

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
 Data File : BN030624.D
 Acq On : 03 Apr 2024 12:12
 Operator : MA/JU
 Sample : P1934-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0R40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030624.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	32	35	46	rVB	49543	75179	0.91%	0.110%
2	3.605	102	105	126	rBV	161438	277408	3.38%	0.407%
3	3.922	154	159	166	rVB2	10182	18673	0.23%	0.027%
4	6.857	650	658	669	rVB	212645	332099	4.04%	0.487%
5	7.034	681	688	703	rBV	962360	1499699	18.25%	2.201%
6	7.222	713	720	731	rBV	865803	1337261	16.28%	1.963%
7	7.316	733	736	742	rVB5	6971	10064	0.12%	0.015%
8	7.693	792	800	815	rVB	927743	1448362	17.63%	2.126%
9	8.287	897	901	906	rVB7	5735	9628	0.12%	0.014%
10	8.393	911	919	933	rBV	668396	1057070	12.87%	1.551%
11	8.846	989	996	1007	rBV	1125188	1814122	22.08%	2.662%
12	9.257	1060	1066	1072	rVB	20222	31365	0.38%	0.046%
13	9.563	1110	1118	1133	rBV	734792	1176086	14.31%	1.726%
14	10.093	1201	1208	1227	rBV	1245247	2064092	25.12%	3.029%
15	10.475	1264	1273	1286	rBV	1315510	2225686	27.09%	3.267%
16	10.616	1289	1297	1312	rVV	788100	1337864	16.28%	1.963%
17	11.257	1402	1406	1415	rBV9	4544	8918	0.11%	0.013%
18	11.751	1484	1490	1495	rVB	14290	22449	0.27%	0.033%
19	12.069	1538	1544	1550	rVB2	24565	37269	0.45%	0.055%
20	13.234	1736	1742	1749	rBV3	18052	30387	0.37%	0.045%
21	13.751	1823	1830	1842	rBV	2737242	3687925	44.88%	5.413%
22	14.028	1867	1877	1888	rBV	3102965	4501486	54.79%	6.607%
23	14.334	1922	1929	1943	rBV	2121612	3076373	37.44%	4.515%
24	14.534	1958	1963	1979	rBV	161671	270566	3.29%	0.397%
25	14.757	1995	2001	2007	rBV9	4998	11387	0.14%	0.017%
26	15.145	2063	2067	2075	rBV4	9409	20277	0.25%	0.030%
27	15.334	2092	2099	2111	rBV	3974282	5756921	70.07%	8.449%
28	15.445	2111	2118	2135	rVV	994256	1343727	16.35%	1.972%
29	15.569	2135	2139	2144	rVB3	19296	29025	0.35%	0.043%
30	16.116	2226	2232	2237	rBV3	13498	17524	0.21%	0.026%
31	16.763	2338	2342	2346	rBV5	7119	10186	0.12%	0.015%
32	17.080	2390	2396	2406	rBV	2516555	3716996	45.24%	5.455%
33	17.186	2407	2414	2432	rVB	4737488	7035579	85.63%	10.326%
34	17.980	2545	2549	2554	rBV2	31460	41187	0.50%	0.060%
35	18.057	2559	2562	2568	rVB2	7186	10109	0.12%	0.015%
36	19.045	2725	2730	2735	rBV3	59319	80952	0.99%	0.119%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030624.D
Acq On : 03 Apr 2024 12:12
Operator : MA/JU
Sample : P1934-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R40

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	19.110	2738	2741	2746	rVV2	46853	63792	0.78%	0.094%
38	19.269	2765	2768	2774	rBV4	26790	35246	0.43%	0.052%
39	19.427	2792	2795	2798	rVB4	12133	10531	0.13%	0.015%
40	19.486	2798	2805	2813	rBV	5813103	8216536	100.00%	12.059%
41	21.321	3111	3117	3128	rBV	2790783	4006774	48.76%	5.880%
42	24.062	3574	3583	3595	rBV2	3252886	7510739	91.41%	11.023%
43	24.262	3609	3617	3640	rVB	1498425	3869191	47.09%	5.679%




Sum of corrected areas: 68136710

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030624.D
Acq On : 03 Apr 2024 12:12
Operator : MA/JU
Sample : P1934-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R40

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

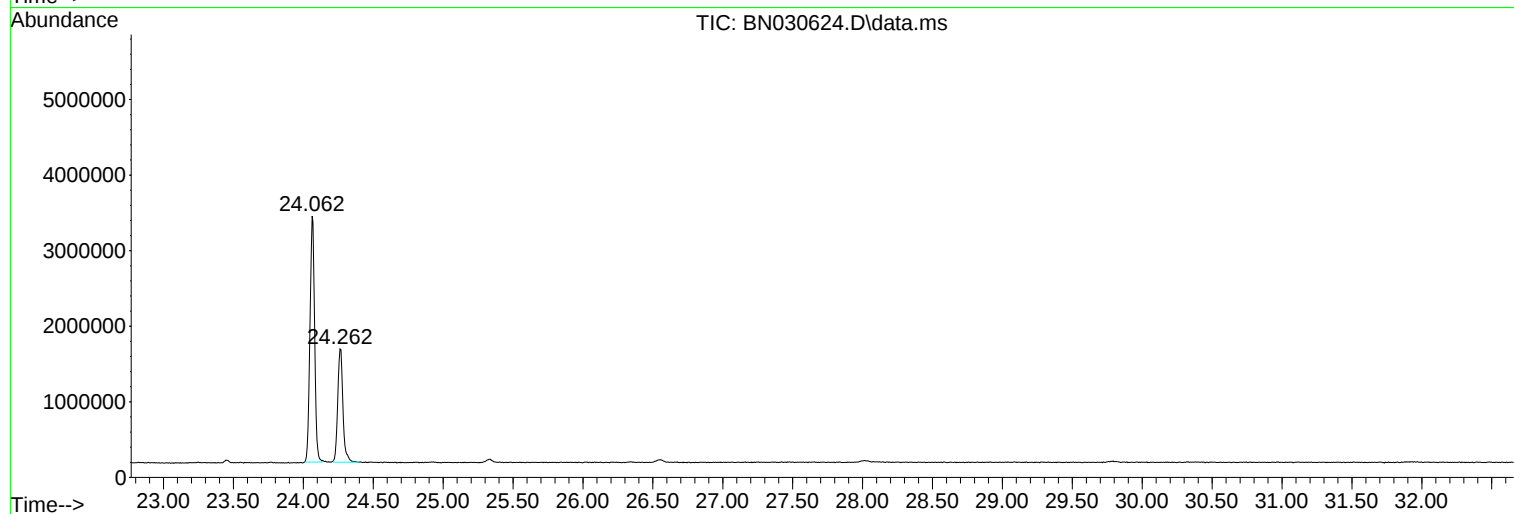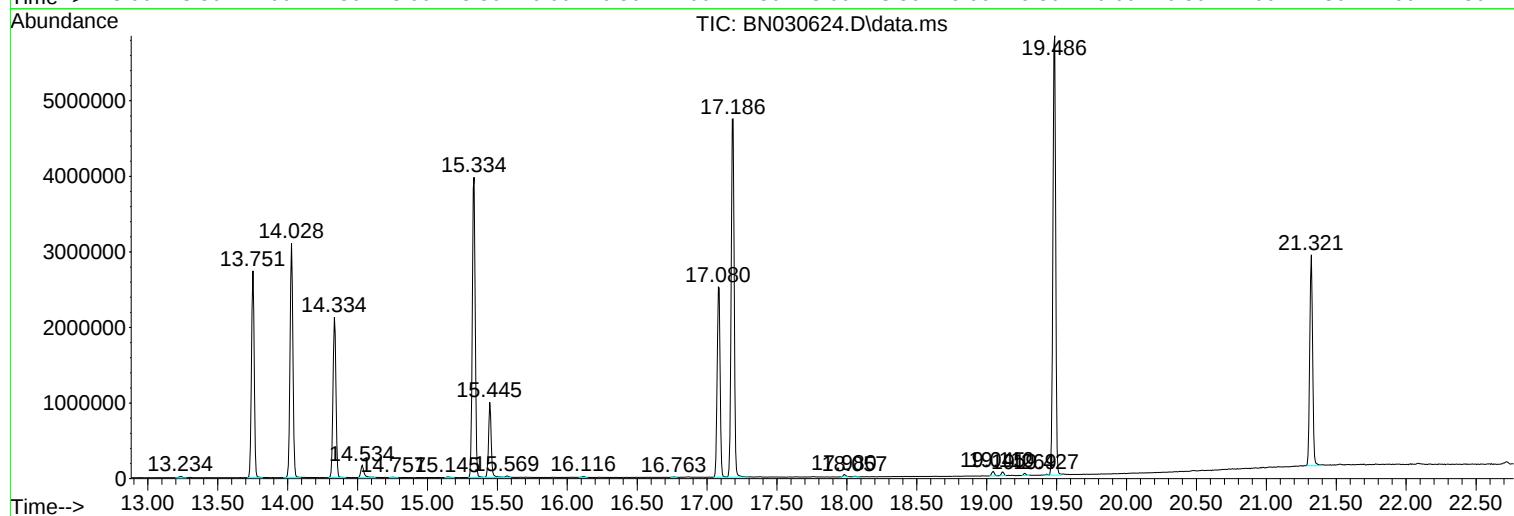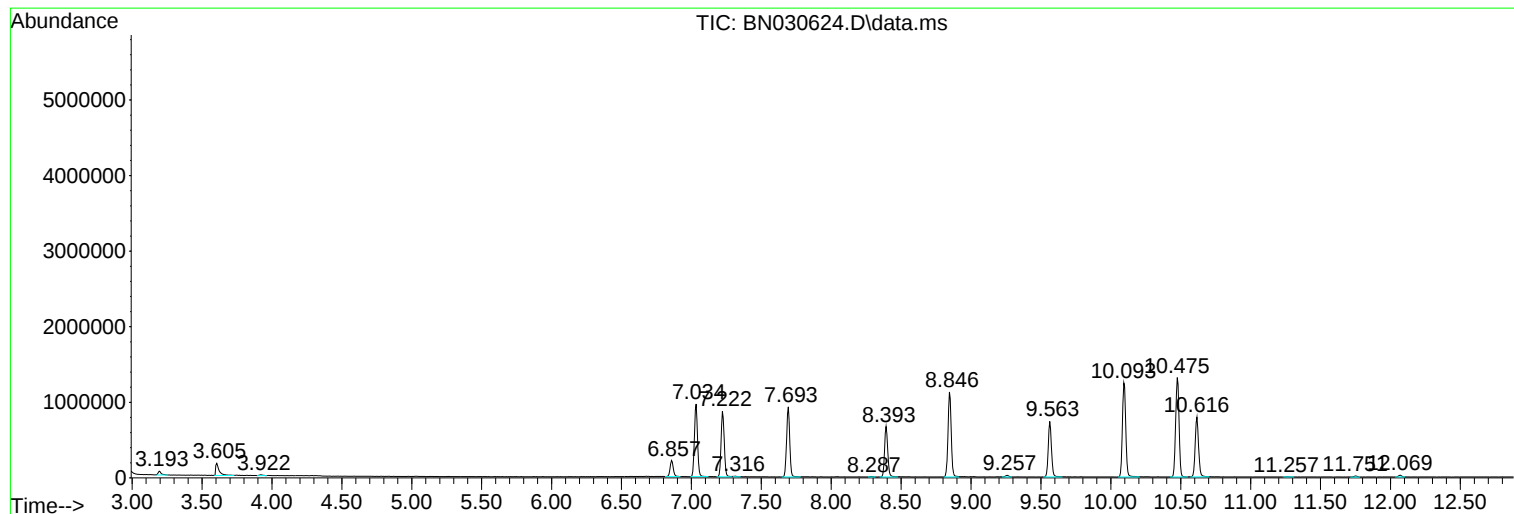

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030624.D
Acq On : 03 Apr 2024 12:12
Operator : MA/JU
Sample : P1934-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R40

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030624.D
Acq On : 03 Apr 2024 12:12
Operator : MA/JU
Sample : P1934-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R40

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------