

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
 Data File : BN030630.D
 Acq On : 03 Apr 2024 16:09
 Operator : MA/JU
 Sample : P1934-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0R38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030630.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	45	rVB	50100	77085	0.93%	0.110%
2	3.605	103	105	123	rBV	164230	268772	3.25%	0.385%
3	3.922	156	159	165	rVB2	13275	15857	0.19%	0.023%
4	6.858	652	658	668	rVB	261253	415891	5.02%	0.595%
5	7.034	680	688	704	rVB	1008484	1562137	18.86%	2.236%
6	7.222	713	720	732	rBV	966214	1521313	18.37%	2.177%
7	7.311	732	735	739	rVB5	6032	8836	0.11%	0.013%
8	7.693	792	800	808	rBV	825082	1305868	15.77%	1.869%
9	8.287	897	901	906	rVB7	7531	11374	0.14%	0.016%
10	8.393	911	919	931	rBV	791226	1257413	15.18%	1.800%
11	8.846	989	996	1006	rBV	1203781	1963120	23.71%	2.810%
12	9.257	1061	1066	1071	rVV2	19019	28429	0.34%	0.041%
13	9.563	1109	1118	1131	rBV	919197	1487845	17.97%	2.129%
14	10.093	1200	1208	1220	rBV	1391111	2334494	28.19%	3.341%
15	10.475	1265	1273	1281	rBV	1250376	2033564	24.56%	2.910%
16	10.616	1289	1297	1312	rBV	786013	1355391	16.37%	1.940%
17	11.751	1484	1490	1495	rVB3	14637	23611	0.29%	0.034%
18	12.069	1538	1544	1552	rVB	29954	46186	0.56%	0.066%
19	13.146	1722	1727	1731	rBV4	10756	16845	0.20%	0.024%
20	13.234	1737	1742	1747	rVB2	27173	40999	0.50%	0.059%
21	13.751	1823	1830	1847	rBV	2923342	4047624	48.88%	5.793%
22	14.028	1867	1877	1885	rBV2	3338385	4942600	59.69%	7.074%
23	14.334	1922	1929	1938	rBV	1958474	2823069	34.09%	4.040%
24	14.534	1957	1963	1971	rBV	245341	379238	4.58%	0.543%
25	14.757	1996	2001	2007	rVB9	9101	16274	0.20%	0.023%
26	15.145	2063	2067	2076	rBV4	8793	14827	0.18%	0.021%
27	15.334	2091	2099	2104	rBV	4226098	6206058	74.94%	8.882%
28	15.445	2112	2118	2131	rBV	1169846	1671679	20.19%	2.393%
29	15.569	2134	2139	2147	rVB2	22619	38681	0.47%	0.055%
30	15.904	2189	2196	2198	rBV7	4803	10117	0.12%	0.014%
31	16.034	2210	2218	2221	rBV8	4365	10302	0.12%	0.015%
32	16.116	2228	2232	2238	rVB4	15311	21170	0.26%	0.030%
33	16.763	2338	2342	2345	rBV5	7941	9673	0.12%	0.014%
34	17.081	2390	2396	2406	rBV	2328323	3399564	41.05%	4.866%
35	17.181	2406	2413	2425	rBV2	4878748	7236938	87.39%	10.358%
36	17.375	2442	2446	2451	rVB3	5612	9125	0.11%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030630.D
Acq On : 03 Apr 2024 16:09
Operator : MA/JU
Sample : P1934-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R38

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	17.763	2509	2512	2516	rVB6	6467	9779	0.12%	0.014%
38	17.857	2524	2528	2533	rBV7	7040	11339	0.14%	0.016%
39	17.981	2545	2549	2555	rBV3	45626	68681	0.83%	0.098%
40	19.045	2725	2730	2735	rBV2	73476	100964	1.22%	0.145%
41	19.116	2738	2742	2746	rVV	61920	76501	0.92%	0.109%
42	19.275	2765	2769	2775	rBV5	31394	43221	0.52%	0.062%
43	19.428	2792	2795	2798	rBV4	14796	17544	0.21%	0.025%
44	19.486	2798	2805	2813	rVV	5998078	8280974	100.00%	11.852%
45	21.322	3112	3117	3130	rVB2	2561570	3616142	43.67%	5.175%
46	24.068	3574	3584	3597	rBV2	3019012	7597621	91.75%	10.874%
47	24.268	3609	3618	3635	rVB	1300076	3436001	41.49%	4.918%




Sum of corrected areas: 69870736

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030630.D
Acq On : 03 Apr 2024 16:09
Operator : MA/JU
Sample : P1934-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R38

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

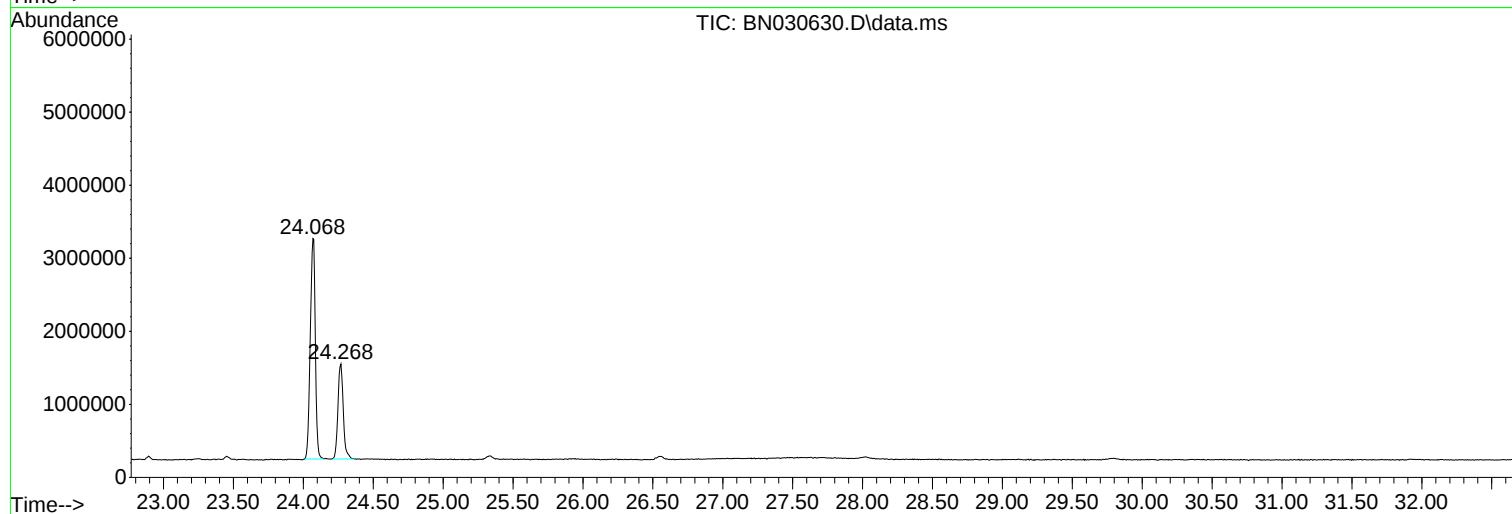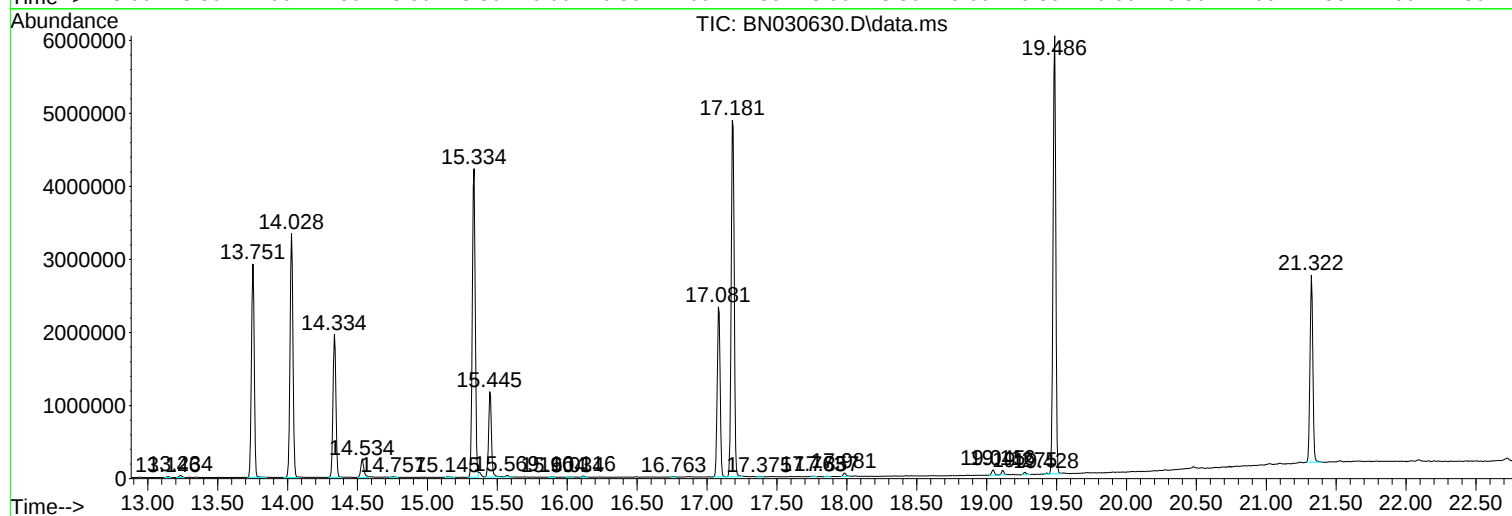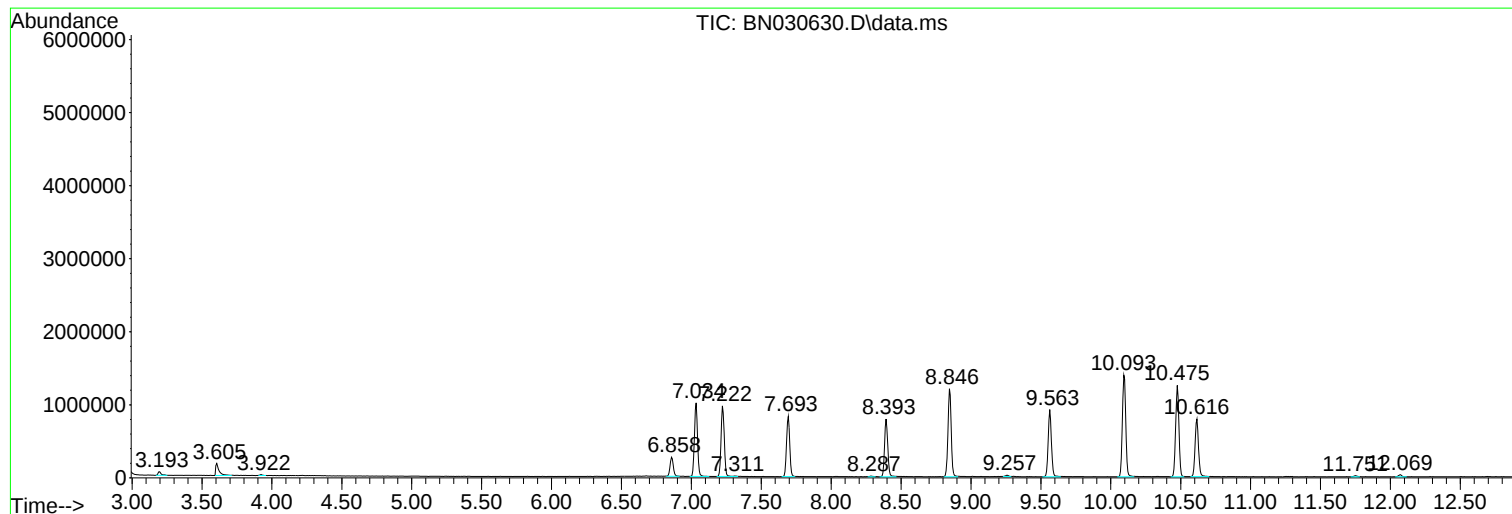

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030630.D
Acq On : 03 Apr 2024 16:09
Operator : MA/JU
Sample : P1934-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R38

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030630.D
Acq On : 03 Apr 2024 16:09
Operator : MA/JU
Sample : P1934-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0R38

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
