

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
 Data File : BN030636.D
 Acq On : 03 Apr 2024 20:46
 Operator : MA/JU
 Sample : PB159839BL
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK839

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030636.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	46	rVB	72129	99814	1.46%	0.143%
2	3.599	101	104	124	rBV	1007356	1594542	23.35%	2.278%
3	3.917	156	158	163	rVB3	10592	13388	0.20%	0.019%
4	6.858	650	658	674	rVB	1145424	1793284	26.27%	2.562%
5	7.034	681	688	702	rBV	934414	1457331	21.34%	2.082%
6	7.222	713	720	732	rBV	1161453	1800459	26.37%	2.572%
7	7.693	792	800	810	rBV	897596	1441340	21.11%	2.059%
8	8.393	912	919	931	rBV	1467991	2303144	33.73%	3.290%
9	8.846	988	996	1008	rBV	1107896	1802613	26.40%	2.575%
10	9.563	1105	1118	1129	rBV	890943	1456707	21.34%	2.081%
11	10.093	1201	1208	1224	rBV	1445838	2392305	35.04%	3.417%
12	10.475	1265	1273	1283	rBV	1348897	2243782	32.86%	3.205%
13	10.616	1289	1297	1313	rBV	1202862	2033450	29.78%	2.905%
14	11.740	1481	1488	1494	rBV8	4250	11607	0.17%	0.017%
15	12.069	1539	1544	1550	rVB	24843	39257	0.57%	0.056%
16	13.234	1736	1742	1749	rVB4	25440	40543	0.59%	0.058%
17	13.298	1749	1753	1757	rBV5	5118	7700	0.11%	0.011%
18	13.751	1820	1830	1841	rBV	2613247	3634026	53.23%	5.191%
19	14.028	1869	1877	1887	rBV	3115740	4464086	65.38%	6.376%
20	14.334	1922	1929	1940	rBV	2099143	3141318	46.01%	4.487%
21	14.422	1940	1944	1949	rVB6	4135	6919	0.10%	0.010%
22	14.534	1957	1963	1975	rBV	1229908	1782200	26.10%	2.546%
23	14.751	1997	2000	2004	rVB6	6212	7514	0.11%	0.011%
24	15.334	2091	2099	2108	rBV	3775819	5476419	80.21%	7.822%
25	15.445	2112	2118	2130	rBV	1050881	1420032	20.80%	2.028%
26	15.569	2135	2139	2144	rVB3	18246	28217	0.41%	0.040%
27	16.116	2228	2232	2237	rBV4	13304	16812	0.25%	0.024%
28	16.763	2338	2342	2345	rVB4	5706	7308	0.11%	0.010%
29	16.869	2356	2360	2363	rBV4	7070	8891	0.13%	0.013%
30	17.087	2389	2397	2407	rBV	2559762	3731304	54.65%	5.330%
31	17.181	2407	2413	2426	rVV2	4180894	5891319	86.29%	8.415%
32	17.986	2546	2550	2553	rBV6	7943	9978	0.15%	0.014%
33	18.316	2604	2606	2612	rVB6	6107	8321	0.12%	0.012%
34	19.045	2726	2730	2735	rBV2	56242	70933	1.04%	0.101%
35	19.116	2737	2742	2747	rBV	49105	71895	1.05%	0.103%
36	19.428	2792	2795	2798	rBV3	11732	13239	0.19%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030636.D
Acq On : 03 Apr 2024 20:46
Operator : MA/JU
Sample : PB159839BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK839

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	19.480	2798	2804	2813	rVV	4775324	6827592	100.00%	9.752%
38	21.322	3111	3117	3125	rBV	2668636	3810180	55.81%	5.442%
39	24.063	3574	3583	3597	rBV2	2372177	5610573	82.17%	8.014%
40	24.263	3609	3617	3635	rVB2	1366124	3438599	50.36%	4.912%




Sum of corrected areas: 70008941

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030636.D
Acq On : 03 Apr 2024 20:46
Operator : MA/JU
Sample : PB159839BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK839

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

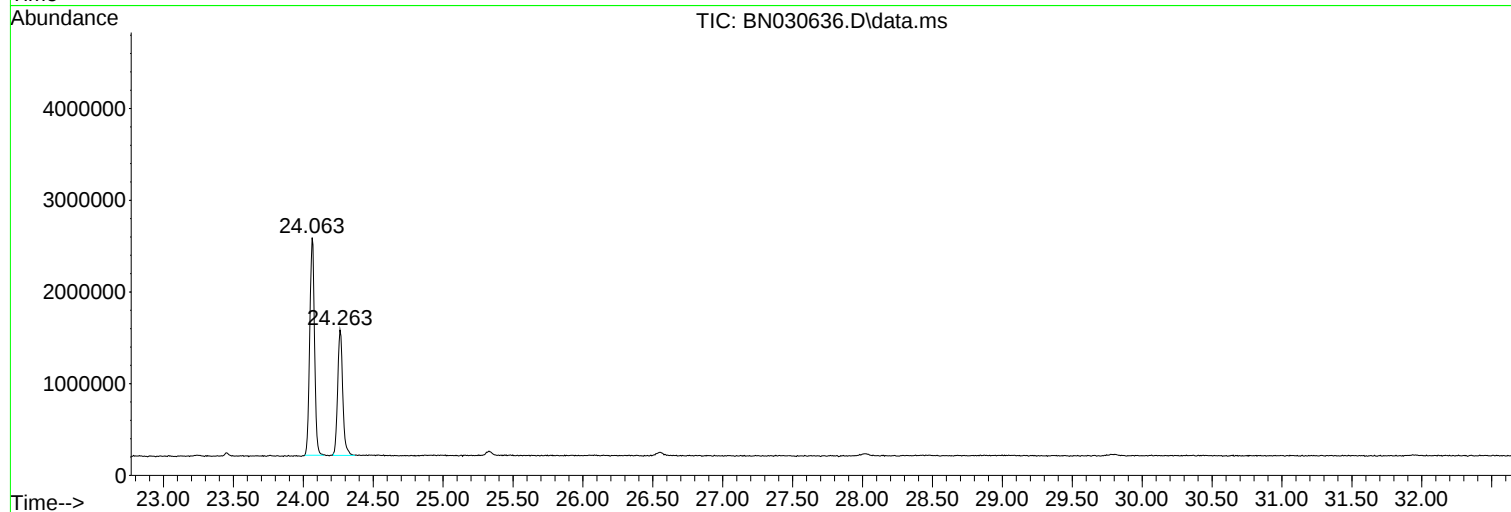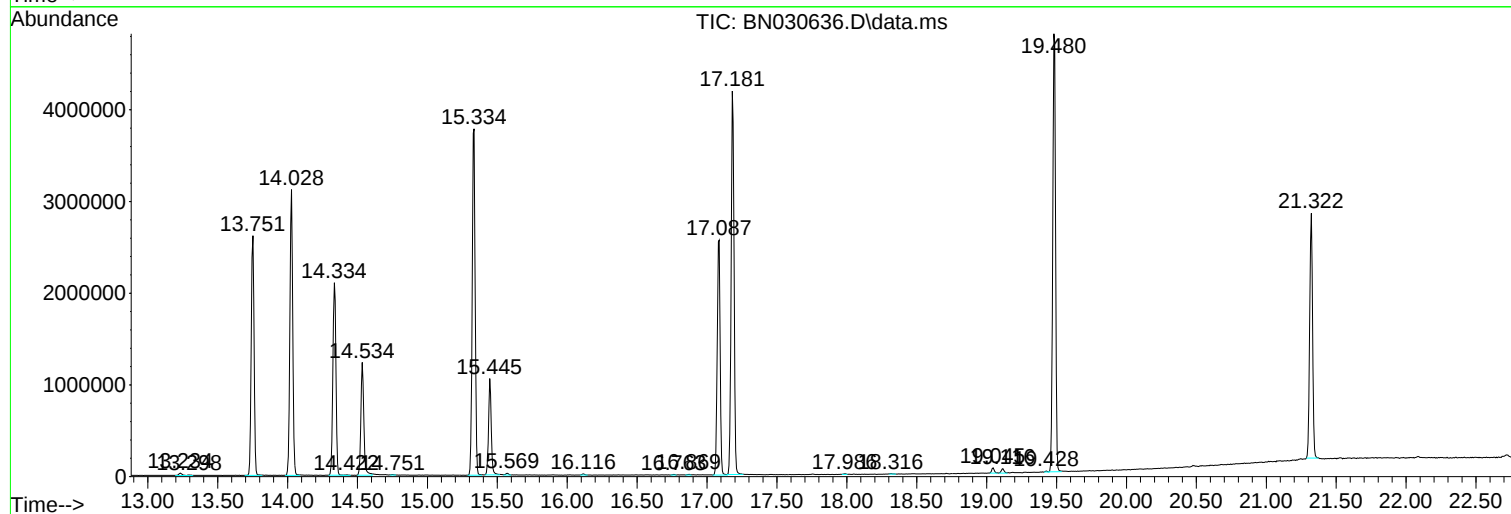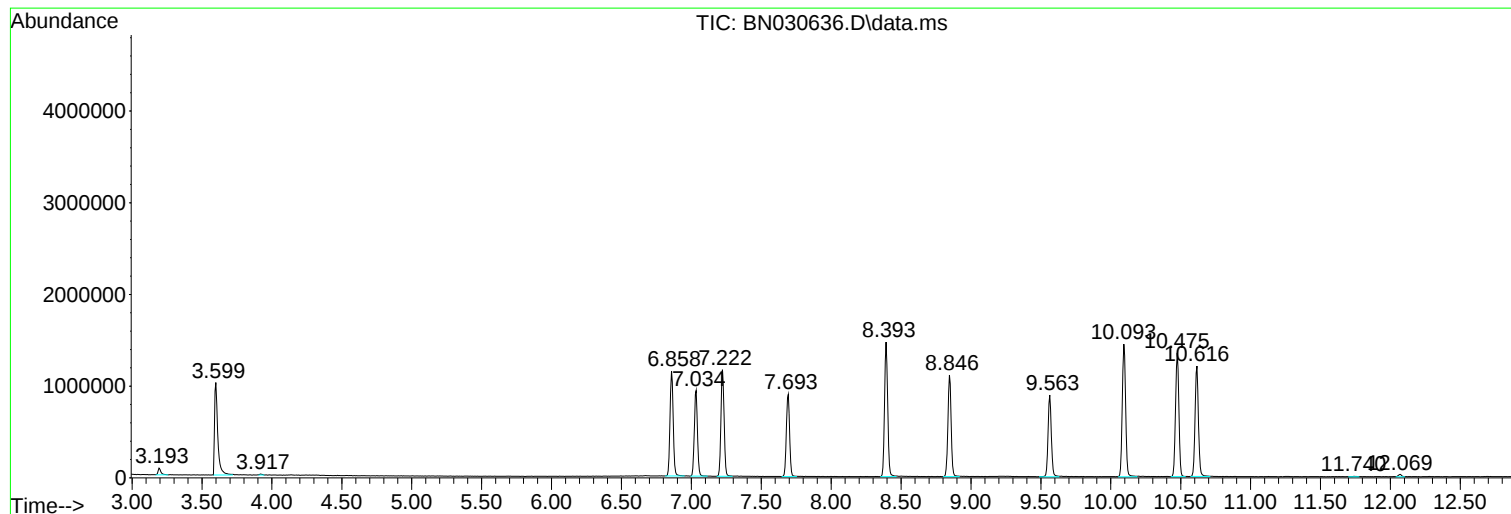

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030636.D
Acq On : 03 Apr 2024 20:46
Operator : MA/JU
Sample : PB159839BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK839

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030636.D
Acq On : 03 Apr 2024 20:46
Operator : MA/JU
Sample : PB159839BL
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK839

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc