

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
 Data File : BN030637.D
 Acq On : 03 Apr 2024 21:25
 Operator : MA/JU
 Sample : PB159947BL
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK947

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030637.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	45	rVB	65231	92401	1.45%	0.138%
2	3.599	100	104	121	rBV	805373	1273018	19.93%	1.900%
3	3.917	155	158	162	rBV3	12266	15875	0.25%	0.024%
4	6.858	651	658	673	rBV	1035159	1612594	25.24%	2.406%
5	7.034	681	688	700	rVB	867900	1333946	20.88%	1.991%
6	7.222	712	720	735	rBV	1048756	1648592	25.81%	2.460%
7	7.693	791	800	808	rBV	912145	1441138	22.56%	2.151%
8	8.393	912	919	930	rBV	1324964	2085484	32.65%	3.112%
9	8.846	989	996	1010	rBV	999237	1627634	25.48%	2.429%
10	9.563	1110	1118	1131	rBV	793238	1280643	20.05%	1.911%
11	10.093	1201	1208	1223	rBV	1283750	2141259	33.52%	3.195%
12	10.475	1264	1273	1281	rBV	1334987	2229224	34.90%	3.327%
13	10.616	1289	1297	1313	rBV	1906811	3171656	49.65%	4.733%
14	12.069	1536	1544	1551	rVB2	23295	38248	0.60%	0.057%
15	13.234	1737	1742	1747	rBV2	16128	25230	0.39%	0.038%
16	13.751	1823	1830	1844	rBV	2414333	3298167	51.63%	4.922%
17	14.028	1869	1877	1892	rBV	2723028	4090909	64.04%	6.105%
18	14.334	1922	1929	1936	rBV	2084648	3107949	48.65%	4.638%
19	14.534	1956	1963	1976	rBV	1114725	1616680	25.31%	2.413%
20	15.328	2091	2098	2108	rBV	3407978	4993505	78.17%	7.452%
21	15.445	2112	2118	2133	rVV	937268	1289270	20.18%	1.924%
22	15.569	2135	2139	2145	rVB3	16391	27347	0.43%	0.041%
23	16.116	2227	2232	2236	rVB4	11640	16881	0.26%	0.025%
24	16.763	2339	2342	2346	rBV5	5401	6661	0.10%	0.010%
25	16.875	2357	2361	2369	rVB3	5724	11302	0.18%	0.017%
26	17.081	2389	2396	2407	rBV	2572363	3694370	57.83%	5.513%
27	17.181	2407	2413	2427	rVV2	3900835	5465801	85.56%	8.156%
28	17.986	2546	2550	2555	rVB8	4978	7471	0.12%	0.011%
29	18.310	2601	2605	2612	rBV8	5274	9879	0.15%	0.015%
30	19.045	2725	2730	2736	rBV2	49294	70332	1.10%	0.105%
31	19.116	2738	2742	2748	rVV	41882	56851	0.89%	0.085%
32	19.427	2792	2795	2797	rBV4	12566	13772	0.22%	0.021%
33	19.486	2798	2805	2813	rBV	4478180	6387937	100.00%	9.533%
34	21.322	3111	3117	3133	rVB	2676666	3845052	60.19%	5.738%
35	24.063	3574	3583	3603	rVB2	2233584	5461318	85.49%	8.150%
36	24.263	3609	3617	3631	rVB	1397219	3523283	55.16%	5.258%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030637.D
Acq On : 03 Apr 2024 21:25
Operator : MA/JU
Sample : PB159947BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK947

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 67011679

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030637.D
Acq On : 03 Apr 2024 21:25
Operator : MA/JU
Sample : PB159947BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK947

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

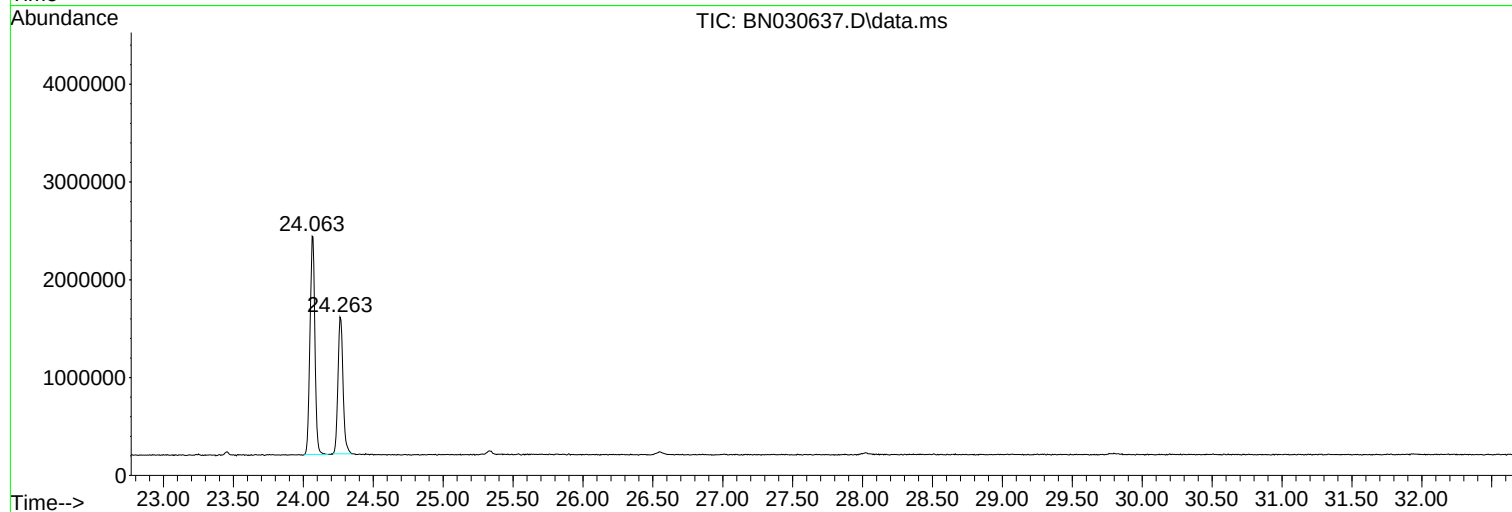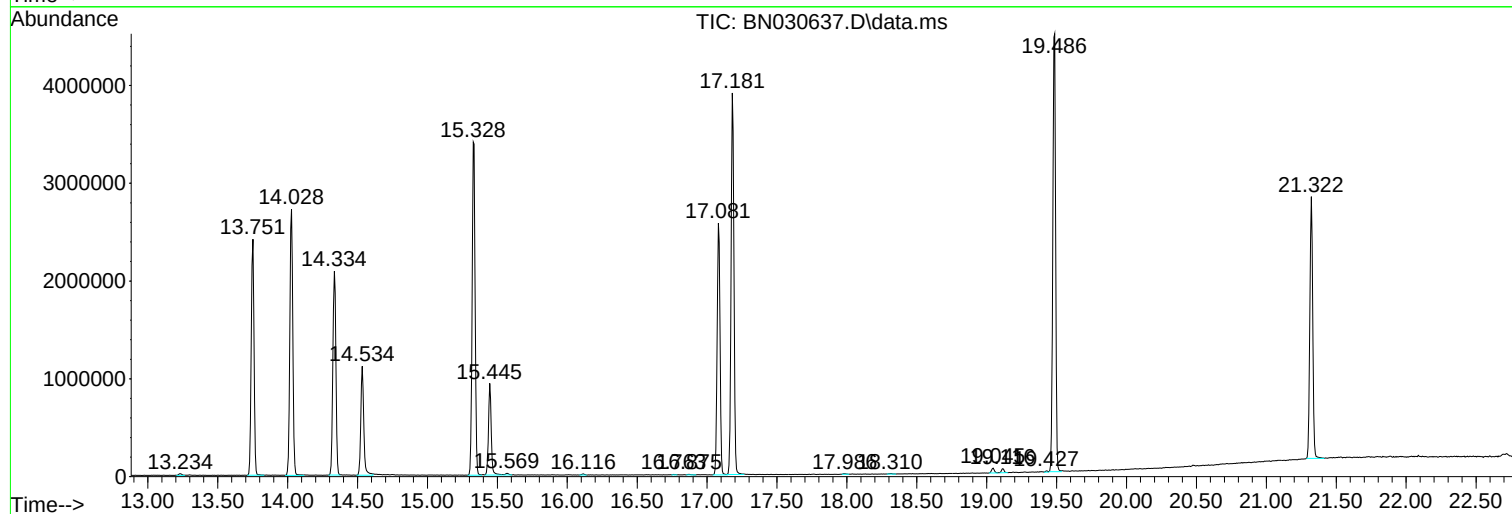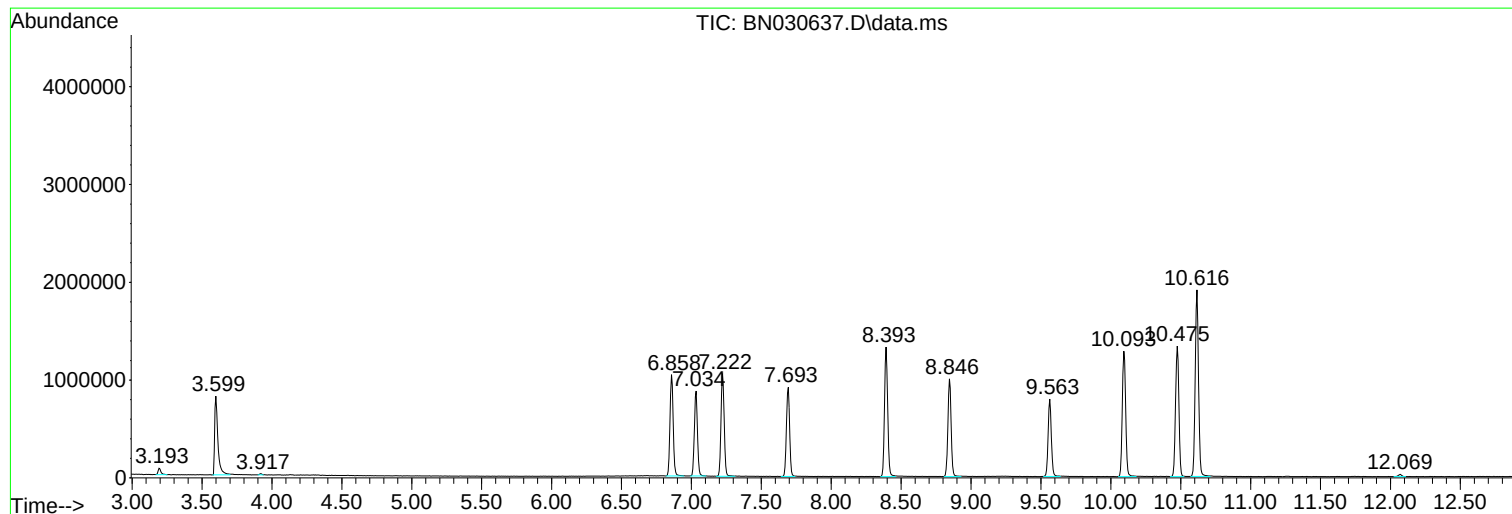

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030637.D
Acq On : 03 Apr 2024 21:25
Operator : MA/JU
Sample : PB159947BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK947

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030637.D
Acq On : 03 Apr 2024 21:25
Operator : MA/JU
Sample : PB159947BL
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK947

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------