

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
 Data File : BN030651.D
 Acq On : 04 Apr 2024 07:13
 Operator : MA/JU
 Sample : PB159945BL
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK945

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	44	rVB	88079	123314	1.54%	0.137%
2	3.599	101	104	126	rBV	1188076	1807899	22.51%	2.014%
3	3.923	155	159	165	rVB	17254	23369	0.29%	0.026%
4	6.687	625	629	634	rVB7	5390	9810	0.12%	0.011%
5	6.864	651	659	675	rBV	1532339	2432346	30.29%	2.710%
6	7.034	681	688	701	rVB	1273673	1936559	24.11%	2.157%
7	7.222	712	720	731	rBV	1542343	2455813	30.58%	2.736%
8	7.693	793	800	811	rBV	1192966	1872312	23.31%	2.086%
9	8.393	912	919	931	rBV	1908248	3132339	39.00%	3.489%
10	8.846	989	996	1006	rBV	1488611	2454444	30.56%	2.734%
11	9.563	1110	1118	1130	rBV	1263900	2089271	26.02%	2.327%
12	10.099	1201	1209	1221	rBV	1945060	3259342	40.59%	3.631%
13	10.475	1266	1273	1285	rBV	1752316	2923298	36.40%	3.256%
14	10.616	1289	1297	1314	rBV	2516269	4262414	53.08%	4.748%
15	11.263	1403	1407	1410	rBV5	7155	10910	0.14%	0.012%
16	12.069	1538	1544	1552	rVB2	36368	64397	0.80%	0.072%
17	13.234	1737	1742	1748	rBV	26976	43036	0.54%	0.048%
18	13.304	1749	1754	1759	rVB5	6552	11557	0.14%	0.013%
19	13.751	1823	1830	1847	rVB	3534301	4834856	60.20%	5.386%
20	14.028	1868	1877	1886	rBV2	4018344	5969598	74.33%	6.650%
21	14.334	1922	1929	1939	rBV	2713052	4042771	50.34%	4.504%
22	14.540	1955	1964	1984	rBV	1631133	2481028	30.89%	2.764%
23	14.693	1988	1990	1996	rVV7	8170	17487	0.22%	0.019%
24	14.751	1996	2000	2007	rVB9	7169	16855	0.21%	0.019%
25	15.334	2092	2099	2108	rBV	4941341	7132480	88.81%	7.945%
26	15.451	2112	2119	2132	rVV	1458783	2004390	24.96%	2.233%
27	15.569	2135	2139	2145	rVB2	24117	38776	0.48%	0.043%
28	16.116	2225	2232	2238	rBV4	18625	32070	0.40%	0.036%
29	16.763	2338	2342	2347	rBV5	8303	11910	0.15%	0.013%
30	16.869	2357	2360	2365	rBV2	7356	9969	0.12%	0.011%
31	17.087	2390	2397	2407	rBV	3277858	4663122	58.07%	5.195%
32	17.187	2407	2414	2430	rVB	5236399	7594221	94.56%	8.460%
33	17.334	2435	2439	2445	rVV8	10060	20021	0.25%	0.022%
34	17.751	2508	2510	2516	rVB7	6691	9417	0.12%	0.010%
35	17.981	2546	2549	2554	rBV6	12646	16190	0.20%	0.018%
36	18.316	2602	2606	2609	rBV6	5184	9091	0.11%	0.010%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030651.D
Acq On : 04 Apr 2024 07:13
Operator : MA/JU
Sample : PB159945BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK945

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	19.045	2726	2730	2735	rBV	73000	101157	1.26%	0.113%
38	19.116	2738	2742	2748	rVV	60467	84312	1.05%	0.094%
39	19.428	2792	2795	2798	rBV3	23532	28140	0.35%	0.031%
40	19.486	2799	2805	2812	rVV	5831114	8030798	100.00%	8.946%
41	21.327	3112	3118	3125	rVB	2629822	3840910	47.83%	4.279%
42	24.074	3575	3585	3594	rBV2	2664023	6123914	76.26%	6.822%
43	24.274	3610	3619	3635	rVB	1431643	3742410	46.60%	4.169%




Sum of corrected areas: 89768323

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030651.D
Acq On : 04 Apr 2024 07:13
Operator : MA/JU
Sample : PB159945BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK945

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

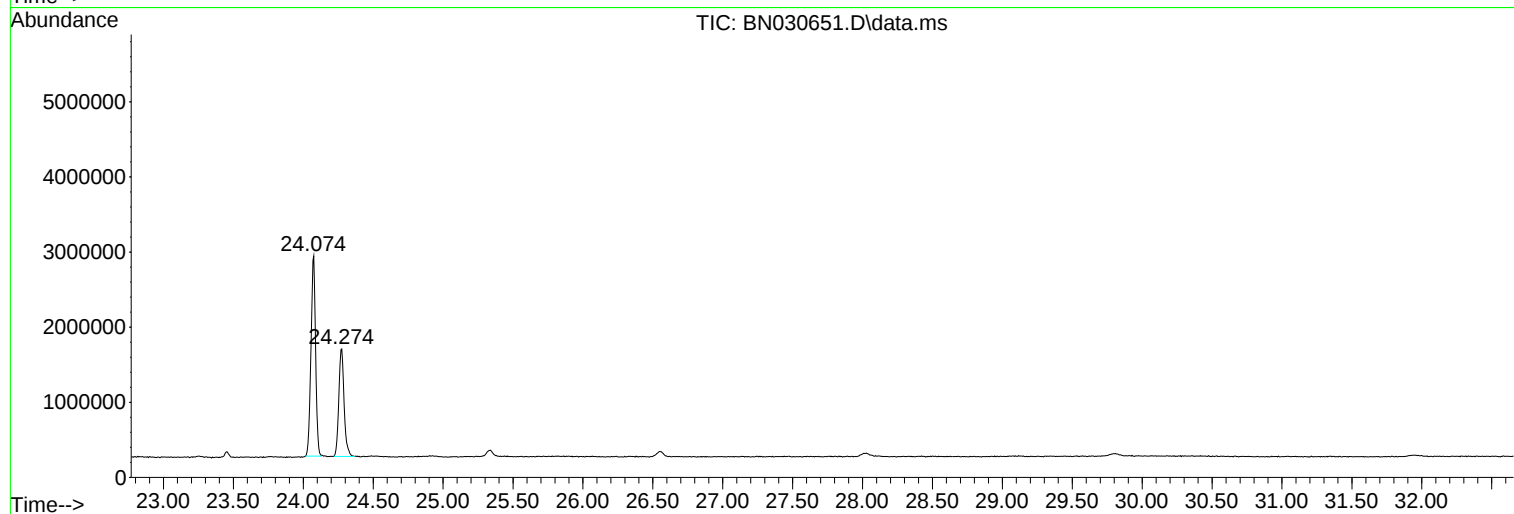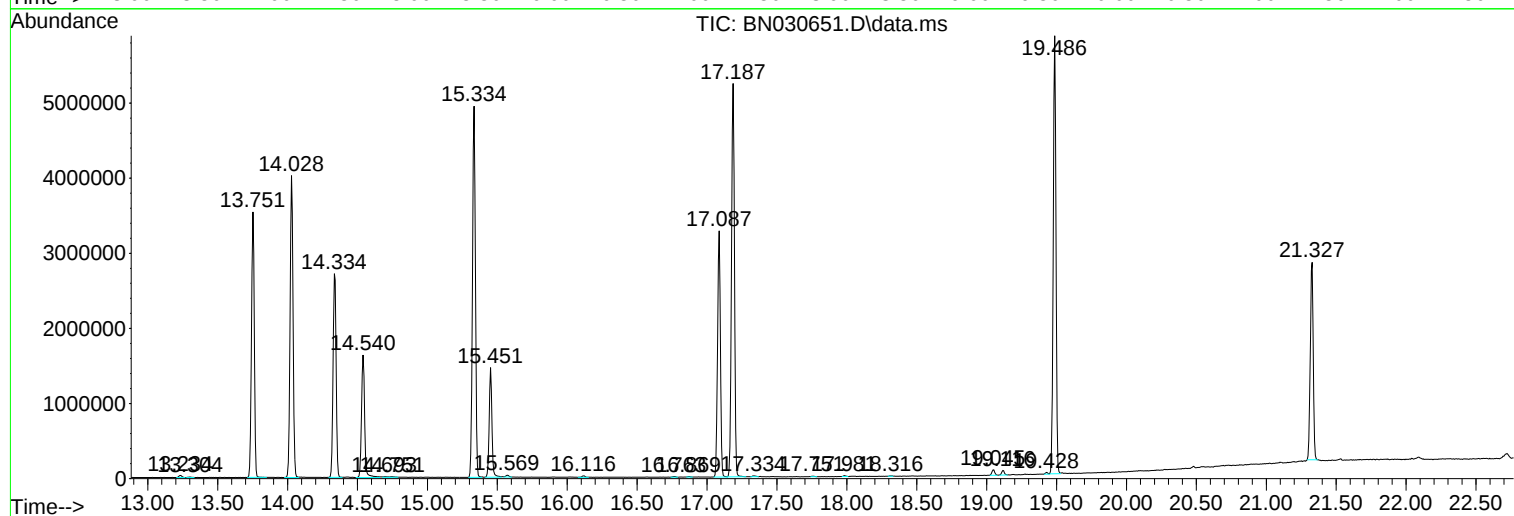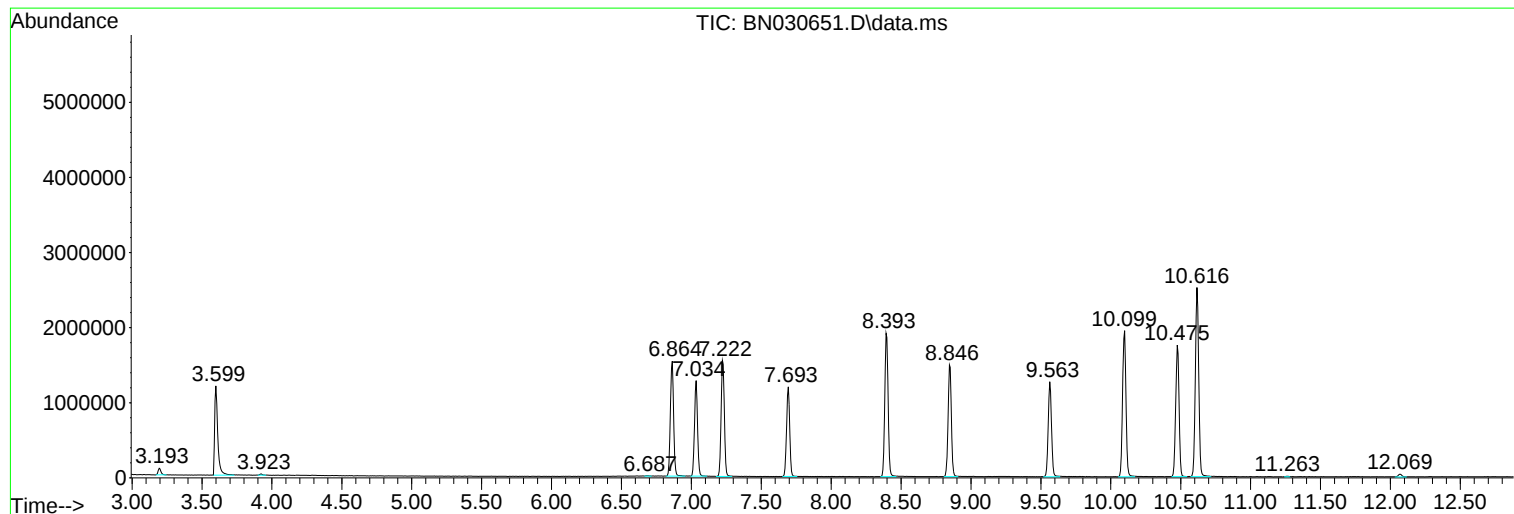

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030651.D
Acq On : 04 Apr 2024 07:13
Operator : MA/JU
Sample : PB159945BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK945

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030651.D
Acq On : 04 Apr 2024 07:13
Operator : MA/JU
Sample : PB159945BL
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK945

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc