

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
 Data File : BN030656.D
 Acq On : 04 Apr 2024 10:32
 Operator : MA/JU
 Sample : P1948-09
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AK7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	38	rBV	49094	63003	0.79%	0.091%
2	3.228	38	41	52	rVB	57719	83895	1.05%	0.122%
3	3.605	102	105	119	rBV	203310	315508	3.96%	0.458%
4	3.922	155	159	163	rVB2	12276	17189	0.22%	0.025%
5	6.675	621	627	634	rBV10	6580	17504	0.22%	0.025%
6	6.858	649	658	669	rVB	219948	365136	4.58%	0.530%
7	7.034	681	688	700	rBV	1058620	1645749	20.65%	2.390%
8	7.222	713	720	732	rBV	953242	1506227	18.90%	2.187%
9	7.316	732	736	741	rVB6	5077	9826	0.12%	0.014%
10	7.693	793	800	808	rBV	808803	1282001	16.09%	1.862%
11	8.393	910	919	931	rBV	729623	1156081	14.51%	1.679%
12	8.846	989	996	1006	rBV	1284629	2101157	26.37%	3.051%
13	9.010	1020	1024	1031	rVB9	6556	12039	0.15%	0.017%
14	9.257	1062	1066	1074	rVB6	7728	16276	0.20%	0.024%
15	9.563	1110	1118	1130	rBV	1028013	1664788	20.89%	2.418%
16	9.893	1169	1174	1182	rBV6	9791	17980	0.23%	0.026%
17	10.093	1200	1208	1221	rBV	1425631	2433034	30.53%	3.533%
18	10.475	1265	1273	1284	rBV	1229306	2011282	25.24%	2.921%
19	10.616	1288	1297	1317	rVB	1270500	2138326	26.83%	3.105%
20	11.263	1401	1407	1414	rVB8	7998	14732	0.18%	0.021%
21	12.069	1536	1544	1550	rBV	32578	53105	0.67%	0.077%
22	13.234	1737	1742	1748	rBV2	30134	49481	0.62%	0.072%
23	13.304	1748	1754	1759	rVB5	5019	8921	0.11%	0.013%
24	13.751	1823	1830	1840	rBV	2953916	4179068	52.44%	6.069%
25	14.028	1870	1877	1886	rBV2	3527138	5261509	66.03%	7.641%
26	14.334	1922	1929	1939	rBV	1926958	2847308	35.73%	4.135%
27	14.428	1942	1945	1951	rVB6	5254	8781	0.11%	0.013%
28	14.534	1957	1963	1976	rBV	211758	367115	4.61%	0.533%
29	14.763	1996	2002	2006	rVB7	10686	16619	0.21%	0.024%
30	15.334	2092	2099	2111	rBV	4415522	6407416	80.41%	9.305%
31	15.451	2112	2119	2133	rVV	1350839	1854718	23.28%	2.693%
32	15.569	2135	2139	2149	rVB2	24376	46139	0.58%	0.067%
33	15.898	2190	2195	2199	rBV7	5777	12055	0.15%	0.018%
34	16.116	2228	2232	2240	rVB6	19710	30715	0.39%	0.045%
35	16.763	2338	2342	2346	rVB5	8490	11305	0.14%	0.016%
36	16.863	2354	2359	2364	rBV4	6134	15337	0.19%	0.022%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
 Data File : BN030656.D
 Acq On : 04 Apr 2024 10:32
 Operator : MA/JU
 Sample : P1948-09
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AK7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	17.086	2387	2397	2406	rBV	2288271	3281527	41.18%	4.765%
38	17.186	2407	2414	2428	rVV2	4979924	7402782	92.90%	10.750%
39	17.333	2435	2439	2444	rVB8	8128	12031	0.15%	0.017%
40	17.375	2444	2446	2453	rVB4	5537	9281	0.12%	0.013%
41	17.451	2453	2459	2473	rBV	84420	168325	2.11%	0.244%
42	17.986	2545	2550	2556	rBV	68025	100781	1.26%	0.146%
43	18.057	2559	2562	2566	rVB2	10654	15243	0.19%	0.022%
44	18.422	2620	2624	2628	rVB4	22943	28357	0.36%	0.041%
45	19.045	2726	2730	2735	rBV2	75210	98471	1.24%	0.143%
46	19.116	2738	2742	2746	rBV	58600	83294	1.05%	0.121%
47	19.275	2765	2769	2776	rBV	52483	70357	0.88%	0.102%
48	19.427	2792	2795	2798	rBV3	21562	22255	0.28%	0.032%
49	19.486	2798	2805	2814	rBV	5761972	7968507	100.00%	11.572%
50	21.321	3112	3117	3130	rVB2	1888632	2791335	35.03%	4.054%
51	24.068	3575	3584	3598	rBV2	2599591	6135566	77.00%	8.910%
52	24.268	3610	3618	3636	rVB	1019349	2632322	33.03%	3.823%




Sum of corrected areas: 68861759

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030656.D
Acq On : 04 Apr 2024 10:32
Operator : MA/JU
Sample : P1948-09
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

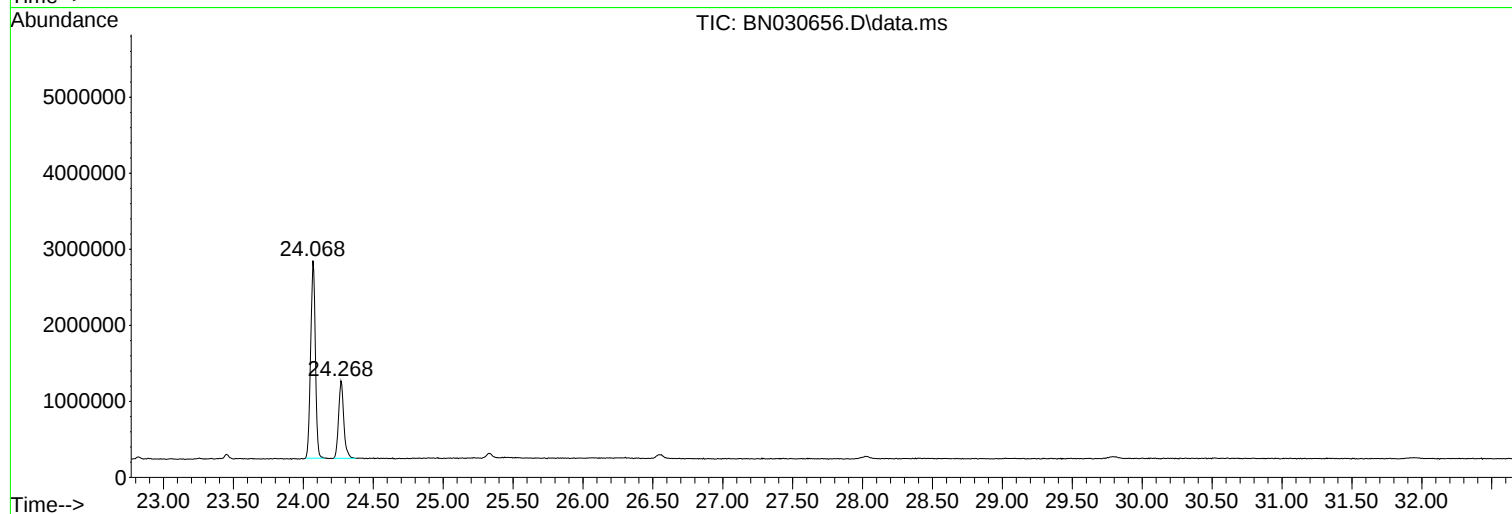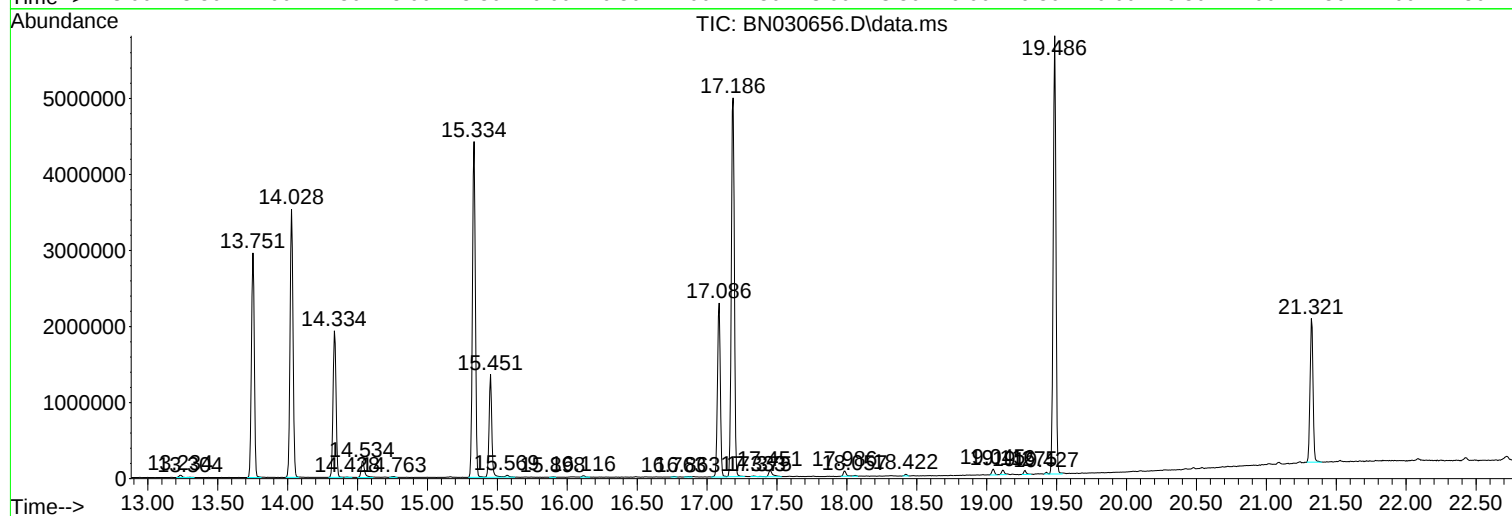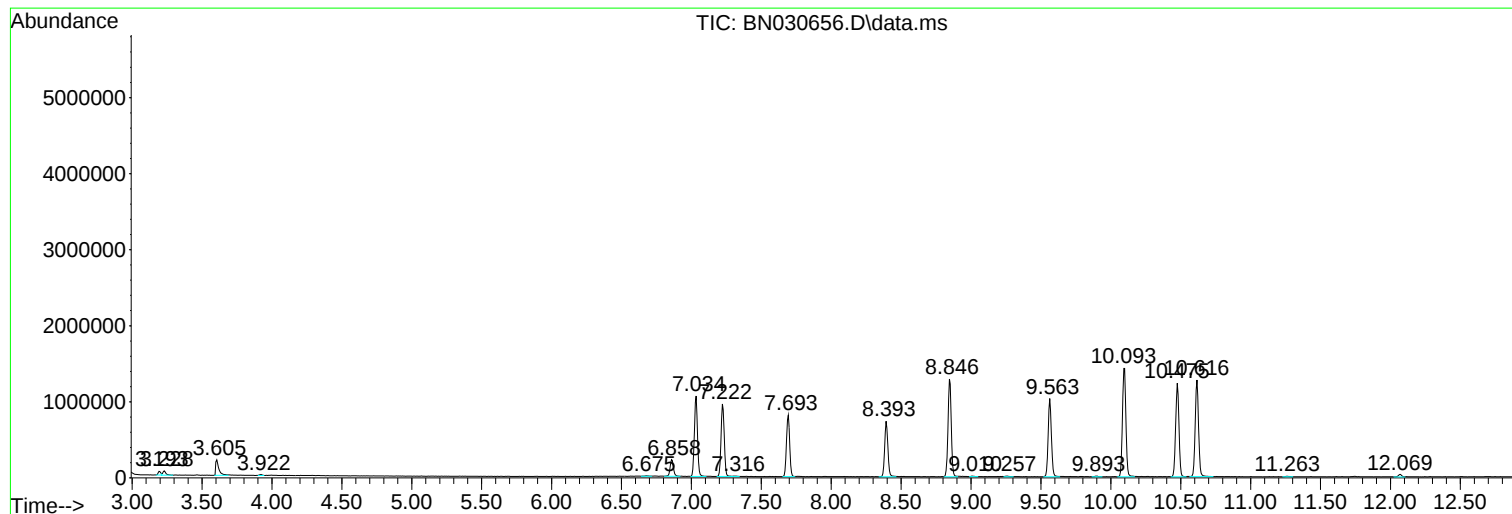

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030656.D
Acq On : 04 Apr 2024 10:32
Operator : MA/JU
Sample : P1948-09
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040424\
Data File : BN030656.D
Acq On : 04 Apr 2024 10:32
Operator : MA/JU
Sample : P1948-09
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc