


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040522\
 Data File : BN019347.D
 Acq On : 05 Apr 2022 11:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Apr 04 17:40:00 2022

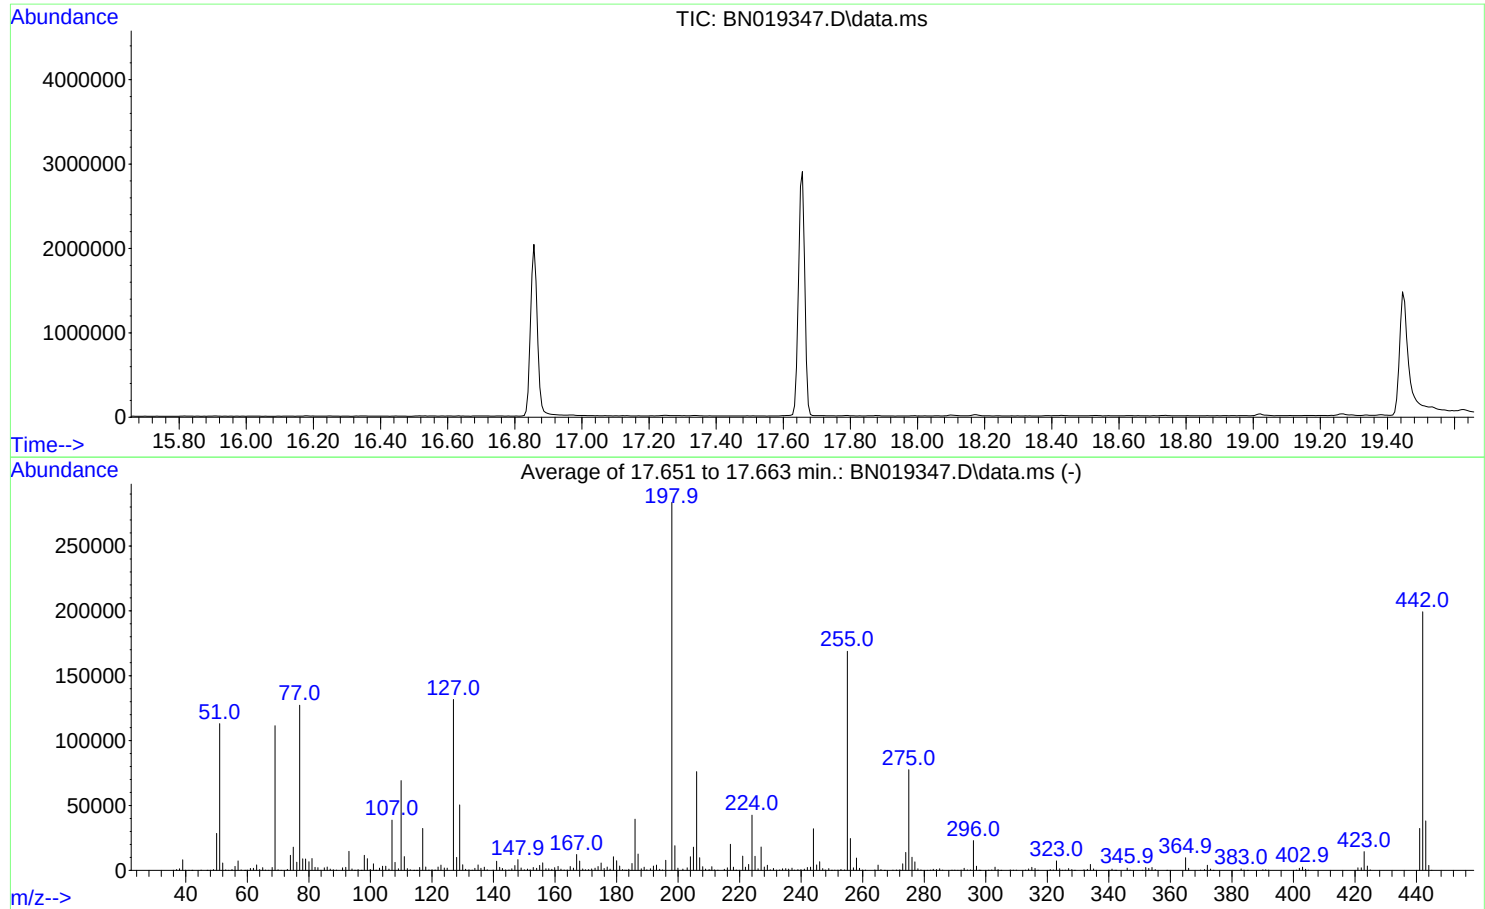




AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2486

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	113116	PASS
68	69	0.00	2	2.0	2222	PASS
69	198	0.00	100	39.3	111433	PASS
70	69	0.00	2	0.5	503	PASS
127	198	10	80	46.5	131693	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	283499	PASS
199	198	5	9	6.7	19004	PASS
275	198	10	60	27.4	77560	PASS
365	198	1	100	3.4	9728	PASS
441	198	0.01	100	11.4	32341	PASS
442	442	50	100	100.0	199253	PASS
443	442	15	24	19.1	38104	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040522\
 Data File : BN019347.D
 Acq On : 05 Apr 2022 11:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Apr 06 03:22:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 23 16:56:32 2022
 Response via : Initial Calibration

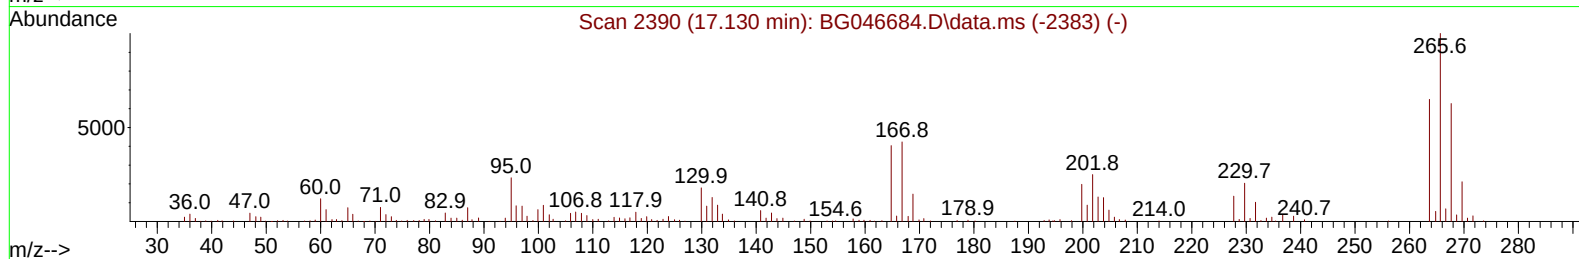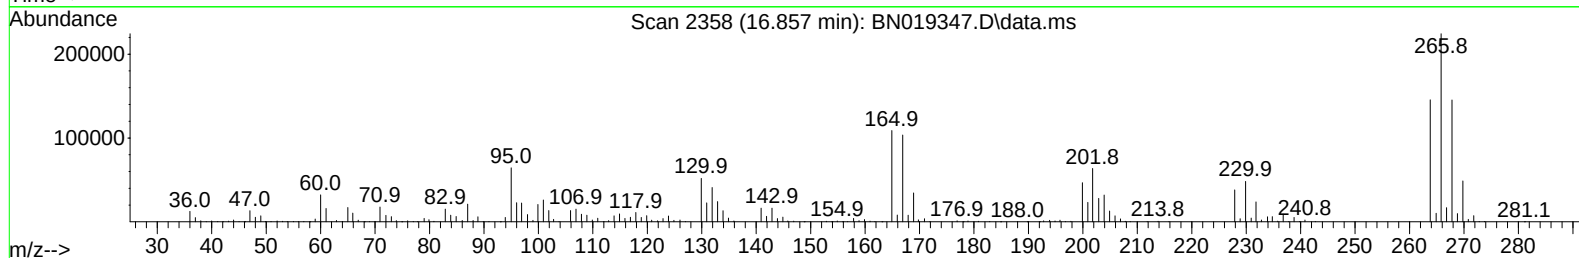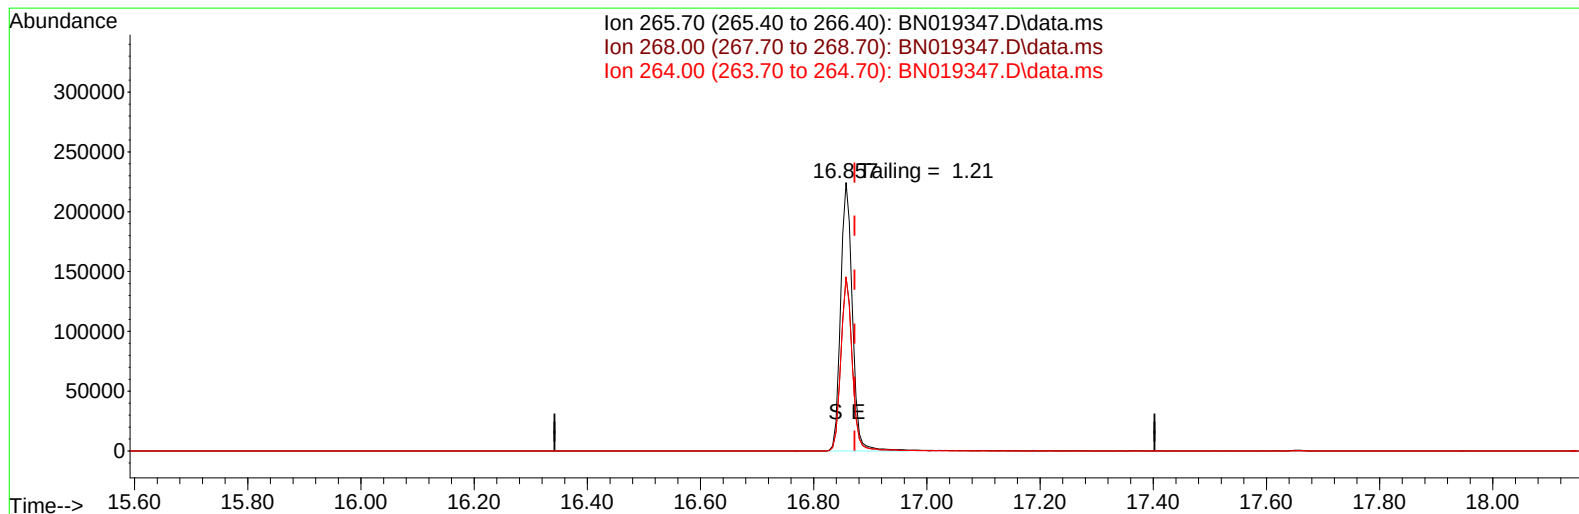

TIC: BN019347.D\data.ms

(70) Pentachlorophenol (C)

16.857min (-0.015) 0.00 ng




response 324872

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.76
264.00	61.60	64.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040522\
Data File : BN019347.D
Acq On : 05 Apr 2022 11:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 06 03:22:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 23 16:56:32 2022
Response via : Initial Calibration

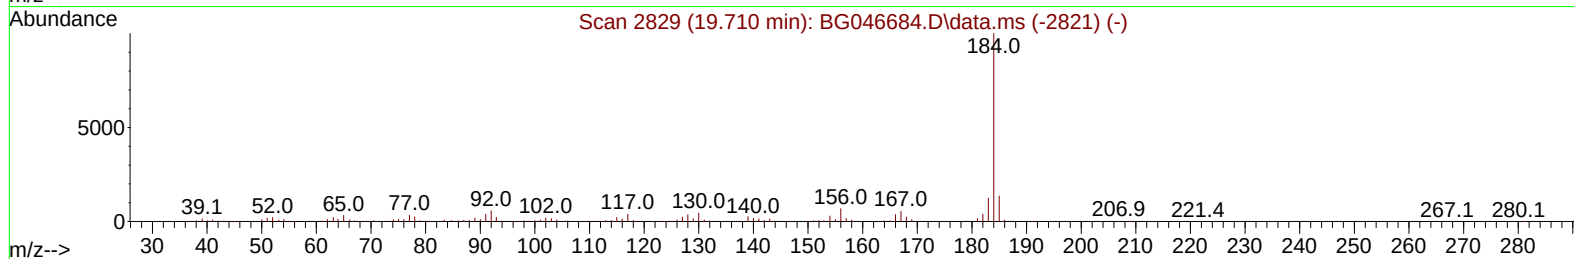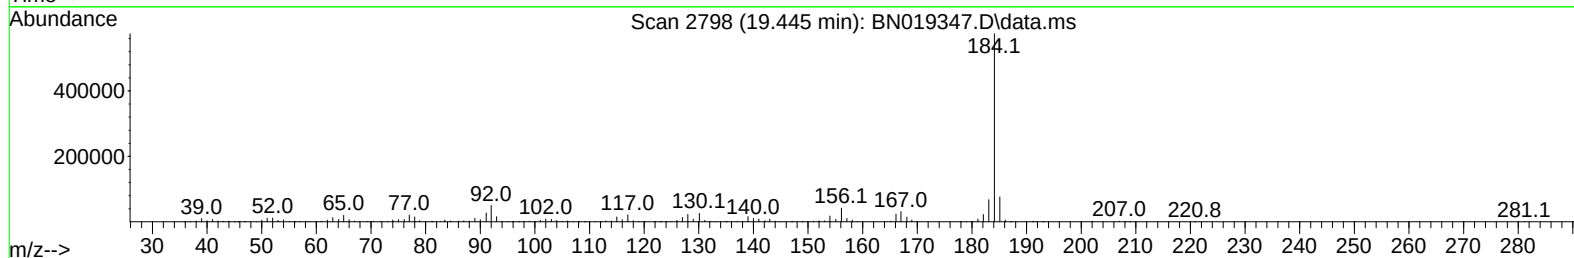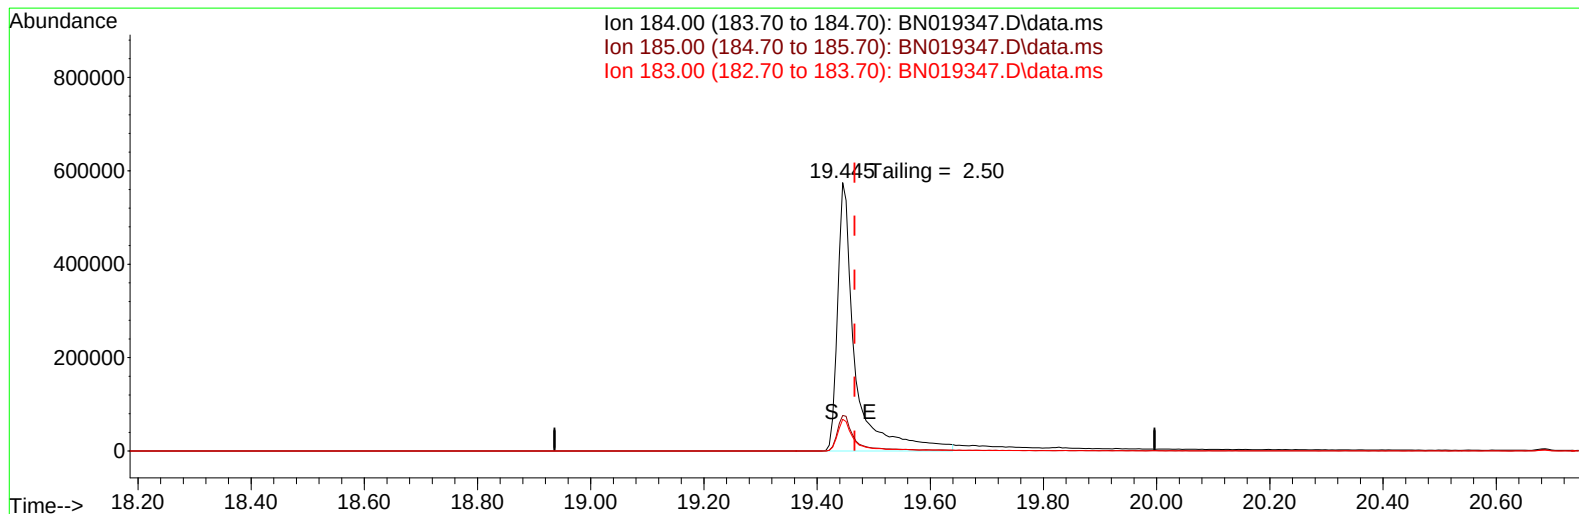

TIC: BN019347.D\data.ms

(77) Benzidine

19.445min (-0.021) 744033.50 ng

response 1261431

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.24
183.00	13.20	11.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/5/2022	BNA_N	<u>BN019347.D</u>
Compound Name	Response	Retention Time
DDT	1005053	20.686
DDD	15222	20.245
DDE	1181	19.739
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16403	1021456	1.61

Instrument :
BNA_N
ClientSampleId :
DFTPP