
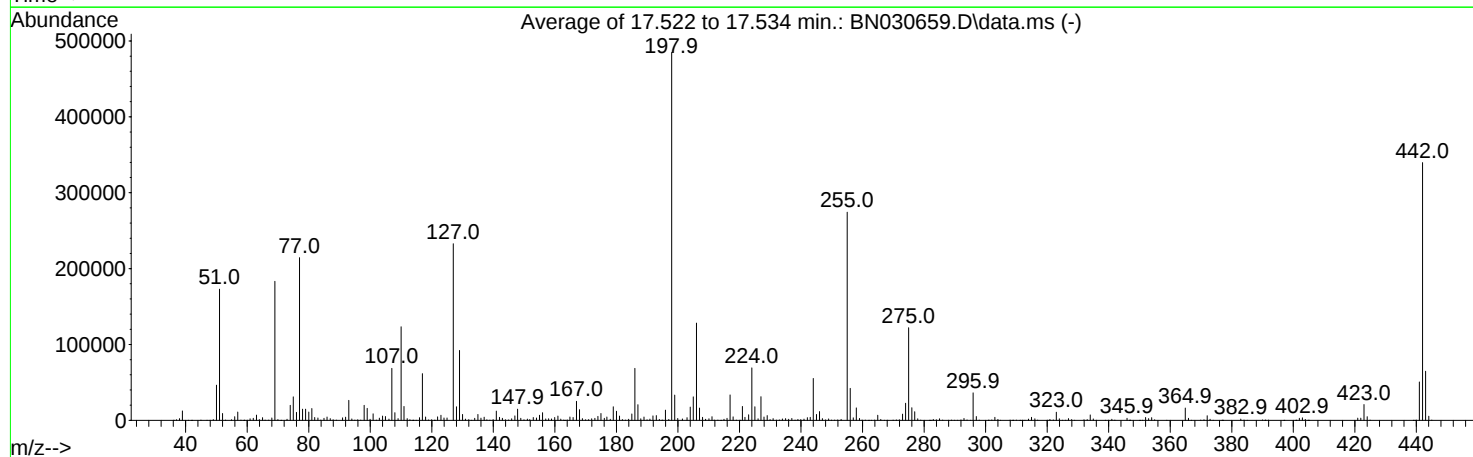


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040524\
Data File : BN030659.D
Acq On : 04 Apr 2024 13:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN033024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Mar 30 00:04:36 2024

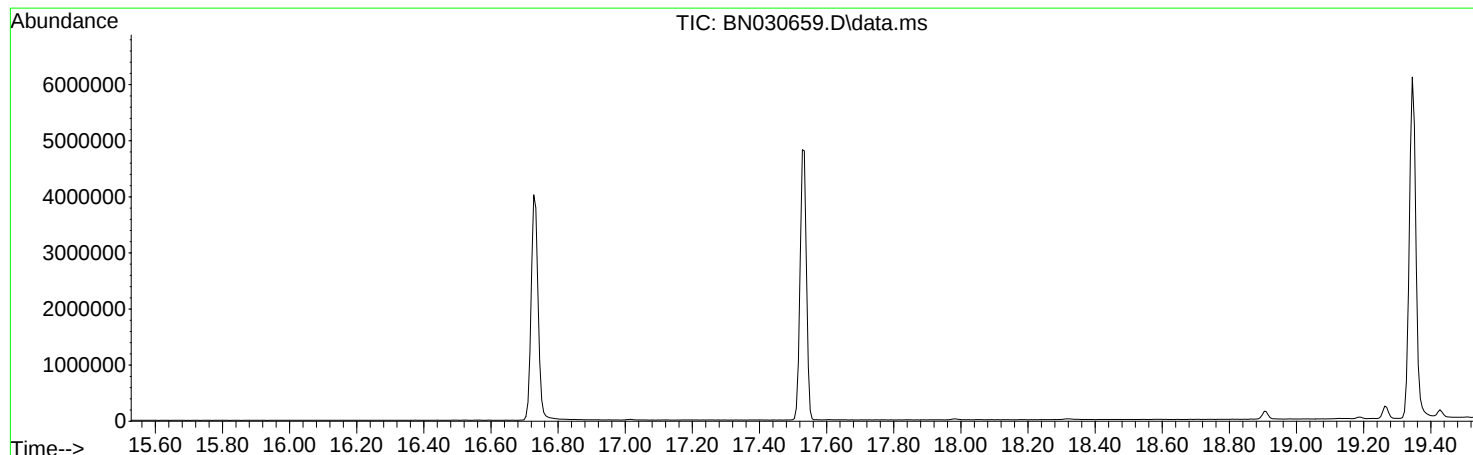




AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2465

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.7	172949	PASS
68	69	0.00	2	1.7	3133	PASS
69	198	0.00	100	37.8	183147	PASS
70	69	0.00	2	0.5	977	PASS
127	198	10	80	48.0	232811	PASS
197	198	0.00	2	0.3	1261	PASS
198	198	100	100	100.0	484779	PASS
199	198	5	9	6.9	33275	PASS
275	198	10	60	25.2	122152	PASS
365	198	1	100	3.3	16184	PASS
441	198	0.01	100	10.4	50611	PASS
442	442	50	100	100.0	339755	PASS
443	442	15	24	19.1	64755	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040524\
Data File : BN030659.D
Acq On : 04 Apr 2024 13:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 05 00:03:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 05 00:03:52 2024
Response via : Initial Calibration

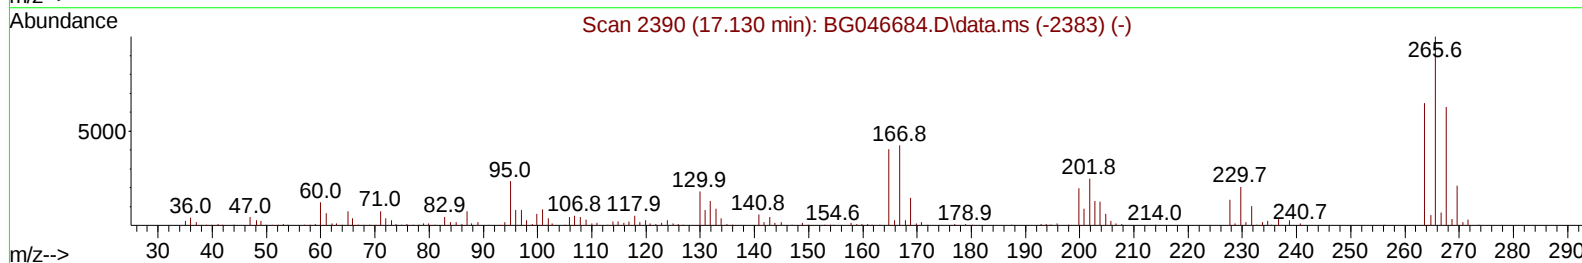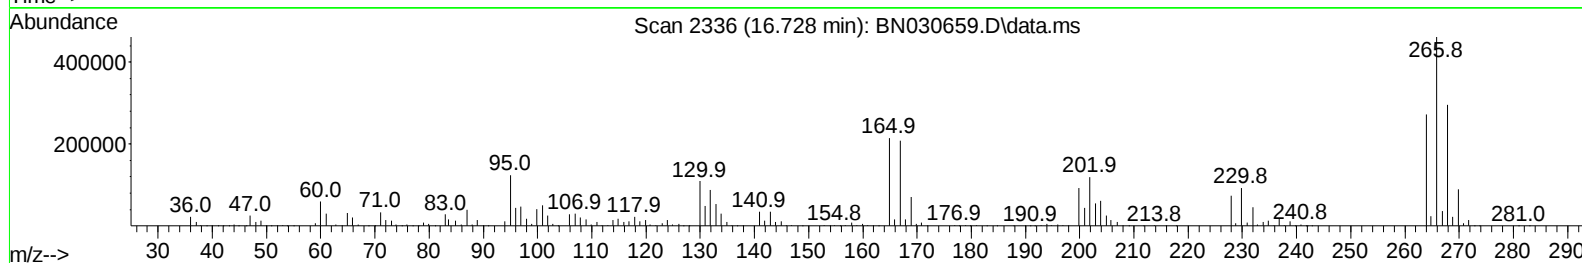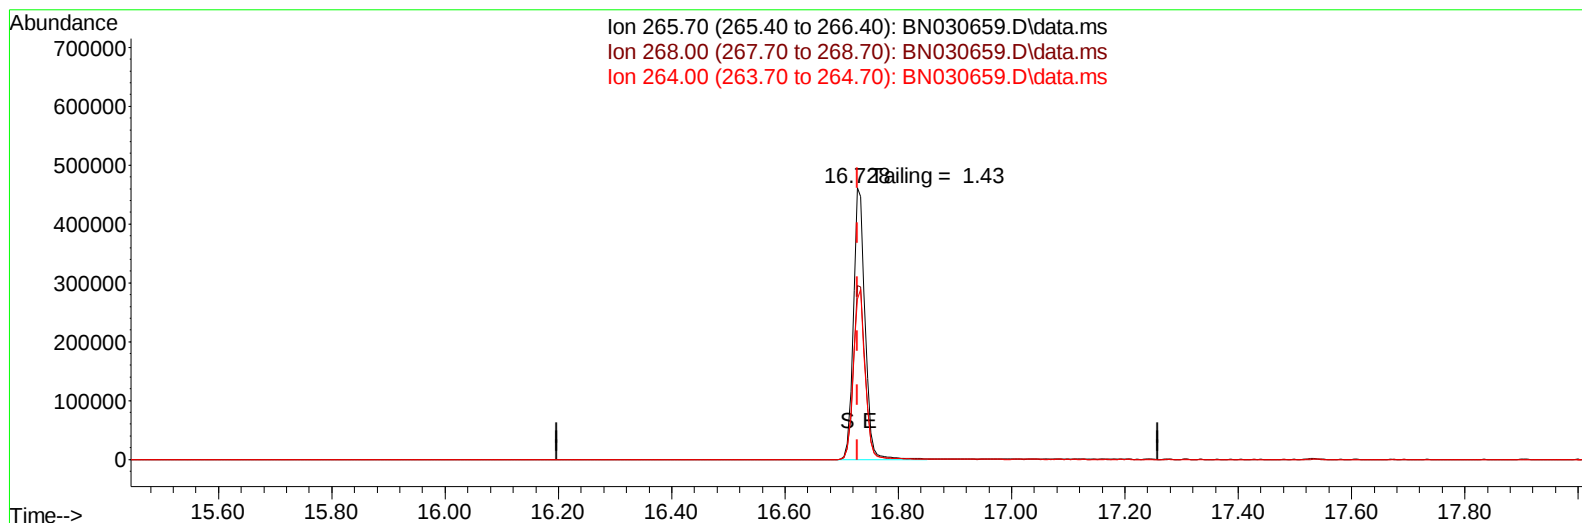

TIC: BN030659.D\data.ms

(70) Pentachlorophenol (C)

16.728min (0.000) 27372.88 ng




response 662491

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.10
264.00	61.60	59.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040524\
Data File : BN030659.D
Acq On : 04 Apr 2024 13:10
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 05 00:03:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 05 00:03:52 2024
Response via : Initial Calibration

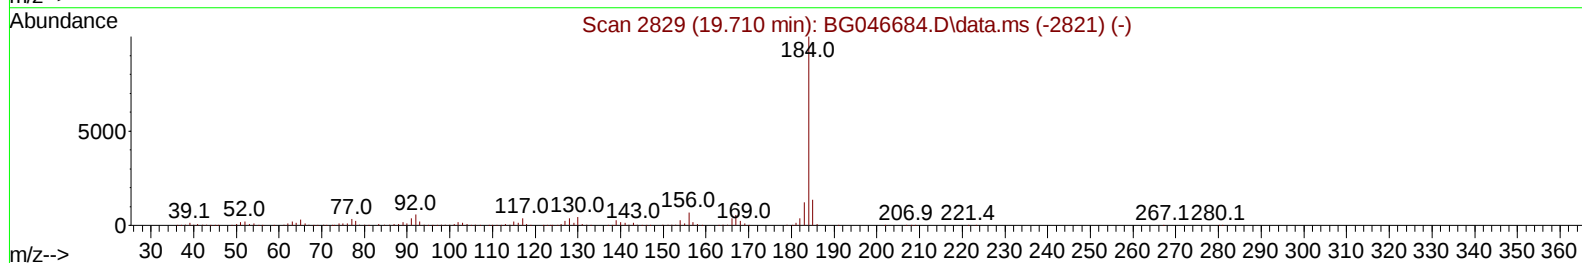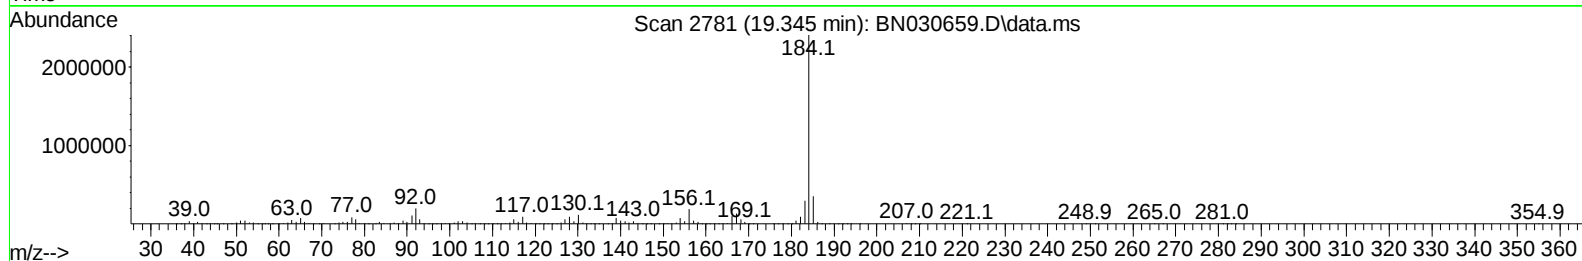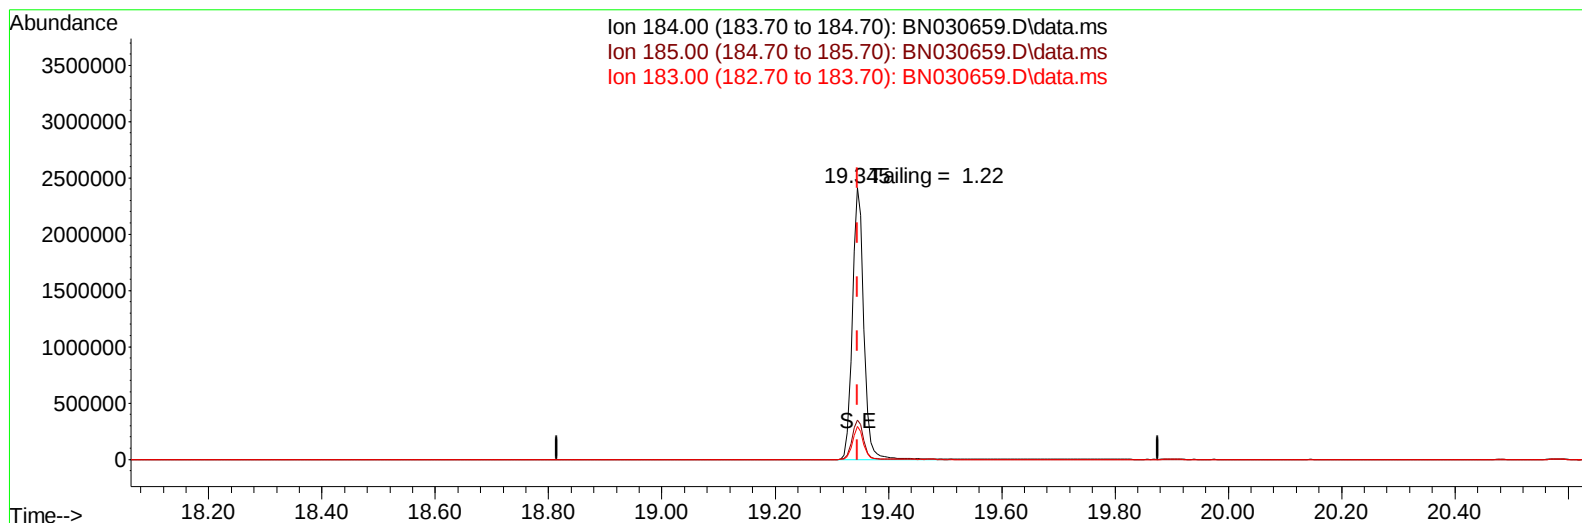

TIC: BN030659.D\data.ms

(77) Benzidine

19.345min (0.000) 0.00 ng

response 3408827

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.54
183.00	13.20	12.06
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/5/2024	BNA_N	<u>BN030659.D</u>
Compound Name	Response	Retention Time
DDT	1546966	20.58
DDD	152809	20.139
DDE	2995	19.633
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
155804	1702770	9.15

Instrument :
BNA_N
ClientSampleId :
DFTPP