

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040621\
 Data File : BN014212.D
 Acq On : 05 Apr 2021 20:14
 Operator : CG/JU
 Sample : SSTDIC3.2
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC3.2

Quant Time: Apr 06 01:10:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Apr 05 18:58:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.644	152	5824	0.40	ng	0.00
7) Naphthalene-d8	10.429	136	21559	0.40	ng	0.00
13) Acenaphthene-d10	14.283	164	13804	0.40	ng	0.00
19) Phenanthrene-d10	17.031	188	29133	0.40	ng	0.00
29) Chrysene-d12	21.229	240	32801	0.40	ng	# 0.01
36) Perylene-d12	23.428	264	30636	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.236	112	44982	3.14	ng	0.00
5) Phenol-d6	6.814	99	60651	3.31	ng	0.00
8) Nitrobenzene-d5	8.794	82	53463	3.54	ng	0.00
11) 2-Methylnaphthalene-d10	12.017	152	162429	3.48	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	19396	4.42	ng	0.00
15) 2-Fluorobiphenyl	12.900	172	165380	3.16	ng	0.00
27) Fluoranthene-d10	19.069	212	392930	3.50	ng	0.00
31) Terphenyl-d14	19.670	244	237786	3.07	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.166	88	21093	2.93	ng	95
3) n-Nitrosodimethylamine	3.488	42	20491	3.77	ng	# 95
6) bis(2-Chloroethyl)ether	7.080	93	52703	3.27	ng	100
9) Naphthalene	10.467	128	189346	3.27	ng	99
10) Hexachlorobutadiene	10.758	225	34064	3.19	ng	# 100
12) 2-Methylnaphthalene	12.093	142	134361	3.47	ng	99
16) Acenaphthylene	14.004	152	205373	3.67	ng	100
17) Acenaphthene	14.346	154	134146	3.37	ng	97
18) Fluorene	15.336	166	173383	3.44	ng	100
20) 4,6-Dinitro-2-methylph...	15.412	198	17899	4.81	ng	# 89
21) 4-Bromophenyl-phenylether	16.228	248	55692	3.36	ng	99
22) Hexachlorobenzene	16.337	284	58681	3.20	ng	100
23) Atrazine	16.496	200	41033	4.02	ng	98
24) Pentachlorophenol	16.690	266	19408	5.93	ng	98
25) Phenanthrene	17.068	178	281081	3.31	ng	100
26) Anthracene	17.165	178	255524	3.58	ng	100
28) Fluoranthene	19.099	202	337124	3.48	ng	100
30) Pyrene	19.461	202	341344	3.15	ng	100
32) Benzo(a)anthracene	21.208	228	348530	3.49	ng	100
33) Chrysene	21.261	228	365781	3.28	ng	100
34) Bis(2-ethylhexyl)phtha...	21.144	149	121870	3.95	ng	100
35) Indeno(1,2,3-cd)pyrene	25.635	276	435170	3.43	ng	100
37) Benzo(b)fluoranthene	22.767	252	383189	3.26	ng	# 95
38) Benzo(k)fluoranthene	22.811	252	370587	3.25	ng	98
39) Benzo(a)pyrene	23.332	252	344076	3.42	ng	# 90
40) Dibenzo(a,h)anthracene	25.646	278	362947	3.36	ng	99
41) Benzo(g,h,i)perylene	26.306	276	371078	3.27	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040621\
Data File : BN014212.D
Acq On : 05 Apr 2021 20:14
Operator : CG/JU
Sample : SSTDICC3.2
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Quant Time: Apr 06 01:10:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Apr 05 18:58:13 2021
Response via : Initial Calibration




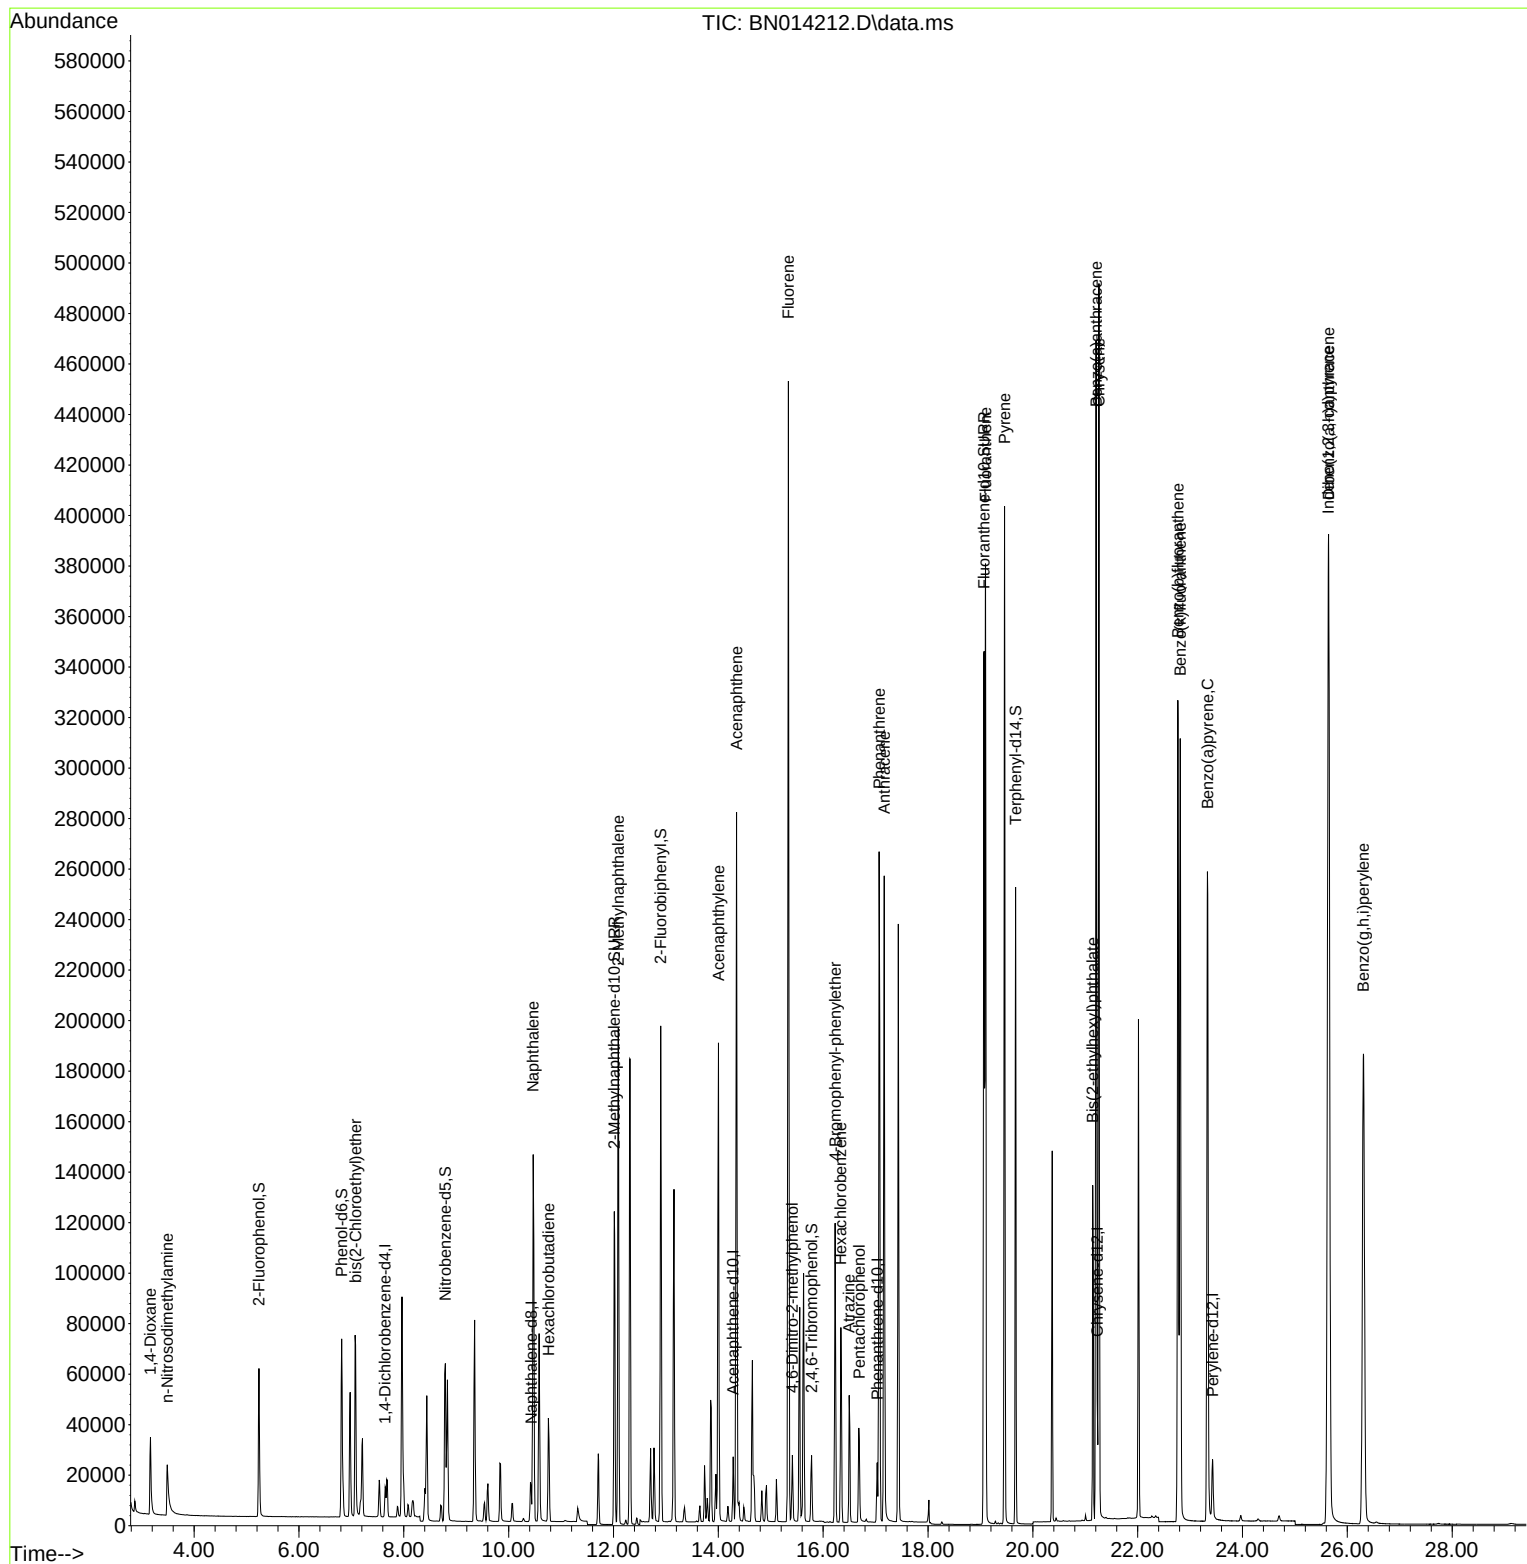




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.644 min Scan# 604
 Delta R.T. -0.000 min
 Lab File: BN014212.D
 Acq: 05 Apr 2021 20:14




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2


Tgt Ion:152 Resp: 5824
 Ion Ratio Lower Upper
 152 100
 150 158.9 127.4 191.0
 115 62.7 50.3 75.5

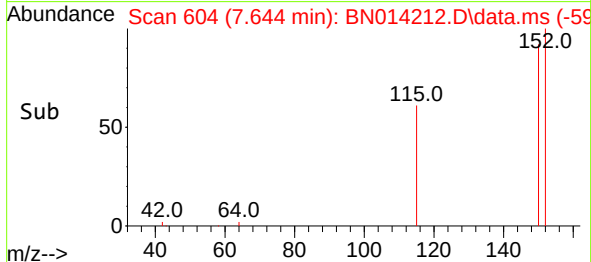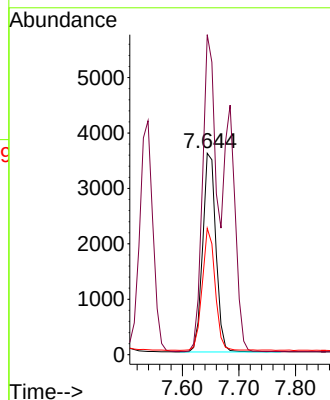

#2
 1,4-Dioxane
 Concen: 2.93 ng
 RT: 3.166 min Scan# 48
 Delta R.T. -0.008 min
 Lab File: BN014212.D
 Acq: 05 Apr 2021 20:14

Tgt Ion: 88 Resp: 21093
 Ion Ratio Lower Upper
 88 100
 58 80.0 59.4 89.0
 43 33.4 25.8 38.8


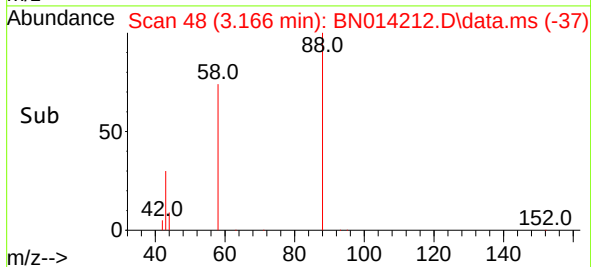
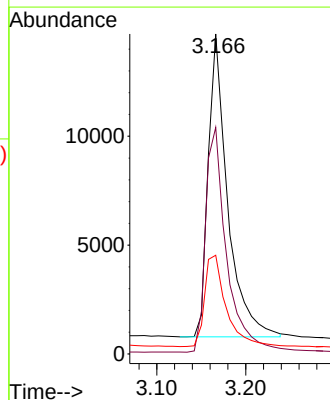
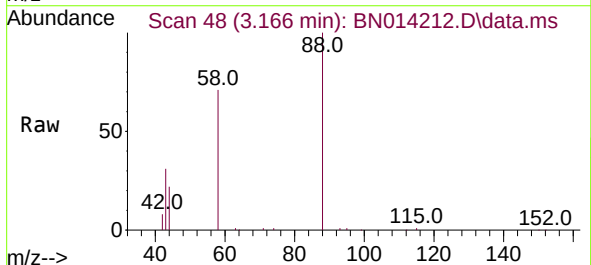


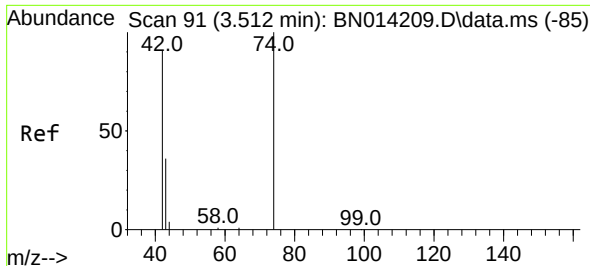

#3
n-Nitrosodimethylamine
Concen: 3.77 ng
RT: 3.488 min Scan# 88
Delta R.T. -0.024 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion: 42 Resp: 20491
Ion Ratio Lower Upper
42 100
74 113.5 95.1 142.7
44 6.9 4.2 6.2#

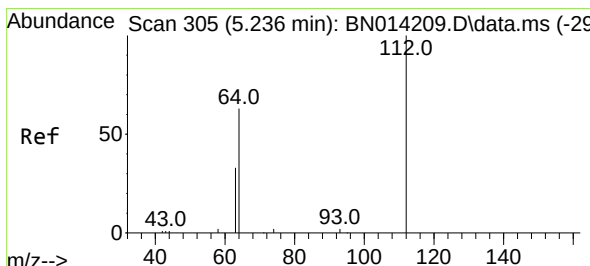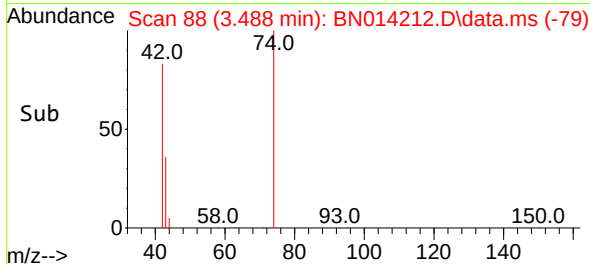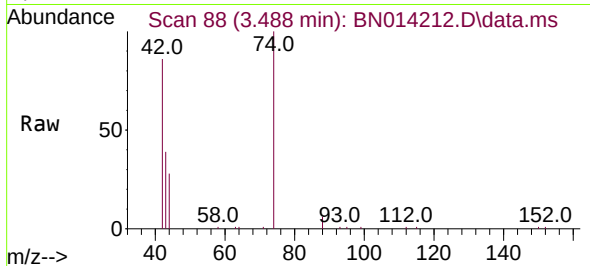

#4
2-Fluorophenol
Concen: 3.14 ng
RT: 5.236 min Scan# 305
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion: 112 Resp: 44982
Ion Ratio Lower Upper
112 100
64 60.2 48.2 72.4
63 32.0 25.5 38.3


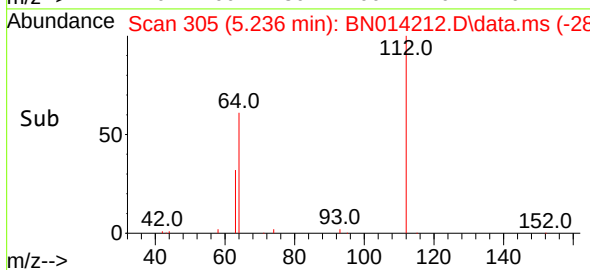

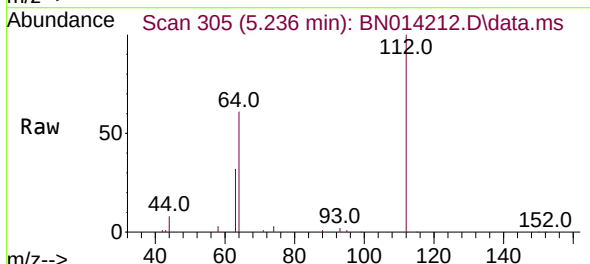


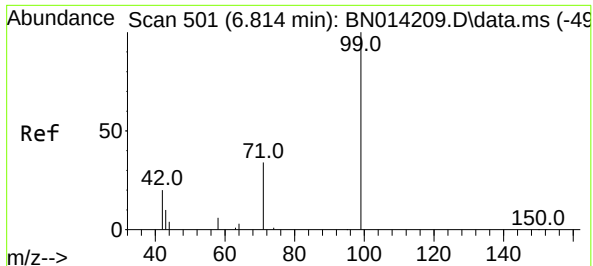

#5
Phenol-d6
Concen: 3.31 ng
RT: 6.814 min Scan# 501
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion: 99 Resp: 60651
Ion Ratio Lower Upper
99 100
42 22.1 18.2 27.2
71 33.7 26.9 40.3

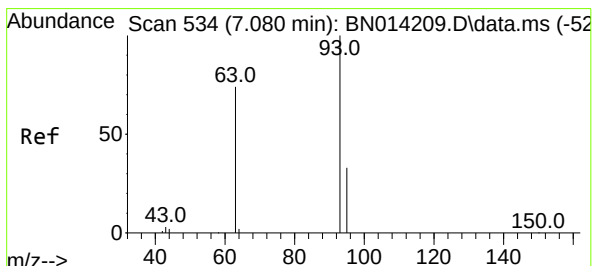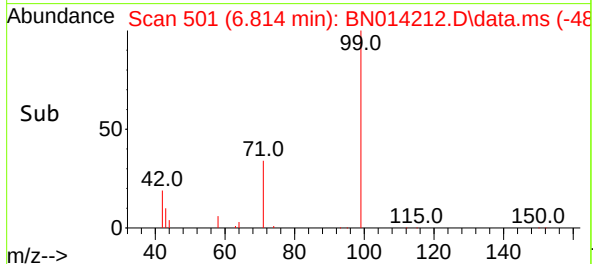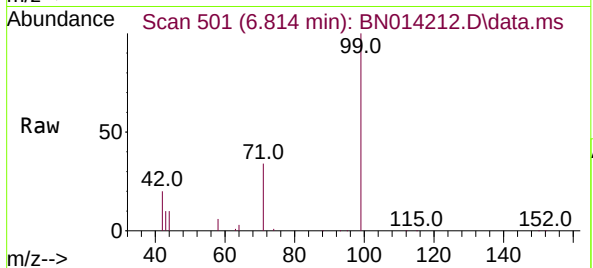

#6
bis(2-Chloroethyl)ether
Concen: 3.27 ng
RT: 7.080 min Scan# 534
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion: 93 Resp: 52703
Ion Ratio Lower Upper
93 100
63 81.3 65.0 97.6
95 32.9 26.8 40.2


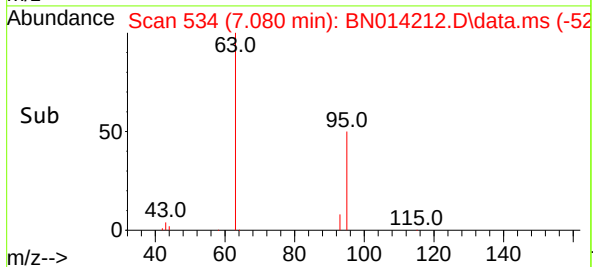

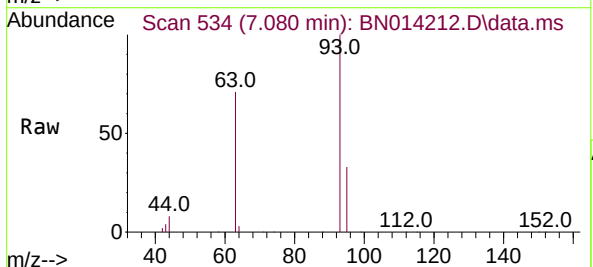




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.429 min Scan# 854
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:	136	Resp:	21559
Ion Ratio	Lower	Upper	
136	100		
137	11.4	9.2	13.8
54	5.0	4.3	6.5
68	4.1	3.6	5.4



#8
Nitrobenzene-d5
Concen: 3.54 ng
RT: 8.794 min Scan# 725
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:	82	Resp:	53463
Ion Ratio	Lower	Upper	
82	100		
128	45.7	34.1	51.1
54	47.3	39.5	59.3


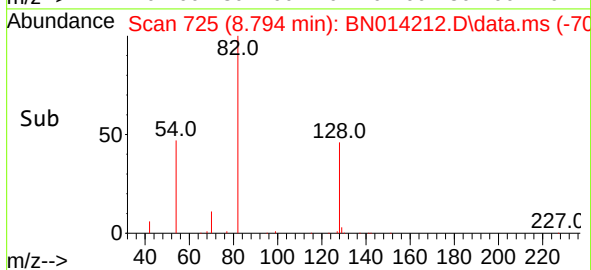






#9
Naphthalene
Concen: 3.27 ng
RT: 10.467 min Scan# 857
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:128 Resp: 189346
Ion Ratio Lower Upper
128 100
129 10.9 8.9 13.3
127 13.1 10.7 16.1

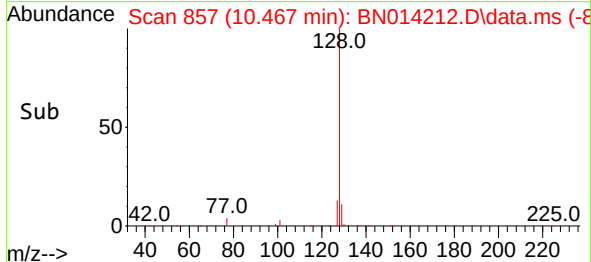

#10
Hexachlorobutadiene
Concen: 3.19 ng
RT: 10.758 min Scan# 880
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:225 Resp: 34064
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 64.2 51.2 76.8


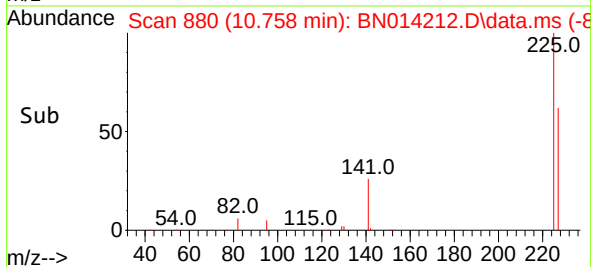

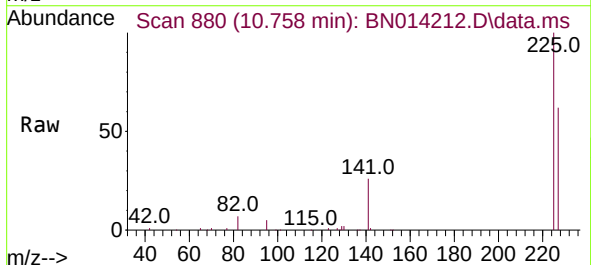




#11
2-Methylnaphthalene-d10
Concen: 3.48 ng
RT: 12.017 min Scan# 1054
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:152 Resp: 162429
Ion Ratio Lower Upper
152 100
151 20.1 16.2 24.2



#12
2-Methylnaphthalene
Concen: 3.47 ng
RT: 12.093 min Scan# 1071
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:142 Resp: 134361
Ion Ratio Lower Upper
142 100
141 87.3 70.5 105.7
115 34.1 28.3 42.5


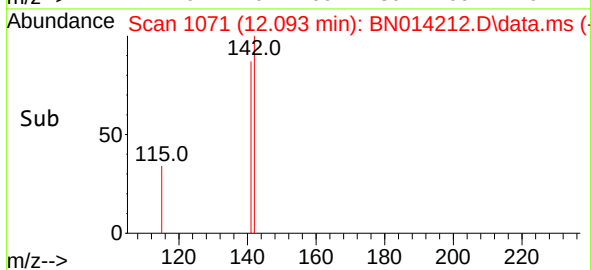

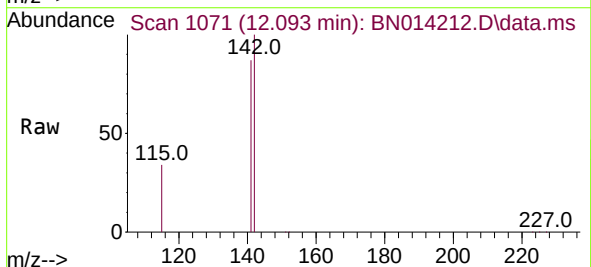




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.283 min Scan# 1304
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:164 Resp: 13804
Ion Ratio Lower Upper
164 100
162 102.0 81.2 121.8
160 45.8 37.5 56.3

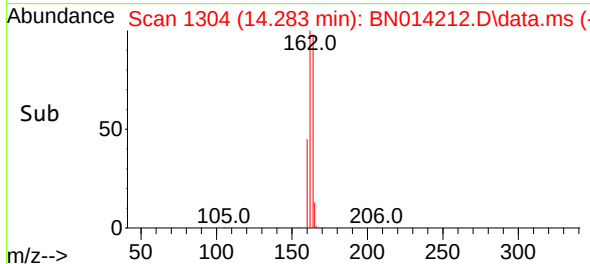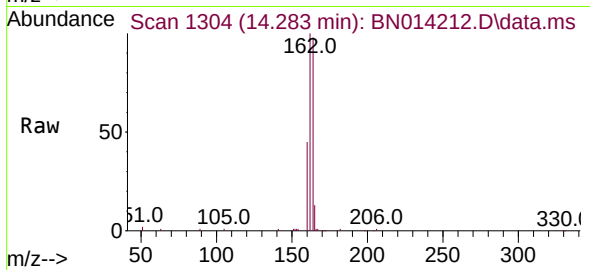

#14
2,4,6-Tribromophenol
Concen: 4.42 ng
RT: 15.780 min Scan# 1422
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:330 Resp: 19396
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 38.4 30.5 45.7


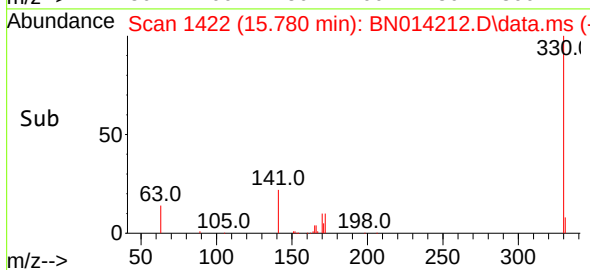

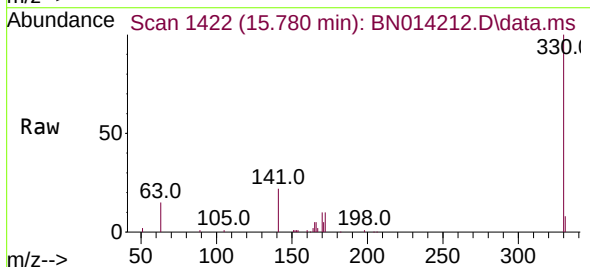




#15
2-Fluorobiphenyl
Concen: 3.16 ng
RT: 12.900 min Scan# 1195
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:172 Resp: 165380
Ion Ratio Lower Upper
172 100
171 34.6 28.0 42.0
170 23.4 19.1 28.7



#16
Acenaphthylene
Concen: 3.67 ng
RT: 14.004 min Scan# 1282
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:152 Resp: 205373
Ion Ratio Lower Upper
152 100
151 19.2 15.5 23.3
153 13.0 10.2 15.4


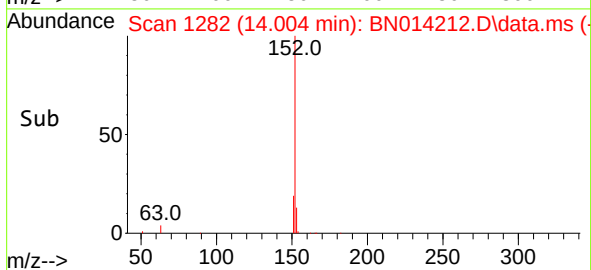

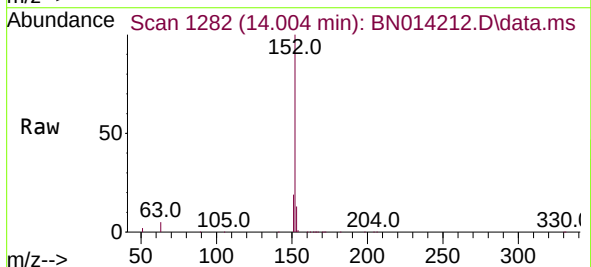




#17
Acenaphthene
Concen: 3.37 ng
RT: 14.346 min Scan# 1309
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:154 Resp: 134146
Ion Ratio Lower Upper
154 100
153 108.7 89.4 134.2
152 52.4 43.9 65.9

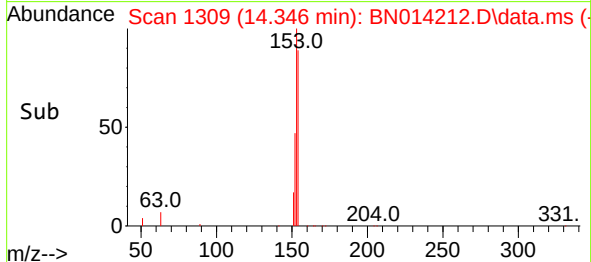

#18
Fluorene
Concen: 3.44 ng
RT: 15.336 min Scan# 1387
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:166 Resp: 173383
Ion Ratio Lower Upper
166 100
165 97.3 78.1 117.1
167 13.4 10.8 16.2


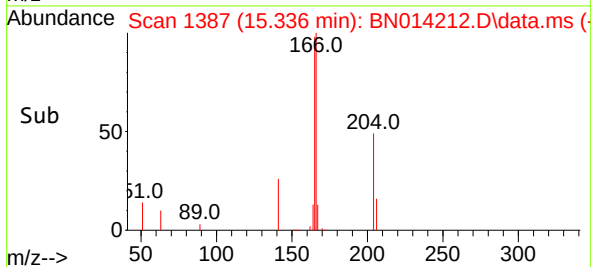

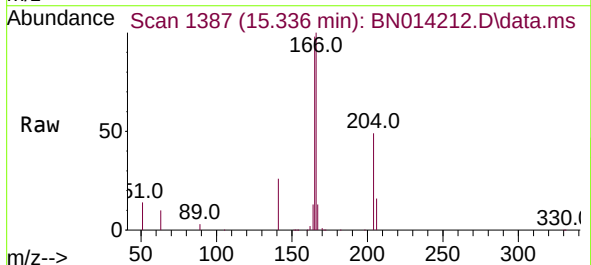


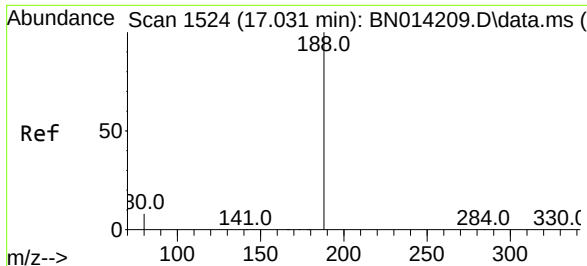

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.031 min Scan# 1524
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:188 Resp: 29133
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.6 6.9 10.3

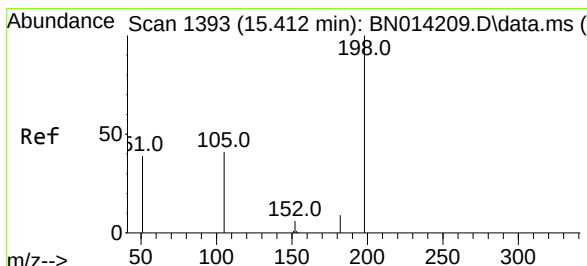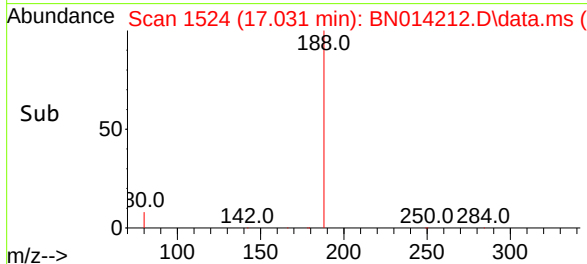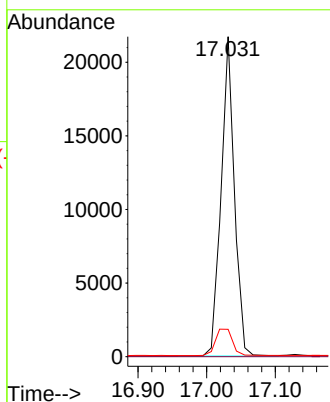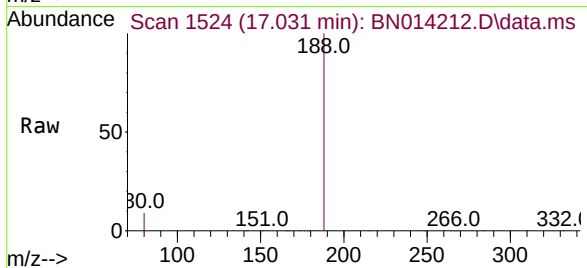

#20
4,6-Dinitro-2-methylphenol
Concen: 4.81 ng
RT: 15.412 min Scan# 1393
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:198 Resp: 17899
Ion Ratio Lower Upper
198 100
51 49.8 51.7 77.5#
105 47.6 38.2 57.2


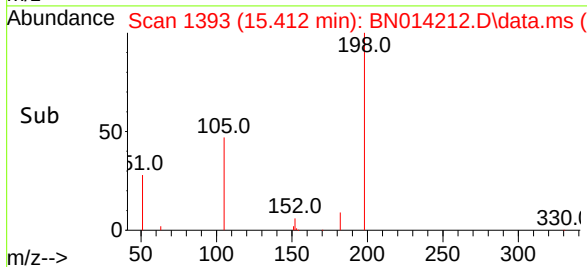
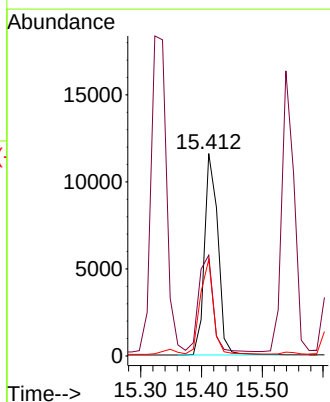
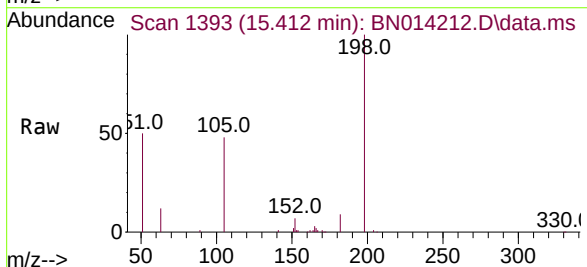


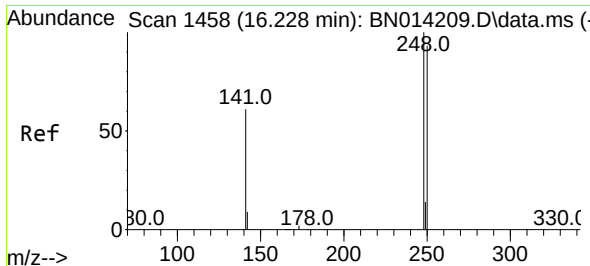

#21
4-Bromophenyl-phenylether
Concen: 3.36 ng
RT: 16.228 min Scan# 1458
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:248 Resp: 55692
Ion Ratio Lower Upper
248 100
250 94.6 74.6 111.8
141 62.1 49.4 74.0

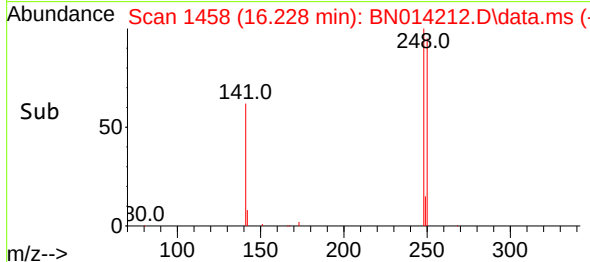

#22
Hexachlorobenzene
Concen: 3.20 ng
RT: 16.337 min Scan# 1467
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:284 Resp: 58681
Ion Ratio Lower Upper
284 100
142 36.3 29.0 43.4
249 31.2 25.2 37.8


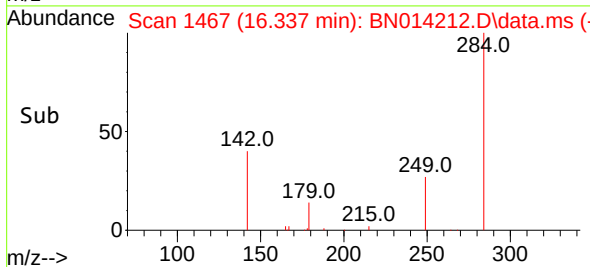

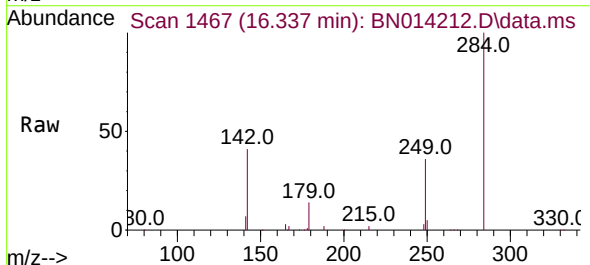


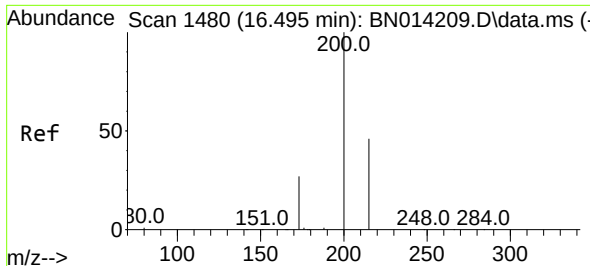

#23
Atrazine
Concen: 4.02 ng
RT: 16.496 min Scan# 1480
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:200 Resp: 41033
Ion Ratio Lower Upper
200 100
173 30.2 22.9 34.3
215 46.6 37.7 56.5

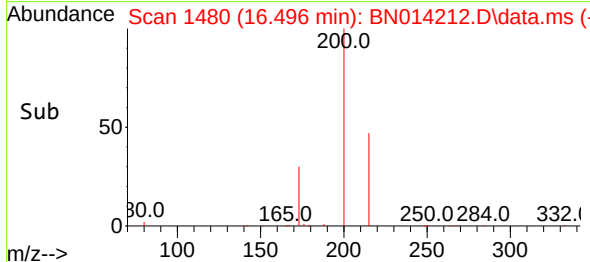

#24
Pentachlorophenol
Concen: 5.93 ng
RT: 16.690 min Scan# 1496
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:266 Resp: 19408
Ion Ratio Lower Upper
266 100
264 63.0 49.0 73.4
268 64.3 50.3 75.5


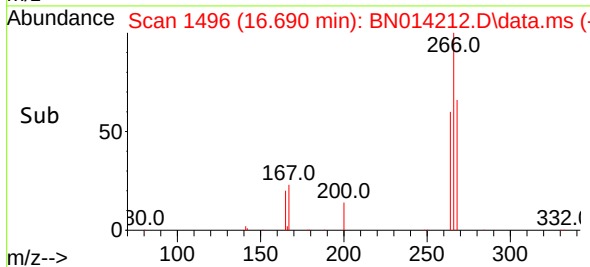

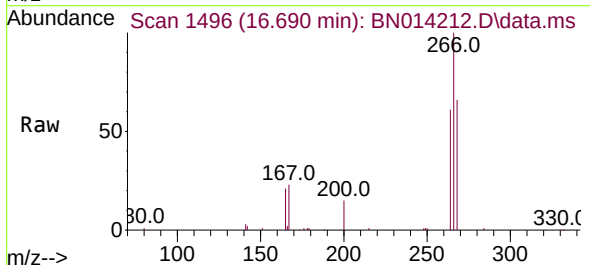


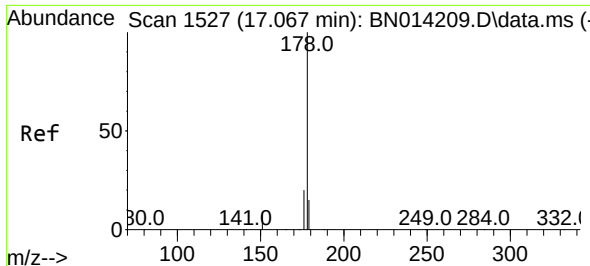

#25
Phenanthrene
Concen: 3.31 ng
RT: 17.068 min Scan# 1527
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:178 Resp: 281081
Ion Ratio Lower Upper
178 100
176 18.8 15.1 22.7
179 15.3 12.4 18.6

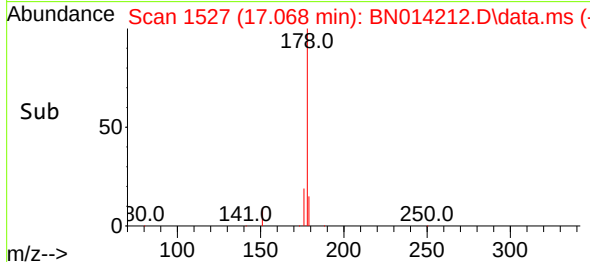

#26
Anthracene
Concen: 3.58 ng
RT: 17.165 min Scan# 1535
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:178 Resp: 255524
Ion Ratio Lower Upper
178 100
176 18.2 14.6 21.8
179 15.3 12.2 18.2


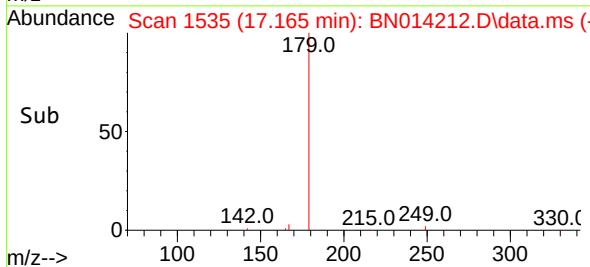

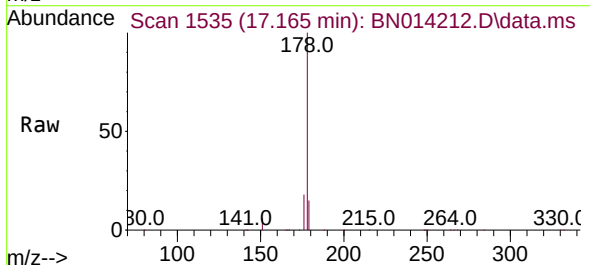


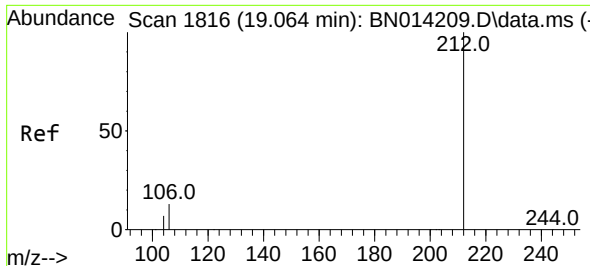

#27
Fluoranthene-d10
Concen: 3.50 ng
RT: 19.069 min Scan# 1817
Delta R.T. 0.005 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:212 Resp: 392930
Ion Ratio Lower Upper
212 100
106 12.6 10.0 15.0
104 7.0 5.6 8.4

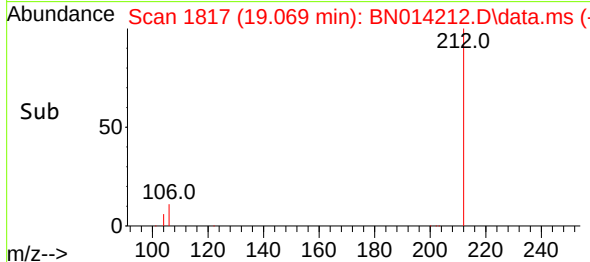

#28
Fluoranthene
Concen: 3.48 ng
RT: 19.099 min Scan# 1823
Delta R.T. 0.005 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:202 Resp: 337124
Ion Ratio Lower Upper
202 100
101 10.9 8.7 13.1
203 17.4 13.8 20.6


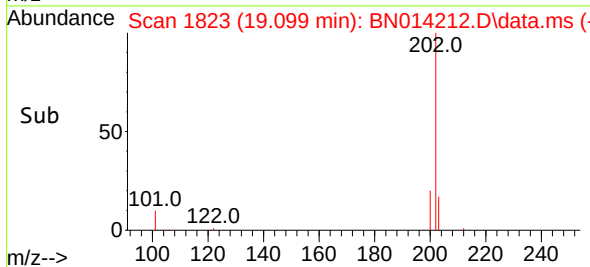

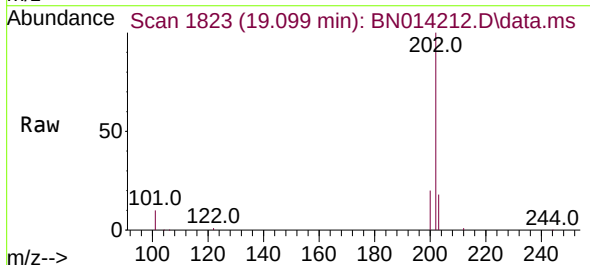




#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.229 min Scan# 2121
Delta R.T. 0.011 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:240 Resp: 32801
Ion Ratio Lower Upper
240 100
120 4.9 10.3 15.5#
236 25.0 21.4 32.0

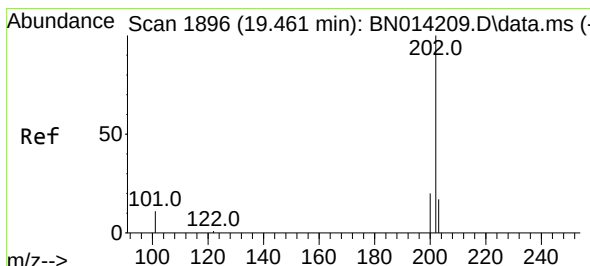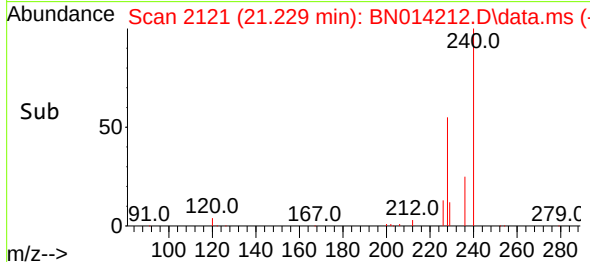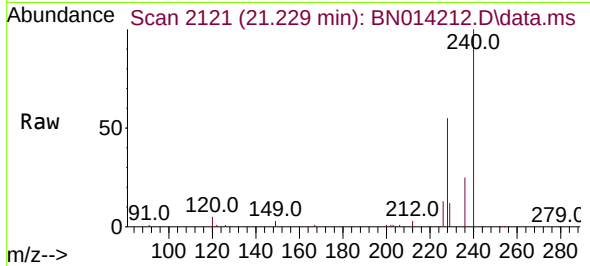

#30
Pyrene
Concen: 3.15 ng
RT: 19.461 min Scan# 1896
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:202 Resp: 341344
Ion Ratio Lower Upper
202 100
200 20.4 16.2 24.4
203 17.5 13.9 20.9


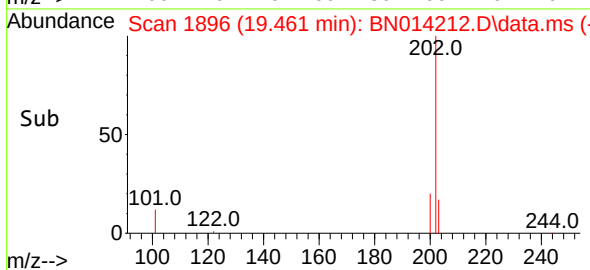

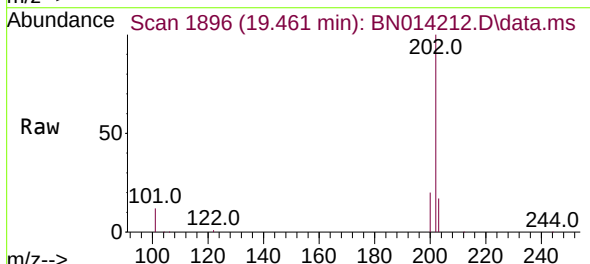




#31
 Terphenyl-d14
 Concen: 3.07 ng
 RT: 19.670 min Scan# 1938
 Delta R.T. 0.000 min
 Lab File: BN014212.D
 Acq: 05 Apr 2021 20:14




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2


Tgt Ion:244 Resp: 237786
 Ion Ratio Lower Upper
 244 100
 212 7.5 6.0 9.0
 122 12.2 9.4 14.0



#32
 Benzo(a)anthracene
 Concen: 3.49 ng
 RT: 21.208 min Scan# 2119
 Delta R.T. 0.000 min
 Lab File: BN014212.D
 Acq: 05 Apr 2021 20:14

Tgt Ion:228 Resp: 348530
 Ion Ratio Lower Upper
 228 100
 226 26.6 21.1 31.7
 229 19.7 15.7 23.5

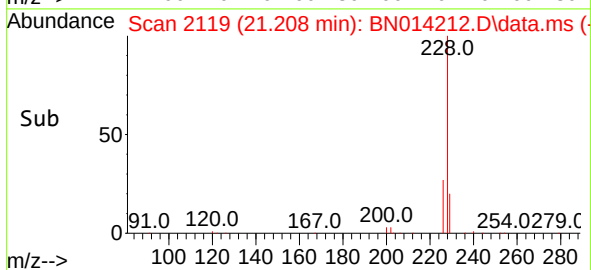







#33
Chrysene
Concen: 3.28 ng
RT: 21.261 min Scan# 2124
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2

Tgt Ion:228 Resp: 365781




Ion	Ratio	Lower	Upper
228	100		
226	28.6	23.0	34.6
229	19.7	15.8	23.8

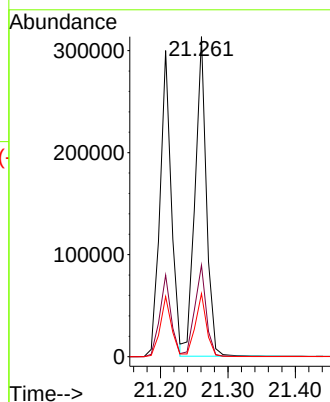


#34
Bis(2-ethylhexyl)phthalate
Concen: 3.95 ng
RT: 21.144 min Scan# 2113
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:149 Resp: 121870

Ion	Ratio	Lower	Upper
149	100		
167	27.0	21.5	32.3
279	3.9	3.1	4.7


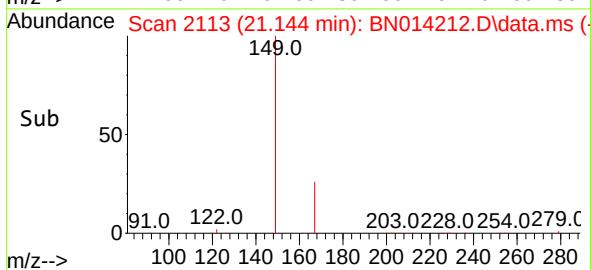
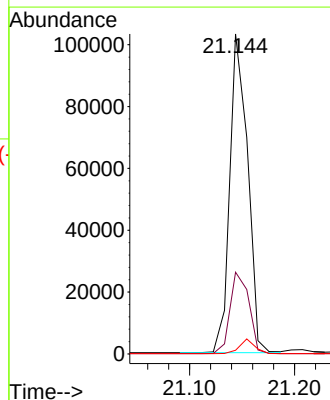





#35
Indeno(1,2,3-cd)pyrene
Concen: 3.43 ng
RT: 25.635 min Scan# 3175
Delta R.T. 0.004 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:276 Resp: 435170
Ion Ratio Lower Upper
276 100
138 23.7 18.6 28.0
277 24.9 19.8 29.8

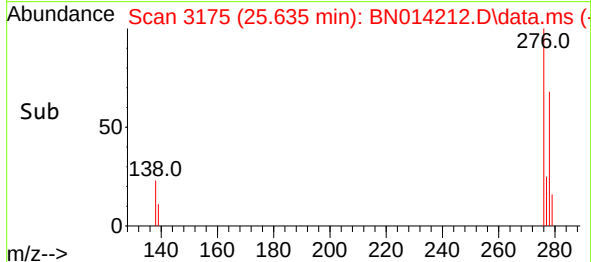

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.428 min Scan# 2530
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:264 Resp: 30636
Ion Ratio Lower Upper
264 100
260 24.6 19.4 29.2
265 25.9 20.7 31.1


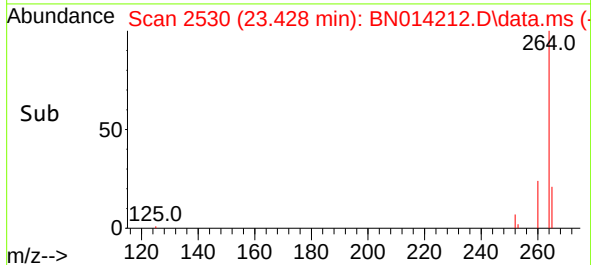

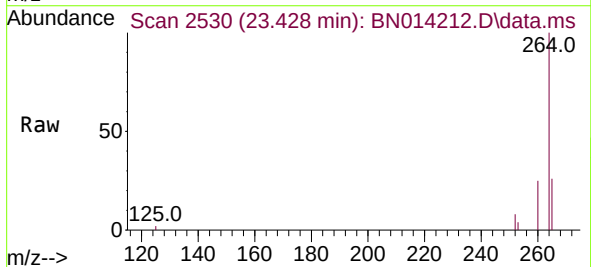




#37
Benzo(b)fluoranthene
Concen: 3.26 ng
RT: 22.767 min Scan# 2337
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:252 Resp: 383189
Ion Ratio Lower Upper
252 100
253 21.8 18.9 28.3
125 9.8 10.1 15.1#



#38
Benzo(k)fluoranthene
Concen: 3.25 ng
RT: 22.811 min Scan# 2350
Delta R.T. 0.000 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:252 Resp: 370587
Ion Ratio Lower Upper
252 100
253 21.7 18.5 27.7
125 9.5 7.9 11.9


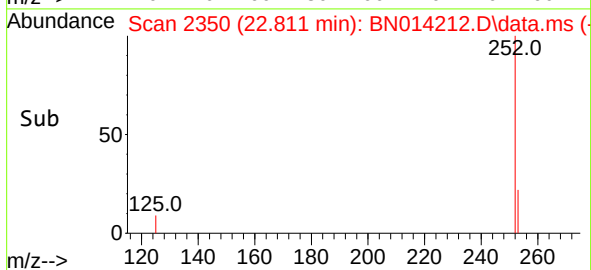

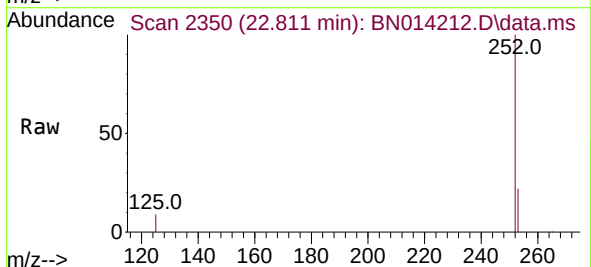




#39
Benzo(a)pyrene
Concen: 3.42 ng
RT: 23.332 min Scan# 2502
Delta R.T. 0.004 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14




Instrument :
BNA_N
ClientSampleId :
SSTDICC3.2


Tgt Ion:252 Resp: 344076
Ion Ratio Lower Upper
252 100
253 22.3 19.4 29.0
125 11.3 15.0 22.6#



#40
Dibenzo(a,h)anthracene
Concen: 3.36 ng
RT: 25.646 min Scan# 3178
Delta R.T. 0.004 min
Lab File: BN014212.D
Acq: 05 Apr 2021 20:14

Tgt Ion:278 Resp: 362947
Ion Ratio Lower Upper
278 100
139 15.9 12.7 19.1
279 23.5 19.4 29.2

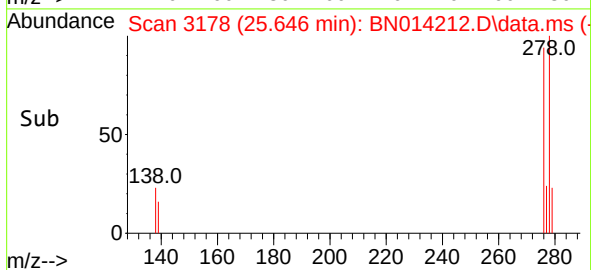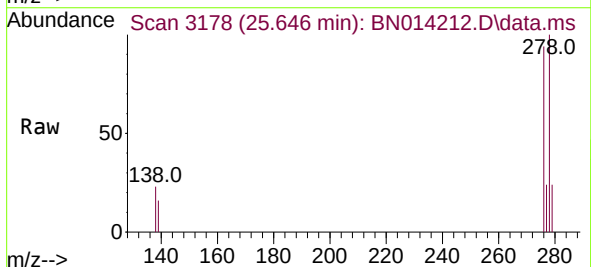

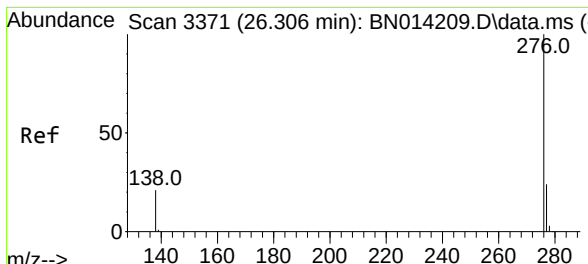

#41
 Benzo(g,h,i)perylene
 Concen: 3.27 ng
 RT: 26.306 min Scan# 3371
 Delta R.T. 0.000 min
 Lab File: BN014212.D
 Acq: 05 Apr 2021 20:14

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC3.2

Tgt Ion:	276	Resp:	371078
Ion	Ratio	Lower	Upper
276	100		
277	23.9	19.2	28.8
138	20.4	16.8	25.2

