
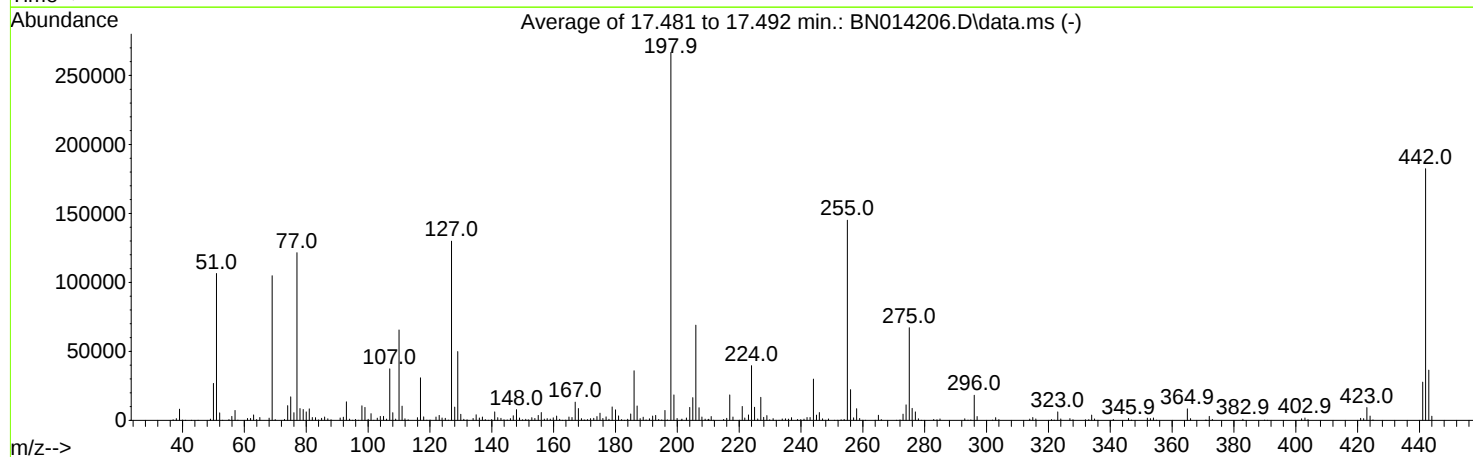


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040621\
 Data File : BN014206.D
 Acq On : 05 Apr 2021 16:38
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 06 03:14:49 2021

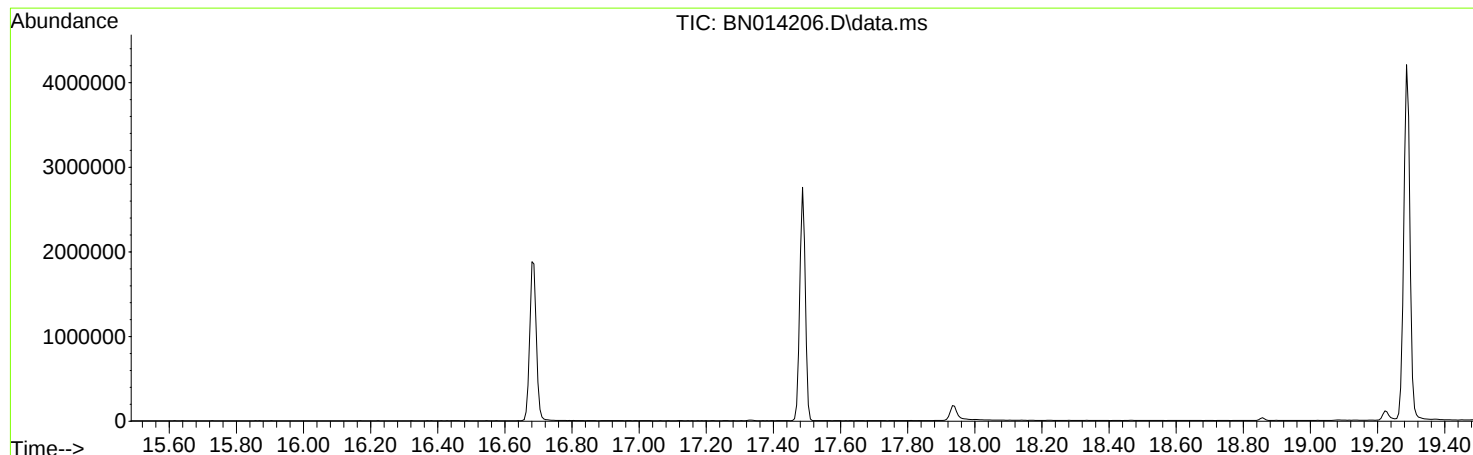

AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.9	106440	PASS
68	69	0.00	2	1.6	1686	PASS
69	198	0.00	100	39.3	104800	PASS
70	69	0.00	2	0.6	606	PASS
127	198	10	80	48.7	129912	PASS
197	198	0.00	2	0.2	402	PASS
198	198	100	100	100.0	266645	PASS
199	198	5	9	6.9	18485	PASS
275	198	10	60	25.2	67136	PASS
365	198	1	100	3.1	8393	PASS
441	198	0.01	100	10.4	27691	PASS
442	442	50	100	100.0	182408	PASS
443	442	15	24	20.0	36392	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/6/2021	BNA_N	<u>BN014206.D</u>
Compound Name	Response	Retention Time
DDT	996715	20.528
DDD	959	20.086
DDE	896	19.575
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1855	998570	0.19

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040621\
Data File : BN014206.D
Acq On : 05 Apr 2021 16:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 06 10:26:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

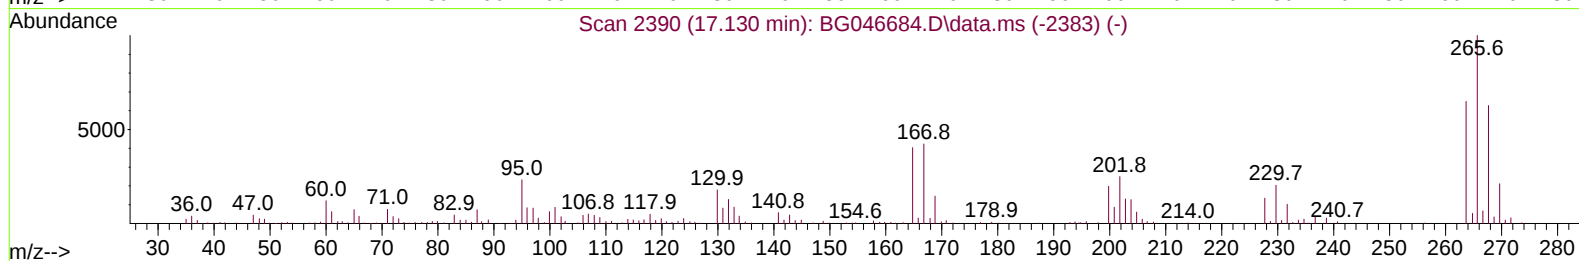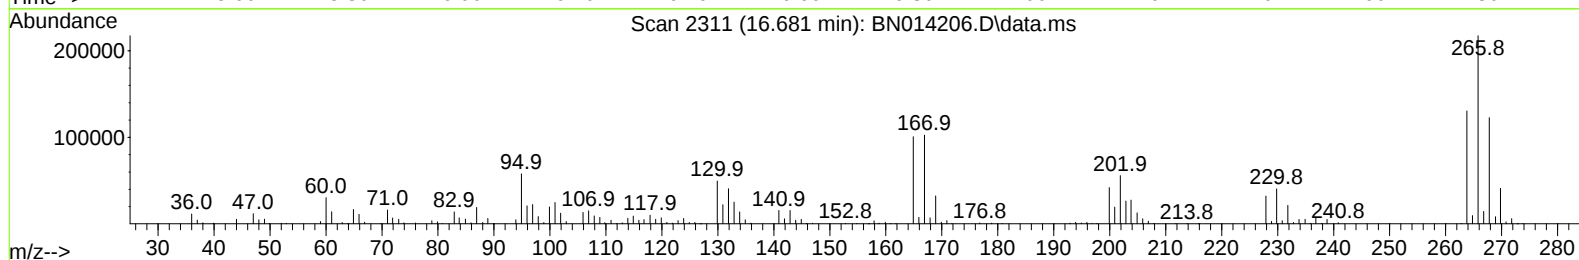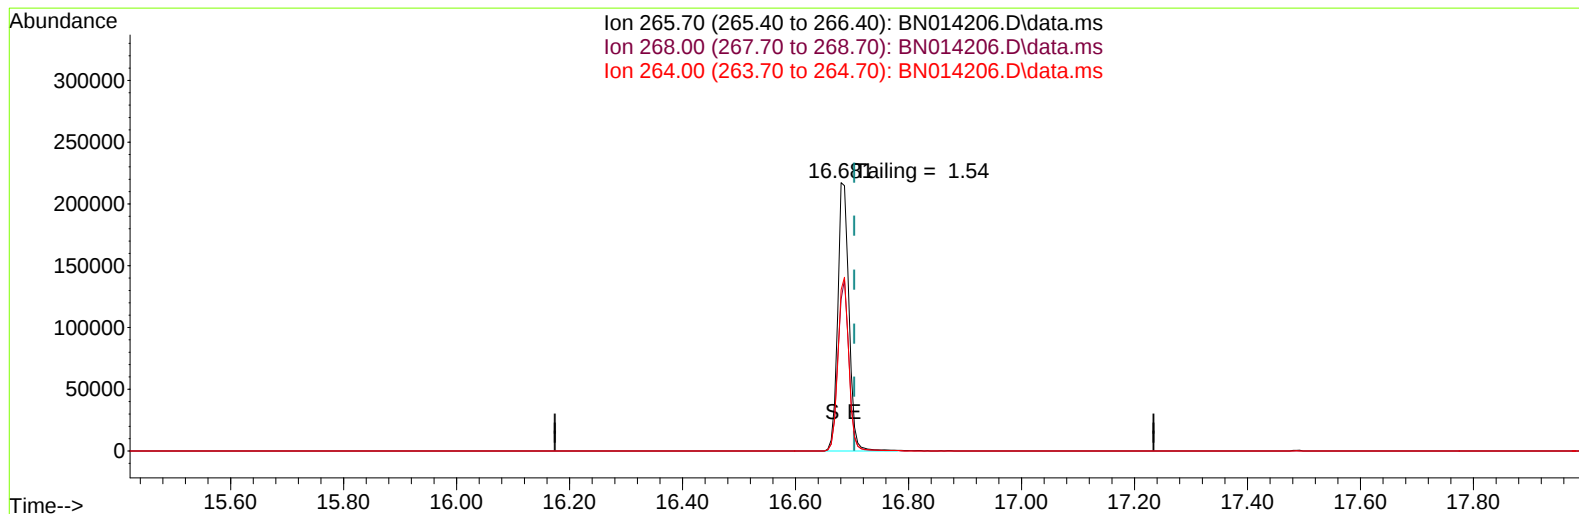

TIC: BN014206.D\data.ms

(70) Pentachlorophenol (C)

16.681min (-0.023) 22449.94 ng




response 298980

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	56.51
264.00	61.60	60.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040621\
Data File : BN014206.D
Acq On : 05 Apr 2021 16:38
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 06 10:26:37 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

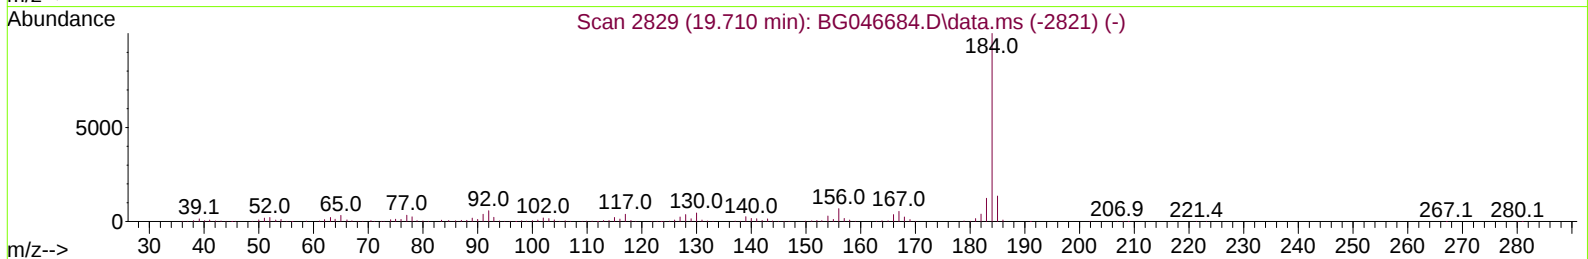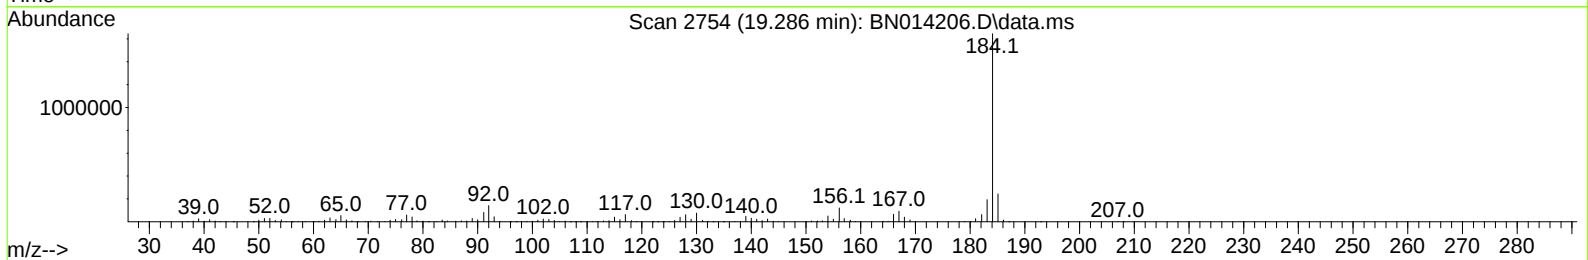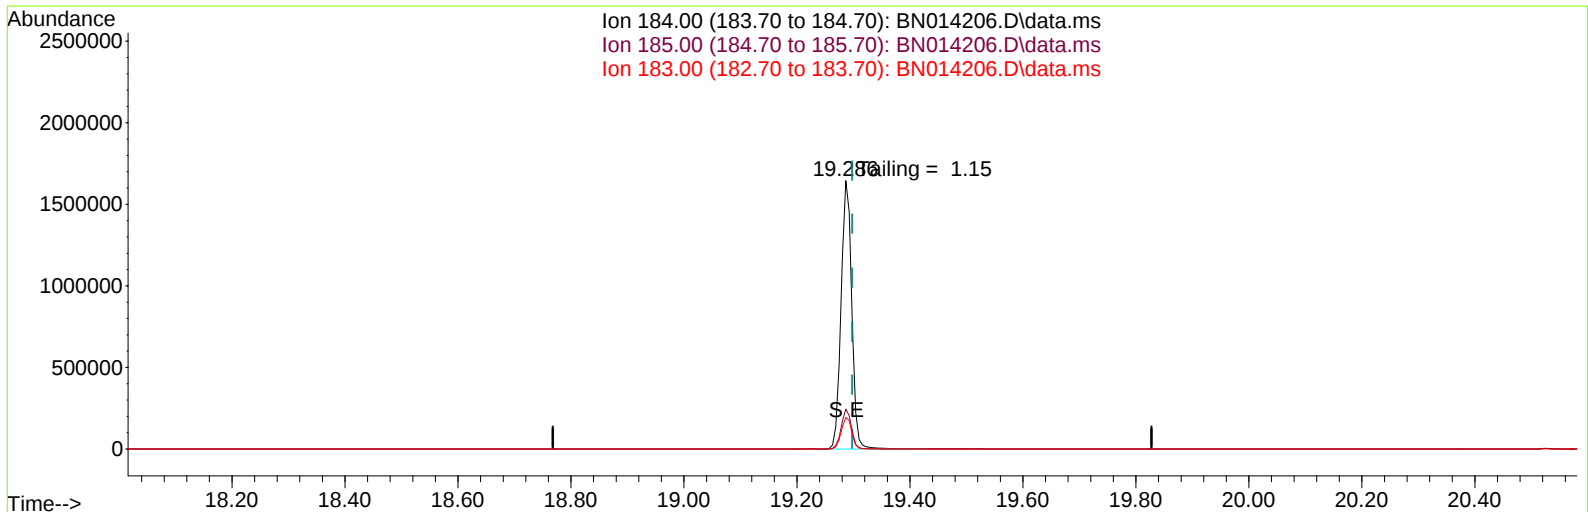

TIC: BN014206.D\data.ms

(77) Benzidine

19.286min (-0.012) 0.00 ng

response 2148456

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.86
183.00	13.20	11.77
0.00	0.00	0.00