

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030677.D
 Acq On : 05 Apr 2024 16:59
 Operator : MA/JU
 Sample : P1989-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07W0

Quant Time: Apr 05 17:54:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 12:24:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.692	152	144453	20.000	ng/u1	0.00
20) Naphthalene-d8	10.475	136	704625	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.333	164	526955	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.086	188	1182378	20.000	ng/u1	0.00
79) Chrysene-d12	21.321	240	1206239	20.000	ng/u1	0.00
88) Perylene-d12	24.268	264	1365260	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	17962	5.830	ng/uL	0.00
4) Pyridine-d5	3.599	84	105963	11.471	ng/u1	0.00
7) Phenol-d5	6.863	99	86819	7.430	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.028	67	279251	38.691	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.222	132	278571	31.425	ng/u1	0.00
15) 4-Methylphenol-d8	8.392	113	180327	18.413	ng/u1	0.00
21) Nitrobenzene-d5	8.845	128	203165	41.565	ng/u1	0.00
24) 2-Nitrophenol-d4	9.563	143	170597	38.152	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.098	165	326427	33.345	ng/u1	0.00
31) 4-Chloroaniline-d4	10.616	131	518365	32.164	ng/u1	0.00
46) Dimethylphthalate-d6	13.751	166	1572859	44.706	ng/u1	0.00
49) Acenaphthylene-d8	14.027	160	1718737	42.489	ng/u1	0.00
54) 4-Nitrophenol-d4	14.539	143	35455	5.268	ng/u1	0.00
60) Fluorene-d10	15.327	176	1368710	44.457	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.451	200	80065	15.341	ng/u1	0.00
73) Anthracene-d10	17.186	188	2458693	48.262	ng/u1	0.00
81) Pyrene-d10	19.486	212	2947229	45.445	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.068	264	3219117	51.172	ng/u1	0.00
Target Compounds						Qvalue
6) Benzaldehyde	6.840	77	6822	1.254	ng/u1	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030677.D
Acq On : 05 Apr 2024 16:59
Operator : MA/JU
Sample : P1989-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07W0


Quant Time: Apr 05 17:54:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

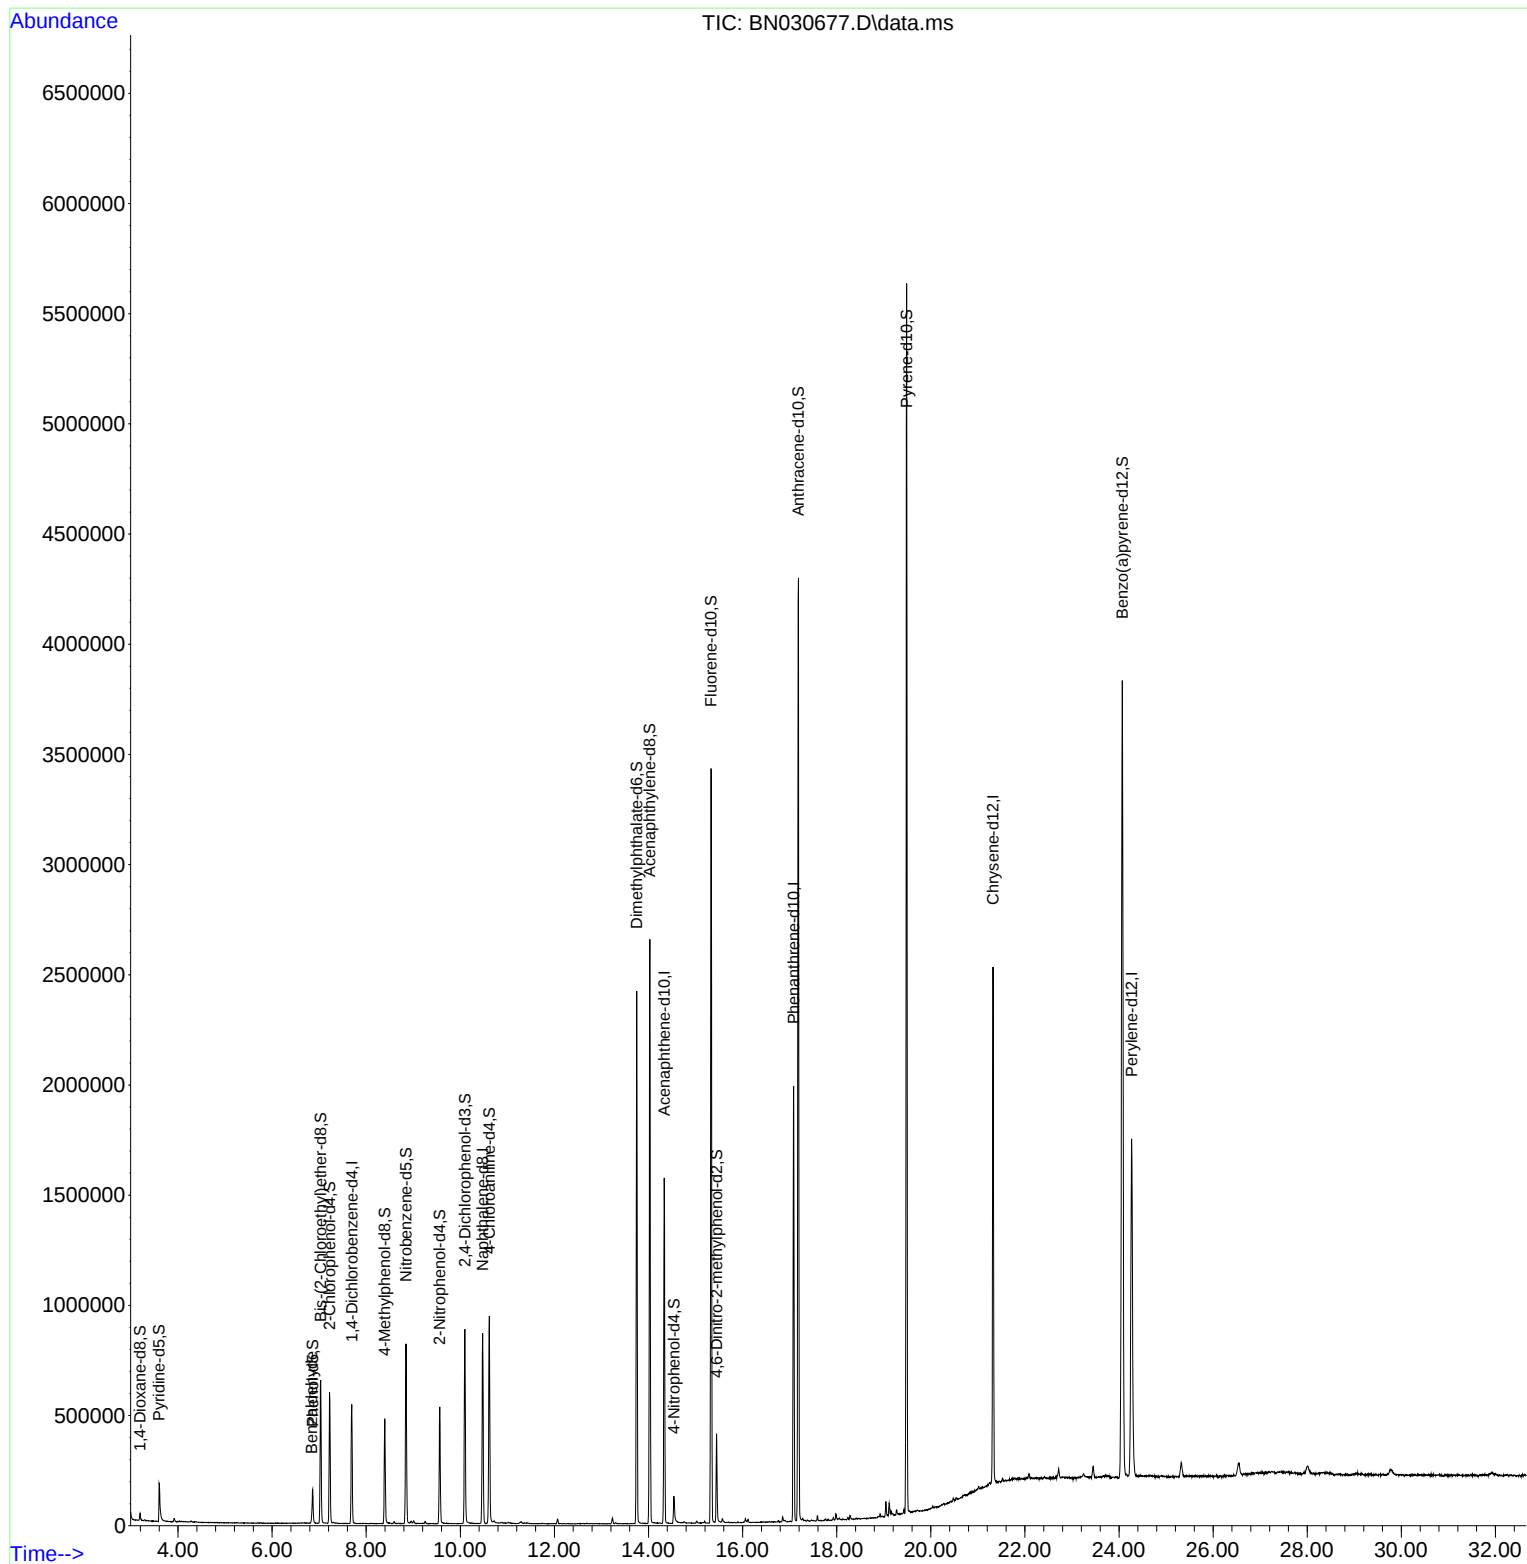

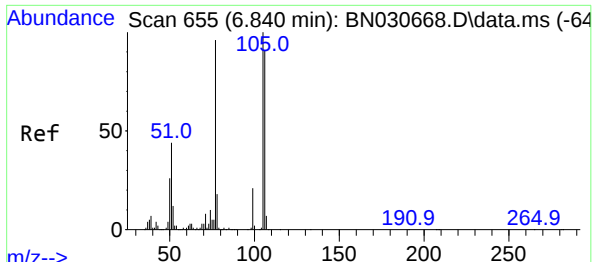

#6
Benzaldehyde
Concen: 1.254 ng/ul
RT: 6.840 min Scan# 61
Delta R.T. -0.006 min
Lab File: BN030677.D
Acq: 05 Apr 2024 16:59

Instrument :
BNA_N
ClientSampleId :
E07W0

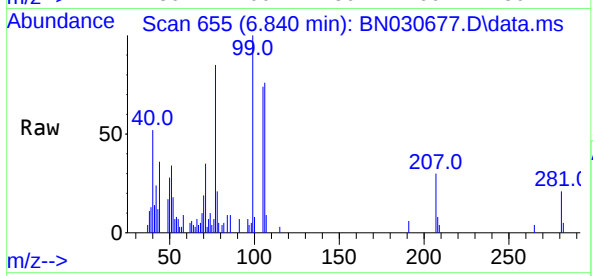

Tgt Ion: 77 Resp: 6822

Ion	Ratio	Lower	Upper
77	100		
105	87.2	78.1	117.1
106	88.7	75.6	113.4

