

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030693.D
 Acq On : 06 Apr 2024 04:07
 Operator : MA/JU
 Sample : P1970-04
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ5

Quant Time: Apr 06 04:36:27 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 12:24:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.687	152	169958	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.475	136	821036	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.334	164	594017	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.081	188	1323990	20.000	ng/u1	0.00
79) Chrysene-d12	21.322	240	1335700	20.000	ng/u1	0.00
88) Perylene-d12	24.263	264	1459542	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	18070	4.985	ng/uL	0.00
4) Pyridine-d5	3.599	84	126048	11.597	ng/u1	0.00
7) Phenol-d5	6.863	99	104025	7.566	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.028	67	292984	34.502	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.222	132	313083	30.018	ng/u1	0.00
15) 4-Methylphenol-d8	8.393	113	221645	19.235	ng/u1	0.00
21) Nitrobenzene-d5	8.846	128	214256	37.619	ng/u1	0.00
24) 2-Nitrophenol-d4	9.563	143	226602	43.491	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.093	165	411596	36.084	ng/u1	0.00
31) 4-Chloroaniline-d4	10.616	131	440621	23.464	ng/u1	0.00
46) Dimethylphthalate-d6	13.751	166	1444323	36.418	ng/u1	0.00
49) Acenaphthylene-d8	14.022	160	1758884	38.572	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.540	143	55242	7.282	ng/u1	0.00
60) Fluorene-d10	15.328	176	1361378	39.226	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.445	200	222280	38.036	ng/u1	0.00
73) Anthracene-d10	17.181	188	2385227	41.812	ng/u1	0.00
81) Pyrene-d10	19.480	212	2829862	39.406	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.063	264	3000404	44.614	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.228	88	15322	3.946	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030693.D
Acq On : 06 Apr 2024 04:07
Operator : MA/JU
Sample : P1970-04
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ5


Quant Time: Apr 06 04:36:27 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

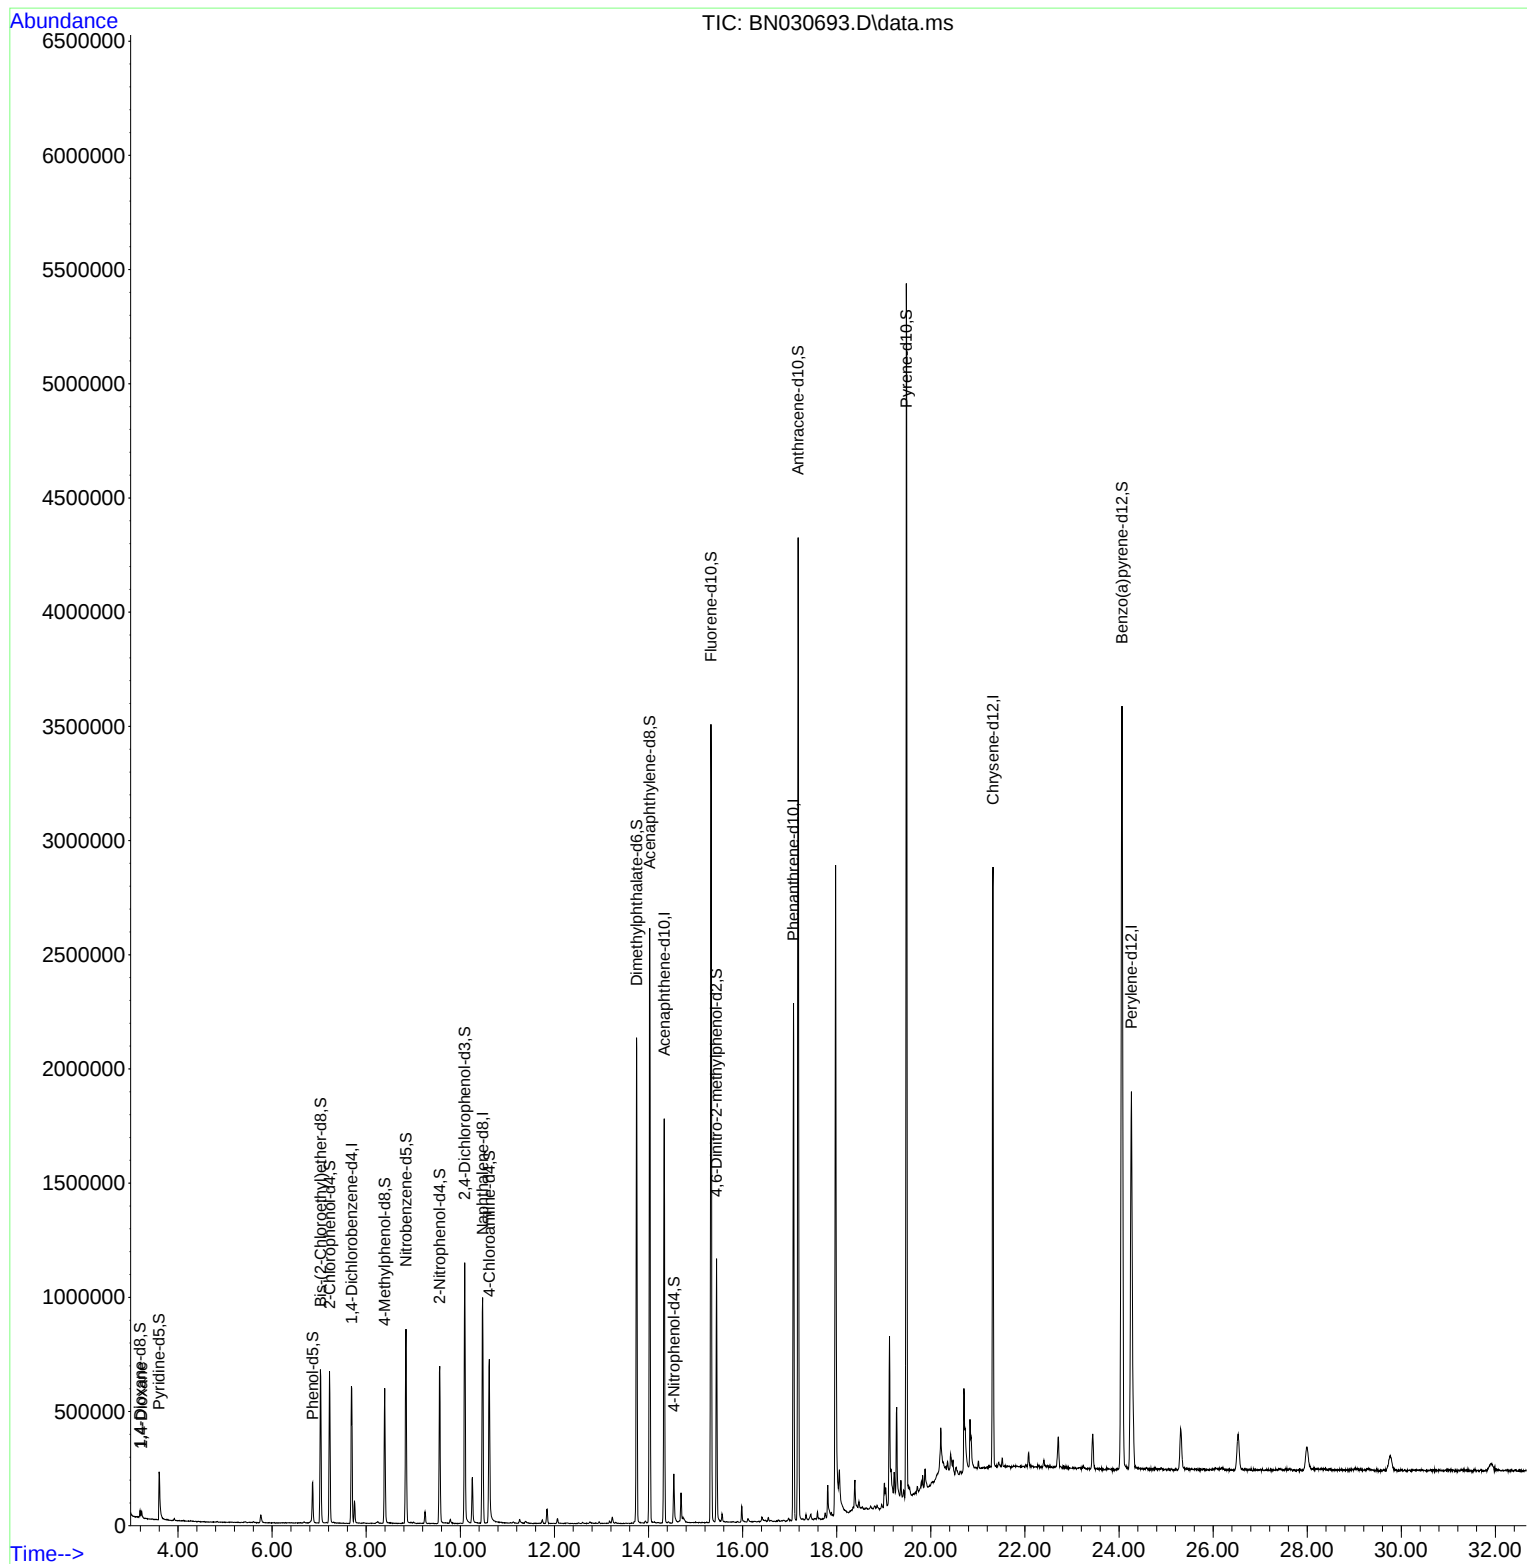

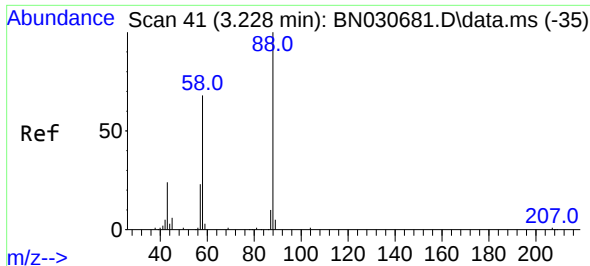

#2
1,4-Dioxane
Concen: 3.946 ng/uL
RT: 3.228 min Scan# 41
Delta R.T. -0.006 min
Lab File: BN030693.D
Acq: 06 Apr 2024 04:07

Instrument :
BNA_N
ClientSampleId :
C0AJ5

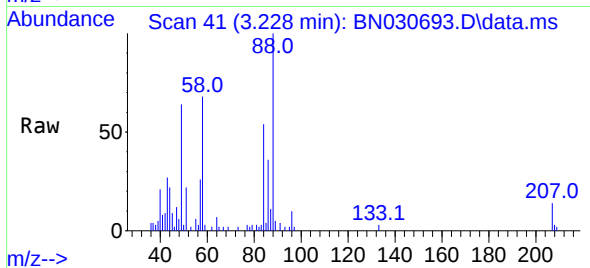

Tgt Ion: 88 Resp: 15322
Ion Ratio Lower Upper
88 100
43 27.2 23.8 35.8
58 68.1 56.6 84.8

