

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030709.D
 Acq On : 06 Apr 2024 15:12
 Operator : MA/JU
 Sample : P1948-12
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ0

Quant Time: Apr 07 12:38:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 12:24:07 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.687	152	158066	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.469	136	738656	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.328	164	554161	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.081	188	1301804	20.000	ng/u1	0.00
79) Chrysene-d12	21.316	240	1331936	20.000	ng/u1	-0.01
88) Perylene-d12	24.257	264	1437277	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	15964	4.735	ng/uL	-0.01
4) Pyridine-d5	3.599	84	48418	4.790	ng/u1	0.00
7) Phenol-d5	6.858	99	65409	5.115	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.028	67	191867	24.294	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.222	132	201913	20.816	ng/u1	0.00
15) 4-Methylphenol-d8	8.393	113	133583	12.465	ng/u1	0.00
21) Nitrobenzene-d5	8.840	128	133475	26.049	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.558	143	134741	28.745	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.093	165	259657	25.303	ng/u1	0.00
31) 4-Chloroaniline-d4	10.610	131	394877	23.373	ng/u1	-0.01
46) Dimethylphthalate-d6	13.746	166	1142554	30.881	ng/u1	-0.01
49) Acenaphthylene-d8	14.022	160	1227808	28.862	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.534	143	30582	4.321	ng/u1	0.00
60) Fluorene-d10	15.328	176	1022024	31.566	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.445	200	145654	25.348	ng/u1	0.00
73) Anthracene-d10	17.175	188	1859139	33.146	ng/u1	-0.01
81) Pyrene-d10	19.481	212	2343879	32.731	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.057	264	2309340	34.870	ng/u1	-0.02
Target Compounds						
2) 1,4-Dioxane	3.223	88	89151	24.686	ng/uL	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030709.D
Acq On : 06 Apr 2024 15:12
Operator : MA/JU
Sample : P1948-12
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ0


Quant Time: Apr 07 12:38:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

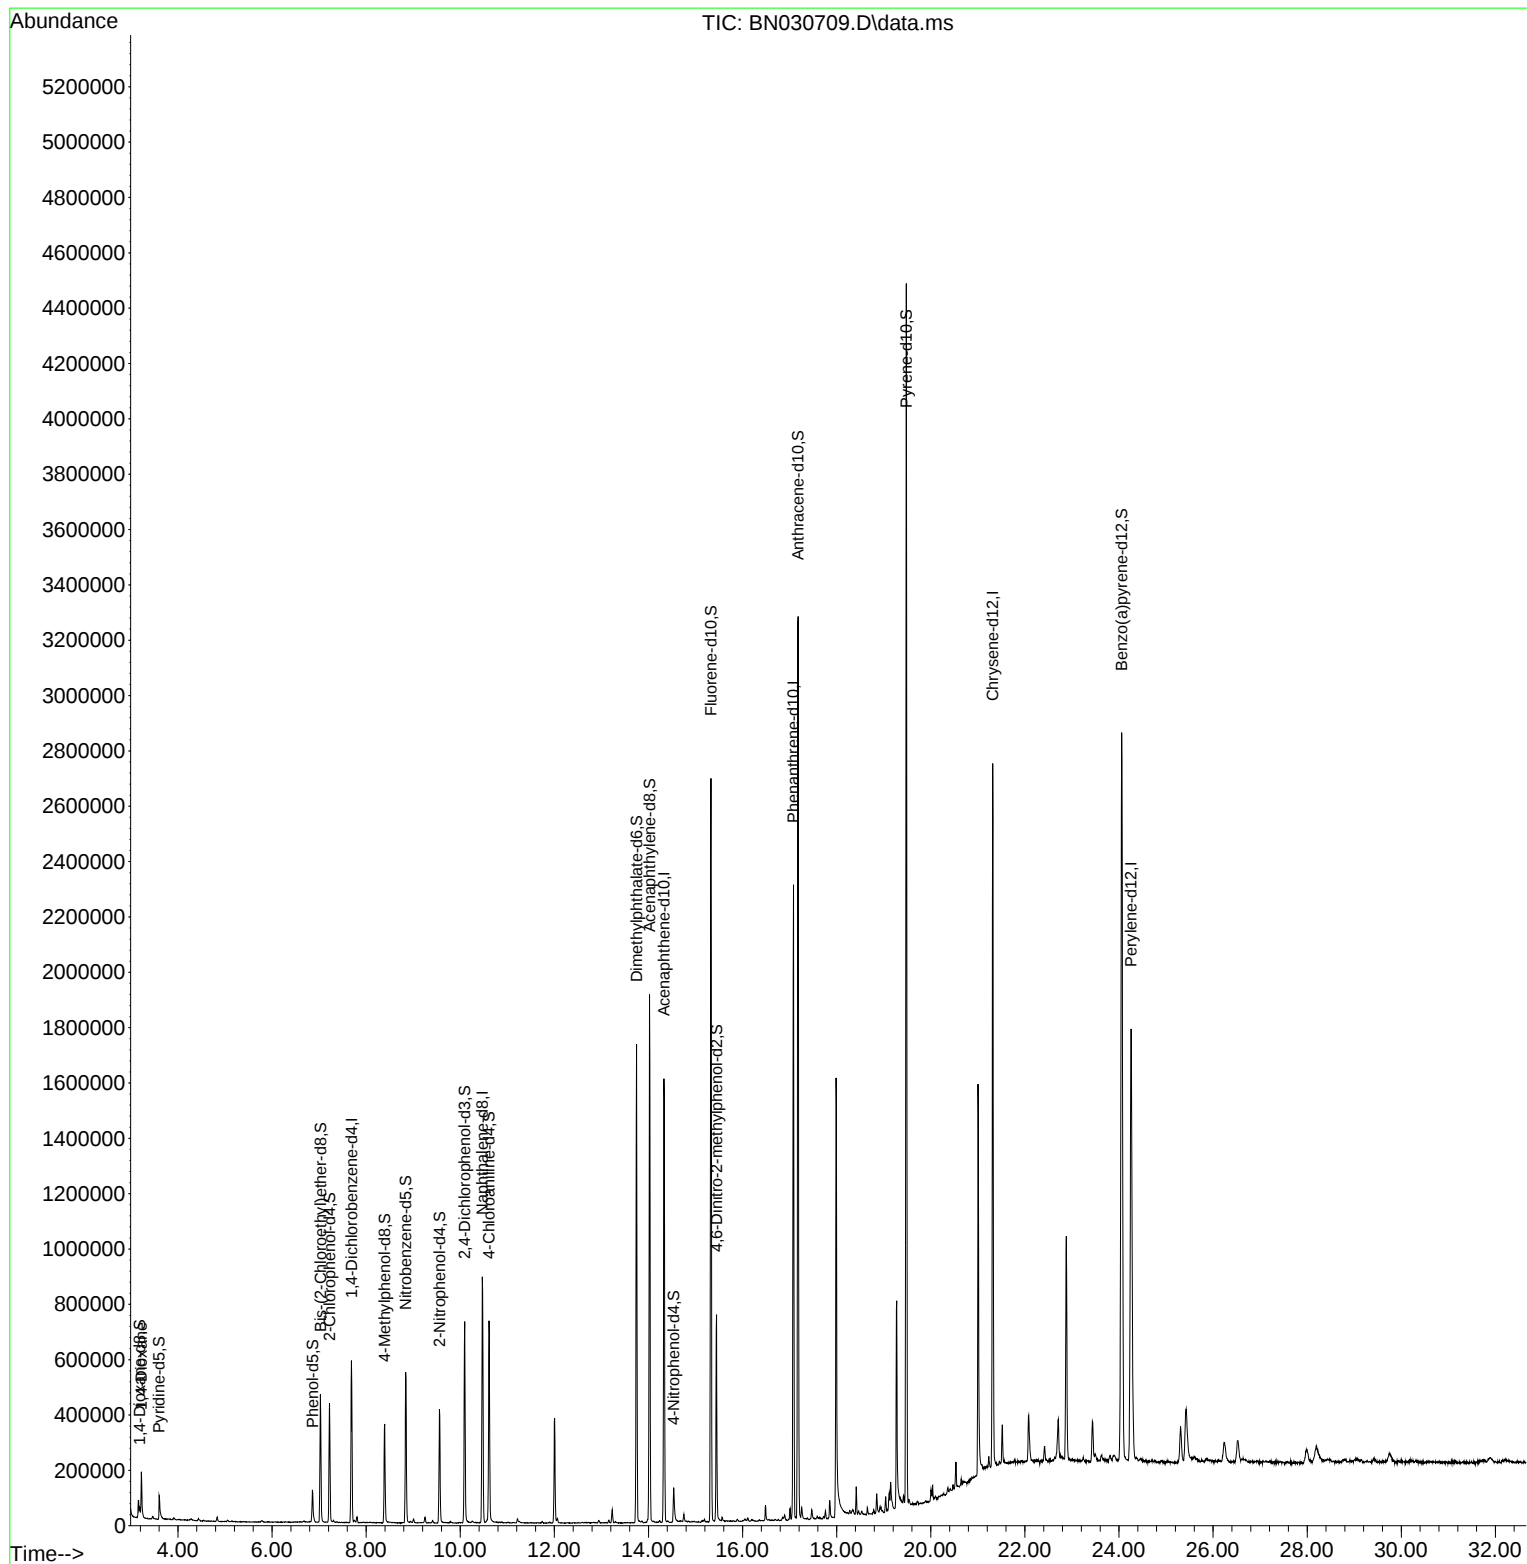

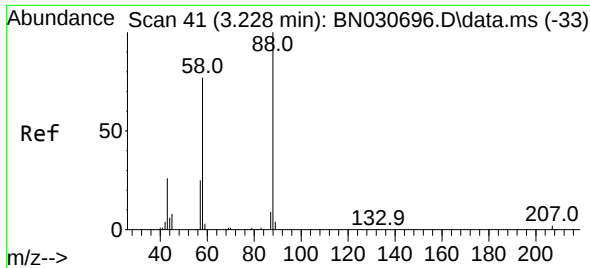

#2
 1,4-Dioxane
 Concen: 24.686 ng/uL
 RT: 3.223 min Scan# 40
 Delta R.T. -0.012 min
 Lab File: BN030709.D
 Acq: 06 Apr 2024 15:12

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ0

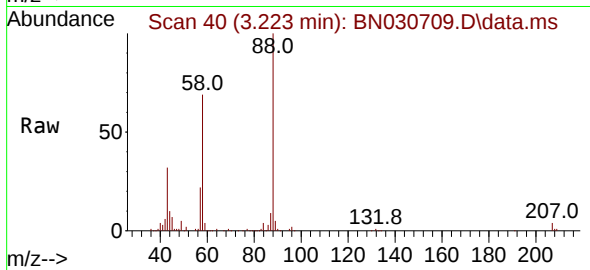

Tgt Ion:	88	Resp:	89151
Ion	Ratio	Lower	Upper
88	100		
43	32.4	23.8	35.8
58	69.1	56.6	84.8

