

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030714.D
 Acq On : 06 Apr 2024 19:07
 Operator : MA/JU
 Sample : P1948-14
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ2

Quant Time: Apr 07 12:54:56 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 12:24:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.687	152	144952	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.469	136	679130	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.328	164	486779	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.080	188	1071029	20.000	ng/u1	0.00
79) Chrysene-d12	21.315	240	1055510	20.000	ng/u1	-0.01
88) Perylene-d12	24.262	264	1191617	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.193	96	18959	6.132	ng/uL	0.00
4) Pyridine-d5	3.599	84	112109	12.094	ng/u1	0.00
7) Phenol-d5	6.857	99	87525	7.464	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.028	67	300434	41.482	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.222	132	296789	33.365	ng/u1	0.00
15) 4-Methylphenol-d8	8.393	113	188607	19.192	ng/u1	0.00
21) Nitrobenzene-d5	8.846	128	212644	45.137	ng/u1	0.00
24) 2-Nitrophenol-d4	9.557	143	212954	49.412	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.093	165	361659	38.331	ng/u1	0.00
31) 4-Chloroaniline-d4	10.610	131	513101	33.033	ng/u1	-0.01
46) Dimethylphthalate-d6	13.745	166	1560220	48.007	ng/u1	-0.01
49) Acenaphthylene-d8	14.022	160	1741471	46.604	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.539	143	41988	6.754	ng/u1	0.00
60) Fluorene-d10	15.328	176	1340493	47.134	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.445	200	195721	41.401	ng/u1	0.00
73) Anthracene-d10	17.180	188	2269034	49.170	ng/u1	0.00
81) Pyrene-d10	19.480	212	2777000	48.935	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.056	264	2771496	50.476	ng/u1	-0.02
Target Compounds						
2) 1,4-Dioxane	3.222	88	29783	8.993	ng/uL	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030714.D
Acq On : 06 Apr 2024 19:07
Operator : MA/JU
Sample : P1948-14
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ2


Quant Time: Apr 07 12:54:56 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

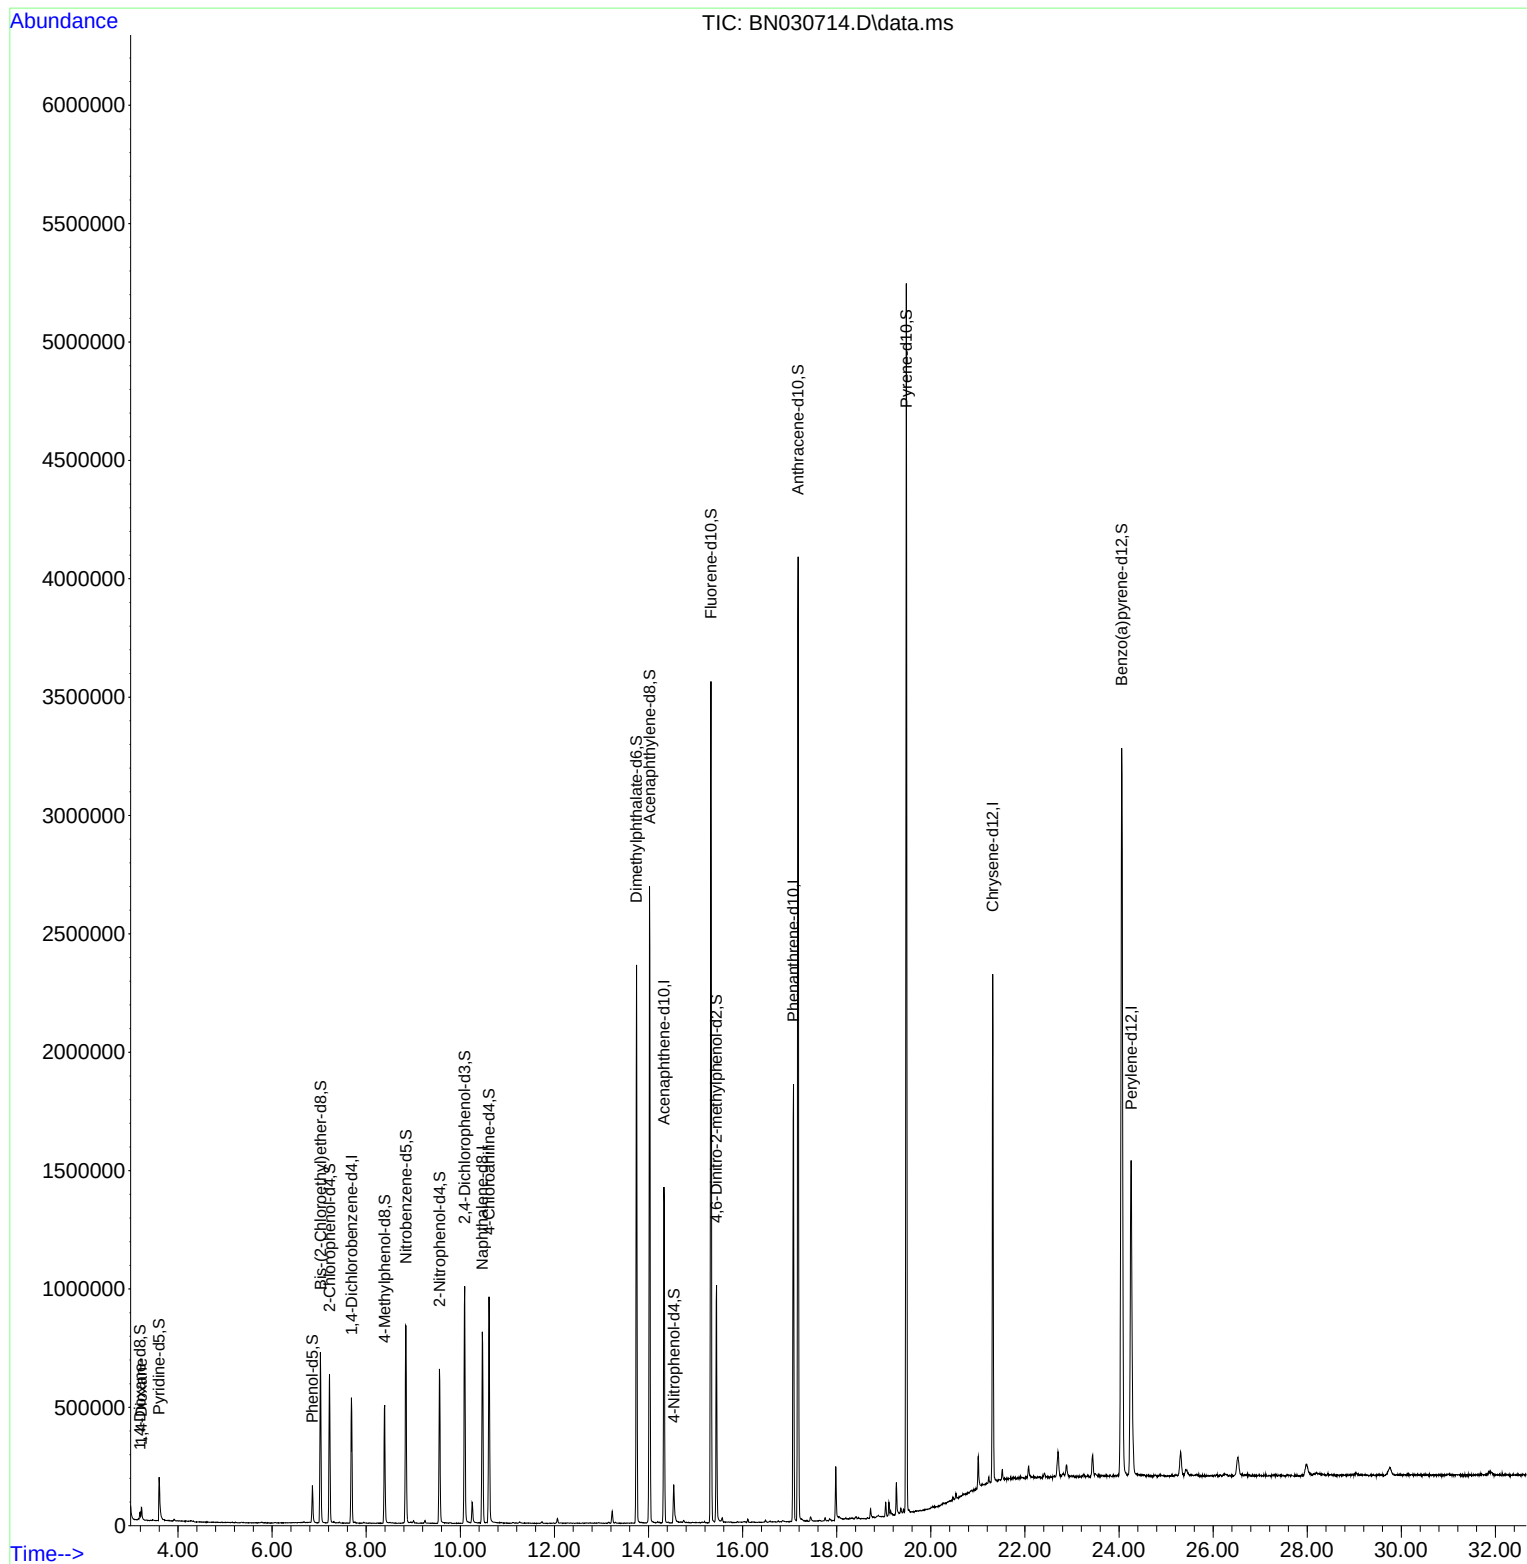

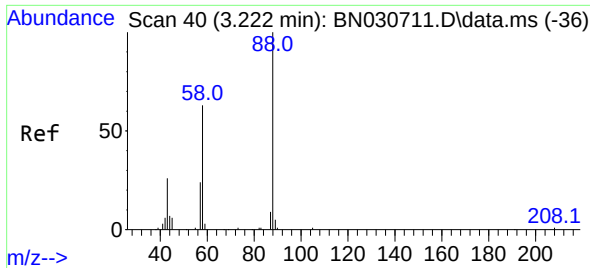

#2
1,4-Dioxane
Concen: 8.993 ng/uL
RT: 3.222 min Scan# 40
Delta R.T. -0.012 min
Lab File: BN030714.D
Acq: 06 Apr 2024 19:07

Instrument :
BNA_N
ClientSampleId :
C0AJ2

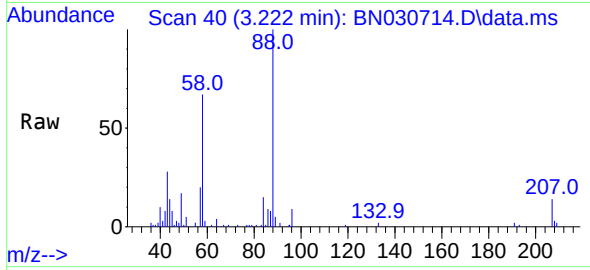

Tgt Ion:	88	Resp:	29783
Ion	Ratio	Lower	Upper
88	100		
43	28.1	23.8	35.8
58	67.2	56.6	84.8

