

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030731.D
 Acq On : 07 Apr 2024 06:51
 Operator : MA/JU
 Sample : P1987-09
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R77

Quant Time: Apr 07 13:39:25 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 12:24:07 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.687	152	154192	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.469	136	760229	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.328	164	553461	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.075	188	1244101	20.000	ng/u1	-0.01
79) Chrysene-d12	21.316	240	1233552	20.000	ng/u1	-0.01
88) Perylene-d12	24.251	264	1359458	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	17852	5.428	ng/uL	-0.01
4) Pyridine-d5	3.599	84	95037	9.638	ng/u1	0.00
7) Phenol-d5	6.858	99	91924	7.370	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.028	67	290486	37.705	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.216	132	290738	30.726	ng/u1	-0.01
15) 4-Methylphenol-d8	8.387	113	191268	18.296	ng/u1	-0.01
21) Nitrobenzene-d5	8.840	128	208263	39.491	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.557	143	205793	42.657	ng/u1	-0.01
28) 2,4-Dichlorophenol-d3	10.087	165	366962	34.744	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.610	131	560600	32.241	ng/u1	-0.01
46) Dimethylphthalate-d6	13.745	166	1576840	42.672	ng/u1	-0.01
49) Acenaphthylene-d8	14.022	160	1703422	40.093	ng/u1	-0.01
54) 4-Nitrophenol-d4	14.534	143	49105	6.947	ng/u1	0.00
60) Fluorene-d10	15.322	176	1371798	42.423	ng/u1	-0.02
65) 4,6-Dinitro-2-methylph...	15.445	200	195834	35.662	ng/u1	0.00
73) Anthracene-d10	17.175	188	2491401	46.478	ng/u1	-0.01
81) Pyrene-d10	19.480	212	2968180	44.755	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.057	264	2999581	47.886	ng/u1	-0.02
Target Compounds						
35) 4-Chloro-3-methylphenol	11.757	107	44324	3.650	ng/u1	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030731.D
Acq On : 07 Apr 2024 06:51
Operator : MA/JU
Sample : P1987-09
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R77


Quant Time: Apr 07 13:39:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

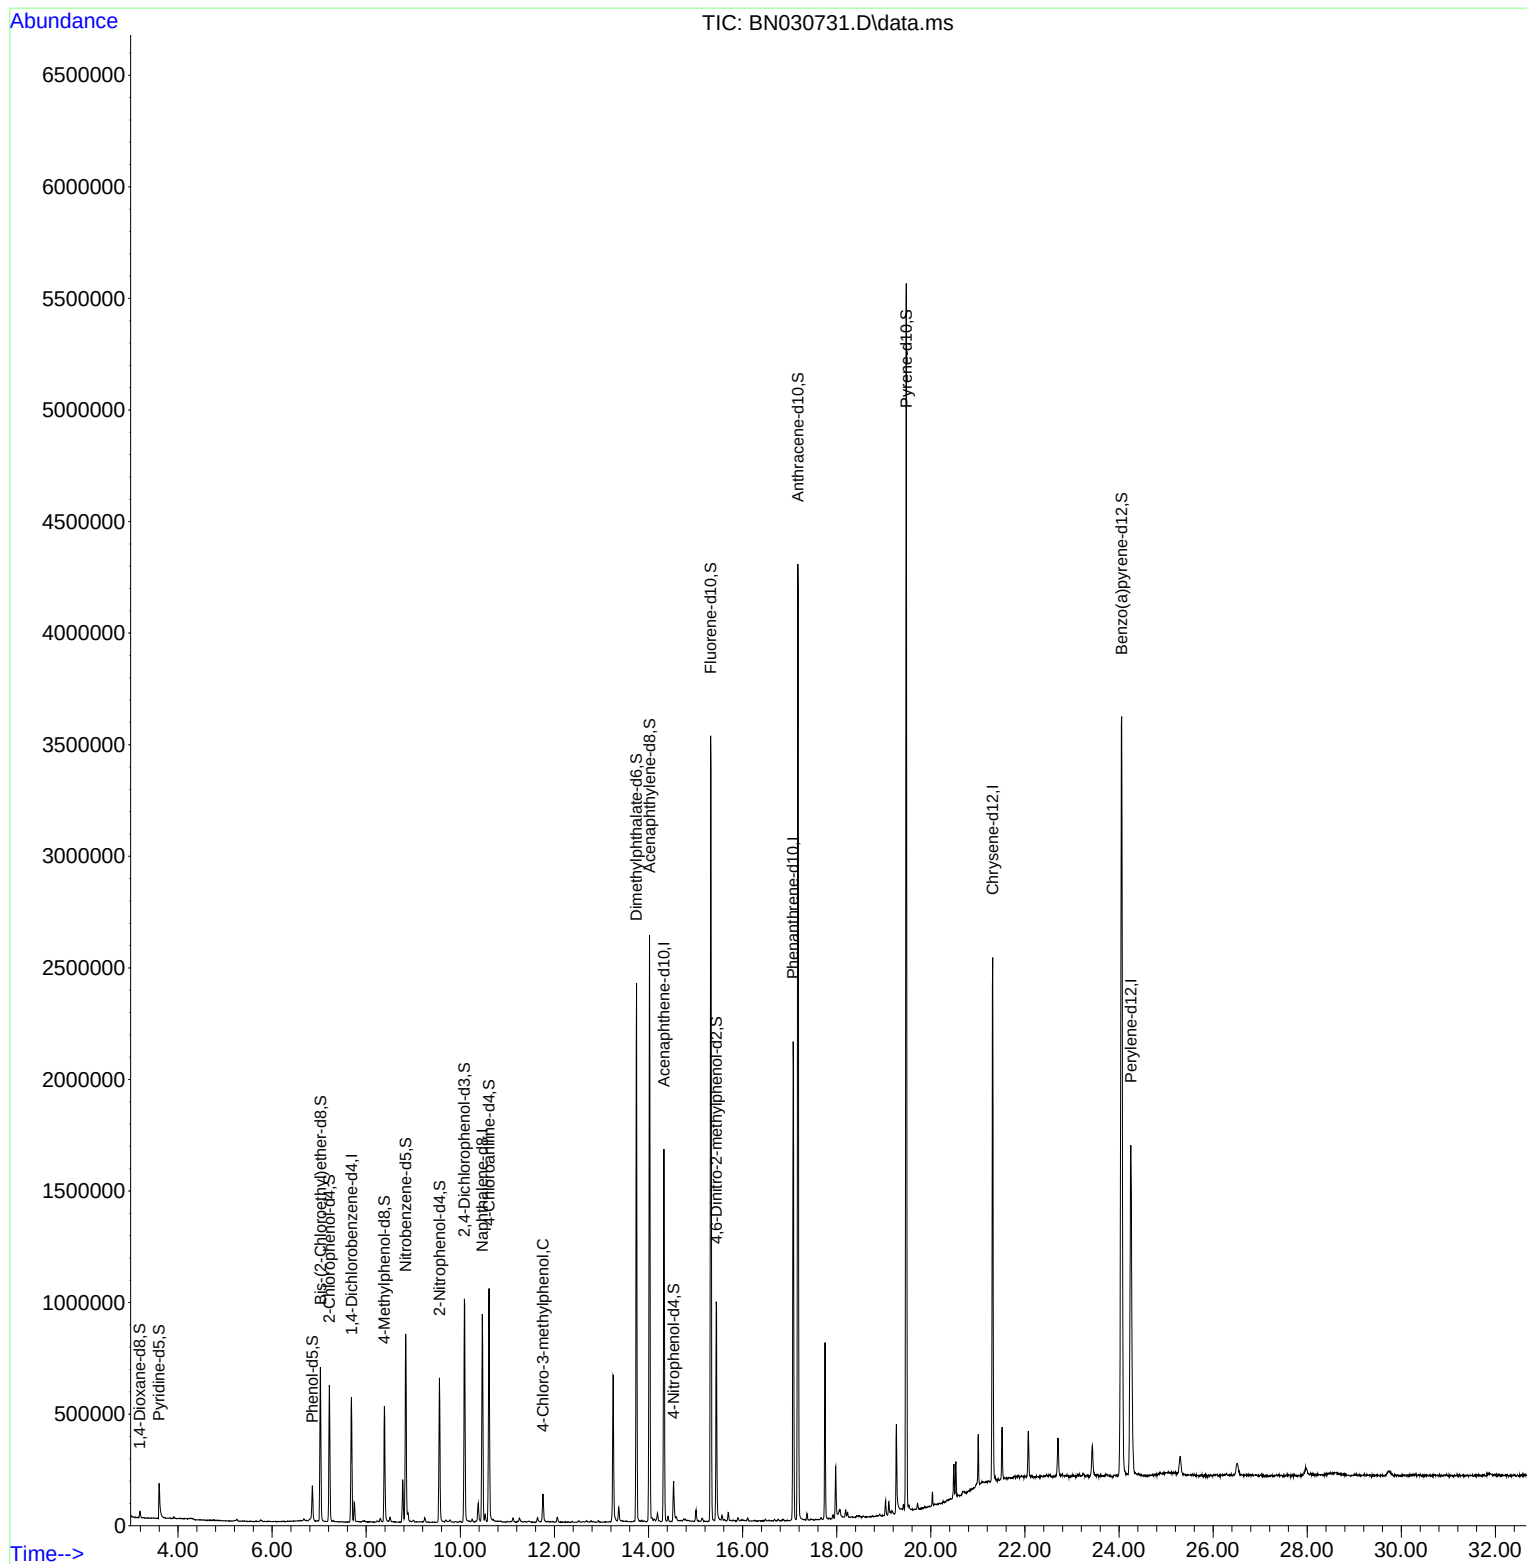

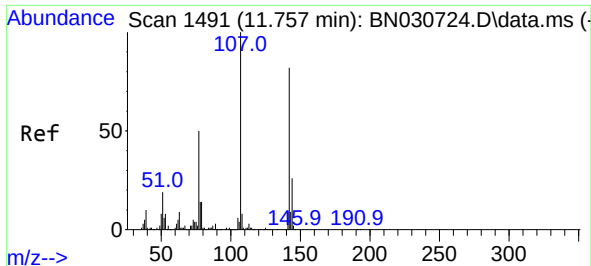

#35
4-Chloro-3-methylphenol
Concen: 3.650 ng/ul
RT: 11.757 min Scan# 1491
Delta R.T. -0.012 min
Lab File: BN030731.D
Acq: 07 Apr 2024 06:51

Instrument :
BNA_N
ClientSampleId :
MC0R77

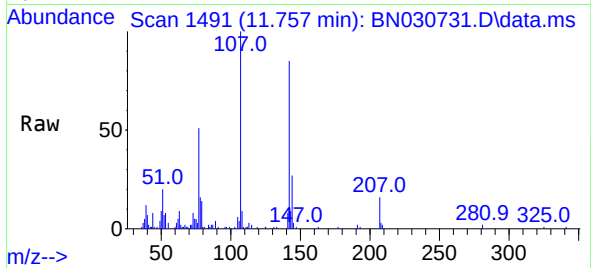

Tgt Ion:107 Resp: 44324
Ion Ratio Lower Upper
107 100
144 27.4 21.4 32.0
142 85.2 65.9 98.9

