

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030670.D
 Acq On : 05 Apr 2024 12:23
 Operator : MA/JU
 Sample : PB160011BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK011

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030670.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	42	rVB	45397	60730	0.90%	0.107%
2	3.599	100	104	121	rBV	584811	945032	14.07%	1.669%
3	3.922	155	159	163	rBV3	7048	11059	0.16%	0.020%
4	6.858	651	658	668	rBV	714801	1143193	17.02%	2.019%
5	7.034	681	688	697	rBV	617070	987970	14.71%	1.745%
6	7.222	714	720	734	rBV	753135	1186356	17.66%	2.095%
7	7.693	792	800	810	rBV	491955	784372	11.68%	1.385%
8	8.393	911	919	934	rBV	950480	1505029	22.41%	2.658%
9	8.846	987	996	1010	rBV	759708	1224806	18.24%	2.163%
10	9.563	1110	1118	1128	rBV	628804	1013492	15.09%	1.790%
11	10.093	1201	1208	1222	rBV	918603	1535375	22.86%	2.711%
12	10.475	1264	1273	1284	rBV	791834	1282904	19.10%	2.265%
13	10.616	1289	1297	1317	rBV	1282537	2169211	32.30%	3.831%
14	12.069	1538	1544	1549	rBV	17596	28062	0.42%	0.050%
15	13.228	1737	1741	1748	rBV2	19221	31397	0.47%	0.055%
16	13.751	1823	1830	1841	rBV	2154928	3014989	44.89%	5.324%
17	14.028	1870	1877	1890	rBV	2296330	3400902	50.63%	6.006%
18	14.334	1921	1929	1939	rBV	1374501	1992459	29.66%	3.519%
19	14.534	1957	1963	1977	rBV	902522	1484664	22.10%	2.622%
20	14.745	1998	1999	2006	rVB7	5257	8592	0.13%	0.015%
21	15.328	2091	2098	2112	rBV	2999880	4294550	63.94%	7.584%
22	15.445	2112	2118	2131	rVV	942767	1340012	19.95%	2.366%
23	15.569	2135	2139	2145	rVB5	16091	24693	0.37%	0.044%
24	16.116	2226	2232	2236	rBV6	10743	16120	0.24%	0.028%
25	17.081	2390	2396	2406	rBV	1825765	2599839	38.71%	4.591%
26	17.181	2407	2413	2428	rVV2	3616670	4994126	74.35%	8.819%
27	17.980	2545	2549	2557	rBV3	48553	76461	1.14%	0.135%
28	19.045	2726	2730	2736	rVB2	45960	62609	0.93%	0.111%
29	19.116	2738	2742	2747	rVV	37130	52426	0.78%	0.093%
30	19.275	2765	2769	2774	rBV3	33333	51505	0.77%	0.091%
31	19.422	2792	2794	2798	rBV3	9704	11893	0.18%	0.021%
32	19.486	2798	2805	2811	rBV	4245607	6072935	90.42%	10.724%
33	21.321	3111	3117	3124	rBV	2119906	3083729	45.91%	5.446%
34	24.068	3574	3584	3598	rVB2	2783964	6716613	100.00%	11.861%
35	24.262	3609	3617	3633	rVB	1361793	3419896	50.92%	6.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030670.D
Acq On : 05 Apr 2024 12:23
Operator : MA/JU
Sample : PB160011BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK011

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 56628001

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030670.D
Acq On : 05 Apr 2024 12:23
Operator : MA/JU
Sample : PB160011BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK011

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

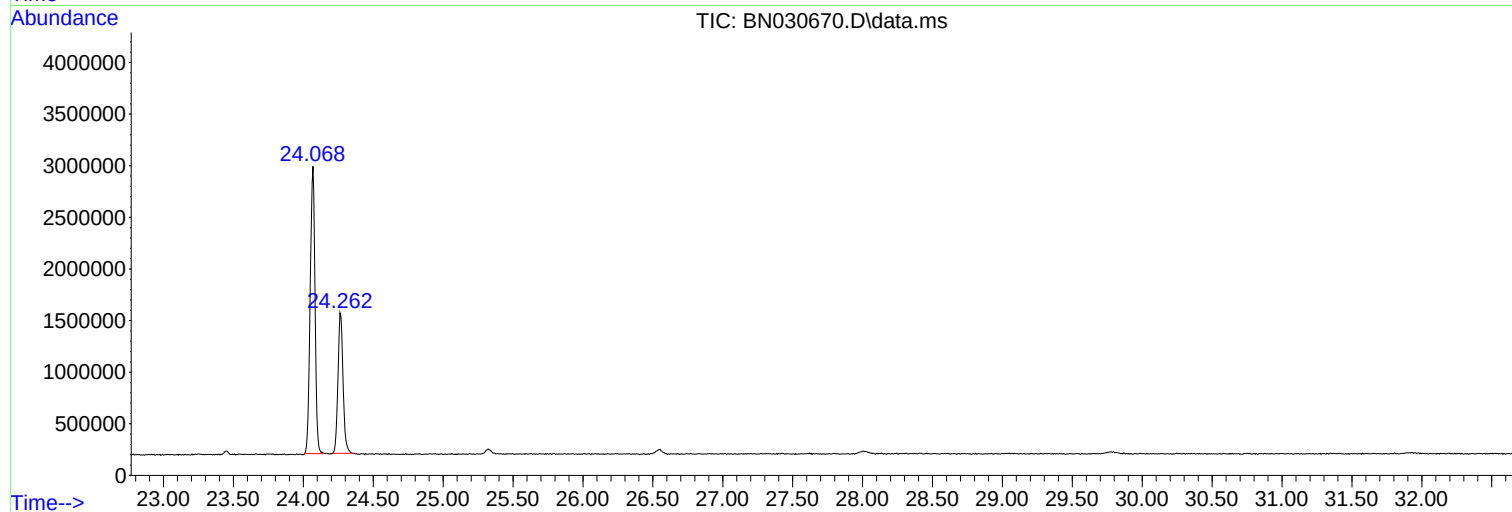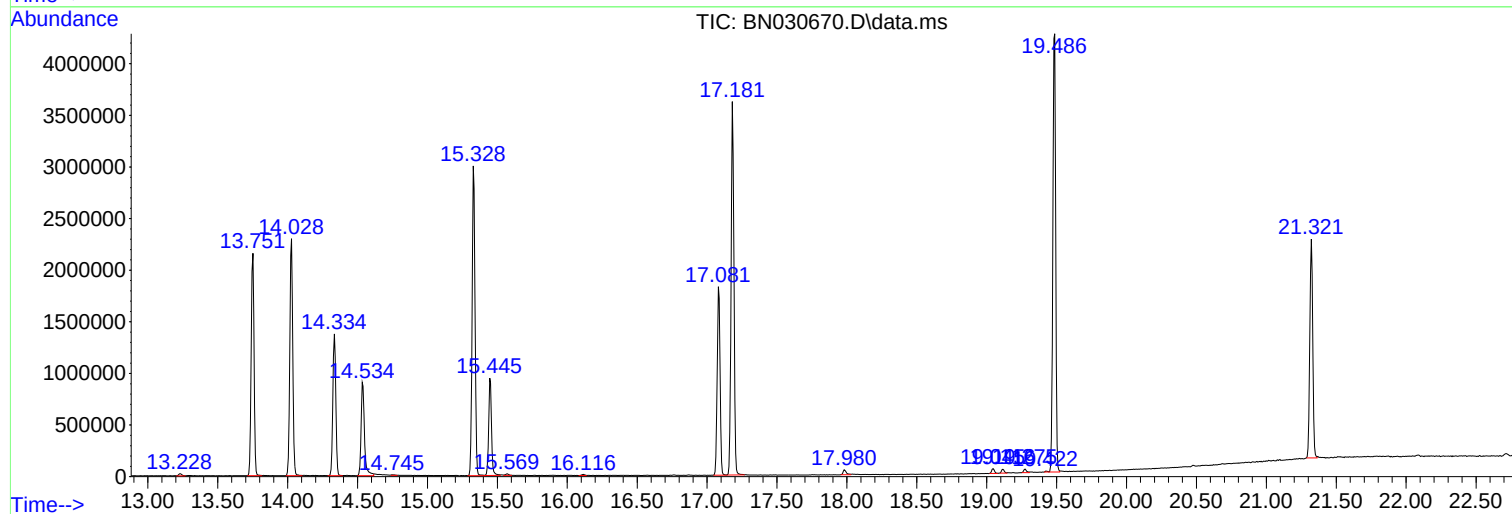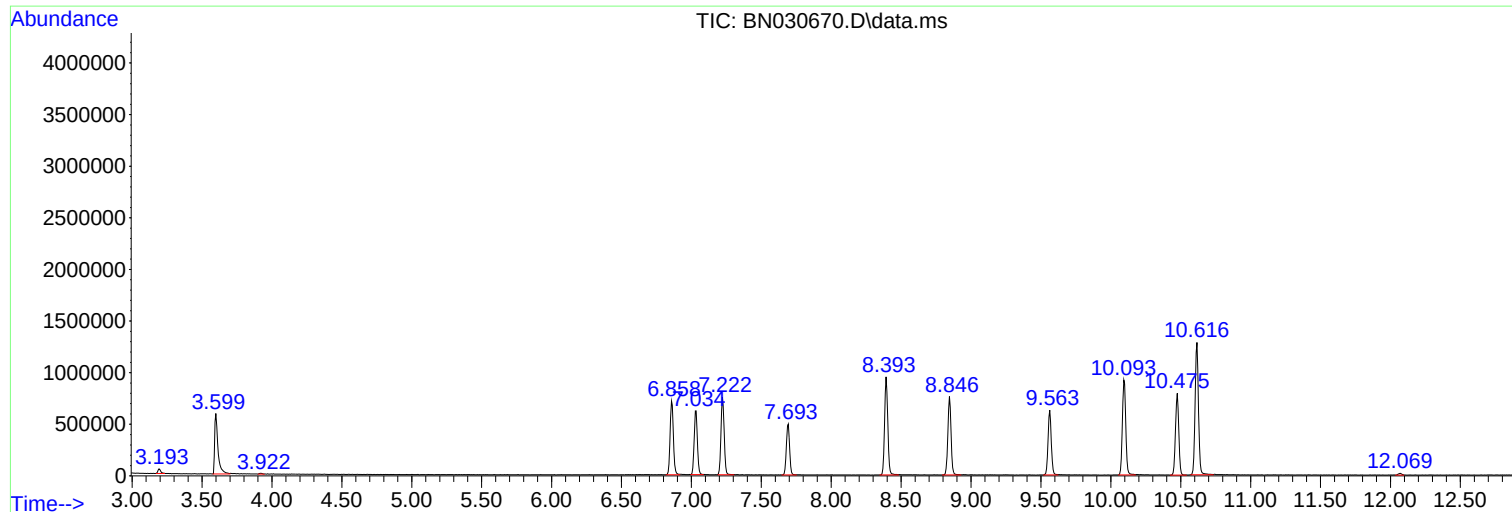

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030670.D
Acq On : 05 Apr 2024 12:23
Operator : MA/JU
Sample : PB160011BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK011

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030670.D
Acq On : 05 Apr 2024 12:23
Operator : MA/JU
Sample : PB160011BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK011

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------