

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030677.D
 Acq On : 05 Apr 2024 16:59
 Operator : MA/JU
 Sample : P1989-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07W0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030677.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	45	rVB	33379	48704	0.56%	0.081%
2	3.599	102	104	119	rBV	173236	299131	3.43%	0.497%
3	3.922	154	159	167	rBV	15500	25881	0.30%	0.043%
4	6.863	650	659	669	rVB	152595	272802	3.13%	0.453%
5	7.034	679	688	700	rBV	649032	1033641	11.86%	1.717%
6	7.222	713	720	732	rBV	594462	950540	10.90%	1.579%
7	7.692	793	800	809	rBV	540425	843923	9.68%	1.402%
8	8.392	912	919	930	rBV	476992	780797	8.96%	1.297%
9	8.592	949	953	960	rVB	9511	14738	0.17%	0.024%
10	8.845	988	996	1006	rBV	815936	1314965	15.09%	2.184%
11	8.957	1009	1015	1019	rVV3	10736	21564	0.25%	0.036%
12	9.010	1019	1024	1031	rVB4	12729	21844	0.25%	0.036%
13	9.251	1058	1065	1069	rBV	10170	14154	0.16%	0.024%
14	9.563	1109	1118	1126	rBV	530651	871491	10.00%	1.447%
15	10.098	1201	1209	1225	rBV	883069	1499936	17.21%	2.491%
16	10.475	1261	1273	1284	rVB	864603	1418896	16.28%	2.357%
17	10.616	1287	1297	1308	rBV	942796	1637391	18.78%	2.719%
18	10.716	1311	1314	1321	rVB5	8759	16376	0.19%	0.027%
19	10.875	1336	1341	1347	rVB9	4349	9560	0.11%	0.016%
20	11.275	1401	1409	1410	rBV7	6802	10791	0.12%	0.018%
21	11.298	1410	1413	1418	rVB6	6867	9714	0.11%	0.016%
22	12.069	1538	1544	1548	rBV	20845	35416	0.41%	0.059%
23	13.233	1735	1742	1748	rBV	27114	45522	0.52%	0.076%
24	13.298	1748	1753	1760	rBV9	5148	10915	0.13%	0.018%
25	13.751	1823	1830	1840	rBV	2417284	3343503	38.36%	5.553%
26	14.027	1867	1877	1885	rBV2	2651544	3877192	44.48%	6.439%
27	14.333	1921	1929	1941	rBV	1568830	2253125	25.85%	3.742%
28	14.539	1959	1964	1981	rBV	123808	245169	2.81%	0.407%
29	14.757	1997	2001	2006	rBV6	7331	13335	0.15%	0.022%
30	15.027	2043	2047	2052	rBV3	8891	13822	0.16%	0.023%
31	15.192	2073	2075	2079	rVB4	9360	10102	0.12%	0.017%
32	15.327	2092	2098	2109	rBV	3423263	5113206	58.66%	8.492%
33	15.445	2112	2118	2135	rVB	402751	592408	6.80%	0.984%
34	15.569	2135	2139	2145	rBV4	16627	28544	0.33%	0.047%
35	16.057	2218	2222	2228	rBV3	16220	26690	0.31%	0.044%
36	16.116	2228	2232	2238	rVB2	15230	23286	0.27%	0.039%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030677.D
 Acq On : 05 Apr 2024 16:59
 Operator : MA/JU
 Sample : P1989-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07W0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	16.851	2353	2357	2363	rBV3	22280	33572	0.39%	0.056%
38	17.086	2390	2397	2406	rBV	1975452	2909218	33.37%	4.832%
39	17.186	2407	2414	2424	rVV	4276956	6350358	72.85%	10.547%
40	17.280	2427	2430	2433	rVB4	10187	12973	0.15%	0.022%
41	17.592	2479	2483	2488	rBV2	22643	28144	0.32%	0.047%
42	17.763	2509	2512	2516	rVB5	8298	10399	0.12%	0.017%
43	17.927	2537	2540	2544	rVB4	11751	13372	0.15%	0.022%
44	17.980	2546	2549	2556	rBV2	28052	39396	0.45%	0.065%
45	18.239	2590	2593	2597	rVB5	11573	15446	0.18%	0.026%
46	18.286	2597	2601	2605	rBV	21980	32434	0.37%	0.054%
47	18.880	2700	2702	2706	rBV5	5952	8747	0.10%	0.015%
48	18.921	2706	2709	2712	rVB3	15296	16863	0.19%	0.028%
49	19.045	2725	2730	2735	rBV2	72272	99993	1.15%	0.166%
50	19.115	2738	2742	2746	rBV	58197	81910	0.94%	0.136%
51	19.151	2746	2748	2751	rVV4	15481	17035	0.20%	0.028%
52	19.268	2766	2768	2776	rBV6	22277	35761	0.41%	0.059%
53	19.427	2792	2795	2798	rVB3	17145	15353	0.18%	0.025%
54	19.486	2798	2805	2813	rBV	5580980	7694700	88.27%	12.780%
55	21.321	3111	3117	3126	rBV2	2338709	3438985	39.45%	5.712%
56	24.068	3574	3584	3596	rBV2	3606841	8716985	100.00%	14.478%
57	24.268	3609	3618	3632	rVB2	1527526	3888955	44.61%	6.459%


Sum of corrected areas: 60209673

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030677.D
Acq On : 05 Apr 2024 16:59
Operator : MA/JU
Sample : P1989-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07W0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

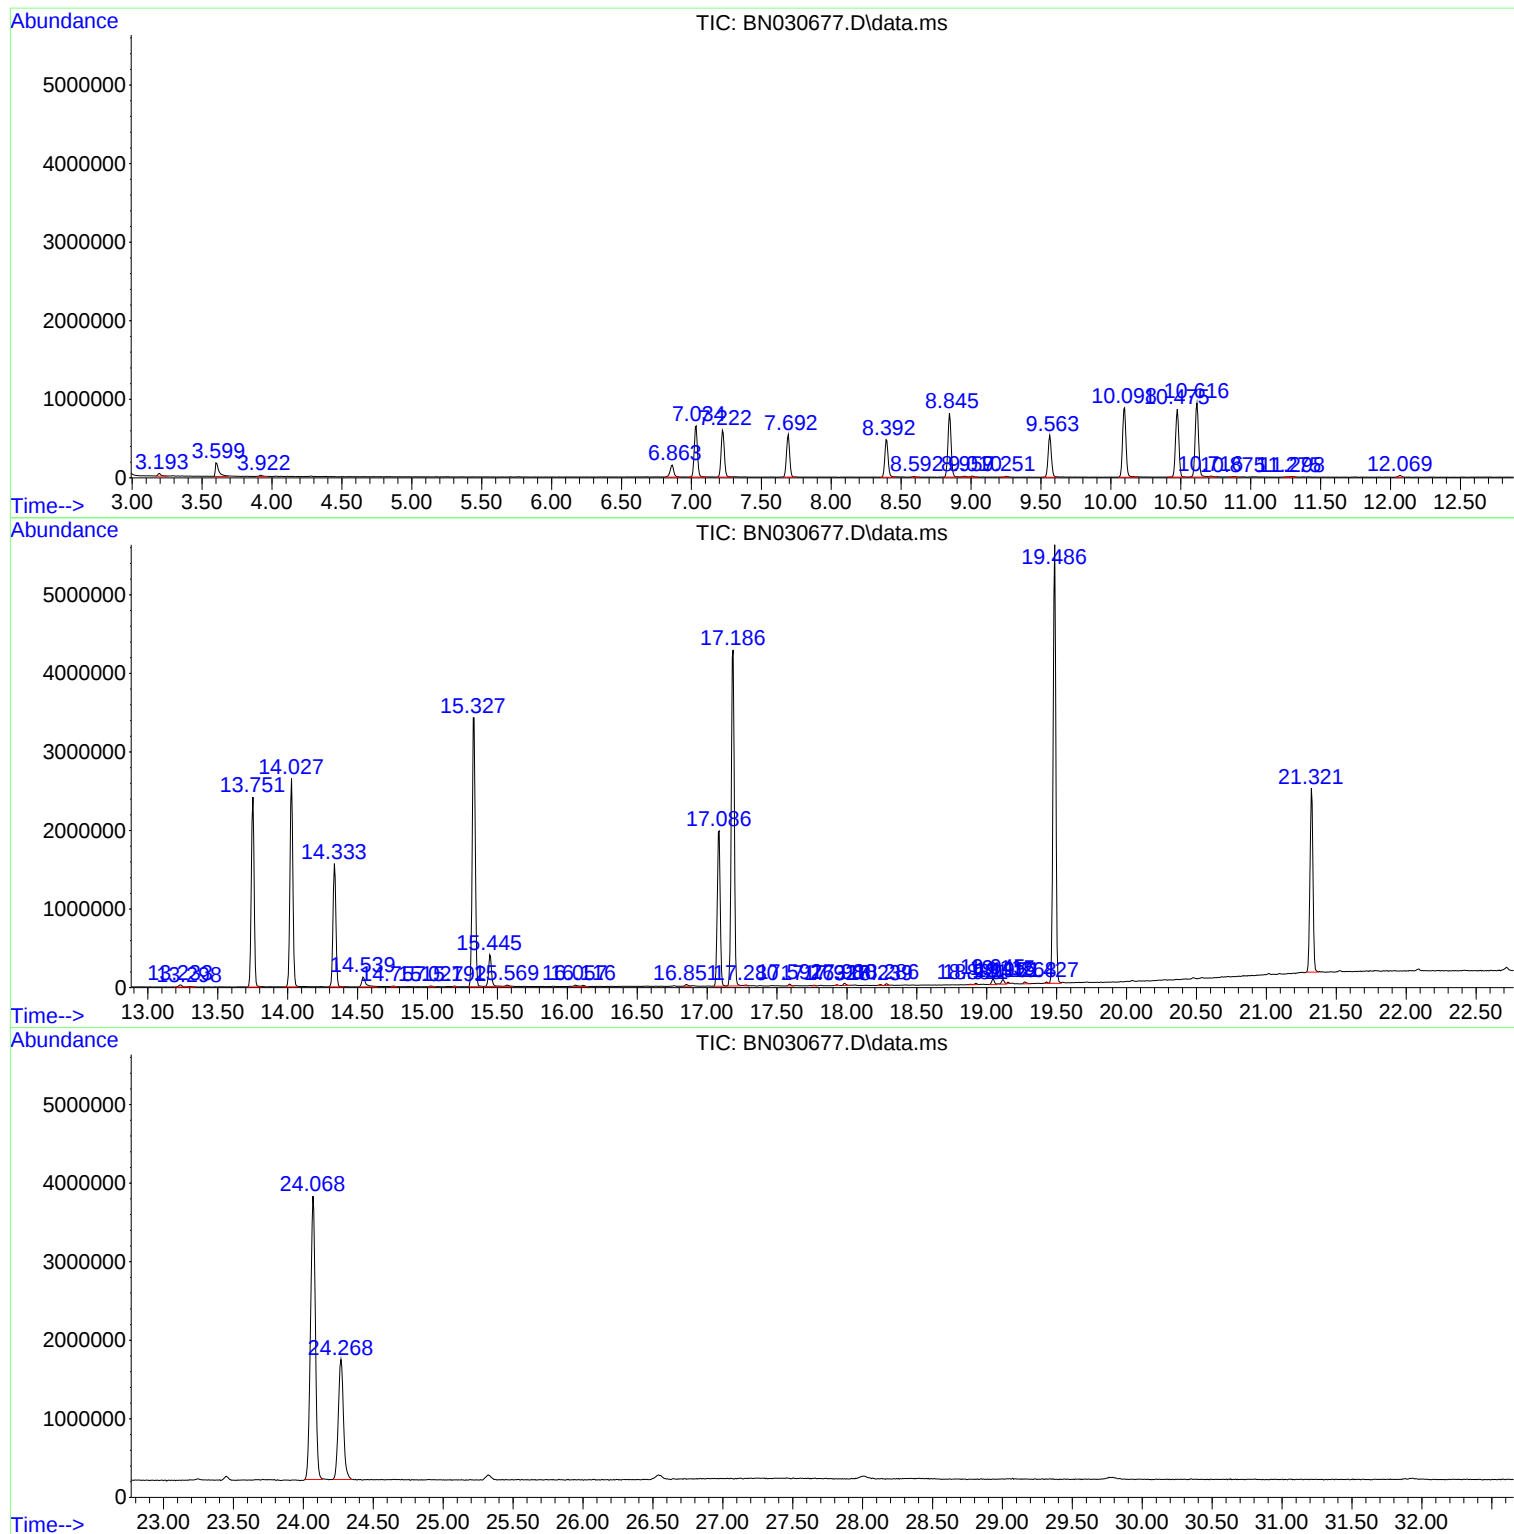

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030677.D
Acq On : 05 Apr 2024 16:59
Operator : MA/JU
Sample : P1989-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07W0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030677.D
Acq On : 05 Apr 2024 16:59
Operator : MA/JU
Sample : P1989-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07W0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------