

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030683.D
Acq On : 05 Apr 2024 21:34
Operator : MA/JU
Sample : PB160016BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK016

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BN030683.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	46	rVB	40661	60152	1.03%	0.111%
2	3.599	100	104	130	rVB	514404	848367	14.50%	1.571%
3	3.917	155	158	161	rBV2	5530	6646	0.11%	0.012%
4	6.858	652	658	673	rBV	641932	1035024	17.69%	1.916%
5	7.028	681	687	699	rVB	556995	878795	15.02%	1.627%
6	7.222	713	720	732	rBV	678231	1067649	18.24%	1.977%
7	7.693	792	800	810	rBV	546107	891947	15.24%	1.652%
8	8.393	912	919	933	rBV	855446	1359478	23.23%	2.517%
9	8.846	987	996	1005	rBV	667727	1093033	18.68%	2.024%
10	9.563	1110	1118	1128	rBV	555589	906294	15.49%	1.678%
11	10.093	1201	1208	1217	rBV	842955	1416524	24.21%	2.623%
12	10.475	1264	1273	1282	rBV	866999	1456134	24.88%	2.696%
13	10.616	1289	1297	1313	rBV	1162253	2025425	34.61%	3.750%
14	12.069	1538	1544	1551	rBV2	17460	27235	0.47%	0.050%
15	13.228	1737	1741	1747	rVB	17302	27580	0.47%	0.051%
16	13.751	1823	1830	1837	rBV	1919727	2674505	45.70%	4.952%
17	14.028	1870	1877	1893	rBV	2048062	3114370	53.22%	5.767%
18	14.334	1922	1929	1939	rBV	1600722	2287166	39.08%	4.235%
19	14.540	1957	1964	1977	rBV	801712	1311564	22.41%	2.429%
20	15.328	2091	2098	2107	rBV	2776702	3962698	67.71%	7.337%
21	15.445	2112	2118	2130	rVV	756488	1118642	19.12%	2.071%
22	15.569	2134	2139	2143	rVB2	13320	20757	0.35%	0.038%
23	16.116	2226	2232	2236	rBV6	10152	15840	0.27%	0.029%
24	16.869	2355	2360	2363	rBV4	5276	7143	0.12%	0.013%
25	17.081	2390	2396	2405	rBV	2038812	3009899	51.43%	5.573%
26	17.181	2407	2413	2429	rVV2	3220982	4476962	76.50%	8.290%
27	17.980	2543	2549	2552	rBV6	11750	18434	0.31%	0.034%
28	19.045	2726	2730	2735	rBV2	40750	56826	0.97%	0.105%
29	19.116	2737	2742	2746	rBV	37514	52908	0.90%	0.098%
30	19.269	2766	2768	2774	rBV6	8045	9987	0.17%	0.018%
31	19.422	2791	2794	2798	rBV3	12653	16595	0.28%	0.031%
32	19.480	2798	2804	2813	rBV	3965415	5452933	93.18%	10.097%
33	21.322	3111	3117	3124	rBV	2355380	3557280	60.79%	6.587%
34	24.063	3574	3583	3600	rVB2	2407330	5852150	100.00%	10.836%
35	24.263	3608	3617	3634	rVB	1560584	3890090	66.47%	7.203%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030683.D
Acq On : 05 Apr 2024 21:34
Operator : MA/JU
Sample : PB160016BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK016

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 54007032

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030683.D
Acq On : 05 Apr 2024 21:34
Operator : MA/JU
Sample : PB160016BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK016

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

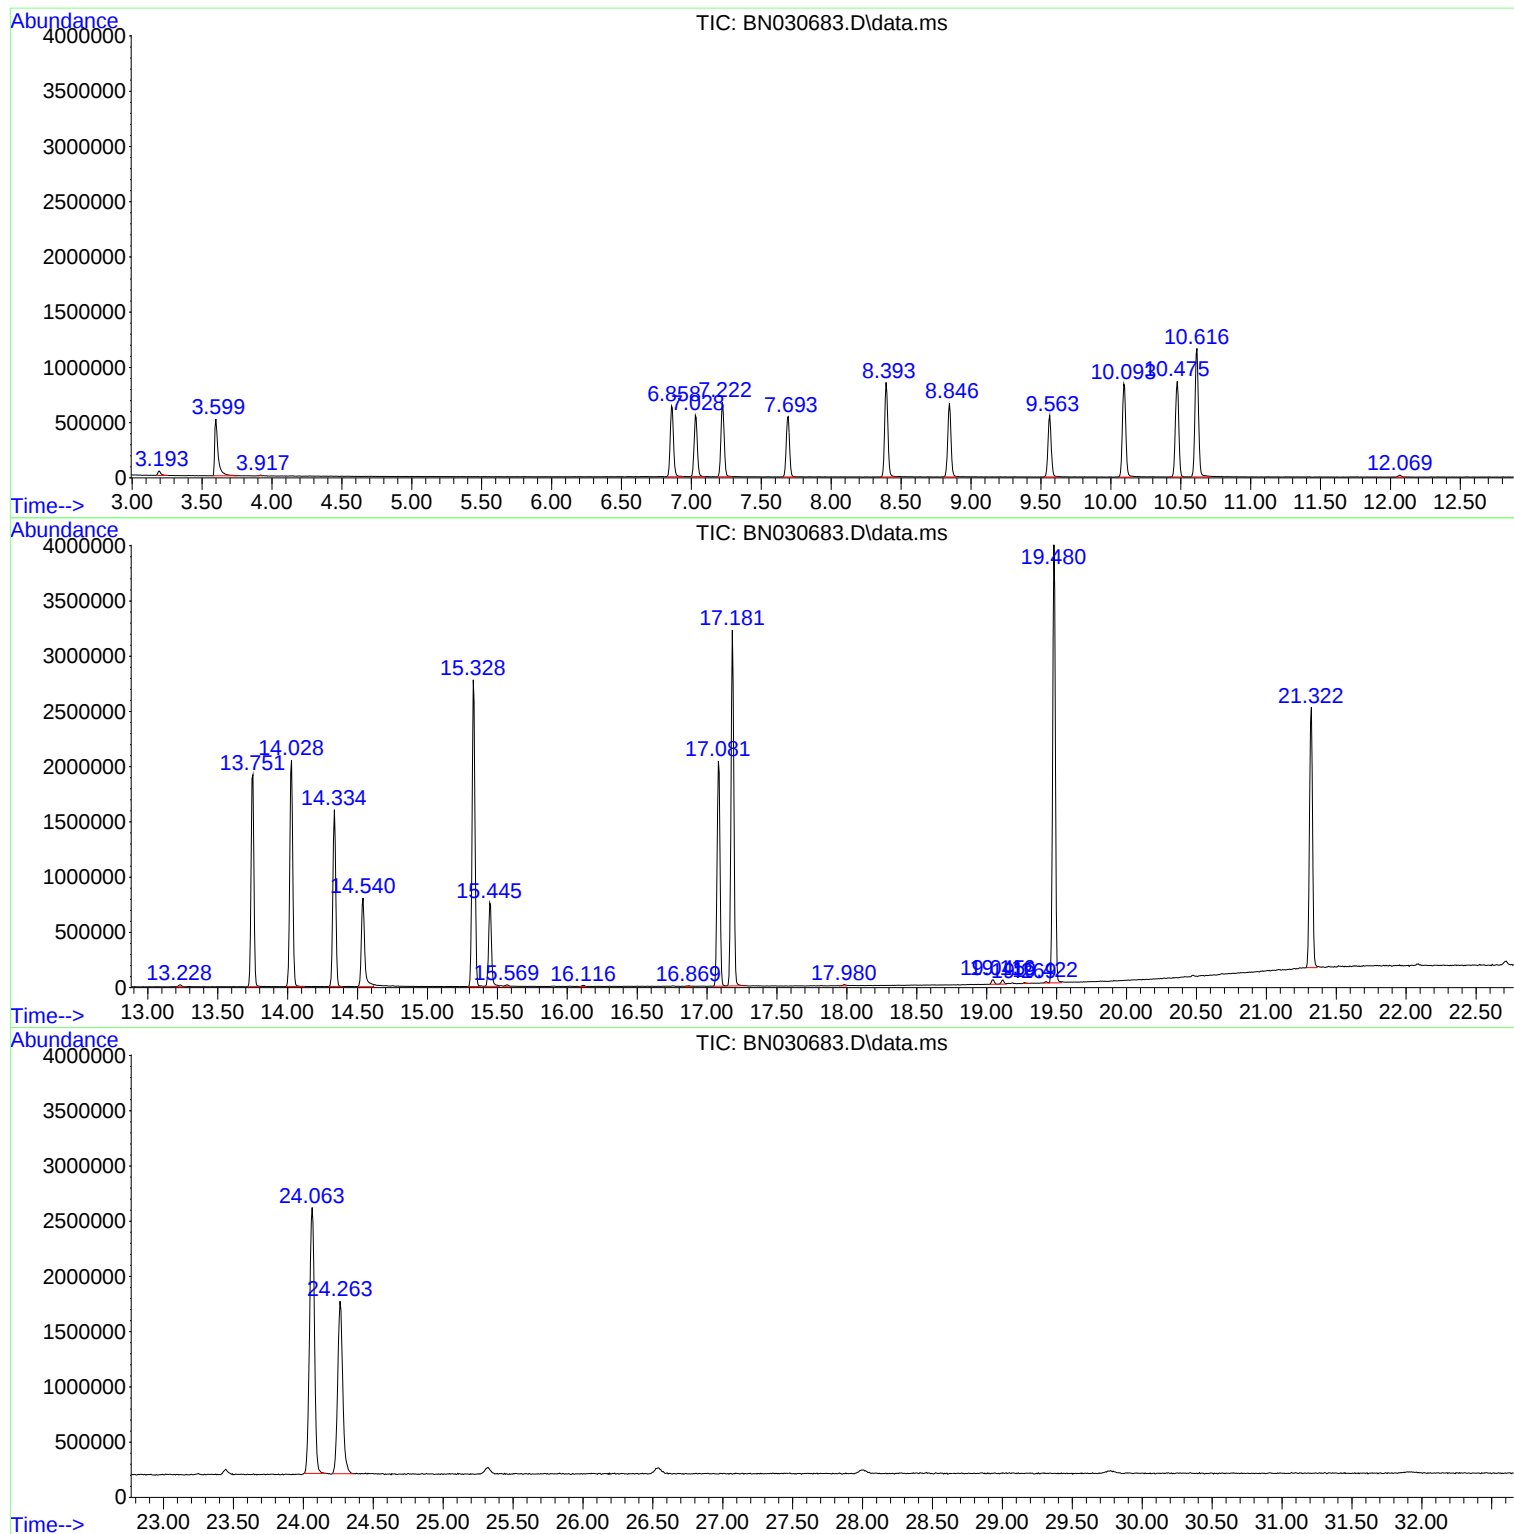

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030683.D
Acq On : 05 Apr 2024 21:34
Operator : MA/JU
Sample : PB160016BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK016

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030683.D
Acq On : 05 Apr 2024 21:34
Operator : MA/JU
Sample : PB160016BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK016

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------