

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030707.D
 Acq On : 06 Apr 2024 13:54
 Operator : MA/JU
 Sample : P1970-08
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030707.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.158	25	29	32	rBV	87049	117926	1.33%	0.170%
2	3.193	32	35	37	rVV	51266	71439	0.81%	0.103%
3	3.228	37	41	50	rVB	241110	340724	3.84%	0.493%
4	3.605	103	105	117	rBV	147773	230056	2.60%	0.333%
5	3.917	155	158	162	rVB2	8569	10450	0.12%	0.015%
6	4.434	241	246	255	rVB	41436	67661	0.76%	0.098%
7	5.811	476	480	484	rVB5	7549	11764	0.13%	0.017%
8	6.858	651	658	668	rBV	173693	275224	3.10%	0.398%
9	7.028	680	687	700	rVB	804215	1256295	14.17%	1.816%
10	7.222	712	720	731	rBV	717881	1148038	12.95%	1.659%
11	7.311	731	735	741	rVB7	5297	9903	0.11%	0.014%
12	7.687	792	799	807	rBV	611859	958143	10.81%	1.385%
13	7.805	815	819	824	rVB5	13333	22609	0.26%	0.033%
14	8.393	912	919	932	rBV	564521	922710	10.41%	1.334%
15	8.846	988	996	1011	rBV	976920	1601684	18.07%	2.315%
16	9.005	1018	1023	1030	rVB8	5276	12282	0.14%	0.018%
17	9.252	1059	1065	1071	rVB2	10212	17434	0.20%	0.025%
18	9.558	1108	1117	1130	rBV	783395	1301802	14.69%	1.882%
19	10.093	1200	1208	1228	rBV	1173563	1955250	22.06%	2.826%
20	10.258	1229	1236	1250	rVB	21126	43622	0.49%	0.063%
21	10.469	1263	1272	1283	rBV	983075	1617954	18.25%	2.339%
22	10.610	1288	1296	1313	rBV	1041208	1783584	20.12%	2.578%
23	12.063	1537	1543	1550	rVB2	23721	40075	0.45%	0.058%
24	13.228	1735	1741	1748	rVB	33868	51045	0.58%	0.074%
25	13.746	1822	1829	1841	rBV	2735182	3877900	43.75%	5.605%
26	14.022	1869	1876	1892	rBV	3005804	4526932	51.07%	6.544%
27	14.334	1922	1929	1941	rBV	1657785	2503927	28.25%	3.619%
28	14.534	1957	1963	1976	rBV	185142	336804	3.80%	0.487%
29	14.751	1993	2000	2005	rVB10	9352	14670	0.17%	0.021%
30	15.328	2091	2098	2111	rBV	4084286	5910040	66.67%	8.543%
31	15.445	2112	2118	2132	rVV	1299082	1832045	20.67%	2.648%
32	15.569	2134	2139	2144	rVB2	19201	31269	0.35%	0.045%
33	16.110	2228	2231	2236	rVB3	14744	20792	0.23%	0.030%
34	16.757	2337	2341	2346	rVB6	7122	10601	0.12%	0.015%
35	16.857	2353	2358	2365	rBV6	5671	13390	0.15%	0.019%
36	17.081	2389	2396	2406	rBV	2354719	3230750	36.45%	4.670%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030707.D
 Acq On : 06 Apr 2024 13:54
 Operator : MA/JU
 Sample : P1970-08
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	17.181	2406	2413	2424	rVV	4938073	7061303	79.66%	10.207%
38	17.375	2442	2446	2452	rVB3	9148	12752	0.14%	0.018%
39	17.981	2544	2549	2557	rBV	116984	170749	1.93%	0.247%
40	18.051	2559	2561	2570	rVB4	8702	14960	0.17%	0.022%
41	18.416	2619	2623	2626	rBV4	13169	16357	0.18%	0.024%
42	19.039	2725	2729	2736	rBV2	71833	101593	1.15%	0.147%
43	19.110	2737	2741	2745	rBV	68869	95127	1.07%	0.138%
44	19.269	2764	2768	2774	rBV	83438	113912	1.29%	0.165%
45	19.422	2791	2794	2797	rVB2	20795	20245	0.23%	0.029%
46	19.481	2797	2804	2811	rBV	6335241	8558464	96.55%	12.371%
47	21.010	3061	3064	3069	rVB4	47553	60778	0.69%	0.088%
48	21.316	3110	3116	3123	rBV	2681515	3740336	42.20%	5.407%
49	23.439	3473	3477	3486	rVB3	88438	158359	1.79%	0.229%
50	24.063	3573	3583	3596	rVB2	3750064	8864087	100.00%	12.813%
51	24.257	3607	3616	3632	rBV	1512645	4015257	45.30%	5.804%




Sum of corrected areas: 69181073

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030707.D
Acq On : 06 Apr 2024 13:54
Operator : MA/JU
Sample : P1970-08
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

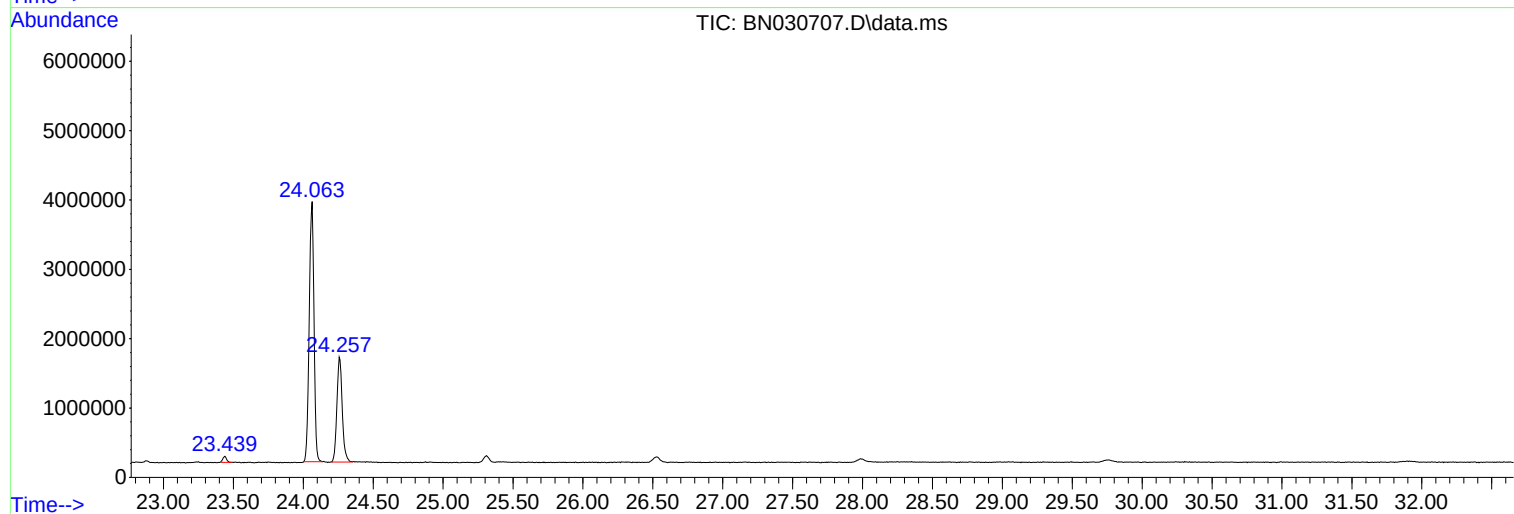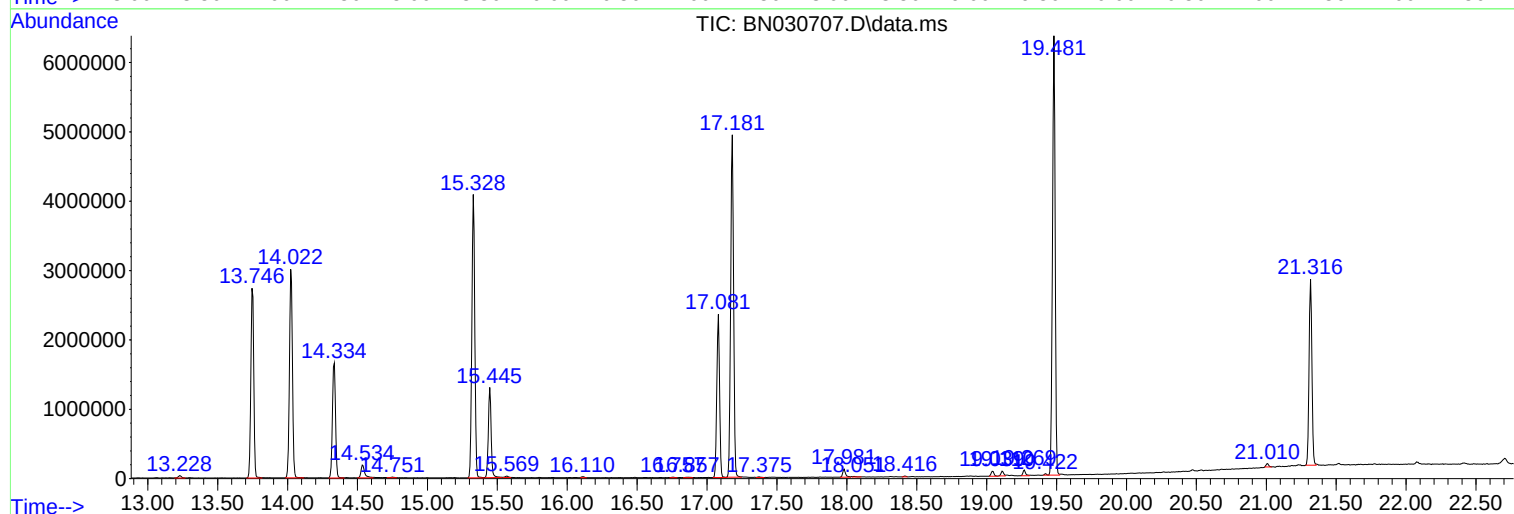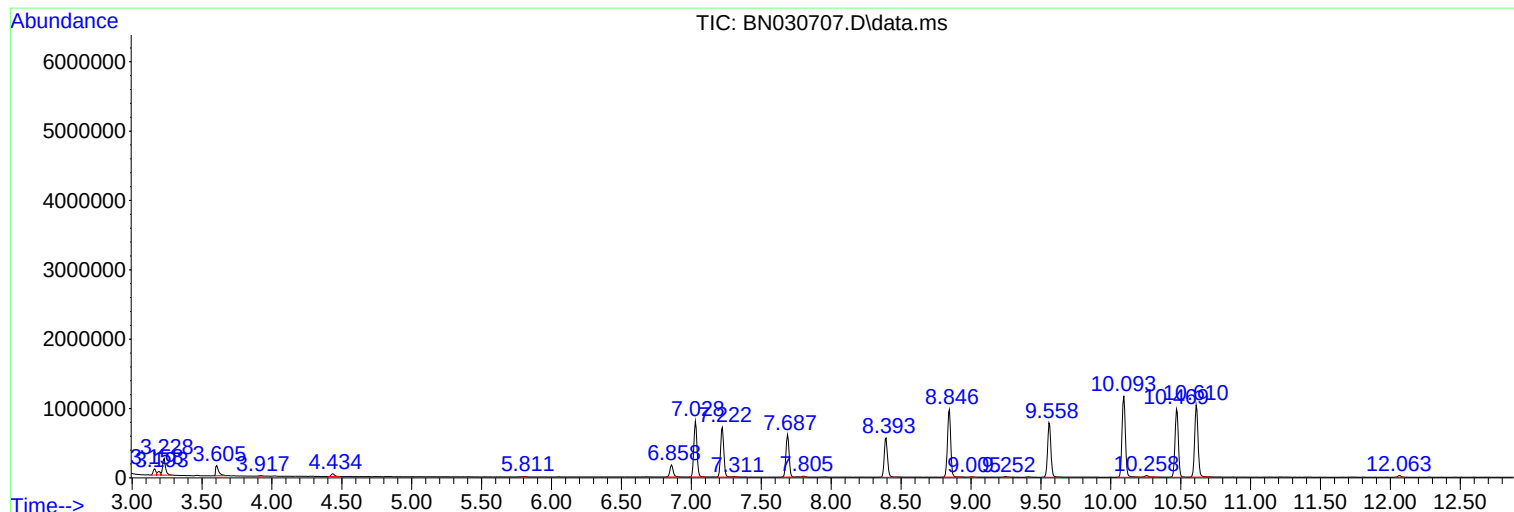

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030707.D
Acq On : 06 Apr 2024 13:54
Operator : MA/JU
Sample : P1970-08
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030707.D
Acq On : 06 Apr 2024 13:54
Operator : MA/JU
Sample : P1970-08
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AJ9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc