

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030713.D
 Acq On : 06 Apr 2024 18:28
 Operator : MA/JU
 Sample : PB159989BL
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK989

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030713.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	31	34	46	rVB	60507	94481	1.45%	0.164%
2	3.593	100	103	125	rBV	563088	946982	14.57%	1.642%
3	3.911	155	157	164	rVB2	6584	11010	0.17%	0.019%
4	6.858	651	658	669	rBV	771205	1195034	18.38%	2.073%
5	7.028	681	687	696	rVB	652185	1001639	15.41%	1.737%
6	7.222	713	720	732	rBV	768039	1215333	18.69%	2.108%
7	7.687	789	799	809	rBV	519144	816798	12.56%	1.417%
8	8.393	910	919	934	rBV	997064	1616960	24.87%	2.804%
9	8.840	987	995	1004	rBV	757071	1250626	19.24%	2.169%
10	9.557	1109	1117	1126	rBV	630765	1037260	15.96%	1.799%
11	10.093	1200	1208	1219	rBV	1025672	1697463	26.11%	2.944%
12	10.469	1265	1272	1280	rBV	834358	1374738	21.15%	2.384%
13	10.610	1289	1296	1308	rBV	1437208	2435780	37.47%	4.224%
14	12.063	1537	1543	1550	rVB2	18869	32384	0.50%	0.056%
15	13.228	1734	1741	1747	rBV3	17439	30490	0.47%	0.053%
16	13.745	1822	1829	1839	rBV	2138008	2903749	44.67%	5.036%
17	14.022	1869	1876	1890	rBV2	2421348	3509101	53.98%	6.086%
18	14.334	1922	1929	1936	rBV	1417731	2112521	32.49%	3.664%
19	14.534	1957	1963	1981	rBV	967004	1504142	23.14%	2.609%
20	15.328	2091	2098	2108	rBV	3191789	4434334	68.21%	7.691%
21	15.445	2112	2118	2134	rVV	860034	1204320	18.52%	2.089%
22	15.563	2134	2138	2143	rVB	14808	24441	0.38%	0.042%
23	16.110	2225	2231	2237	rVB5	11083	17104	0.26%	0.030%
24	16.863	2354	2359	2364	rBV3	4395	7697	0.12%	0.013%
25	17.081	2389	2396	2406	rBV	1926558	2727414	41.95%	4.730%
26	17.181	2406	2413	2426	rVV	3431736	5005598	77.00%	8.681%
27	17.751	2507	2510	2514	rVB5	10497	12824	0.20%	0.022%
28	17.981	2545	2549	2552	rBV4	10050	11949	0.18%	0.021%
29	19.039	2724	2729	2735	rBV2	47645	70457	1.08%	0.122%
30	19.110	2737	2741	2747	rVV	40563	53257	0.82%	0.092%
31	19.422	2792	2794	2797	rVB3	11663	10374	0.16%	0.018%
32	19.480	2798	2804	2812	rVV	4389767	6098785	93.81%	10.577%
33	21.316	3110	3116	3128	rBV2	2178946	3225767	49.62%	5.594%
34	24.063	3573	3583	3597	rVB2	2644034	6501157	100.00%	11.275%
35	24.257	3608	3616	3633	rVB	1321011	3467677	53.34%	6.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030713.D
Acq On : 06 Apr 2024 18:28
Operator : MA/JU
Sample : PB159989BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK989

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 57659646

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030713.D
Acq On : 06 Apr 2024 18:28
Operator : MA/JU
Sample : PB159989BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK989

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

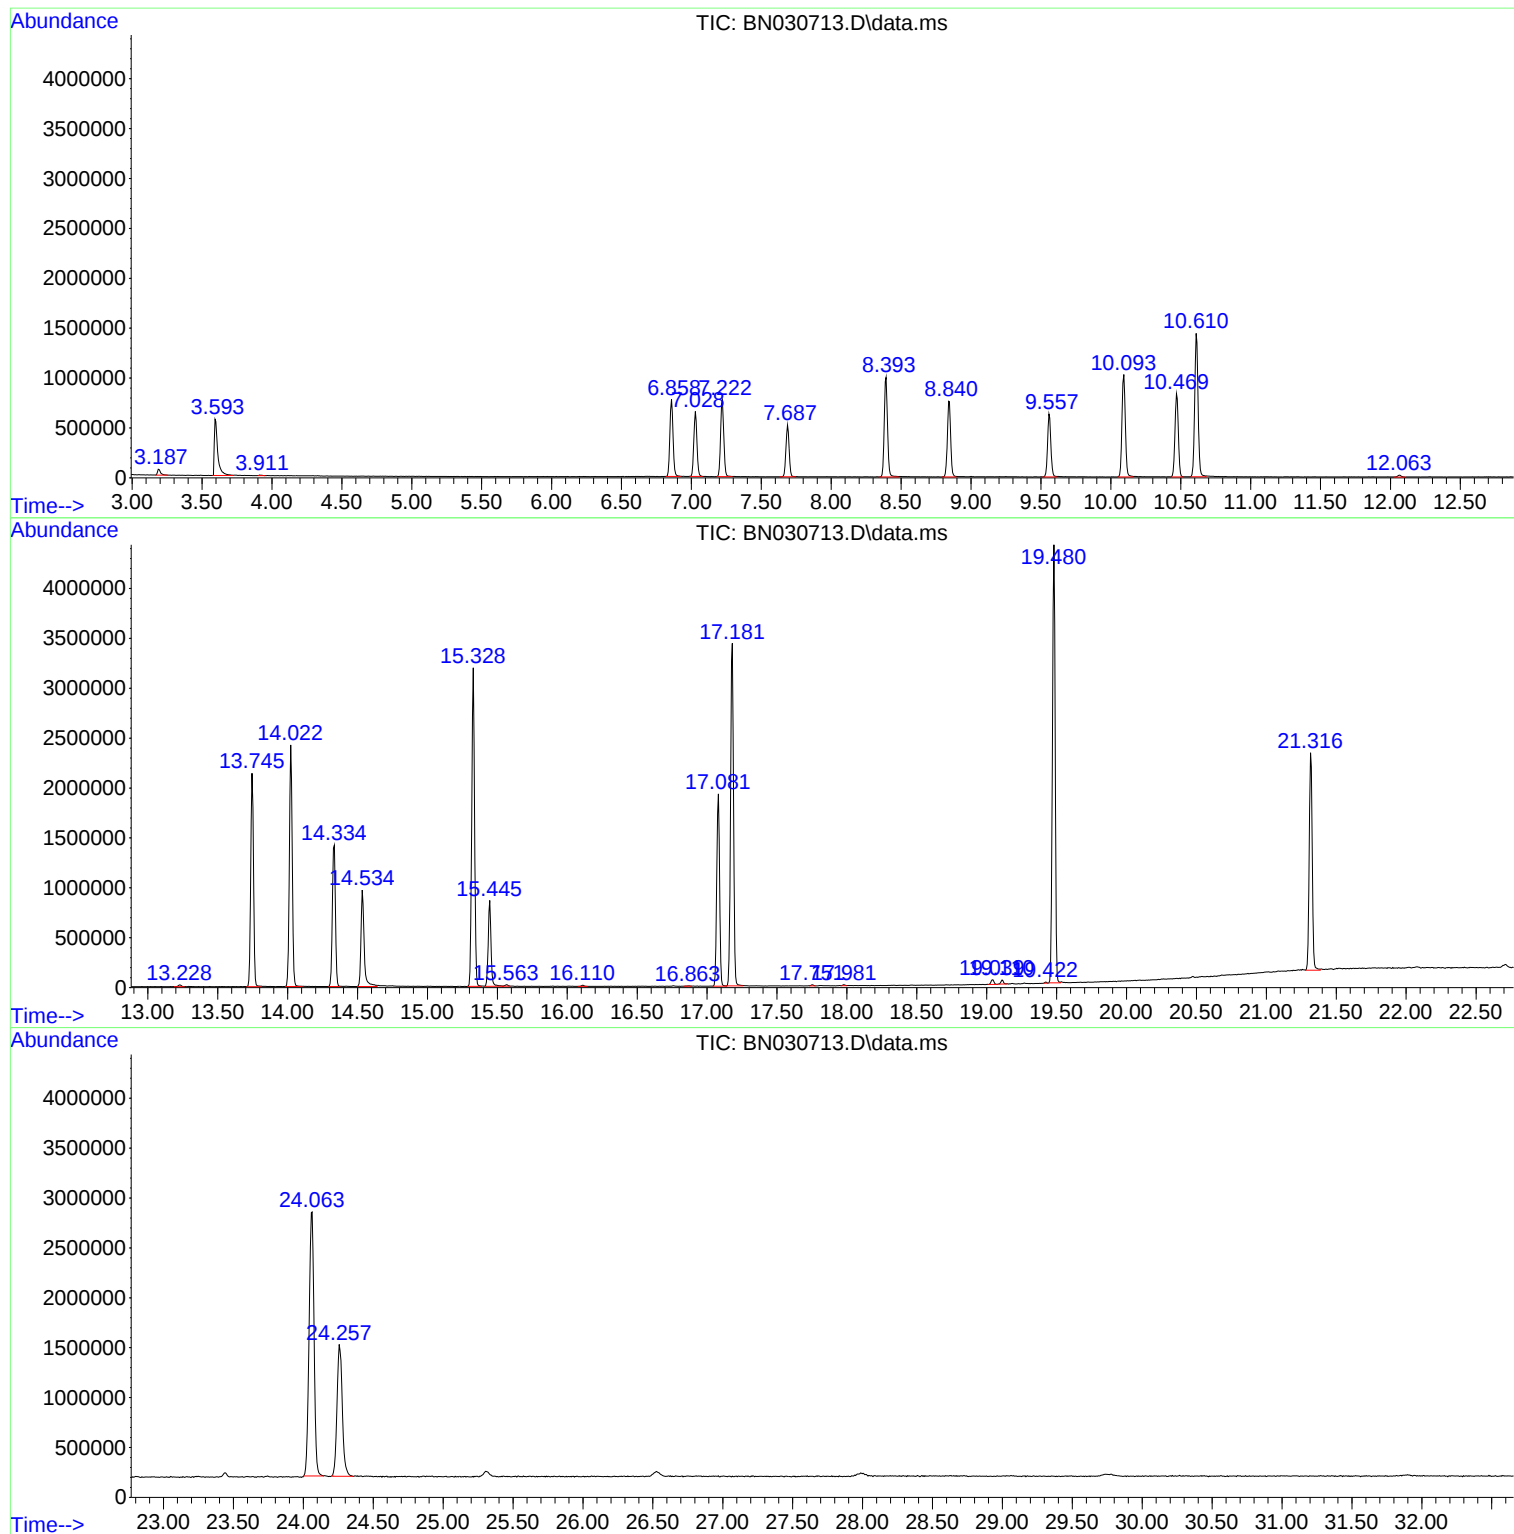

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030713.D
Acq On : 06 Apr 2024 18:28
Operator : MA/JU
Sample : PB159989BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK989

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030713.D
Acq On : 06 Apr 2024 18:28
Operator : MA/JU
Sample : PB159989BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK989

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------