

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030725.D
 Acq On : 07 Apr 2024 02:57
 Operator : MA/JU
 Sample : PB159978BL
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK978

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	44	rVB	49708	73541	1.01%	0.104%
2	3.593	100	103	126	rBV	655660	1130468	15.51%	1.598%
3	3.917	154	158	164	rVB	9828	13747	0.19%	0.019%
4	6.858	651	658	673	rBV	912311	1424331	19.54%	2.013%
5	7.028	680	687	698	rVB	763482	1178085	16.16%	1.665%
6	7.216	712	719	730	rBV	895739	1456149	19.97%	2.058%
7	7.687	792	799	809	rBV	740061	1185376	16.26%	1.675%
8	8.387	911	918	933	rBV	1169151	1914733	26.26%	2.706%
9	8.840	988	995	1005	rBV	884768	1476608	20.25%	2.087%
10	9.557	1108	1117	1129	rBV	773906	1259920	17.28%	1.781%
11	10.093	1199	1208	1224	rBV	1191202	2038752	27.96%	2.882%
12	10.469	1264	1272	1282	rBV	1203719	1967824	26.99%	2.781%
13	10.610	1288	1296	1311	rBV	1654069	2788170	38.24%	3.941%
14	12.063	1537	1543	1551	rBV	22322	36308	0.50%	0.051%
15	13.228	1736	1741	1746	rBV	21624	34278	0.47%	0.048%
16	13.745	1822	1829	1842	rBV	2447514	3341759	45.83%	4.723%
17	14.022	1869	1876	1890	rBV	2861672	4079670	55.96%	5.766%
18	14.328	1921	1928	1936	rBV	2058615	3003764	41.20%	4.246%
19	14.534	1956	1963	1987	rBV	1142119	1792800	24.59%	2.534%
20	15.328	2090	2098	2111	rBV	3479914	5099173	69.94%	7.207%
21	15.440	2111	2117	2130	rVV	954453	1435181	19.68%	2.029%
22	15.563	2134	2138	2144	rVB	16091	27373	0.38%	0.039%
23	16.110	2227	2231	2235	rBV2	14304	17045	0.23%	0.024%
24	17.081	2389	2396	2406	rBV	2580494	3829056	52.52%	5.412%
25	17.181	2406	2413	2427	rVV	3855974	5669627	77.76%	8.014%
26	17.751	2506	2510	2514	rBV5	6070	8765	0.12%	0.012%
27	17.975	2545	2548	2551	rBV3	8888	10937	0.15%	0.015%
28	19.039	2724	2729	2734	rBV	55961	76587	1.05%	0.108%
29	19.110	2737	2741	2746	rVV	48179	64438	0.88%	0.091%
30	19.263	2765	2767	2771	rVB4	7523	9148	0.13%	0.013%
31	19.416	2791	2793	2797	rVB2	14016	14022	0.19%	0.020%
32	19.480	2797	2804	2813	rBV	4911626	6925596	94.99%	9.789%
33	21.316	3110	3116	3125	rBV2	3028343	4522800	62.03%	6.393%
34	23.433	3472	3476	3483	rVB2	104766	192056	2.63%	0.271%
35	24.051	3572	3581	3593	rBV2	2961315	7290890	100.00%	10.305%
36	24.257	3607	3616	3632	rVB	1927188	5034983	69.06%	7.117%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030725.D
Acq On : 07 Apr 2024 02:57
Operator : MA/JU
Sample : PB159978BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK978

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	25.304	3789	3794	3803	rVB4	130354	324942	4.46%	0.459%
----	--------	------	------	------	------	--------	--------	-------	--------


Sum of corrected areas: 70748902

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030725.D
Acq On : 07 Apr 2024 02:57
Operator : MA/JU
Sample : PB159978BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK978

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

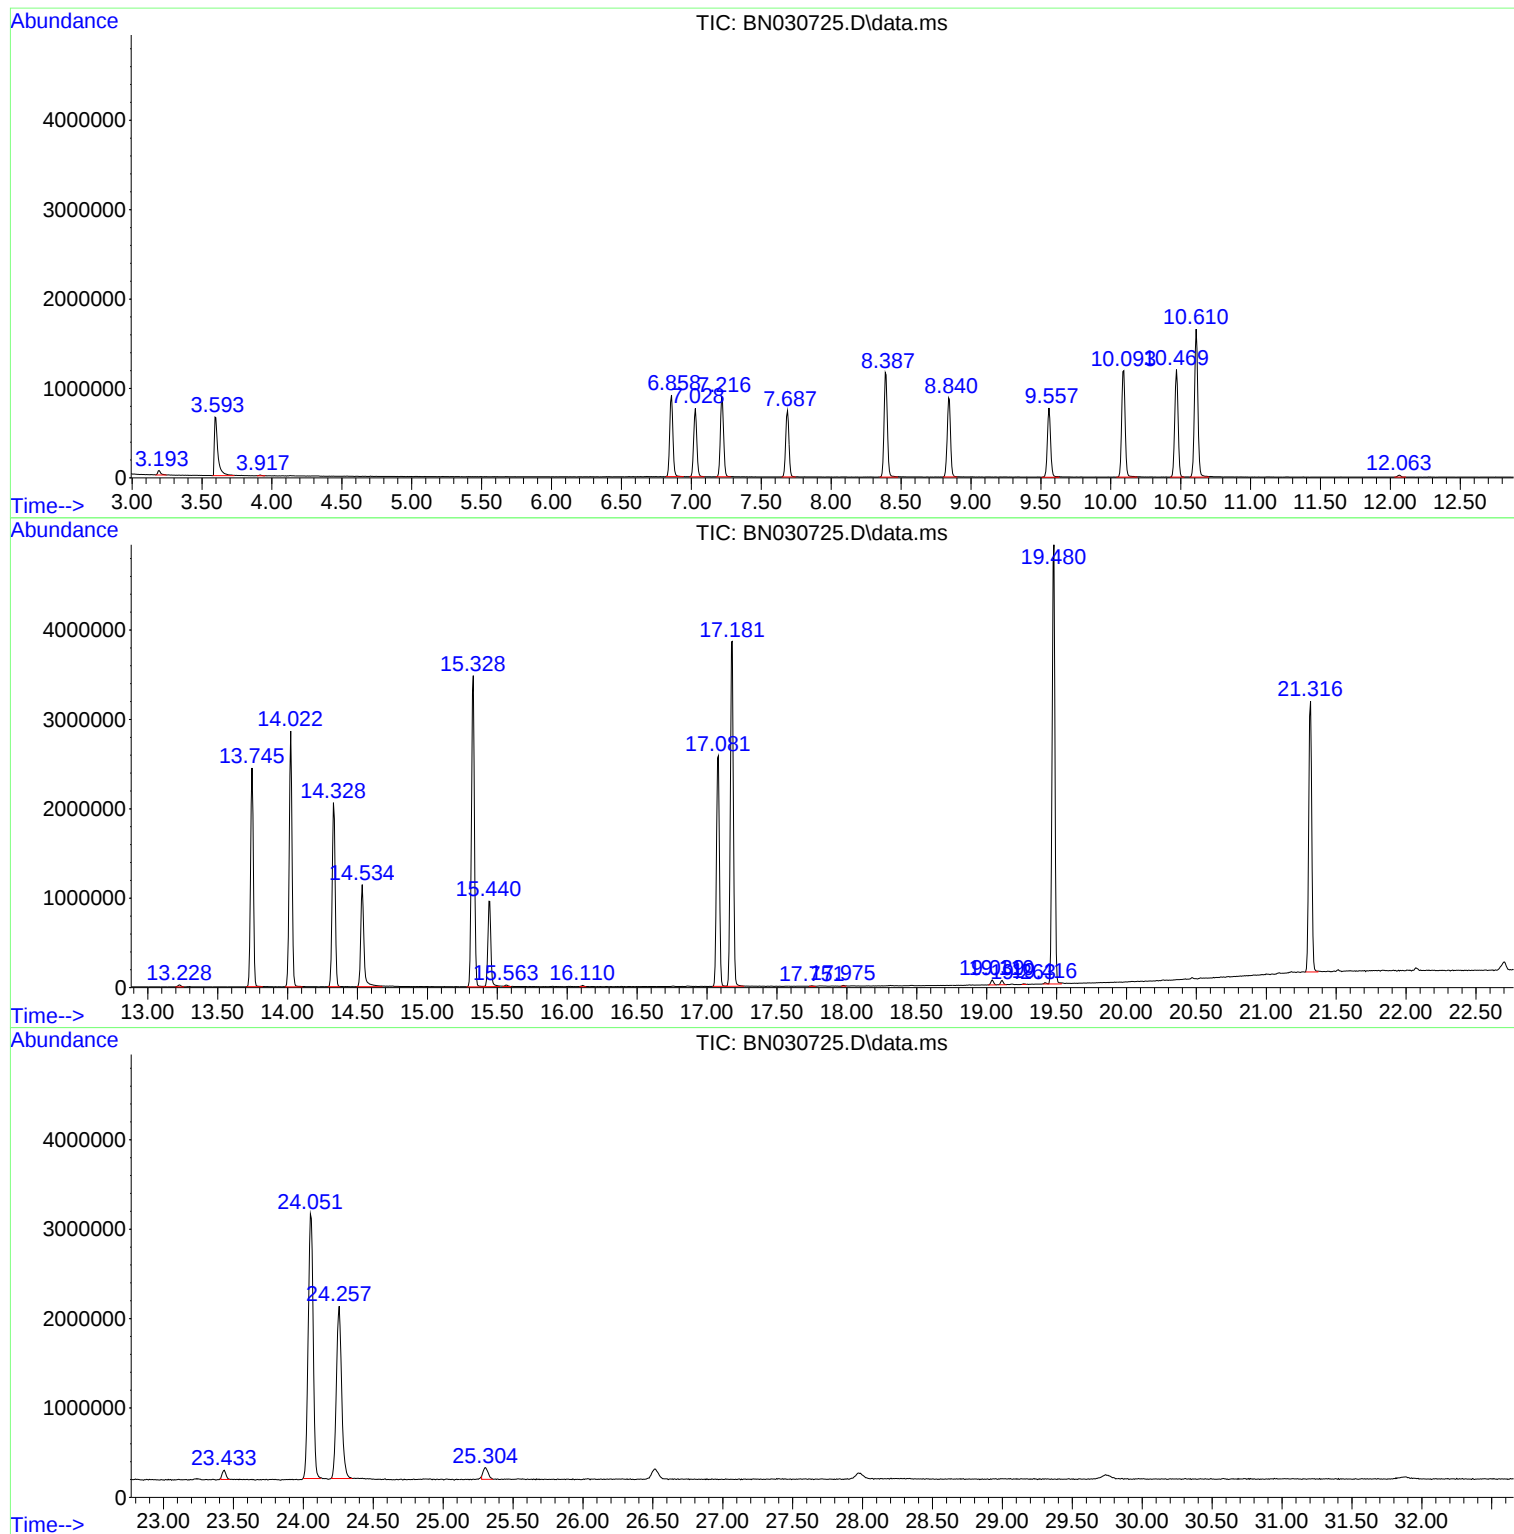

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030725.D
Acq On : 07 Apr 2024 02:57
Operator : MA/JU
Sample : PB159978BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK978

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030725.D
Acq On : 07 Apr 2024 02:57
Operator : MA/JU
Sample : PB159978BL
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK978

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------