

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030726.D
 Acq On : 07 Apr 2024 03:36
 Operator : MA/JU
 Sample : PB160033BL
 Misc :
 ALS Vial : 64 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK033

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030726.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	30	35	43	rBV	36600	54745	0.89%	0.099%
2	3.593	100	103	124	rBV	529519	886821	14.49%	1.596%
3	3.916	154	158	160	rBV3	8688	9850	0.16%	0.018%
4	6.857	651	658	675	rBV	694875	1107757	18.10%	1.994%
5	7.028	681	687	697	rVB	592697	915836	14.96%	1.649%
6	7.216	712	719	731	rBV	693215	1115338	18.22%	2.008%
7	7.687	792	799	807	rBV	571417	884707	14.45%	1.593%
8	8.387	911	918	934	rBV	903303	1476674	24.12%	2.658%
9	8.840	987	995	1009	rBV	703563	1148141	18.76%	2.067%
10	9.557	1107	1117	1126	rBV	587549	946259	15.46%	1.703%
11	10.087	1199	1207	1221	rBV	923956	1569251	25.64%	2.825%
12	10.469	1264	1272	1282	rBV	930557	1523708	24.89%	2.743%
13	10.610	1288	1296	1310	rBV	1159971	1966237	32.12%	3.539%
14	12.057	1536	1542	1551	rVB	16081	27111	0.44%	0.049%
15	13.228	1735	1741	1749	rBV4	12441	19492	0.32%	0.035%
16	13.745	1822	1829	1841	rBV	1901166	2673353	43.67%	4.812%
17	14.022	1869	1876	1891	rBV2	2156151	3228348	52.74%	5.811%
18	14.328	1921	1928	1936	rBV	1612862	2371033	38.73%	4.268%
19	14.534	1957	1963	1984	rBV	847613	1383022	22.59%	2.490%
20	14.739	1994	1998	2005	rVB8	4477	9517	0.16%	0.017%
21	15.328	2091	2098	2106	rBV	2810260	4063225	66.38%	7.314%
22	15.439	2111	2117	2134	rVV	737167	1069616	17.47%	1.925%
23	15.563	2134	2138	2147	rVB2	14519	23681	0.39%	0.043%
24	15.898	2189	2195	2198	rBV8	3515	8014	0.13%	0.014%
25	16.110	2227	2231	2235	rBV4	10052	15338	0.25%	0.028%
26	16.757	2337	2341	2347	rBV7	4940	7813	0.13%	0.014%
27	17.075	2389	2395	2406	rBV	2070139	3024143	49.40%	5.444%
28	17.175	2406	2412	2426	rVV2	3269960	4676064	76.39%	8.417%
29	17.975	2545	2548	2553	rBV6	8212	12141	0.20%	0.022%
30	19.039	2724	2729	2735	rBV2	45626	66804	1.09%	0.120%
31	19.110	2737	2741	2745	rBV	38103	53071	0.87%	0.096%
32	19.174	2750	2752	2755	rVB3	6280	7127	0.12%	0.013%
33	19.263	2765	2767	2774	rBV7	8909	13374	0.22%	0.024%
34	19.422	2790	2794	2797	rBV5	14657	19485	0.32%	0.035%
35	19.474	2797	2803	2810	rBV	4017464	5625701	91.90%	10.127%
36	21.316	3110	3116	3125	rBV	2488691	3573006	58.37%	6.432%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030726.D
Acq On : 07 Apr 2024 03:36
Operator : MA/JU
Sample : PB160033BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK033

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	24.057	3572	3582	3597	rBV2	2539065	6121411	100.00%	11.019%
38	24.257	3607	3616	3630	rVB2	1484901	3855047	62.98%	6.939%


Sum of corrected areas: 55552261

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030726.D
Acq On : 07 Apr 2024 03:36
Operator : MA/JU
Sample : PB160033BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK033

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

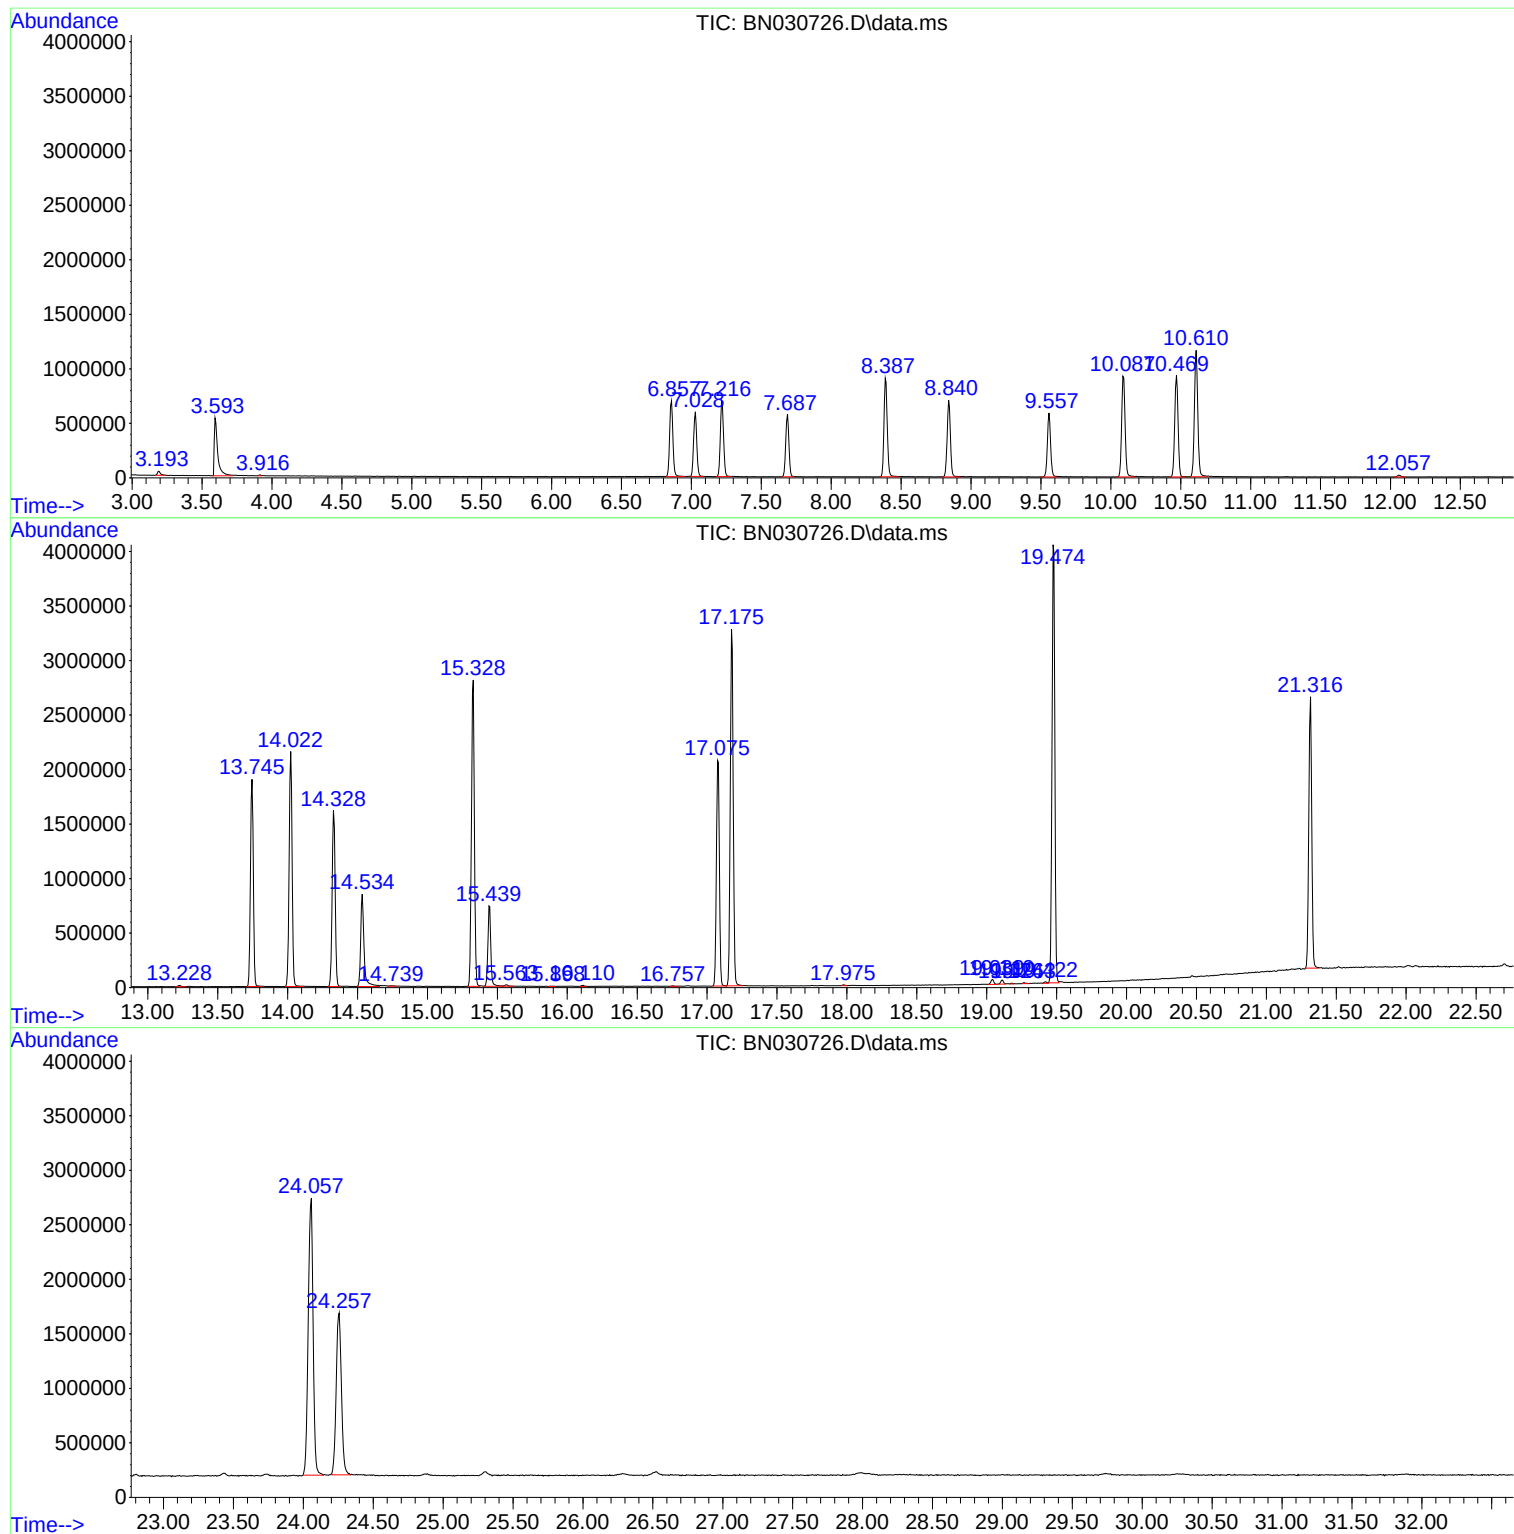

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030726.D
Acq On : 07 Apr 2024 03:36
Operator : MA/JU
Sample : PB160033BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK033

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030726.D
Acq On : 07 Apr 2024 03:36
Operator : MA/JU
Sample : PB160033BL
Misc :
ALS Vial : 64 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK033

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc