

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030727.D
 Acq On : 07 Apr 2024 04:15
 Operator : MA/JU
 Sample : P1966-02
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07S1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030727.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	31	34	47	rVB	27313	45165	0.71%	0.076%
2	3.458	76	80	91	rBV	25202	44126	0.70%	0.074%
3	3.599	100	104	124	rBV	342619	602223	9.52%	1.013%
4	3.916	154	158	164	rVB3	9671	16672	0.26%	0.028%
5	5.787	473	476	480	rBV3	6330	8369	0.13%	0.014%
6	6.857	651	658	669	rBV	548639	886462	14.02%	1.491%
7	7.028	680	687	697	rVB	470722	734400	11.61%	1.235%
8	7.216	712	719	730	rBV	546037	882865	13.96%	1.485%
9	7.687	791	799	807	rBV	888881	1408273	22.27%	2.368%
10	7.757	807	811	817	rVB4	9528	16715	0.26%	0.028%
11	8.387	912	918	929	rBV	743746	1178842	18.64%	1.983%
12	8.840	986	995	1004	rBV	571501	917772	14.51%	1.544%
13	9.004	1018	1023	1028	rVB7	10498	15599	0.25%	0.026%
14	9.245	1060	1064	1070	rVB	13085	20104	0.32%	0.034%
15	9.410	1086	1092	1101	rVB	32824	55090	0.87%	0.093%
16	9.557	1107	1117	1128	rBV	459530	743416	11.76%	1.250%
17	9.987	1184	1190	1195	rBV6	4667	8749	0.14%	0.015%
18	10.093	1200	1208	1228	rBV	757691	1274980	20.16%	2.144%
19	10.251	1230	1235	1243	rBV	29920	50783	0.80%	0.085%
20	10.469	1264	1272	1281	rBV	1415319	2363015	37.37%	3.974%
21	10.610	1287	1296	1315	rBV	789073	1334090	21.10%	2.244%
22	11.016	1361	1365	1374	rVB5	8297	13467	0.21%	0.023%
23	11.216	1392	1399	1404	rBV2	26508	50101	0.79%	0.084%
24	11.898	1510	1515	1522	rBV9	3318	6777	0.11%	0.011%
25	12.063	1536	1543	1549	rVB3	13642	25230	0.40%	0.042%
26	13.151	1724	1728	1734	rVB5	9453	12897	0.20%	0.022%
27	13.228	1734	1741	1748	rBV4	21172	33177	0.52%	0.056%
28	13.745	1822	1829	1840	rBV	1650905	2245526	35.51%	3.777%
29	14.022	1866	1876	1887	rBV	1785812	2688965	42.53%	4.522%
30	14.328	1921	1928	1940	rVV	2490851	3614326	57.16%	6.079%
31	14.533	1957	1963	1980	rBV	697696	1160618	18.35%	1.952%
32	14.745	1996	1999	2006	rVB7	11168	19499	0.31%	0.033%
33	15.186	2069	2074	2079	rVB5	5182	8480	0.13%	0.014%
34	15.322	2091	2097	2109	rBV	2409070	3497484	55.31%	5.882%
35	15.439	2111	2117	2130	rVV	524575	753288	11.91%	1.267%
36	15.569	2134	2139	2143	rVB6	10115	16455	0.26%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030727.D
 Acq On : 07 Apr 2024 04:15
 Operator : MA/JU
 Sample : P1966-02
 Misc :
 ALS Vial : 65 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E07S1

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	16.110	2228	2231	2236	rVB6	11345	15766	0.25%	0.027%
38	16.486	2290	2295	2298	rBV5	5276	7683	0.12%	0.013%
39	16.863	2353	2359	2362	rBV5	6858	14295	0.23%	0.024%
40	17.004	2378	2383	2387	rVB7	7435	11473	0.18%	0.019%
41	17.080	2389	2396	2405	rVV	3130847	4609403	72.90%	7.752%
42	17.175	2405	2412	2423	rVV	2808447	3863566	61.10%	6.498%
43	17.269	2423	2428	2434	rVB7	12980	25069	0.40%	0.042%
44	17.474	2461	2463	2472	rVB8	5260	7956	0.13%	0.013%
45	17.757	2507	2511	2515	rVB4	9414	12129	0.19%	0.020%
46	17.851	2523	2527	2532	rVB8	5028	9539	0.15%	0.016%
47	17.980	2543	2549	2557	rBV	237522	361297	5.71%	0.608%
48	18.280	2596	2600	2602	rBV3	7551	10397	0.16%	0.017%
49	18.416	2619	2623	2627	rVB6	9112	13739	0.22%	0.023%
50	18.463	2627	2631	2636	rBV8	4691	9299	0.15%	0.016%
51	18.851	2693	2697	2700	rBV5	7847	11923	0.19%	0.020%
52	19.039	2724	2729	2734	rBV3	39204	61395	0.97%	0.103%
53	19.110	2737	2741	2745	rBV	44482	72703	1.15%	0.122%
54	19.145	2745	2747	2750	rVB3	16139	16993	0.27%	0.029%
55	19.263	2763	2767	2774	rBV	124237	184277	2.91%	0.310%
56	19.416	2790	2793	2797	rBV3	21835	26137	0.41%	0.044%
57	19.474	2797	2803	2810	rVV	3504864	4803000	75.96%	8.078%
58	19.533	2811	2813	2818	rVB2	20037	23280	0.37%	0.039%
59	20.033	2895	2898	2902	rBV2	37501	39609	0.63%	0.067%
60	20.533	2980	2983	2986	rVB2	49042	54337	0.86%	0.091%
61	21.004	3059	3063	3072	rBV3	266324	440094	6.96%	0.740%
62	21.315	3110	3116	3125	rBV	3840843	5464657	86.42%	9.191%
63	21.515	3147	3150	3155	rVB	73922	88163	1.39%	0.148%
64	22.074	3241	3245	3251	rBV2	85763	135651	2.15%	0.228%
65	22.704	3348	3352	3361	rVB2	122410	214113	3.39%	0.360%
66	23.433	3471	3476	3485	rVB	145466	255885	4.05%	0.430%
67	24.051	3572	3581	3593	rBV2	2074112	5106974	80.77%	8.589%
68	24.256	3606	3616	3633	rVB	2442427	6323249	100.00%	10.635%
69	25.303	3788	3794	3803	rVB2	154544	411118	6.50%	0.691%


Sum of corrected areas: 59459169

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030727.D
Acq On : 07 Apr 2024 04:15
Operator : MA/JU
Sample : P1966-02
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07S1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

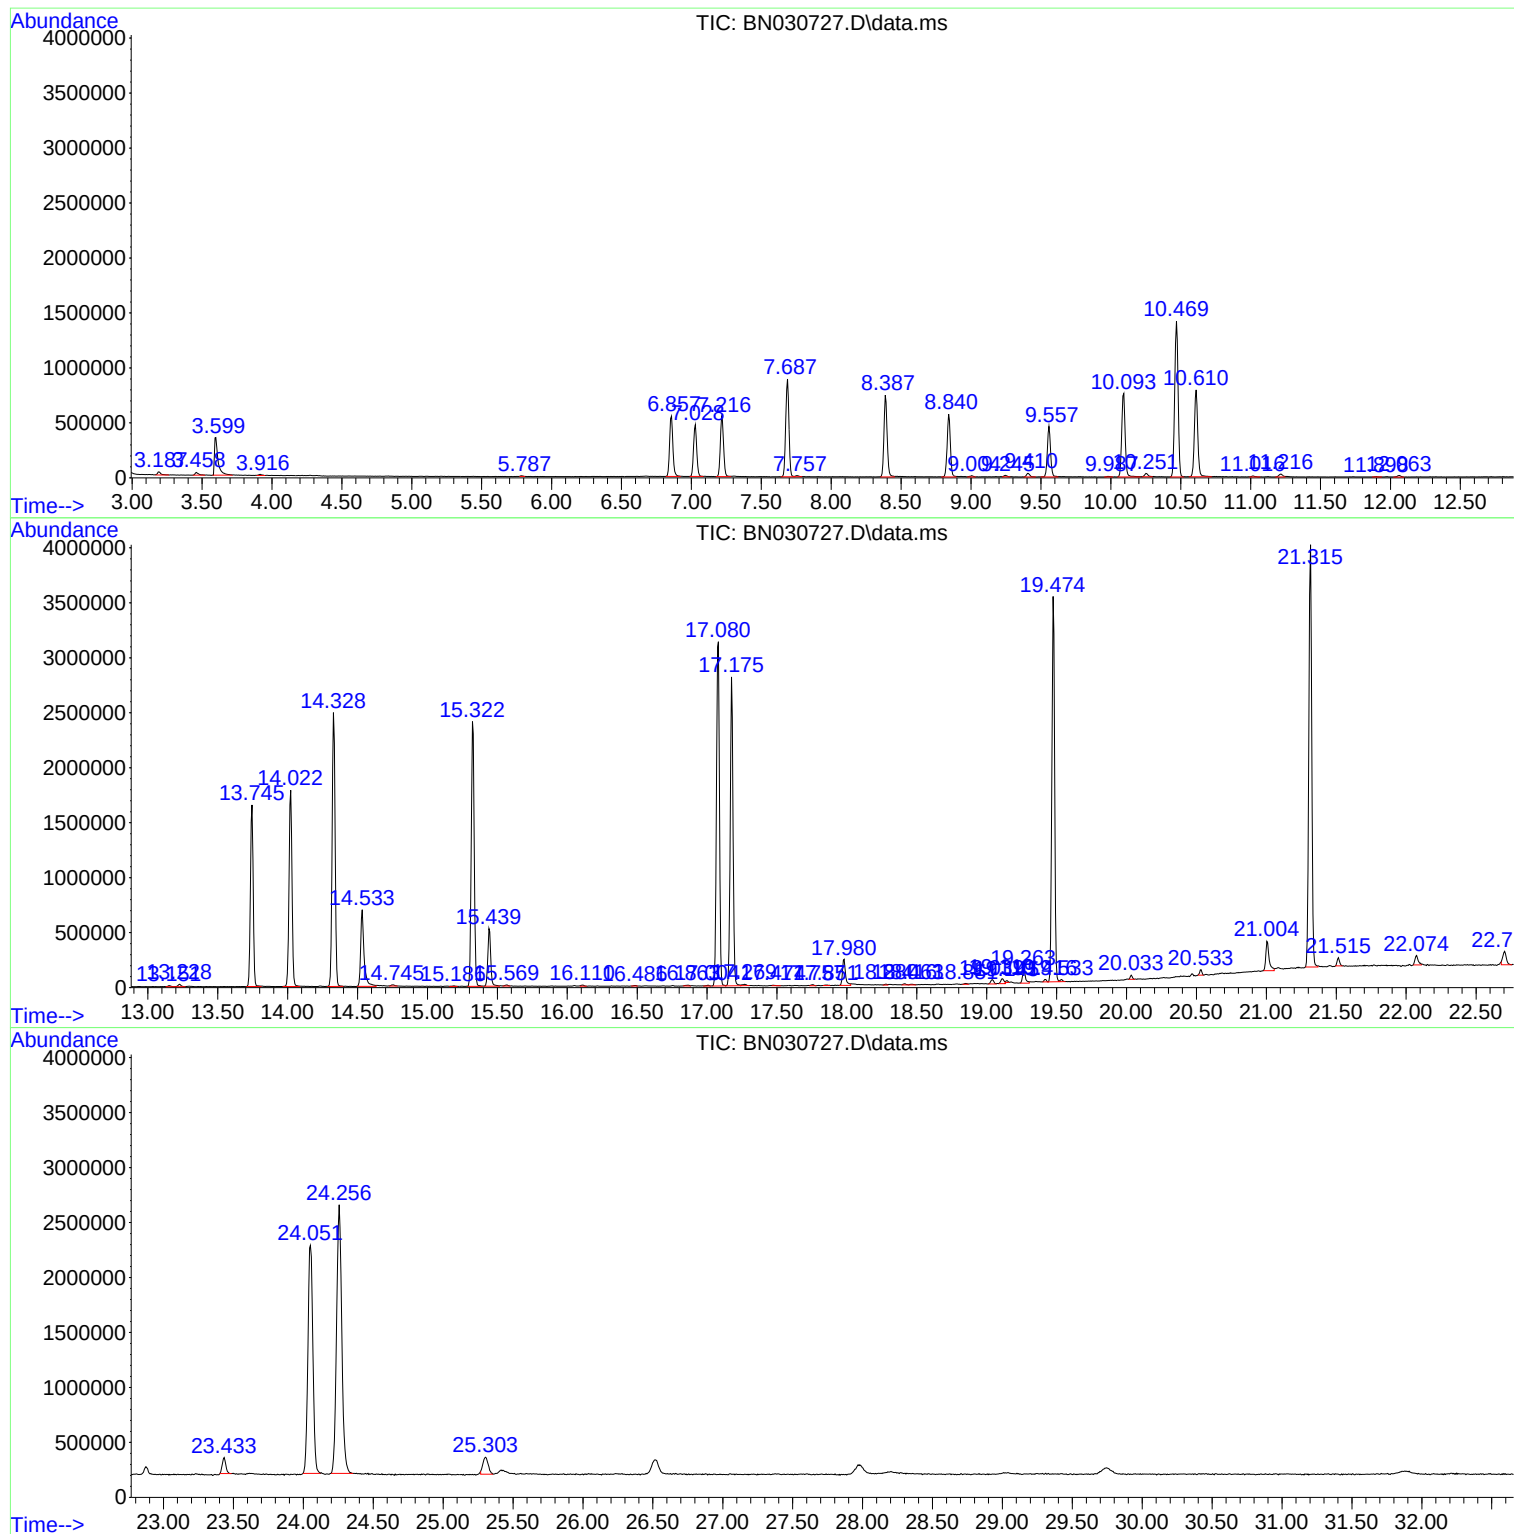

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030727.D
Acq On : 07 Apr 2024 04:15
Operator : MA/JU
Sample : P1966-02
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07S1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030727.D
Acq On : 07 Apr 2024 04:15
Operator : MA/JU
Sample : P1966-02
Misc :
ALS Vial : 65 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E07S1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc