

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030730.D
 Acq On : 07 Apr 2024 06:12
 Operator : MA/JU
 Sample : P1987-08
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030730.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	31	34	41	rVB	31166	42087	0.54%	0.069%
2	3.599	102	104	121	rBV	195416	328067	4.18%	0.538%
3	3.917	154	158	161	rBV3	6667	10246	0.13%	0.017%
4	6.858	651	658	670	rVB	132286	226954	2.89%	0.372%
5	7.028	676	687	701	rVB	678631	1089721	13.90%	1.786%
6	7.216	711	719	729	rBV	546906	873662	11.14%	1.432%
7	7.305	729	734	740	rVB8	7197	13866	0.18%	0.023%
8	7.687	792	799	806	rBV	606978	957423	12.21%	1.569%
9	8.387	911	918	929	rBV	439933	717011	9.14%	1.175%
10	8.840	988	995	1007	rBV	852500	1373549	17.52%	2.251%
11	9.004	1019	1023	1027	rBV5	6559	10328	0.13%	0.017%
12	9.246	1059	1064	1069	rVB3	10347	19175	0.24%	0.031%
13	9.410	1087	1092	1098	rVB2	13881	23006	0.29%	0.038%
14	9.557	1109	1117	1130	rBV	576004	922921	11.77%	1.513%
15	10.093	1200	1208	1220	rBV	846637	1461806	18.64%	2.396%
16	10.251	1232	1235	1243	rVB4	11197	18785	0.24%	0.031%
17	10.469	1264	1272	1283	rBV	985830	1633877	20.84%	2.678%
18	10.610	1283	1296	1307	rBV	942427	1614373	20.59%	2.646%
19	11.216	1393	1399	1405	rBV3	21428	41947	0.53%	0.069%
20	11.740	1481	1488	1493	rVB5	8714	13521	0.17%	0.022%
21	11.857	1503	1508	1515	rBV7	13093	21001	0.27%	0.034%
22	12.063	1537	1543	1550	rVB	21610	37855	0.48%	0.062%
23	12.351	1586	1592	1598	rBV	66867	107684	1.37%	0.177%
24	13.222	1737	1740	1745	rBV5	6544	10897	0.14%	0.018%
25	13.745	1821	1829	1839	rBV	2338101	3279399	41.82%	5.375%
26	14.022	1864	1876	1888	rBV2	2601937	3866937	49.31%	6.338%
27	14.328	1921	1928	1940	rBV	1768631	2558566	32.63%	4.194%
28	14.534	1958	1963	1977	rBV	118757	228162	2.91%	0.374%
29	14.687	1986	1989	1995	rVB6	7486	13403	0.17%	0.022%
30	14.745	1995	1999	2004	rBV7	8674	16426	0.21%	0.027%
31	14.992	2035	2041	2047	rBV9	3916	10229	0.13%	0.017%
32	15.328	2089	2098	2108	rBV	3532028	5177311	66.02%	8.486%
33	15.439	2111	2117	2133	rVV	755569	1085123	13.84%	1.779%
34	15.563	2134	2138	2148	rVB2	18371	34927	0.45%	0.057%
35	15.792	2173	2177	2184	rVB	22949	33054	0.42%	0.054%
36	15.886	2189	2193	2198	rVB6	5881	8982	0.11%	0.015%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030730.D
 Acq On : 07 Apr 2024 06:12
 Operator : MA/JU
 Sample : P1987-08
 Misc :
 ALS Vial : 68 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R72

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	16.110	2227	2231	2237	rVB6	14782	23002	0.29%	0.038%
38	16.486	2290	2295	2301	rBV8	11098	16279	0.21%	0.027%
39	16.545	2301	2305	2313	rVB4	23096	35596	0.45%	0.058%
40	16.757	2337	2341	2347	rBV9	7084	14160	0.18%	0.023%
41	16.845	2353	2356	2359	rBV4	7386	11148	0.14%	0.018%
42	17.010	2377	2384	2387	rBV9	6604	10551	0.13%	0.017%
43	17.075	2389	2395	2402	rBV	2218839	3233787	41.24%	5.301%
44	17.175	2406	2412	2422	rBV2	4206824	6132847	78.21%	10.052%
45	17.586	2479	2482	2486	rBV5	5968	8120	0.10%	0.013%
46	17.757	2508	2511	2516	rVB4	15618	17534	0.22%	0.029%
47	17.845	2523	2526	2532	rVB8	6652	12728	0.16%	0.021%
48	17.975	2543	2548	2560	rBV	138103	238367	3.04%	0.391%
49	18.222	2585	2590	2593	rBV6	7500	12145	0.15%	0.020%
50	18.410	2620	2622	2628	rVB6	9516	11166	0.14%	0.018%
51	19.039	2725	2729	2735	rVB	62206	84340	1.08%	0.138%
52	19.110	2737	2741	2745	rBV	58827	79456	1.01%	0.130%
53	19.145	2745	2747	2750	rVV4	11668	14305	0.18%	0.023%
54	19.263	2764	2767	2773	rBV5	37453	55748	0.71%	0.091%
55	19.422	2791	2794	2797	rVB4	19223	19593	0.25%	0.032%
56	19.480	2797	2804	2811	rBV	5244517	7363891	93.91%	12.070%
57	21.004	3060	3063	3068	rVB2	69433	92744	1.18%	0.152%
58	21.316	3110	3116	3130	rVB	2605198	3752321	47.85%	6.151%
59	24.057	3572	3582	3596	rVB2	3166176	7841734	100.00%	12.854%
60	24.251	3607	3615	3633	rVB	1593497	4044455	51.58%	6.629%


Sum of corrected areas: 61008298

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030730.D
Acq On : 07 Apr 2024 06:12
Operator : MA/JU
Sample : P1987-08
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

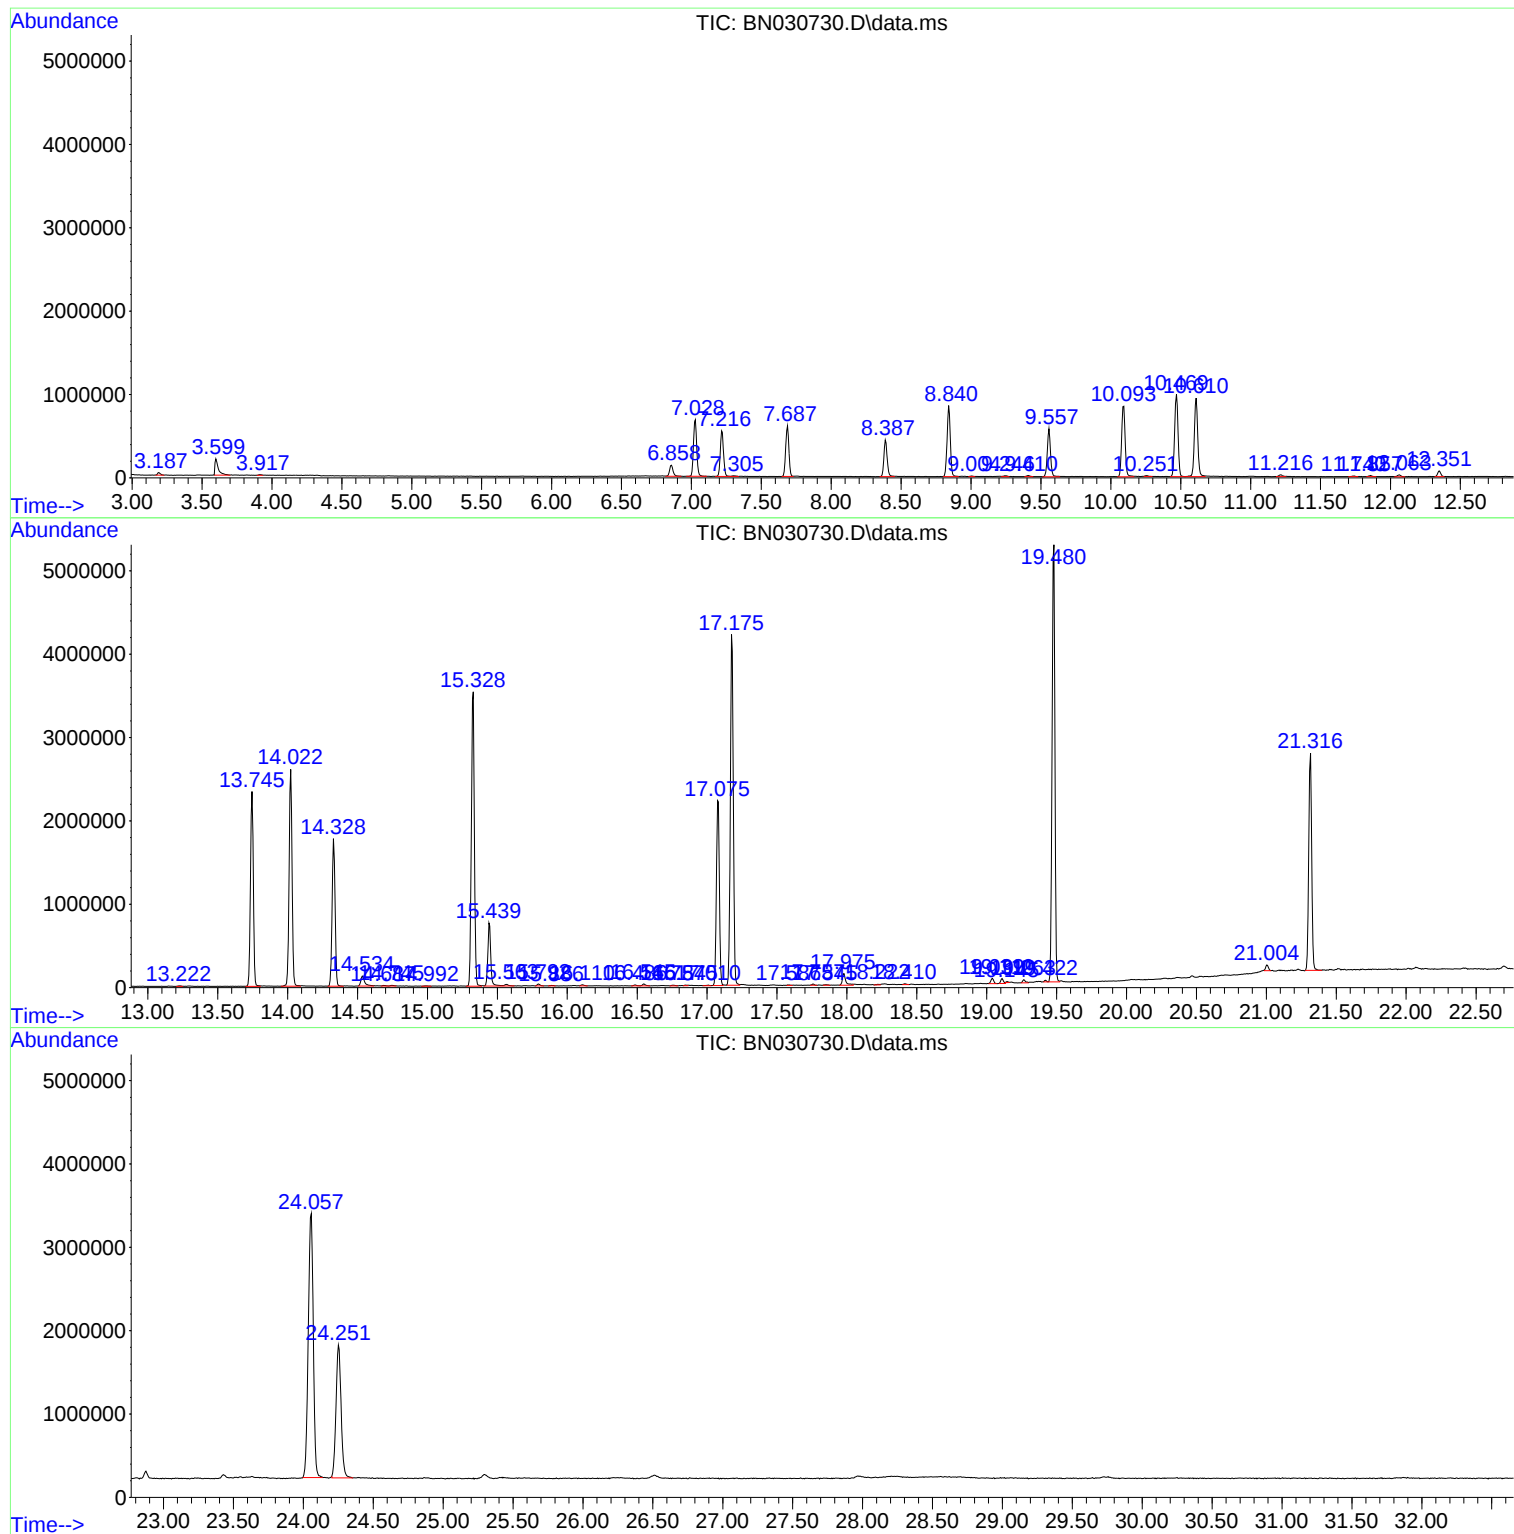

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030730.D
Acq On : 07 Apr 2024 06:12
Operator : MA/JU
Sample : P1987-08
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030730.D
Acq On : 07 Apr 2024 06:12
Operator : MA/JU
Sample : P1987-08
Misc :
ALS Vial : 68 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R72

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc