

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
 Data File : BN030734.D
 Acq On : 07 Apr 2024 08:48
 Operator : MA/JU
 Sample : P1987-12
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MCORH1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030734.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	43	rVB	38776	59154	0.57%	0.079%
2	3.599	101	104	120	rBV	169632	287650	2.79%	0.385%
3	6.858	652	658	665	rVB	204400	324644	3.14%	0.435%
4	7.028	680	687	700	rVB	866999	1369905	13.27%	1.835%
5	7.216	712	719	730	rBV	806259	1274336	12.34%	1.707%
6	7.299	730	733	743	rVB9	7073	14676	0.14%	0.020%
7	7.687	792	799	806	rBV	631320	987773	9.57%	1.323%
8	8.387	911	918	930	rBV	682873	1081065	10.47%	1.448%
9	8.840	987	995	1008	rBV	1114016	1764031	17.08%	2.363%
10	9.246	1058	1064	1069	rVB5	5153	12211	0.12%	0.016%
11	9.558	1109	1117	1130	rBV	832091	1370284	13.27%	1.836%
12	10.087	1200	1207	1224	rBV	1267019	2152807	20.85%	2.884%
13	10.469	1265	1272	1282	rVB	1014965	1692761	16.39%	2.268%
14	10.610	1288	1296	1311	rBV	1208787	2067017	20.02%	2.769%
15	12.063	1536	1543	1550	rVB	27340	48190	0.47%	0.065%
16	13.228	1735	1741	1747	rVB2	26492	39529	0.38%	0.053%
17	13.746	1822	1829	1841	rBV	2978741	4136294	40.06%	5.542%
18	14.022	1865	1876	1888	rBV	3398653	5023782	48.66%	6.731%
19	14.328	1921	1928	1941	rBV	1836581	2588392	25.07%	3.468%
20	14.534	1957	1963	1975	rBV2	266422	497703	4.82%	0.667%
21	14.746	1995	1999	2006	rBV9	9477	15535	0.15%	0.021%
22	14.898	2018	2025	2039	rBV2	65946	234537	2.27%	0.314%
23	15.328	2091	2098	2111	rBV	4339961	6459078	62.56%	8.654%
24	15.445	2111	2118	2134	rVV	1246198	1847590	17.89%	2.475%
25	15.563	2134	2138	2143	rVB2	20075	32941	0.32%	0.044%
26	15.887	2189	2193	2199	rBV7	6349	10929	0.11%	0.015%
27	16.110	2227	2231	2237	rBV4	18395	27388	0.27%	0.037%
28	16.481	2291	2294	2298	rBV5	7670	10697	0.10%	0.014%
29	16.757	2336	2341	2345	rBV5	10532	14797	0.14%	0.020%
30	17.075	2389	2395	2403	rBV	2222688	3293634	31.90%	4.413%
31	17.175	2406	2412	2434	rVB2	5229769	7858844	76.11%	10.529%
32	17.757	2508	2511	2514	rVB3	9627	12710	0.12%	0.017%
33	17.975	2544	2548	2553	rBV	77120	103719	1.00%	0.139%
34	18.410	2620	2622	2627	rVB6	9740	10494	0.10%	0.014%
35	19.039	2725	2729	2734	rBV2	85986	118909	1.15%	0.159%
36	19.110	2737	2741	2744	rBV	77420	101014	0.98%	0.135%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030734.D
Acq On : 07 Apr 2024 08:48
Operator : MA/JU
Sample : P1987-12
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MCORH1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	19.263	2764	2767	2773	rBV4	43795	54919	0.53%	0.074%
38	19.416	2791	2793	2797	rVB5	21689	20263	0.20%	0.027%
39	19.481	2797	2804	2811	rBV	6463002	9397755	91.02%	12.591%
40	21.316	3110	3116	3126	rVB	2529654	3813714	36.94%	5.109%
41	24.057	3572	3582	3596	rVB2	4277881	10325211	100.00%	13.833%
42	24.251	3606	3615	3628	rBV2	1618598	4083023	39.54%	5.470%


Sum of corrected areas: 74639905

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030734.D
Acq On : 07 Apr 2024 08:48
Operator : MA/JU
Sample : P1987-12
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MCORH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

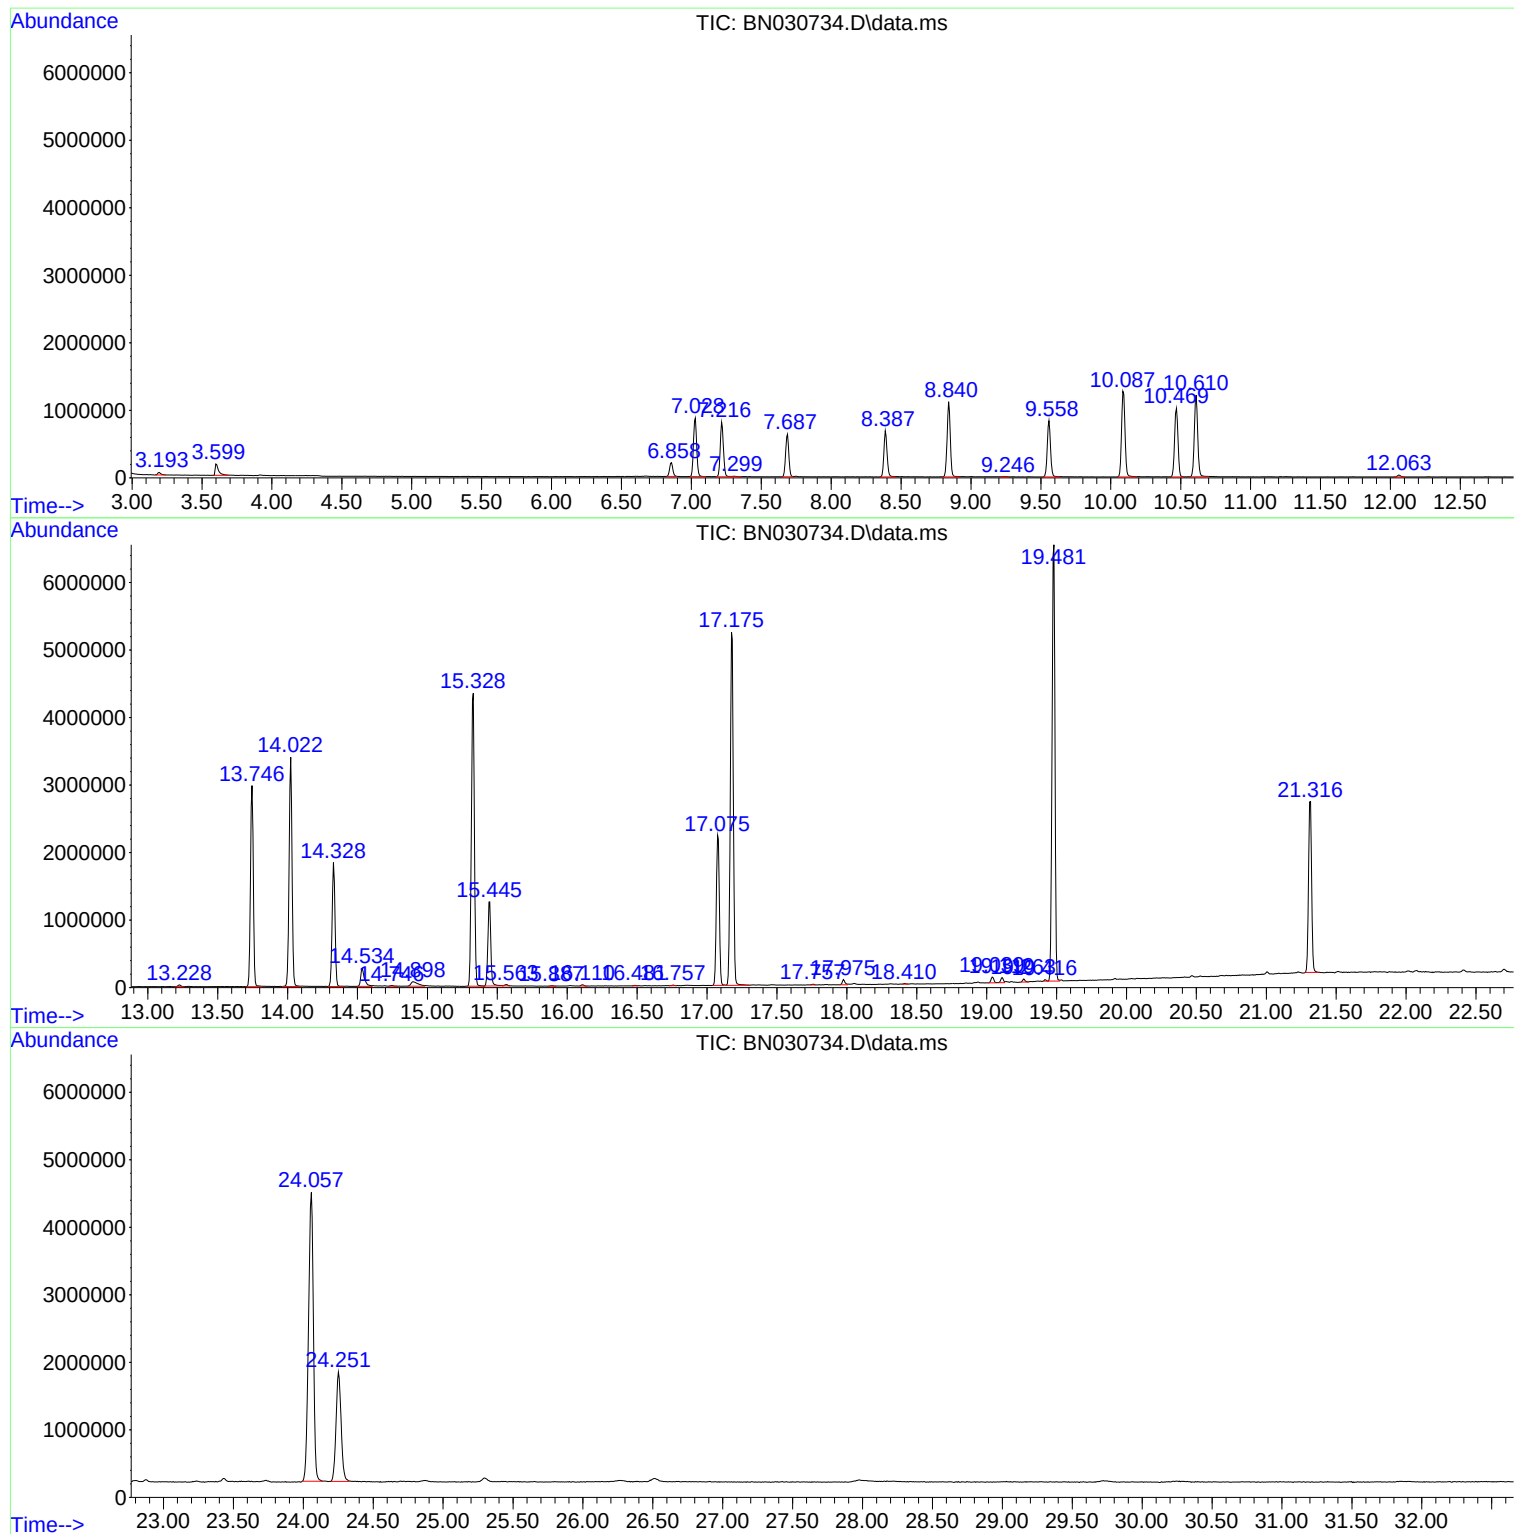

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030734.D
Acq On : 07 Apr 2024 08:48
Operator : MA/JU
Sample : P1987-12
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MCORH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040624\
Data File : BN030734.D
Acq On : 07 Apr 2024 08:48
Operator : MA/JU
Sample : P1987-12
Misc :
ALS Vial : 72 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MCORH1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc