

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040720\
 Data File : BN010423.D
 Acq On : 07 Apr 2020 18:21
 Operator : CG/JU
 Sample : L2173-03
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Apr 08 00:47:55 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 07 11:04:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	511773	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	2188124	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	1469803	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	3341367	20.00	ng/ul	0.00
78) Chrysene-d12	21.18	240	3625212	20.00	ng/ul	0.00
86) Perylene-d12	23.36	264	3897296	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.22	96	13510	1.25	ng/uL	0.01
5) Phenol-d5	6.79	99	261440	6.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	673372	30.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	843879	24.90	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	523242	14.51	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	528332	32.52	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	579312	33.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	1044486	29.29	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	59113	1.40	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	3816779	34.42	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	4488022	34.64	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	105471	5.06	ng/ul	0.00
58) Fluorene-d10	15.23	176	3409513	35.28	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.35	200	520431	27.20	ng/ul	0.00
71) Anthracene-d10	17.08	188	5486240	35.76	ng/ul	0.00
79) Pyrene-d10	19.38	212	6357899	34.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.22	264	7007632	36.14	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.69	163	529084	4.620	ng/ul 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040720\
Data File : BN010423.D
Acq On : 07 Apr 2020 18:21
Operator : CG/JU
Sample : L2173-03
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Apr 08 00:47:55 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 07 11:04:24 2020
Response via : Initial Calibration

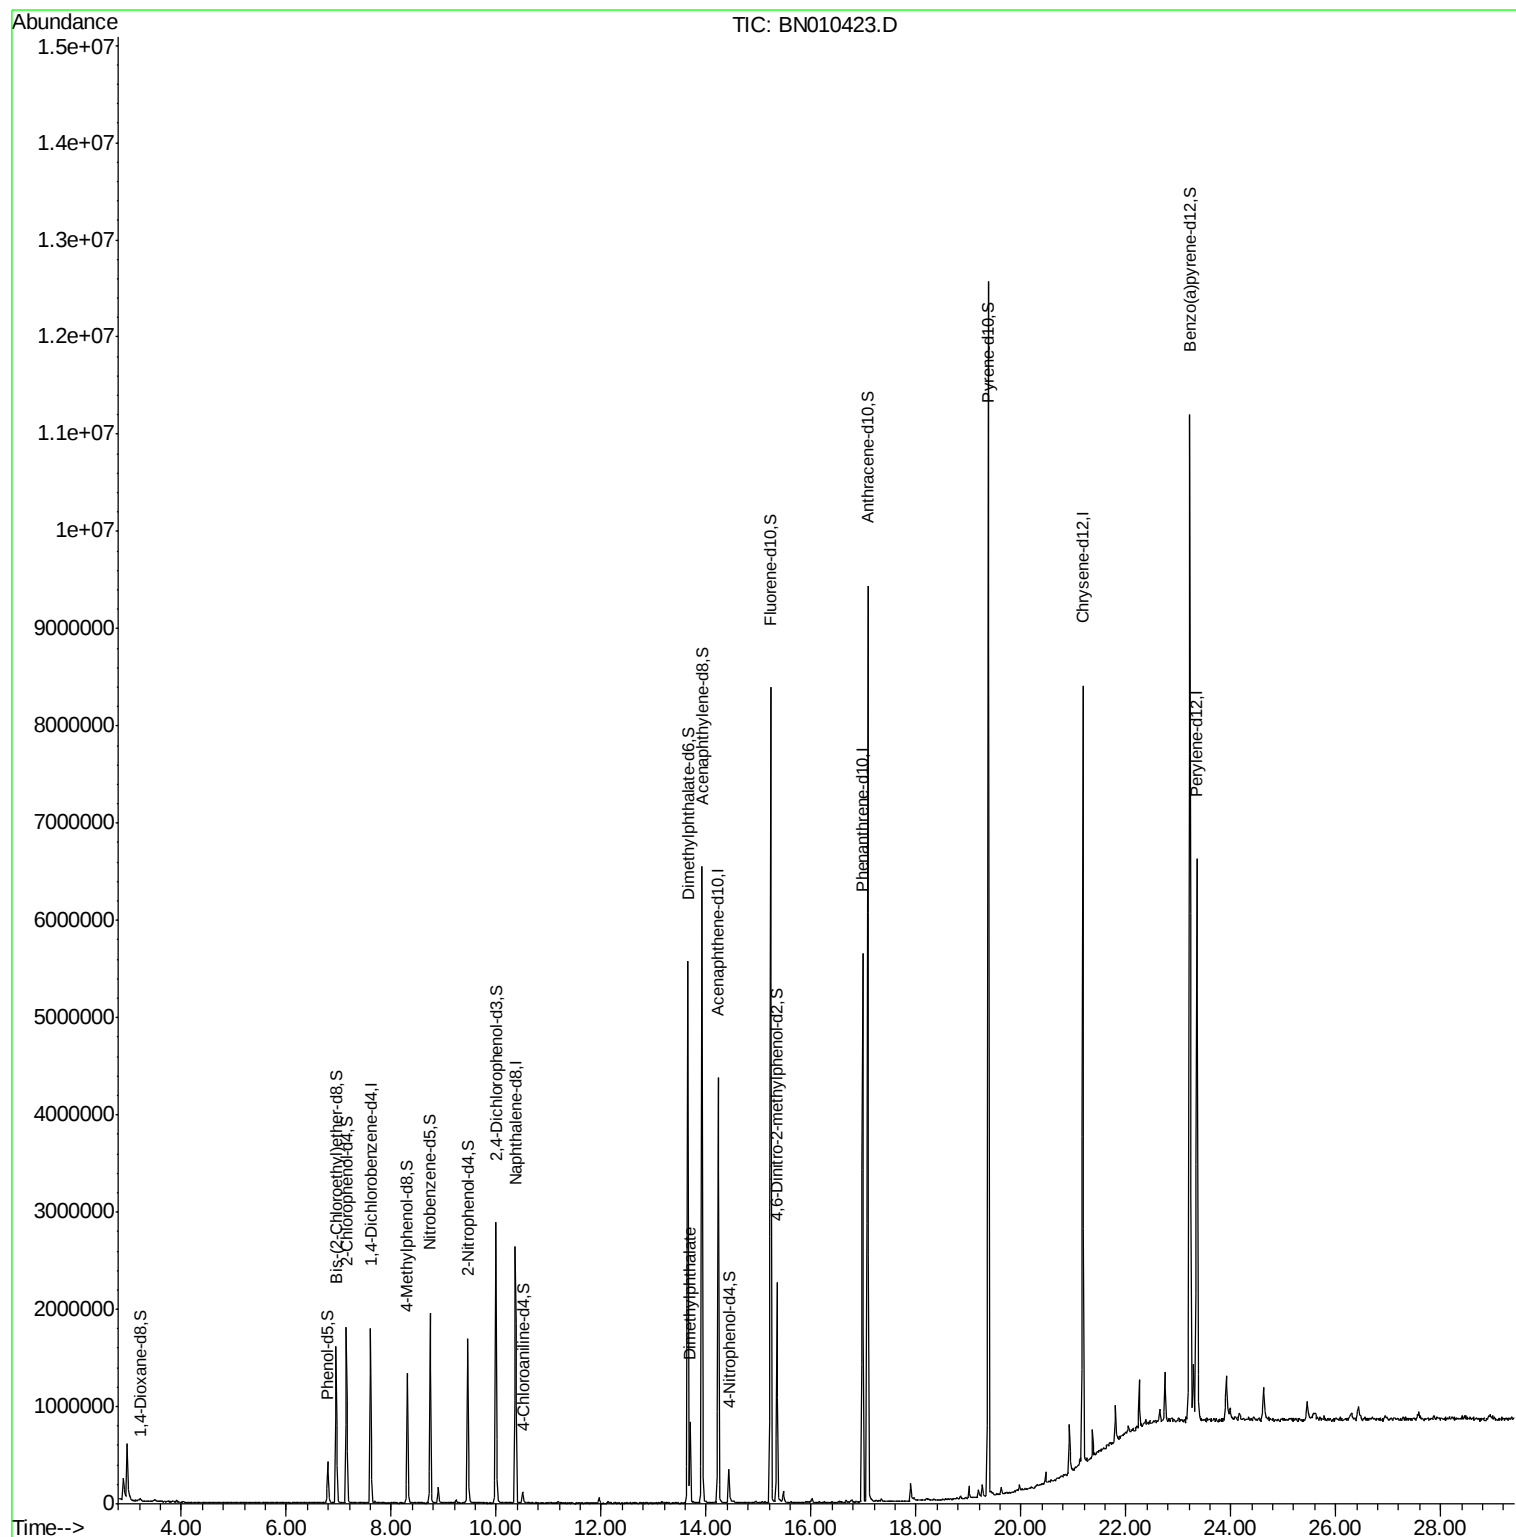

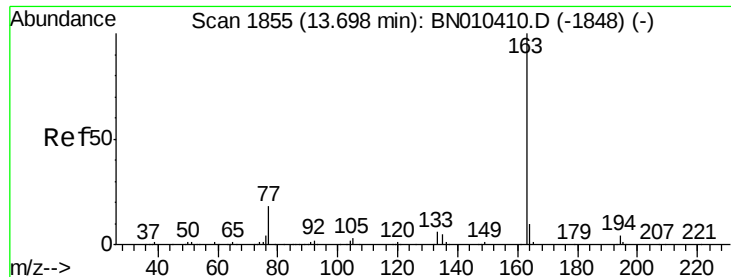

#45

Dimethylphthalate

Concen: 4.620 ng/ul

RT: 13.69 min Scan# 1854

Delta R.T. -0.01 min

Lab File: BN010423.D

Acq: 07 Apr 2020 18:21

Instrument :

BNA_N

ClientSampleId :


Tot Ion:163 Resp: 529084

Ion Ratio Lower Upper

163 100

194 4.0 3.7 5.5

164 11.1 8.0 12.0

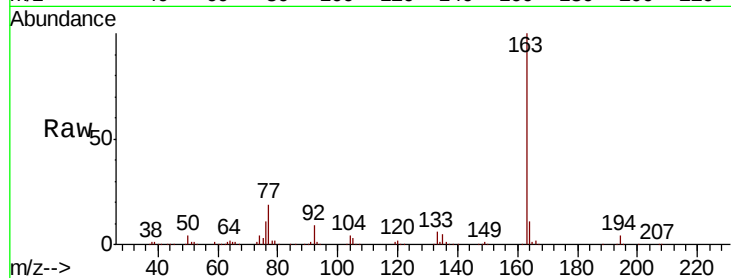

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

