

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040720\
 Data File : BN010425.D
 Acq On : 07 Apr 2020 19:34
 Operator : CG/JU
 Sample : L2173-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Apr 08 00:48:07 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 07 11:04:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.60	152	450150	20.00	ng/ul	0.00
18) Naphthalene-d8	10.36	136	1941997	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	1337242	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	3021600	20.00	ng/ul	0.00
78) Chrysene-d12	21.18	240	3352959	20.00	ng/ul	0.00
86) Perylene-d12	23.36	264	3787868	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.21	96	16400	1.72	ng/uL	0.00
5) Phenol-d5	6.79	99	297434	7.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	726746	36.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	909667	30.52	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	583858	18.40	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	571640	39.65	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	608154	39.84	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	1128962	35.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	67722	1.81	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	3971852	39.36	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	4761518	40.40	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	115106	6.07	ng/ul	0.00
58) Fluorene-d10	15.23	176	3519408	40.02	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.35	200	532656	30.79	ng/ul	0.00
71) Anthracene-d10	17.07	188	5612464	40.45	ng/ul	0.00
79) Pyrene-d10	19.38	212	6705066	38.81	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.22	264	7737952	41.06	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.69	163	449589	4.315	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040720\
Data File : BN010425.D
Acq On : 07 Apr 2020 19:34
Operator : CG/JU
Sample : L2173-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Apr 08 00:48:07 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 07 11:04:24 2020
Response via : Initial Calibration

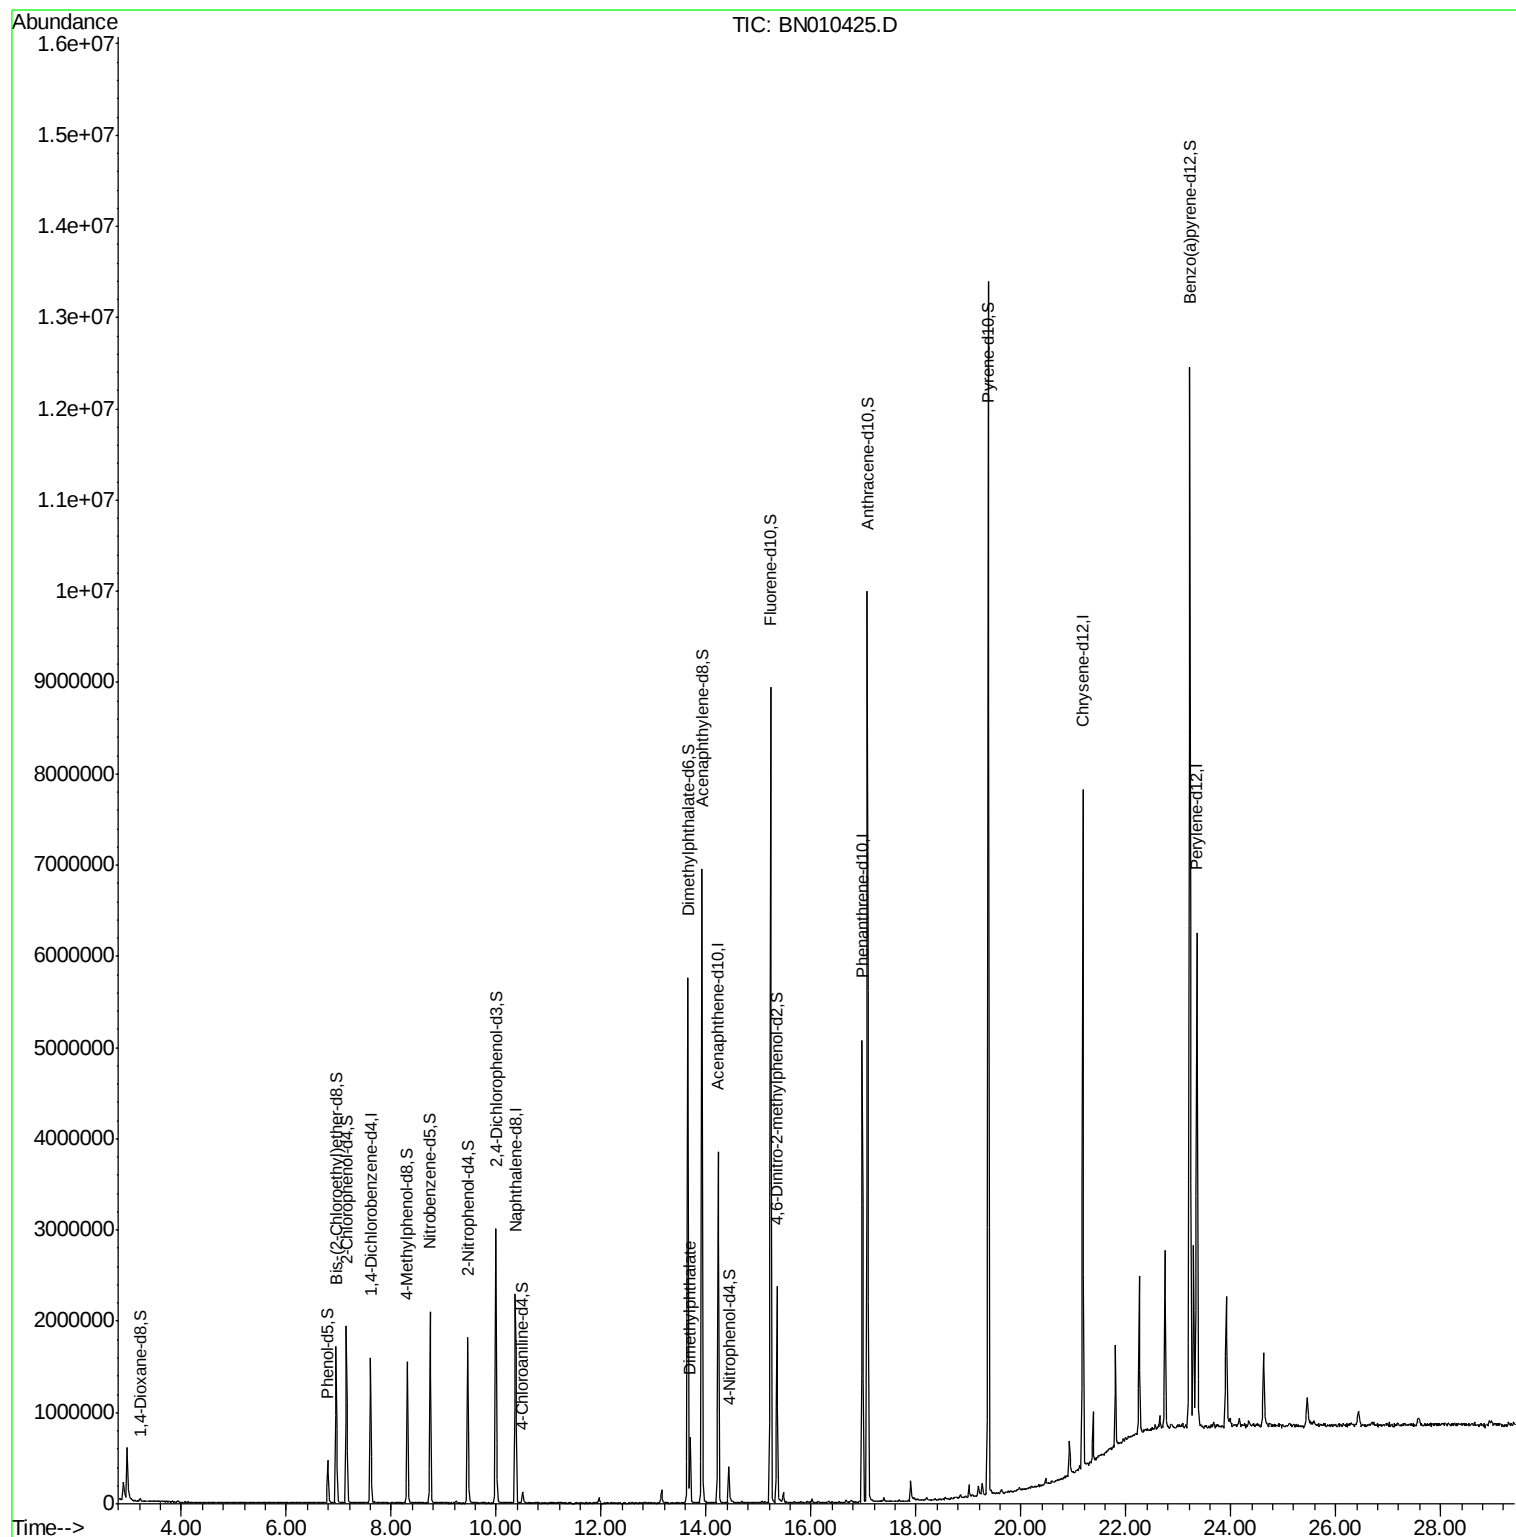

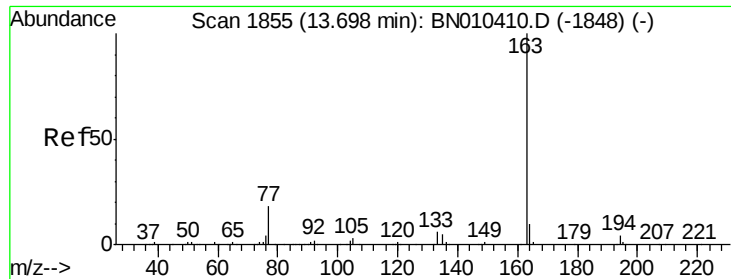

#45

Dimethylphthalate

Concen: 4.315 ng/ul

RT: 13.69 min Scan# 1854

Delta R.T. -0.01 min

Lab File: BN010425.D

Acq: 07 Apr 2020 19:34

Instrument :

BNA_N

ClientSampleId :


Tot Ion:163 Resp: 449589

Ion Ratio Lower Upper

163 100

194 4.3 3.7 5.5

164 9.7 8.0 12.0

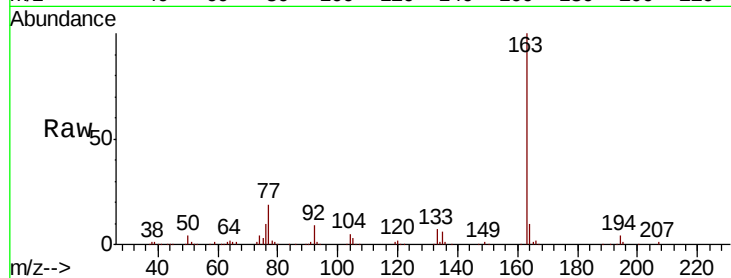

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

