

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040720\
 Data File : BN010416.D
 Acq On : 07 Apr 2020 14:09
 Operator : CG/JU
 Sample : L2158-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0EZ1

Manual Integrations
 APPROVED

mohammad
 4/8/2020 8:11:41 AM

Quant Time: Apr 07 15:20:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 07 11:04:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	441097	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	1944058	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	1291246	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	2942517	20.00	ng/ul	0.00
78) Chrysene-d12	21.18	240	3324284	20.00	ng/ul	0.00
86) Perylene-d12	23.36	264	3699371	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.21	96	21056m	2.26	ng/uL	0.00
5) Phenol-d5	6.79	99	247938	6.74	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	666211	34.56	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	814743	27.89	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	518375	16.68	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	525753	36.43	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	558755	36.57	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	1055025	33.29	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	79251	2.12	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	3807004	39.07	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	4533325	39.83	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	94749	5.18	ng/ul	0.00
58) Fluorene-d10	15.23	176	3417329	40.24	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.35	200	532179	31.59	ng/ul	0.00
71) Anthracene-d10	17.07	188	5347096	39.58	ng/ul	0.00
79) Pyrene-d10	19.38	212	6405353	37.39	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.22	264	7309840	39.72	ng/ul	0.00

Target Compounds					Ovalue	
45) Dimethylphthalate	13.70	163	754931	7.504	ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040720\
Data File : BN010416.D
Acq On : 07 Apr 2020 14:09
Operator : CG/JU
Sample : L2158-03
Misc :
ALS Vial : 8 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0EZ1

Quant Time: Apr 07 15:20:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 07 11:04:24 2020
Response via : Initial Calibration

Manual Integrations
APPROVED

mohammad
4/8/2020 8:11:41 AM

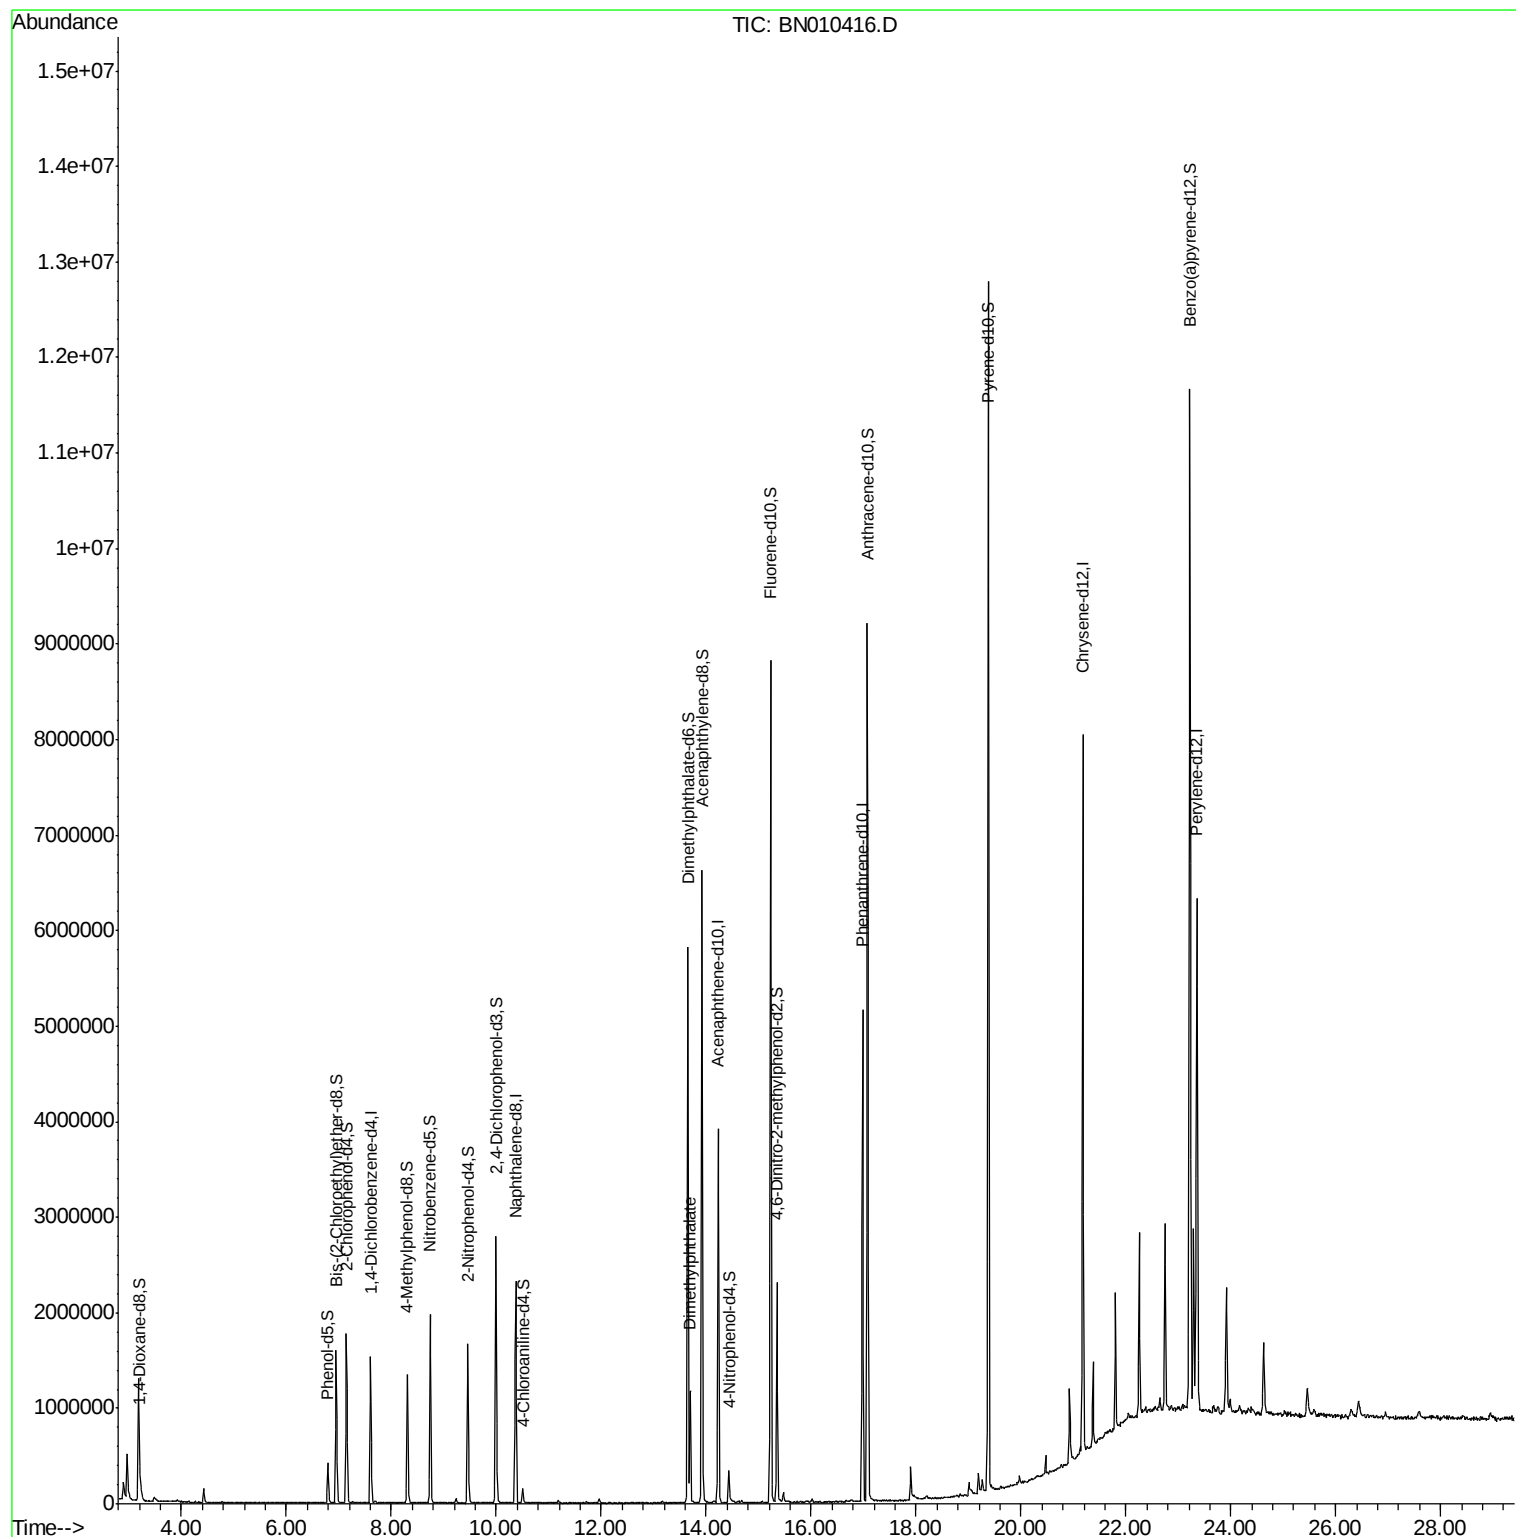

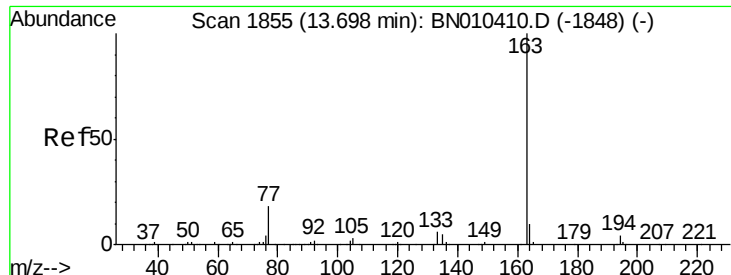

#45
 Dimethylphthalate
 Concen: 7.504 ng/ul
 RT: 13.70 min Scan# 1855
 Delta R.T. 0.00 min
 Lab File: BN010416.D
 Acq: 07 Apr 2020 14:09

Instrument :
 BNA_N
 ClientSampleId :
 C0EZ1

Tot Ion:	163	Resp:	754931
Ion Ratio	Lower	Upper	
163	100		
194	4.5	3.7	5.5
164	9.5	8.0	12.0

Manual Integrations
 APPROVED

mohammad
 4/8/2020 8:11:41 AM

