

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040720\
 Data File : BN010417.D
 Acq On : 07 Apr 2020 14:45
 Operator : CG/JU
 Sample : L2158-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0EZ5

Quant Time: Apr 07 15:23:53 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 07 11:04:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	465425	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	2048918	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	1370344	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.98	188	3166948	20.00	ng/ul	0.00
78) Chrysene-d12	21.18	240	3644258	20.00	ng/ul	0.00
86) Perylene-d12	23.36	264	3933180	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.21	96	15623	1.59	ng/uL	0.00
5) Phenol-d5	6.79	99	254708	6.56	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	584307	28.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	754283	24.47	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	486579	14.84	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	474769	31.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	493803	30.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	936604	28.05	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	76291	1.93	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	3398382	32.87	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	4014368	33.23	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	98694	5.08	ng/ul	0.00
58) Fluorene-d10	15.23	176	3039241	33.73	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.35	200	460344	25.39	ng/ul	0.00
71) Anthracene-d10	17.07	188	4871801	33.50	ng/ul	0.00
79) Pyrene-d10	19.38	212	5613896	29.89	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.22	264	6543402	33.44	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.70	163	767715	7.190	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040720\
Data File : BN010417.D
Acq On : 07 Apr 2020 14:45
Operator : CG/JU
Sample : L2158-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0EZ5

Quant Time: Apr 07 15:23:53 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 07 11:04:24 2020
Response via : Initial Calibration

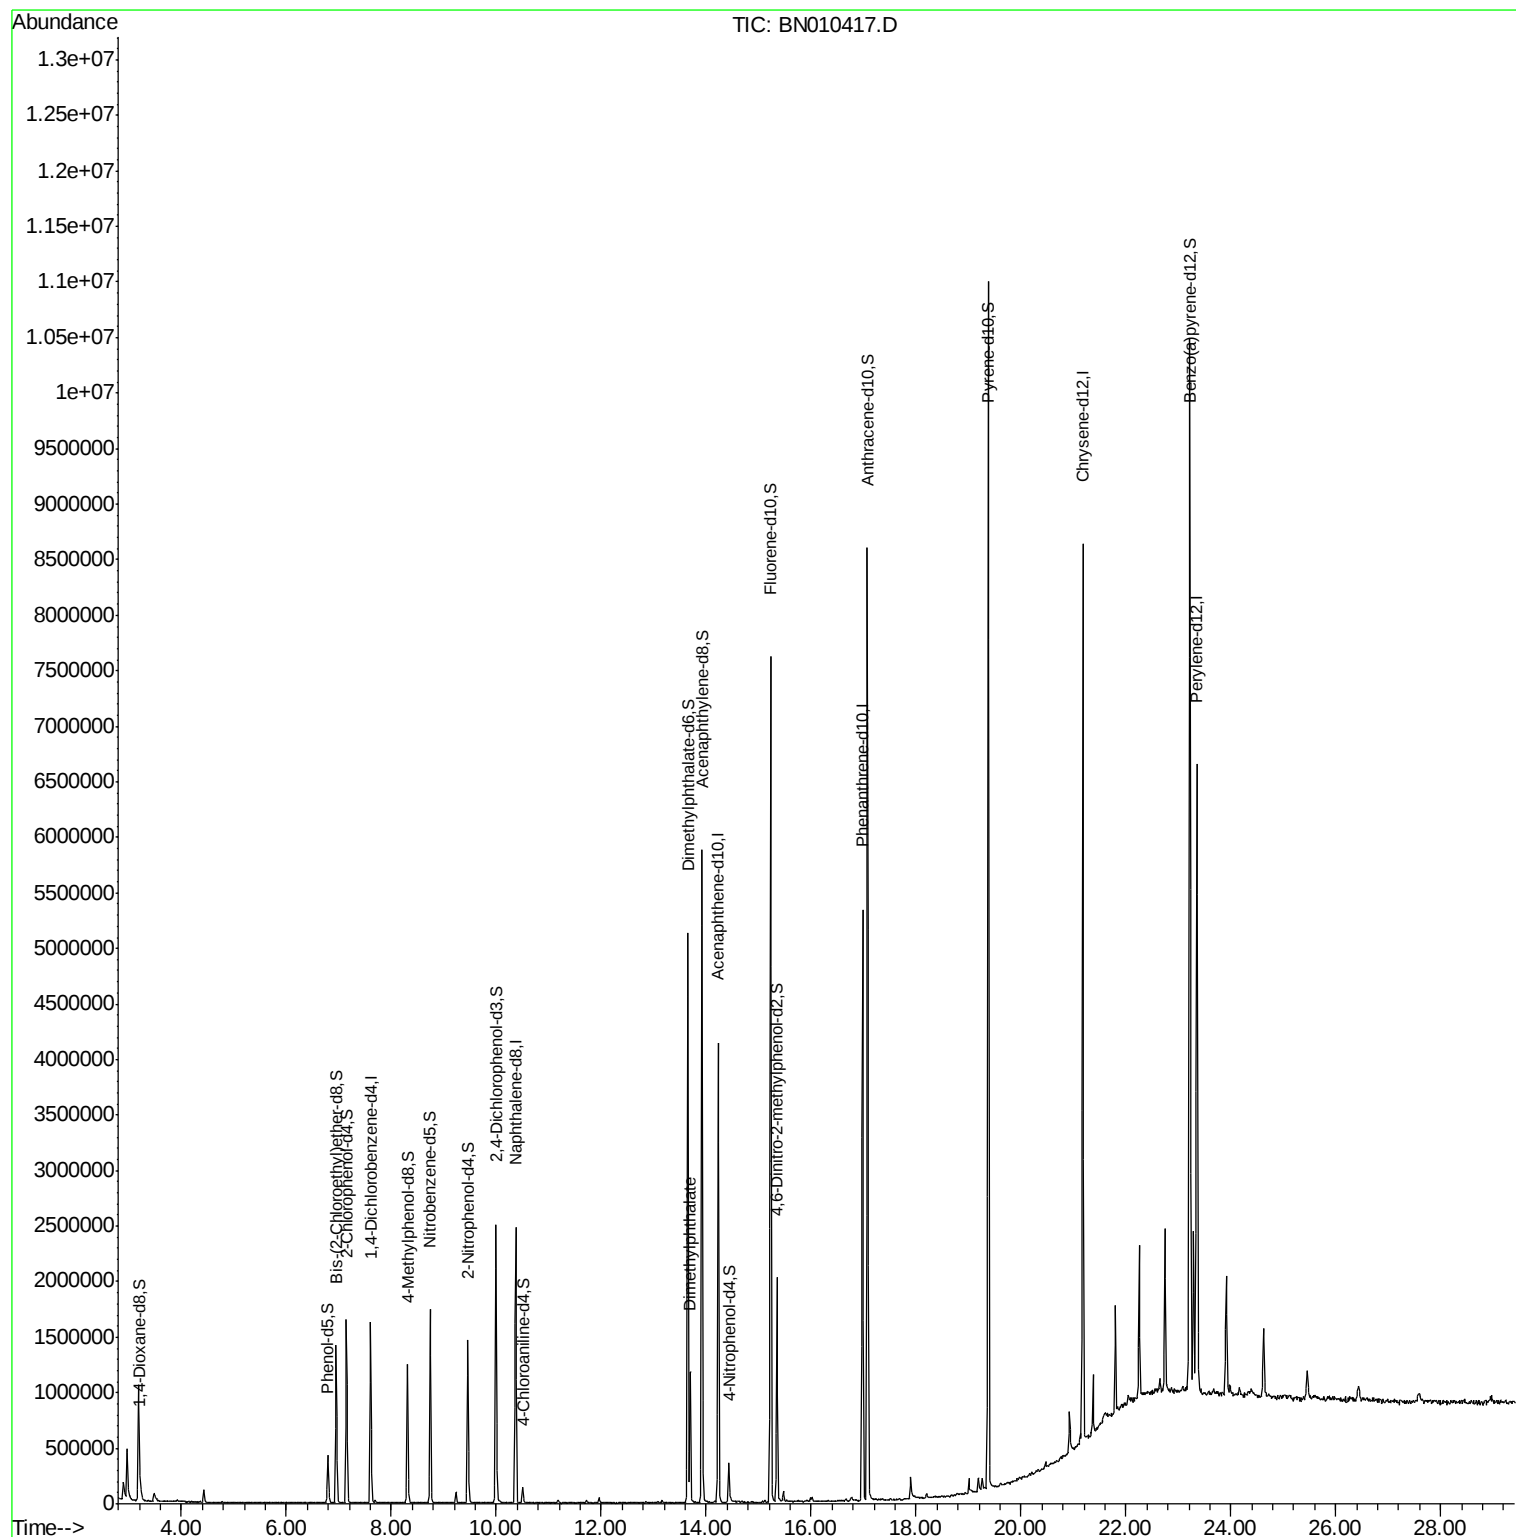

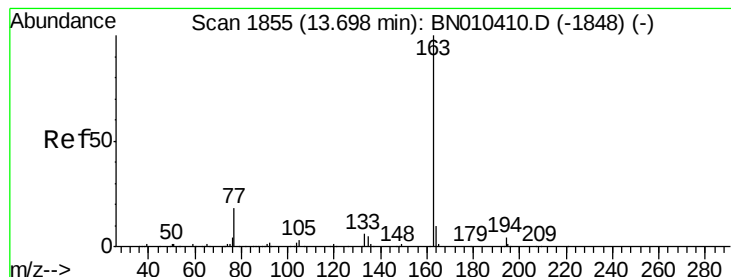

#45

Dimethylphthalate

Concen: 7.190 ng/ul

RT: 13.70 min Scan# 1855

Delta R.T. 0.00 min

Lab File: BN010417.D

Acq: 07 Apr 2020 14:45

Instrument :

BNA_N

ClientSampleId :

C0EZ5


Tot Ion:163 Resp: 767715

Ion Ratio Lower Upper

163 100

194 4.3 3.7 5.5

164 9.4 8.0 12.0

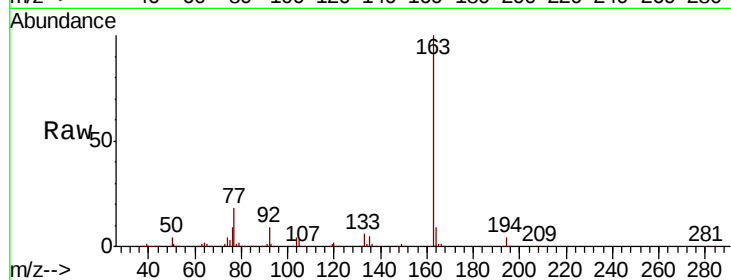

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

