

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040720\
 Data File : BN010420.D
 Acq On : 07 Apr 2020 16:33
 Operator : CG/JU
 Sample : L2158-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0F04

Quant Time: Apr 07 17:05:58 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 07 11:04:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	446765	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	2010971	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	1362520	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	3162888	20.00	ng/ul	0.00
78) Chrysene-d12	21.18	240	3441576	20.00	ng/ul	0.00
86) Perylene-d12	23.35	264	3838696	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	207302	21.94	ng/uL	-0.02
5) Phenol-d5	6.79	99	240133	6.44	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	577918	29.60	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	730467	24.69	ng/ul	0.00
13) 4-Methylphenol-d8	8.30	113	474400	15.07	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	443632	29.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	485549	30.72	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	901656	27.51	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	78487	2.03	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	3209926	31.22	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	3831963	31.91	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	82004	4.25	ng/ul	0.00
58) Fluorene-d10	15.23	176	2911027	32.49	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.35	200	411052	22.70	ng/ul	0.00
71) Anthracene-d10	17.07	188	4538904	31.25	ng/ul	0.00
79) Pyrene-d10	19.38	212	5370475	30.28	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.22	264	6024285	31.55	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.69	163	524654	4.942	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040720\
Data File : BN010420.D
Acq On : 07 Apr 2020 16:33
Operator : CG/JU
Sample : L2158-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0F04

Quant Time: Apr 07 17:05:58 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 07 11:04:24 2020
Response via : Initial Calibration

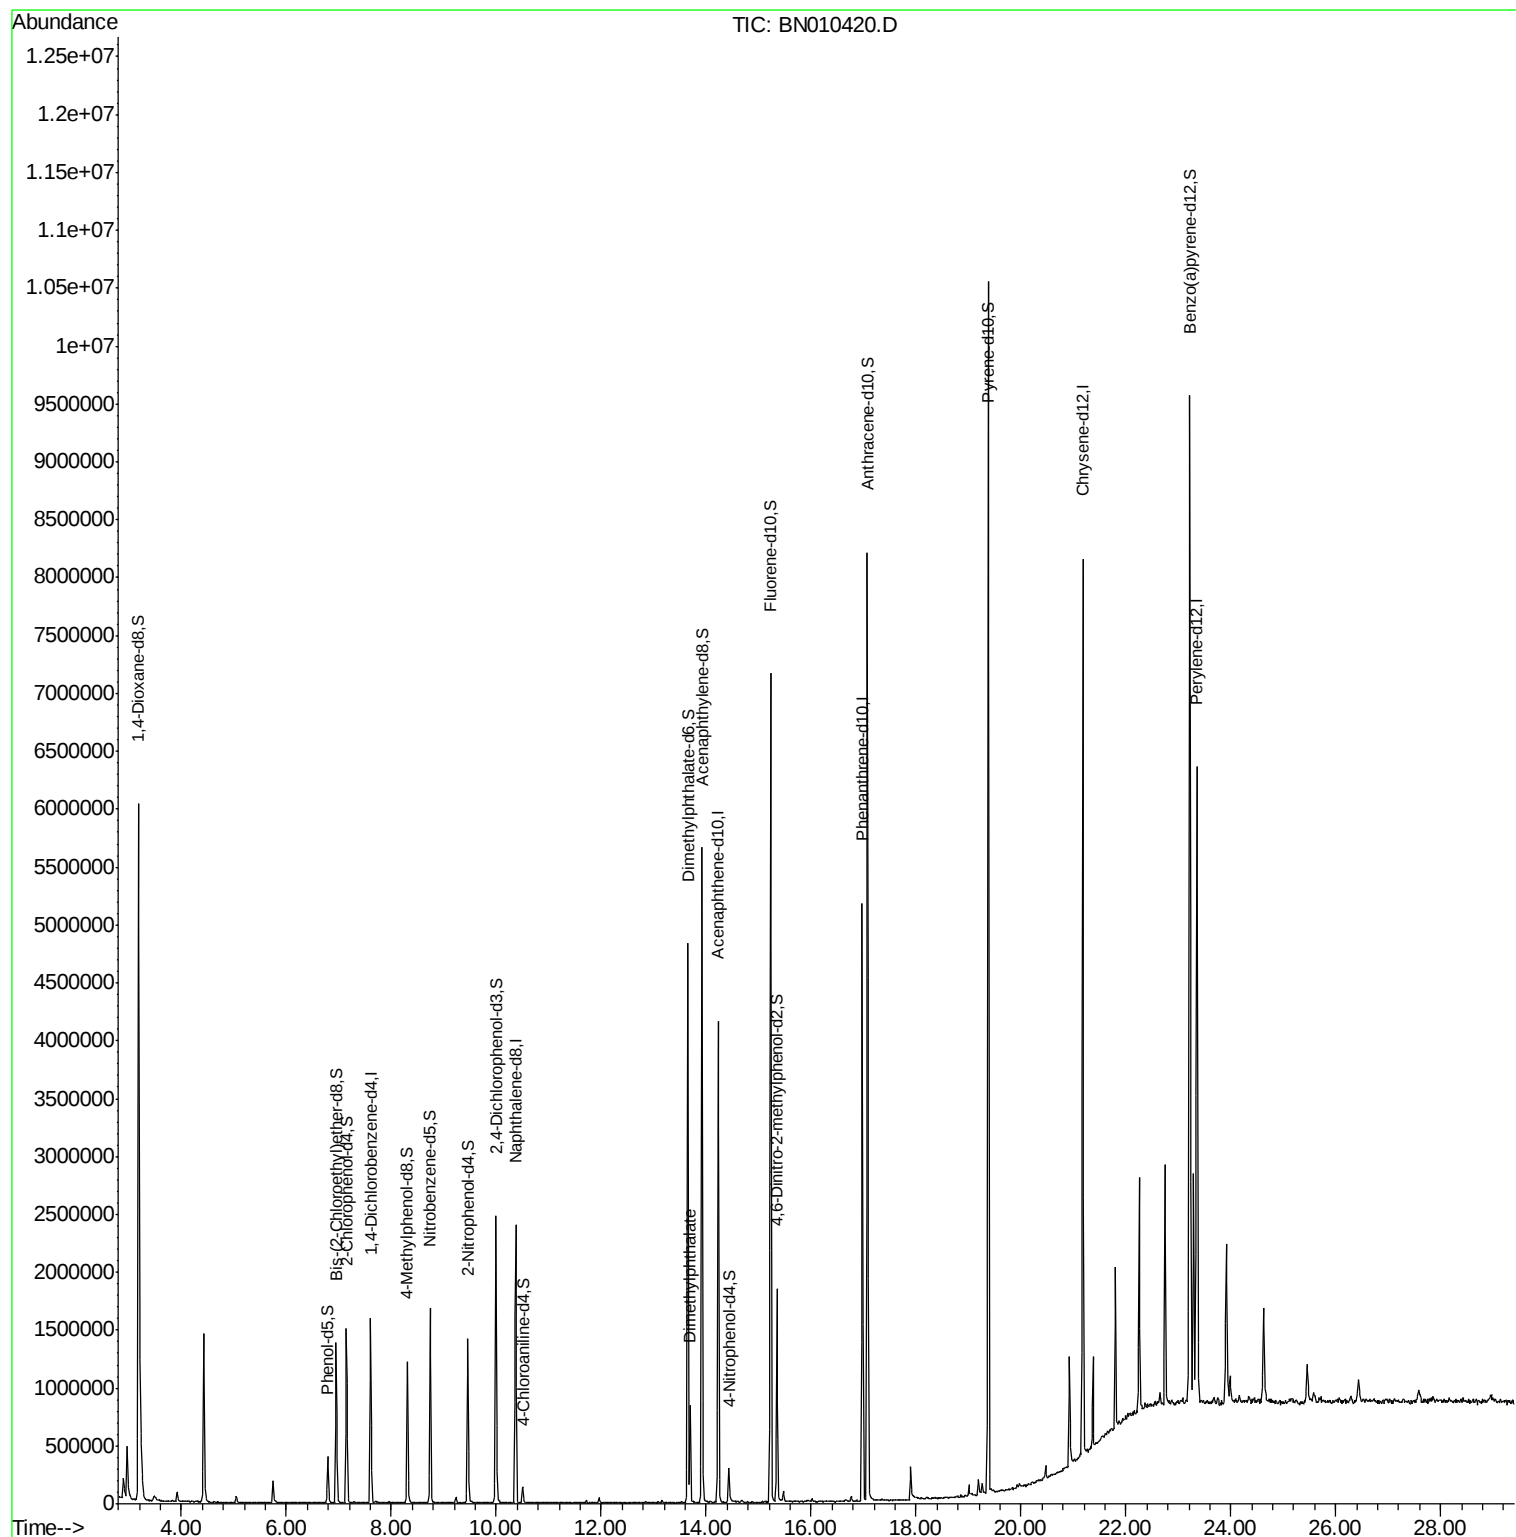

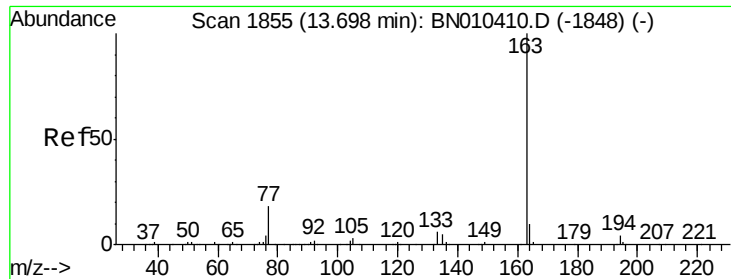

#45

Dimethylphthalate

Concen: 4.942 ng/ul

RT: 13.69 min Scan# 1854

Delta R.T. -0.01 min

Lab File: BN010420.D

Acq: 07 Apr 2020 16:33

Instrument :

BNA_N

ClientSampleId :

C0F04


Tot Ion:163 Resp: 524654

Ion Ratio Lower Upper

163 100

194 3.7 3.7 5.5

164 9.4 8.0 12.0

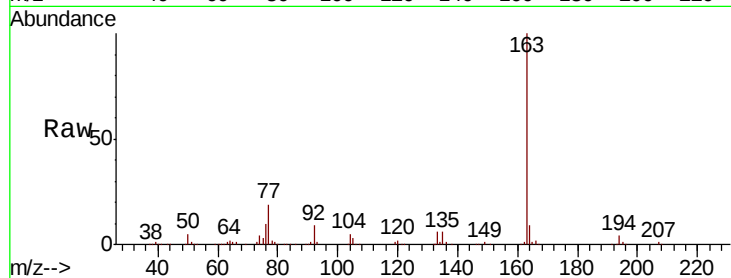

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

