

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN040720\
 Data File : BN010421.D
 Acq On : 07 Apr 2020 17:09
 Operator : CG/JU
 Sample : L2158-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0F05

Quant Time: Apr 07 17:44:12 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 07 11:04:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.61	152	409113	20.00	ng/ul	0.00
18) Naphthalene-d8	10.37	136	1805316	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.23	164	1220039	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.97	188	2770303	20.00	ng/ul	0.00
78) Chrysene-d12	21.18	240	3006512	20.00	ng/ul	0.00
86) Perylene-d12	23.36	264	3356119	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.18	96	352783	40.78	ng/uL	-0.02
5) Phenol-d5	6.79	99	290654	8.52	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	755421	42.25	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	948456	35.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.31	113	589487	20.45	ng/ul	0.00
19) Nitrobenzene-d5	8.75	128	598707	44.67	ng/ul	0.00
22) 2-Nitrophenol-d4	9.46	143	651671	45.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.99	165	1173975	39.90	ng/ul	0.00
29) 4-Chloroaniline-d4	10.50	131	87598	2.52	ng/ul	0.00
44) Dimethylphthalate-d6	13.65	166	4254990	46.22	ng/ul	0.00
47) Acenaphthylene-d8	13.92	160	4945197	45.98	ng/ul	0.00
52) 4-Nitrophenol-d4	14.43	143	109832	6.35	ng/ul	0.00
58) Fluorene-d10	15.23	176	3765922	46.94	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.35	200	599092	37.77	ng/ul	0.00
71) Anthracene-d10	17.08	188	5988874	47.08	ng/ul	0.00
79) Pyrene-d10	19.38	212	7073318	45.66	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.22	264	8133529	48.71	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.70	163	786777	8.277	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN040720\
Data File : BN010421.D
Acq On : 07 Apr 2020 17:09
Operator : CG/JU
Sample : L2158-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0F05

Quant Time: Apr 07 17:44:12 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN040120MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 07 11:04:24 2020
Response via : Initial Calibration

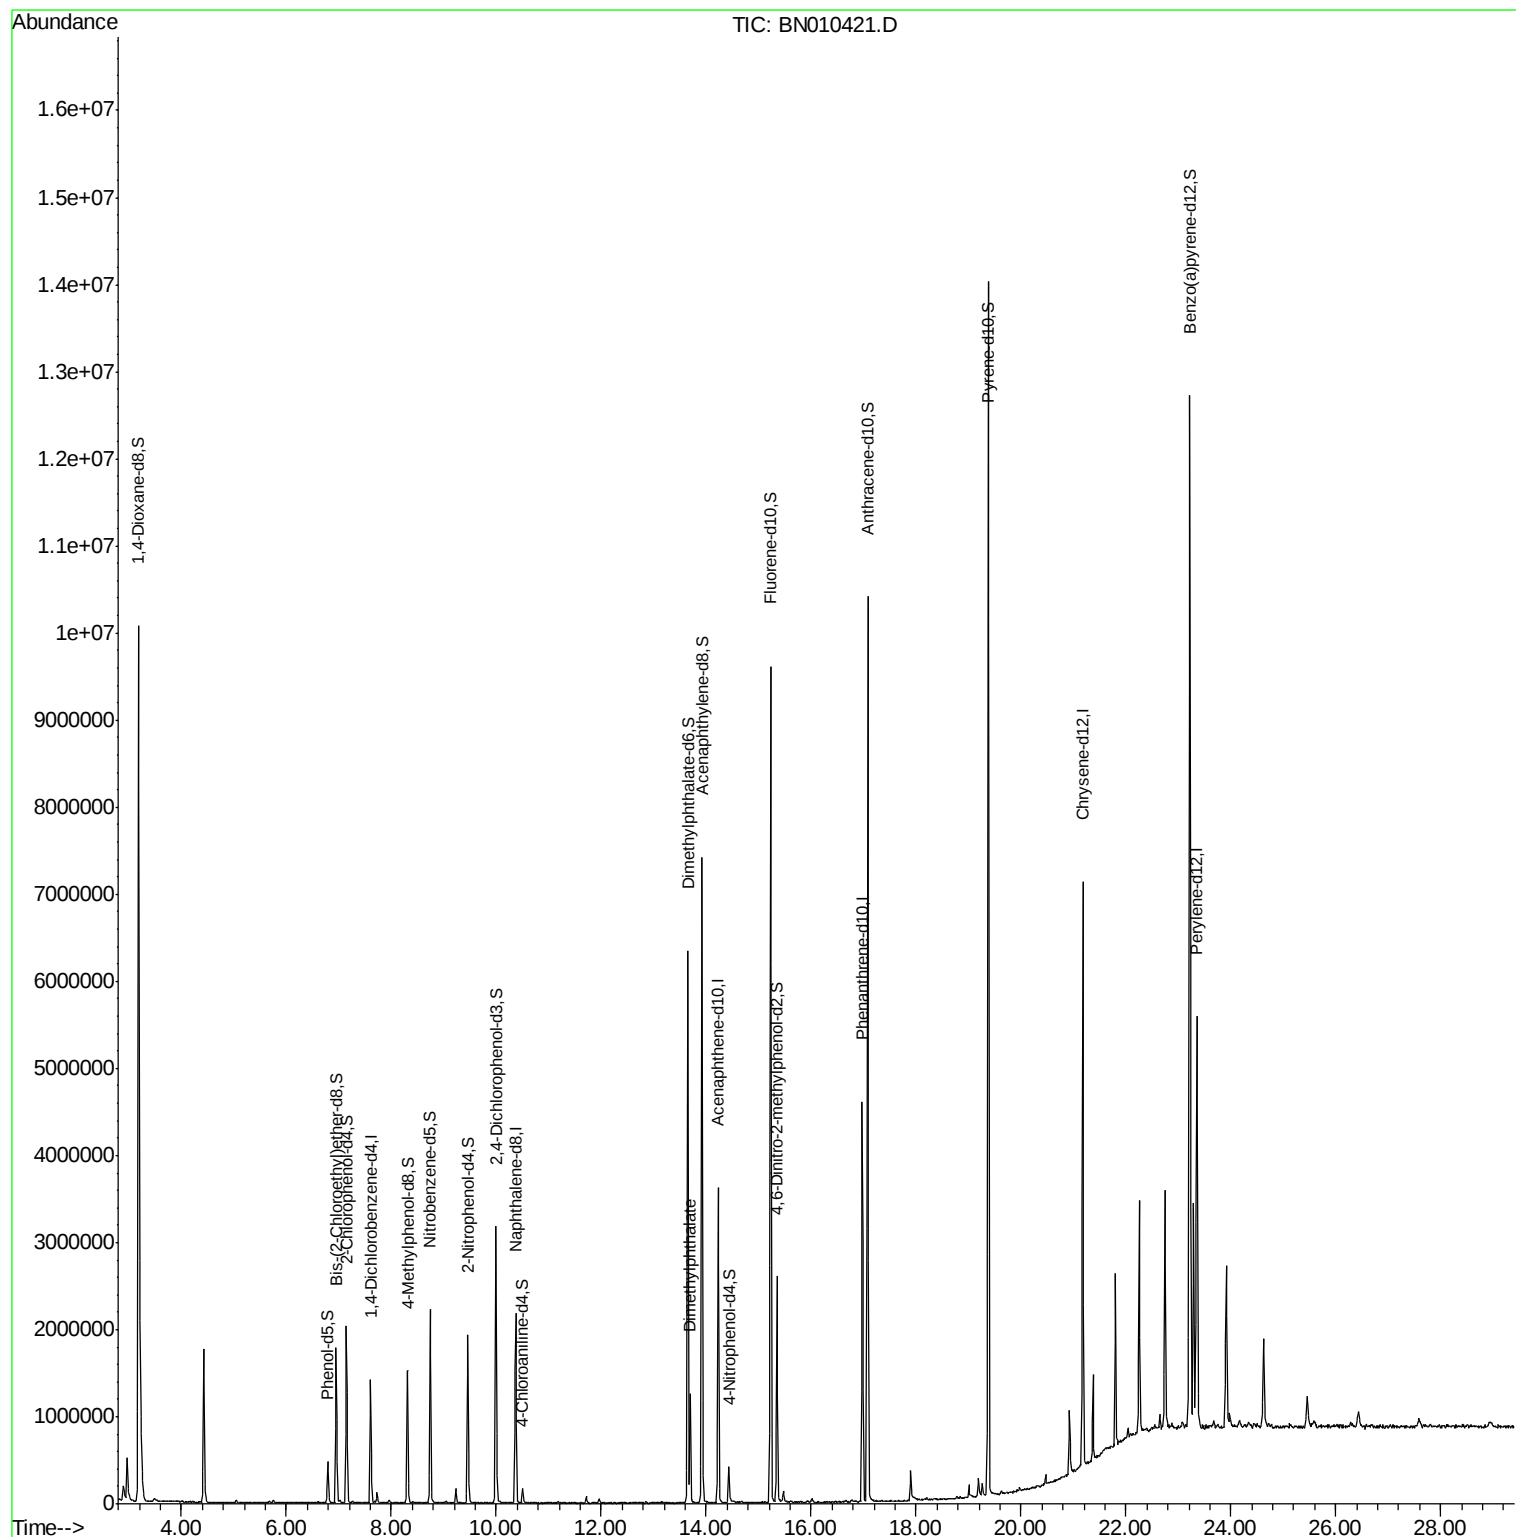

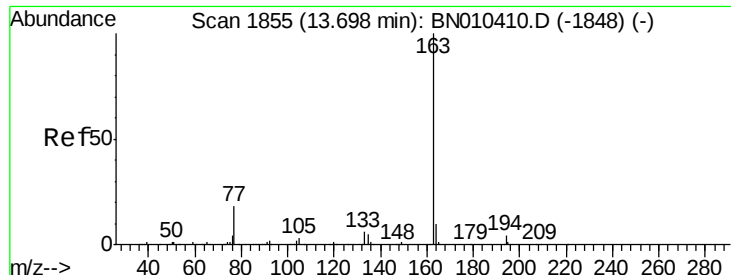

#45

Dimethylphthalate

Concen: 8.277 ng/ul

RT: 13.70 min Scan# 1855

Delta R.T. 0.00 min

Lab File: BN010421.D

Acq: 07 Apr 2020 17:09

Instrument :

BNA_N

ClientSampleId :

C0F05

Tot Ion:163 Resp: 786777

Ion Ratio Lower Upper

163 100

194 3.9 3.7 5.5

164 9.7 8.0 12.0

