

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040721\
 Data File : BN014220.D
 Acq On : 06 Apr 2021 11:54
 Operator : CG/JU
 Sample : SSTDIC0.8
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC0.8

Quant Time: Apr 06 12:23:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 06 12:12:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.644	152	7266	0.40	ng	0.00
7) Naphthalene-d8	10.416	136	28206	0.40	ng	0.00
13) Acenaphthene-d10	14.283	164	17243	0.40	ng	0.00
19) Phenanthrene-d10	17.030	188	38561	0.40	ng	0.00
29) Chrysene-d12	21.226	240	39135	0.40	ng	# 0.00
36) Perylene-d12	23.428	264	33804	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.236	112	14286	0.79	ng	0.00
5) Phenol-d6	6.814	99	18615	0.78	ng	0.00
8) Nitrobenzene-d5	8.794	82	16469	0.80	ng	0.00
11) 2-Methylnaphthalene-d10	12.017	152	37413	0.59	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	5188	0.79	ng	0.00
15) 2-Fluorobiphenyl	12.900	172	53595	0.84	ng	0.00
27) Fluoranthene-d10	19.066	212	88338	0.58	ng	0.00
31) Terphenyl-d14	19.672	244	74214	0.82	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.174	88	7023	0.80	ng	97
3) n-Nitrosodimethylamine	3.496	42	5771	0.80	ng	# 92
6) bis(2-Chloroethyl)ether	7.080	93	16223	0.78	ng	100
9) Naphthalene	10.467	128	57472	0.76	ng	99
10) Hexachlorobutadiene	10.758	225	10646	0.77	ng	# 100
12) 2-Methylnaphthalene	12.093	142	40413	0.76	ng	98
16) Acenaphthylene	14.004	152	55353	0.78	ng	100
17) Acenaphthene	14.346	154	39490	0.78	ng	99
18) Fluorene	15.336	166	50853	0.79	ng	99
20) 4,6-Dinitro-2-methylph...	15.412	198	4104	0.71	ng	94
21) 4-Bromophenyl-phenylether	16.227	248	16551	0.76	ng	96
22) Hexachlorobenzene	16.337	284	17854	0.75	ng	100
23) Atrazine	16.495	200	11887	0.79	ng	99
24) Pentachlorophenol	16.690	266	4547	0.71	ng	97
25) Phenanthrene	17.067	178	85605	0.76	ng	100
26) Anthracene	17.164	178	72139	0.75	ng	100
28) Fluoranthene	19.096	202	98772	0.75	ng	100
30) Pyrene	19.459	202	97271	0.77	ng	100
32) Benzo(a)anthracene	21.205	228	90357	0.75	ng	99
33) Chrysene	21.258	228	98696	0.74	ng	99
34) Bis(2-ethylhexyl)phtha...	21.152	149	26955	0.65	ng	99
35) Indeno(1,2,3-cd)pyrene	25.636	276	95271	0.59	ng	100
37) Benzo(b)fluoranthene	22.768	252	96433	0.76	ng	# 97
38) Benzo(k)fluoranthene	22.812	252	98962	0.80	ng	99
39) Benzo(a)pyrene	23.332	252	84755	0.75	ng	# 90
40) Dibenzo(a,h)anthracene	25.650	278	79362	0.67	ng	100
41) Benzo(g,h,i)perylene	26.307	276	80675	0.67	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040721\
Data File : BN014220.D
Acq On : 06 Apr 2021 11:54
Operator : CG/JU
Sample : SSTDIC0.8
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Quant Time: Apr 06 12:23:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 06 12:12:15 2021
Response via : Initial Calibration




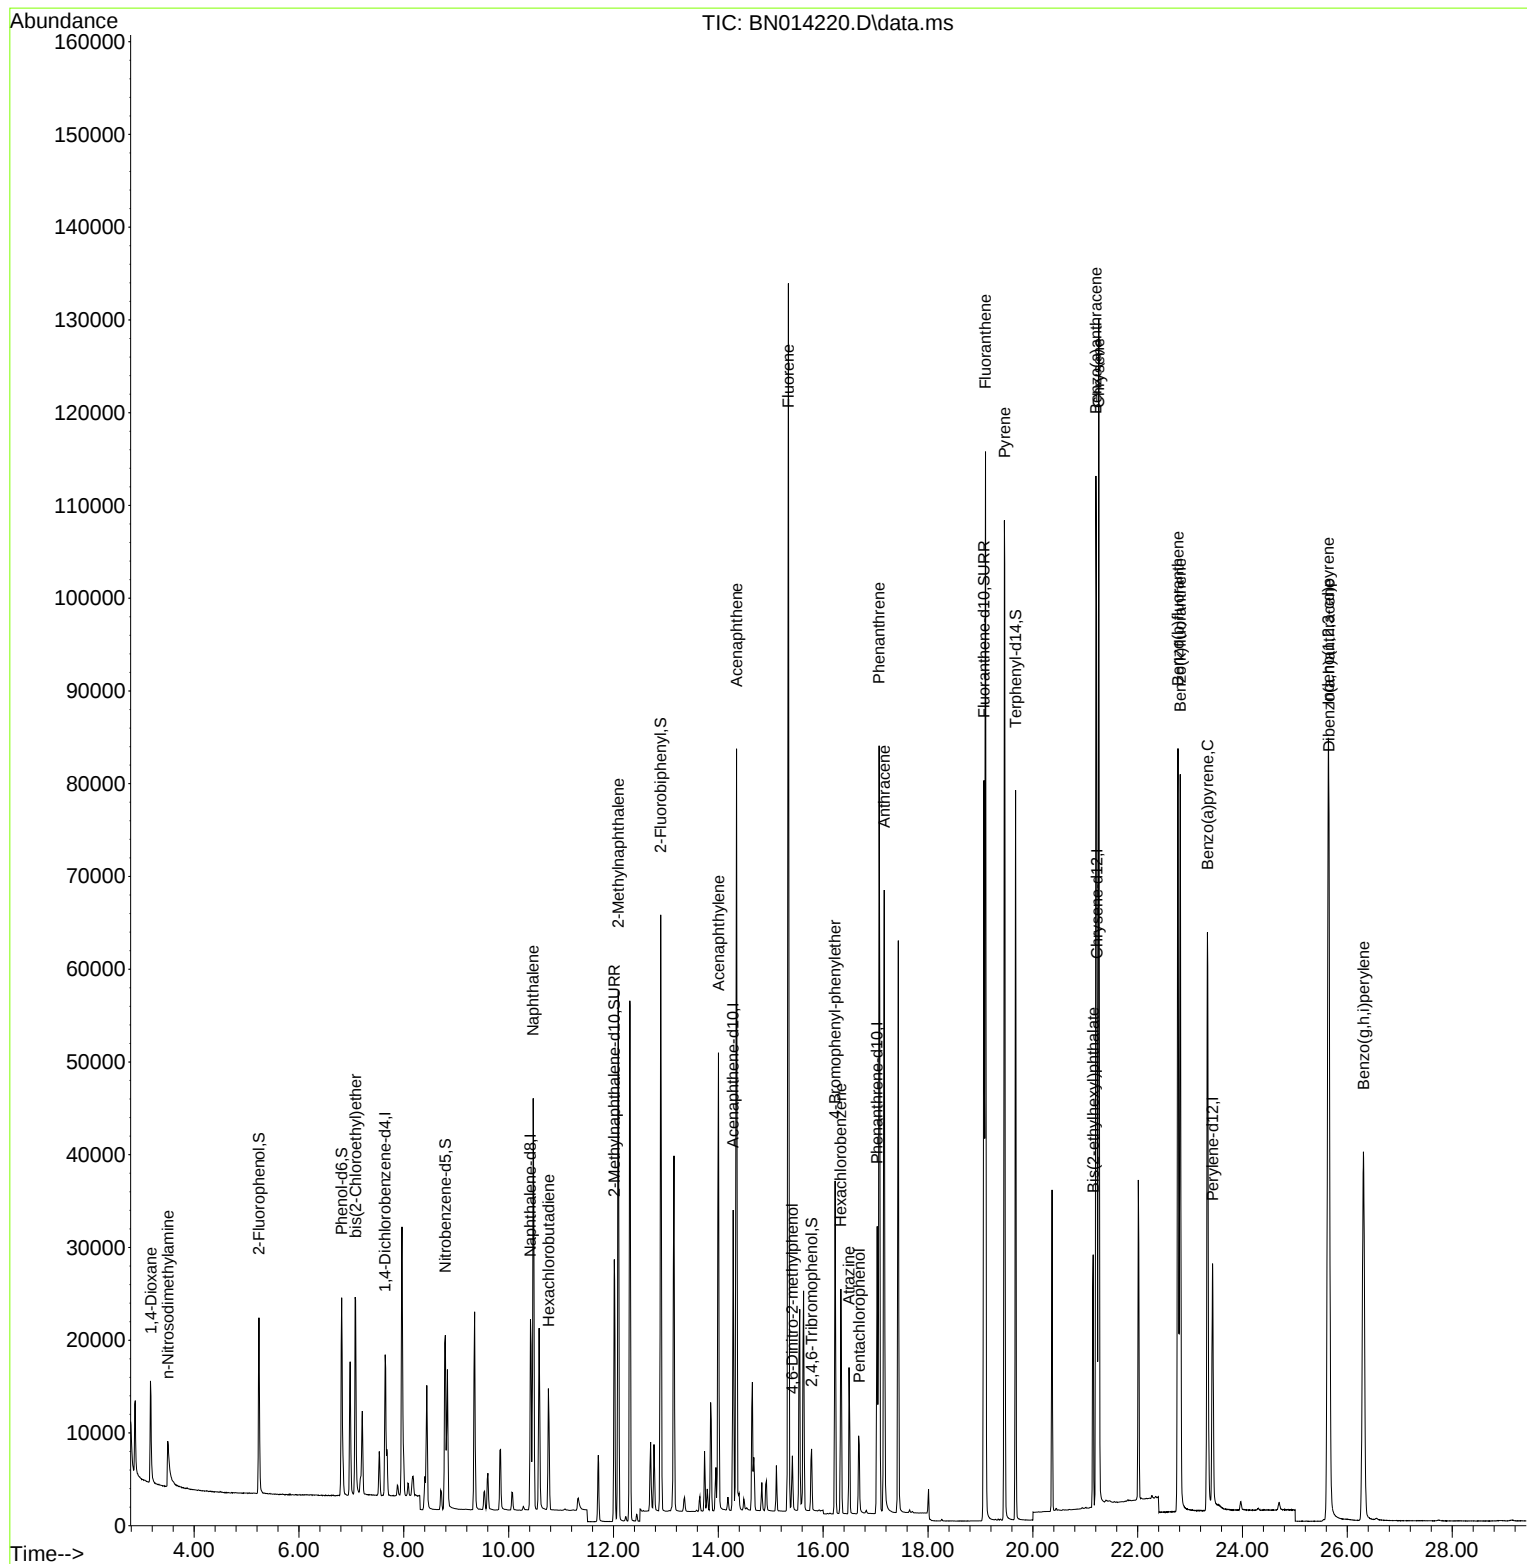




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.644 min Scan# 604
 Delta R.T. -0.000 min
 Lab File: BN014220.D
 Acq: 06 Apr 2021 11:54




Instrument :
 BNA_N
 ClientSampled :
 SSTDICC0.8


Tgt Ion:152 Resp: 7266
 Ion Ratio Lower Upper
 152 100
 150 160.0 126.2 189.2
 115 62.1 49.4 74.0

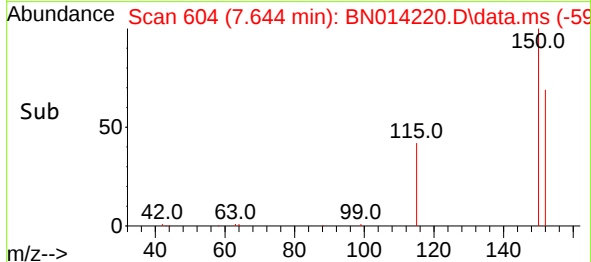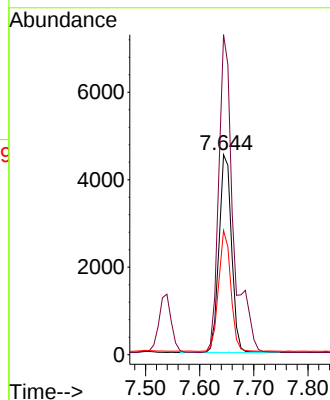

#2
 1,4-Dioxane
 Concen: 0.80 ng
 RT: 3.174 min Scan# 49
 Delta R.T. -0.000 min
 Lab File: BN014220.D
 Acq: 06 Apr 2021 11:54

Tgt Ion: 88 Resp: 7023
 Ion Ratio Lower Upper
 88 100
 58 83.1 70.0 105.0
 43 35.5 28.3 42.5


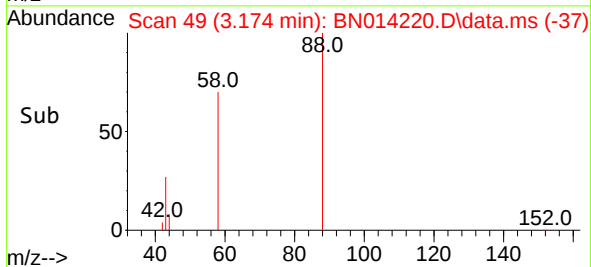
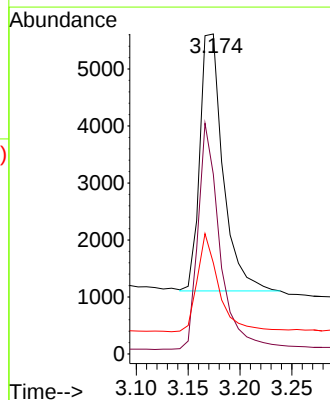
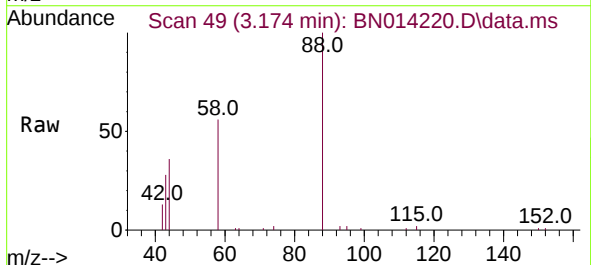




#3
n-Nitrosodimethylamine
Concen: 0.80 ng
RT: 3.496 min Scan# 89
Delta R.T. -0.016 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion: 42 Resp: 5771
Ion Ratio Lower Upper
42 100
74 113.0 85.0 127.6
44 2.2 9.4 14.0#

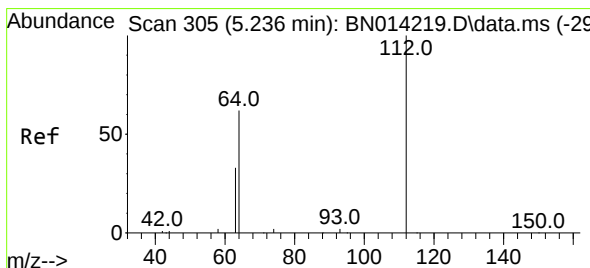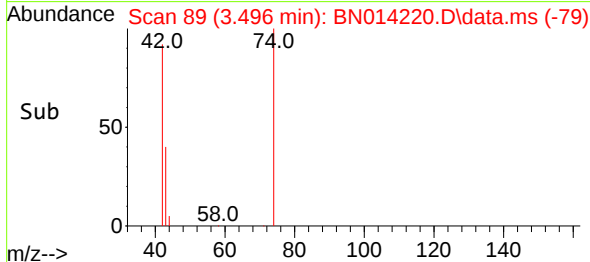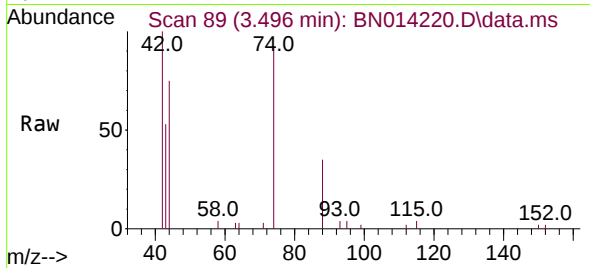

#4
2-Fluorophenol
Concen: 0.79 ng
RT: 5.236 min Scan# 305
Delta R.T. -0.000 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion: 112 Resp: 14286
Ion Ratio Lower Upper
112 100
64 60.5 48.4 72.6
63 32.0 26.1 39.1


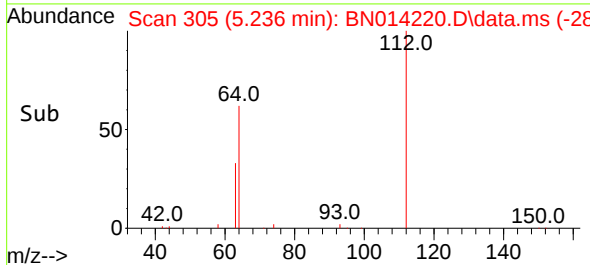

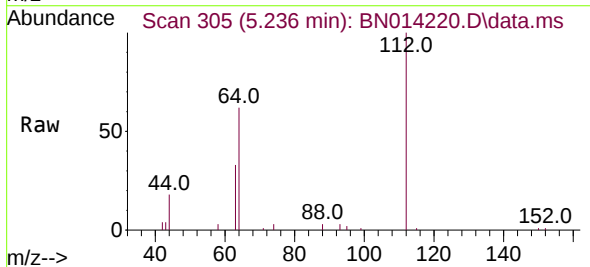


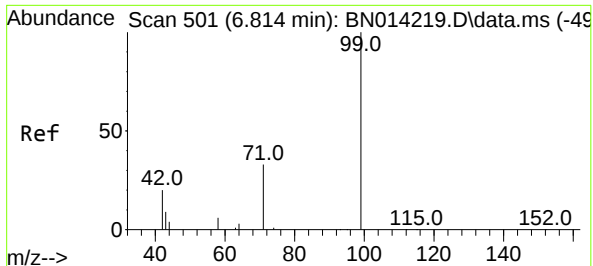

#5
Phenol-d6
Concen: 0.78 ng
RT: 6.814 min Scan# 501
Delta R.T. -0.000 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion: 99 Resp: 18615
Ion Ratio Lower Upper
99 100
42 21.9 17.9 26.9
71 33.8 27.0 40.6

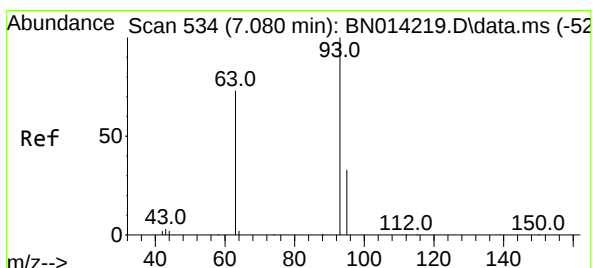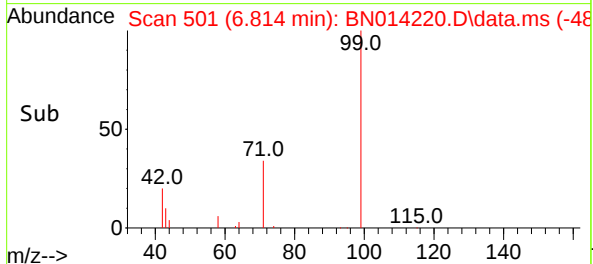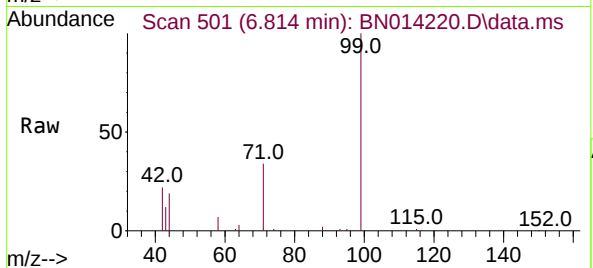

#6
bis(2-Chloroethyl)ether
Concen: 0.78 ng
RT: 7.080 min Scan# 534
Delta R.T. -0.000 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion: 93 Resp: 16223
Ion Ratio Lower Upper
93 100
63 81.5 65.3 97.9
95 32.9 26.3 39.5


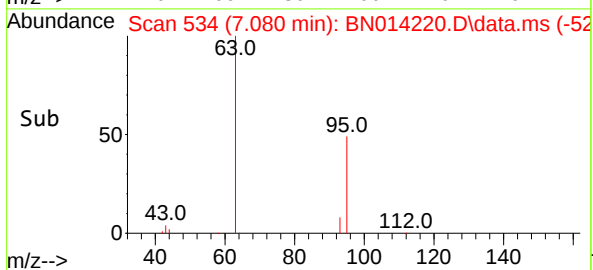

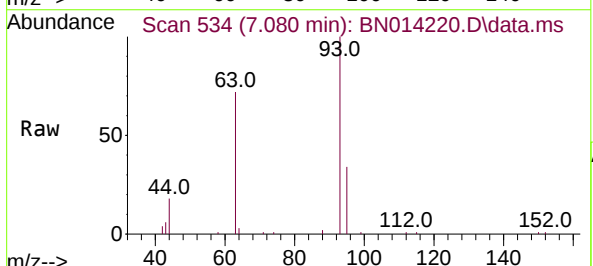




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.416 min Scan# 853
Delta R.T. -0.000 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:	136	Resp:	28206
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.9	13.3
54	11.0	8.4	12.6
68	7.7	5.8	8.8

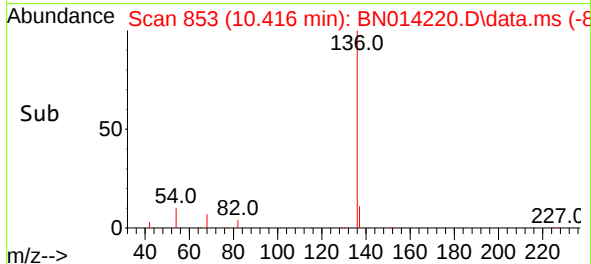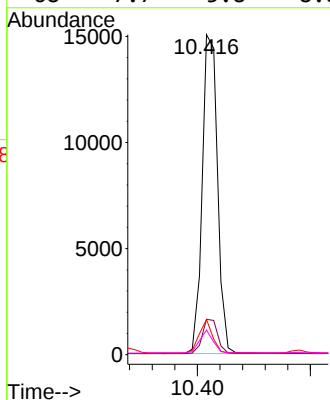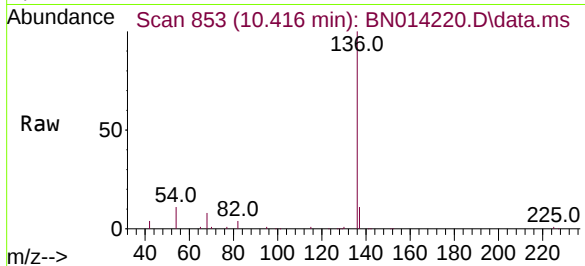

#8
Nitrobenzene-d5
Concen: 0.80 ng
RT: 8.794 min Scan# 725
Delta R.T. -0.000 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:	82	Resp:	16469
Ion	Ratio	Lower	Upper
82	100		
128	44.6	36.1	54.1
54	48.0	39.1	58.7


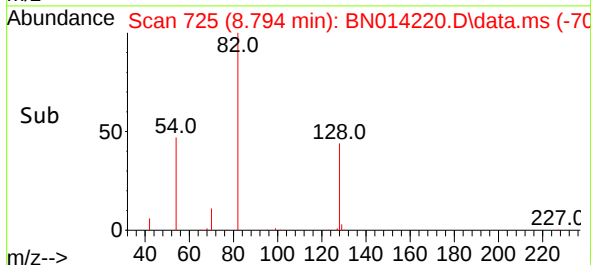
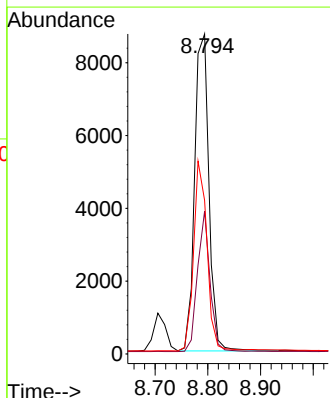
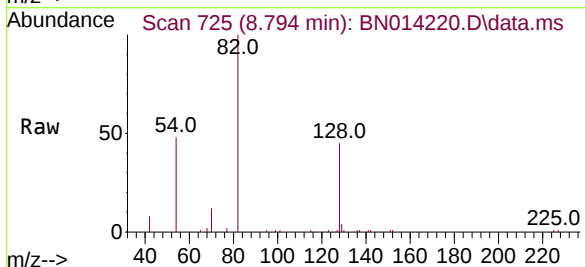


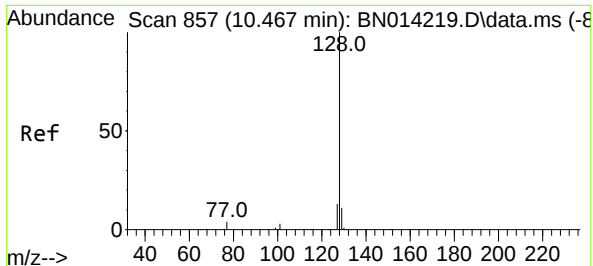

#9
Naphthalene
Concen: 0.76 ng
RT: 10.467 min Scan# 857
Delta R.T. -0.000 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:	128	Resp:	57472
Ion Ratio	Lower	Upper	
128	100		
129	10.8	8.9	13.3
127	13.2	10.6	16.0

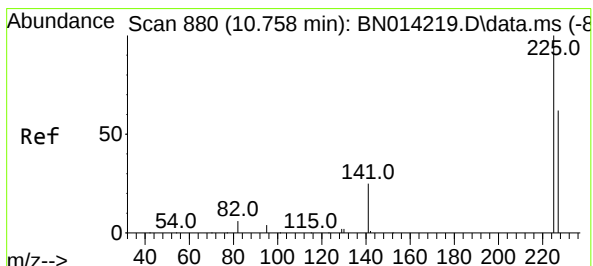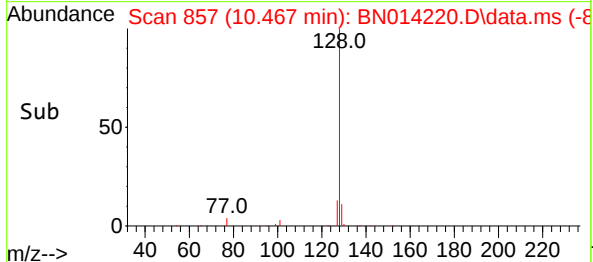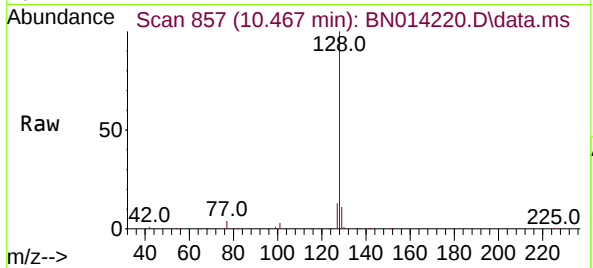

#10
Hexachlorobutadiene
Concen: 0.77 ng
RT: 10.758 min Scan# 880
Delta R.T. -0.000 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:	225	Resp:	10646
Ion Ratio	Lower	Upper	
225	100		
223	0.0	0.0	0.0
227	63.3	50.6	75.8


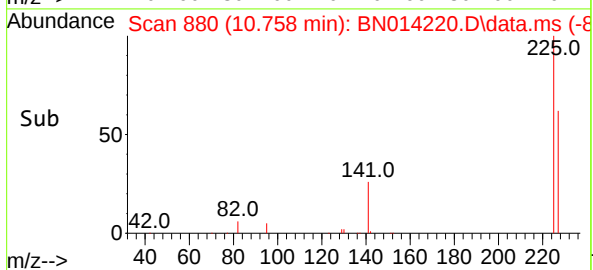

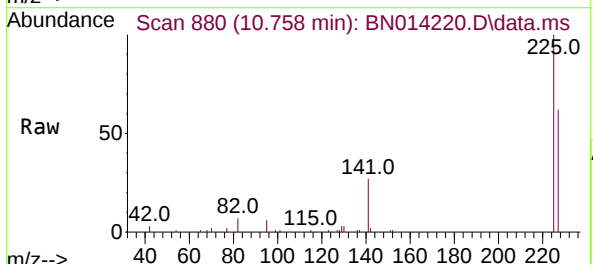




#11
2-Methylnaphthalene-d10
Concen: 0.59 ng
RT: 12.017 min Scan# 1054
Delta R.T. -0.000 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:152 Resp: 37413
Ion Ratio Lower Upper
152 100
151 20.1 16.2 24.2

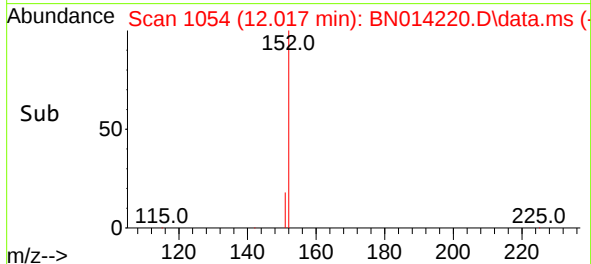

#12
2-Methylnaphthalene
Concen: 0.76 ng
RT: 12.093 min Scan# 1071
Delta R.T. 0.004 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:142 Resp: 40413
Ion Ratio Lower Upper
142 100
141 87.3 71.4 107.2
115 34.5 29.1 43.7


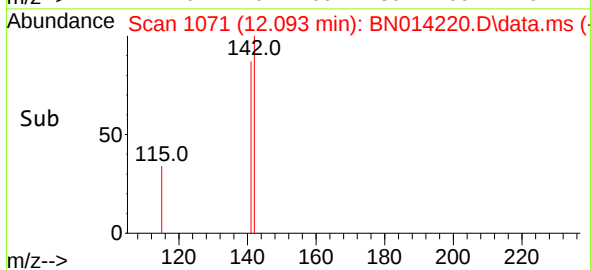

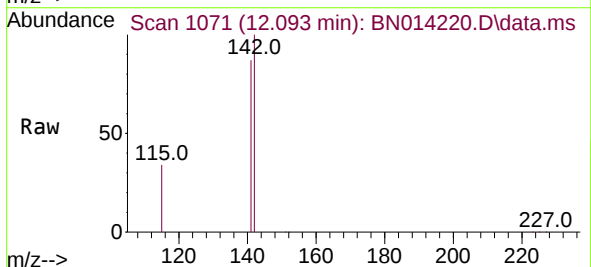


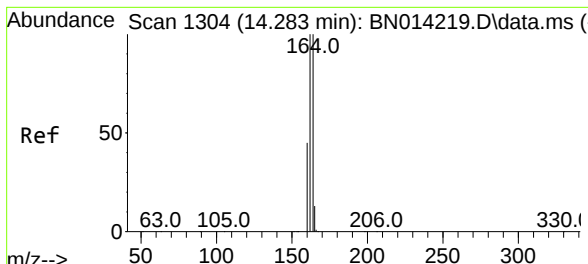

#13
 Acenaphthene-d10
 Concen: 0.40 ng
 RT: 14.283 min Scan# 1304
 Delta R.T. -0.000 min
 Lab File: BN014220.D
 Acq: 06 Apr 2021 11:54




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.8


Tgt Ion:	164	Resp:	17243
Ion Ratio	Lower	Upper	
164	100		
162	103.3	80.4	120.6
160	47.1	36.0	54.0

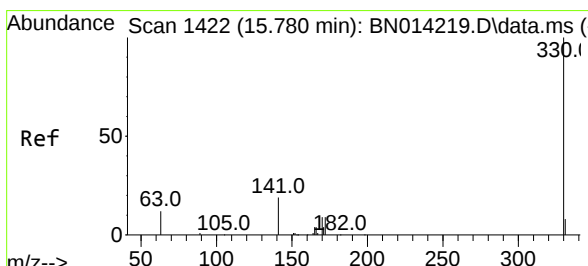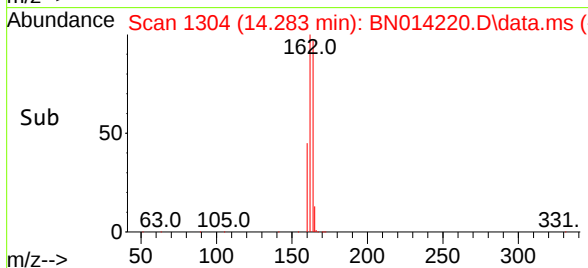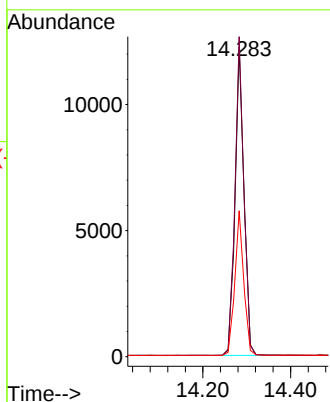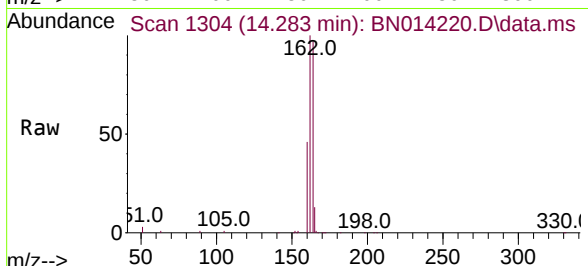

#14
 2,4,6-Tribromophenol
 Concen: 0.79 ng
 RT: 15.780 min Scan# 1422
 Delta R.T. -0.000 min
 Lab File: BN014220.D
 Acq: 06 Apr 2021 11:54

Tgt Ion:	330	Resp:	5188
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	38.1	30.6	45.8


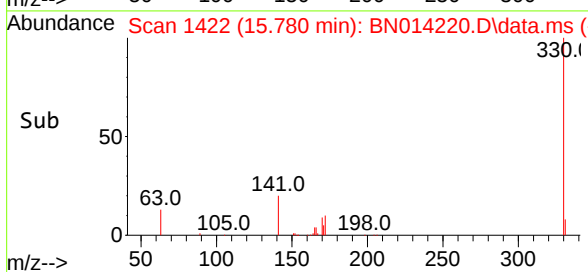
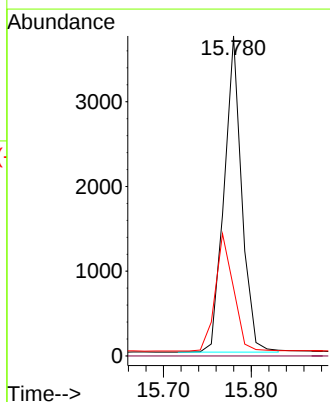
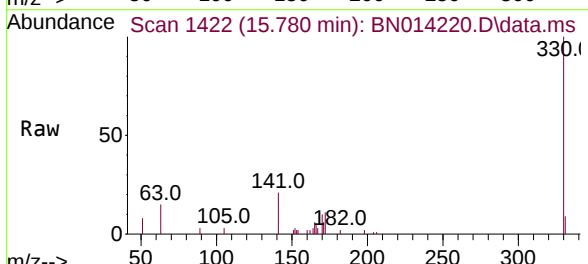




#15
2-Fluorobiphenyl
Concen: 0.84 ng
RT: 12.900 min Scan# 1195
Delta R.T. -0.000 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampled :
SSTDICC0.8


Tgt Ion:172 Resp: 53595
Ion Ratio Lower Upper
172 100
171 34.8 27.8 41.6
170 23.6 18.7 28.1

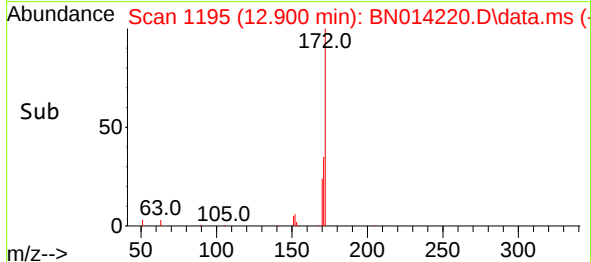

#16
Acenaphthylene
Concen: 0.78 ng
RT: 14.004 min Scan# 1282
Delta R.T. -0.000 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:152 Resp: 55353
Ion Ratio Lower Upper
152 100
151 19.2 15.5 23.3
153 13.0 10.5 15.7


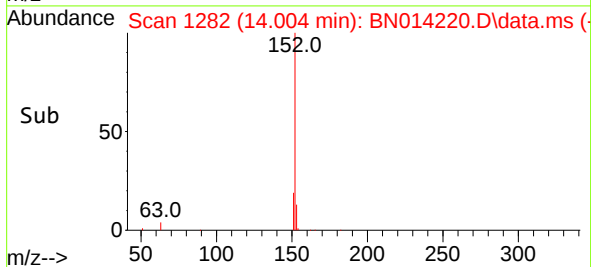

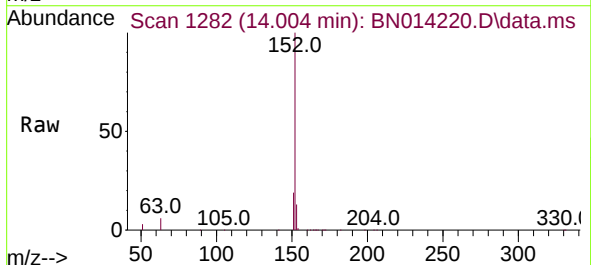




#17
Acenaphthene
Concen: 0.78 ng
RT: 14.346 min Scan# 1309
Delta R.T. -0.000 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:154 Resp: 39490
Ion Ratio Lower Upper
154 100
153 109.8 88.8 133.2
152 53.1 43.8 65.6

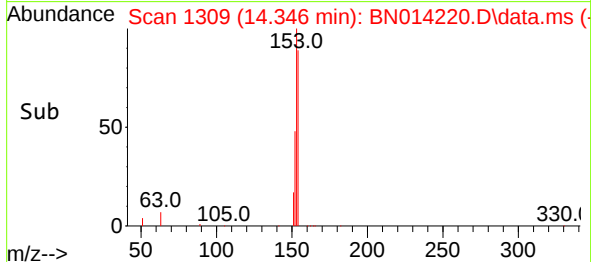

#18
Fluorene
Concen: 0.79 ng
RT: 15.336 min Scan# 1387
Delta R.T. -0.000 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:166 Resp: 50853
Ion Ratio Lower Upper
166 100
165 97.7 78.6 118.0
167 13.4 10.7 16.1


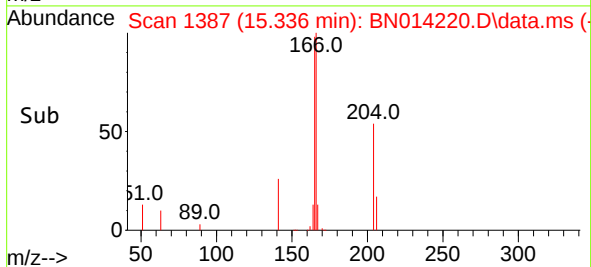

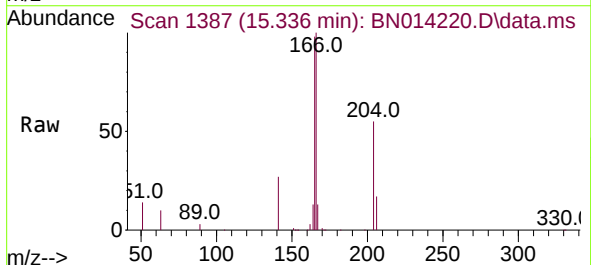




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.030 min Scan# 1524
Delta R.T. -0.001 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:188 Resp: 38561
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.5 6.2 9.2

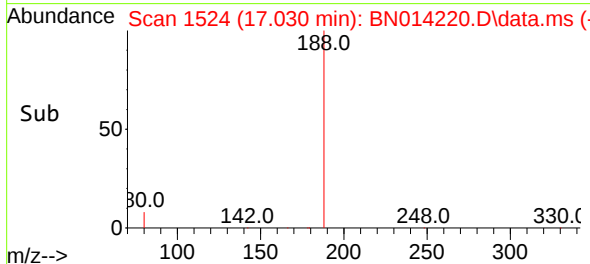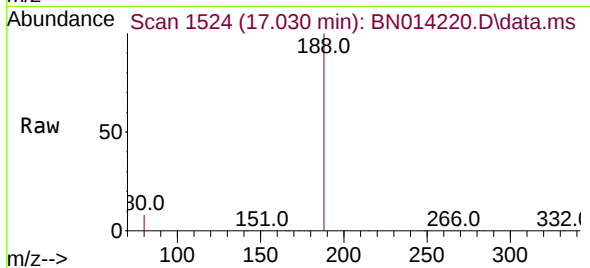

#20
4,6-Dinitro-2-methylphenol
Concen: 0.71 ng
RT: 15.412 min Scan# 1393
Delta R.T. -0.000 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:198 Resp: 4104
Ion Ratio Lower Upper
198 100
51 51.4 46.3 69.5
105 43.4 35.5 53.3


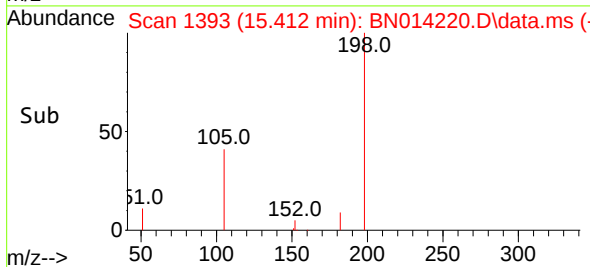

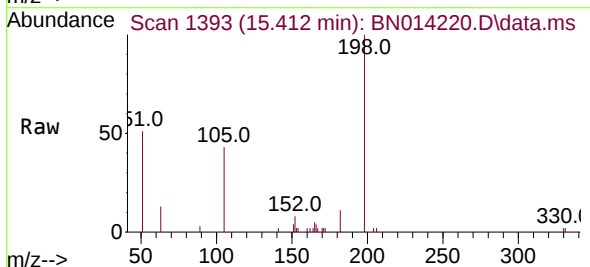




#21
4-Bromophenyl-phenylether
Concen: 0.76 ng
RT: 16.227 min Scan# 1458
Delta R.T. -0.001 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:248 Resp: 16551
Ion Ratio Lower Upper
248 100
250 93.9 76.1 114.1
141 62.4 45.5 68.3

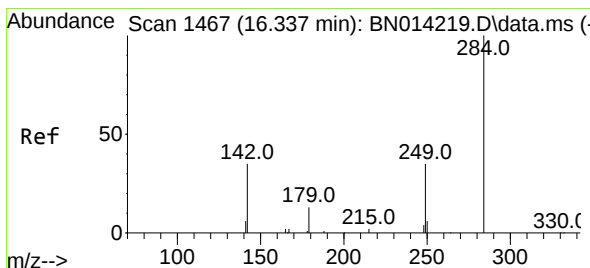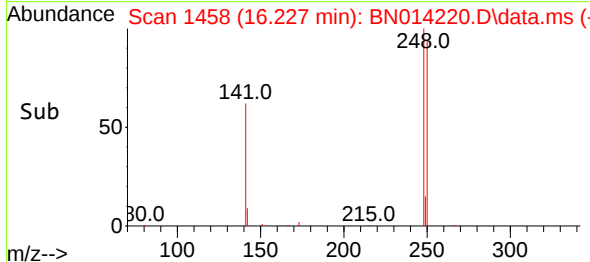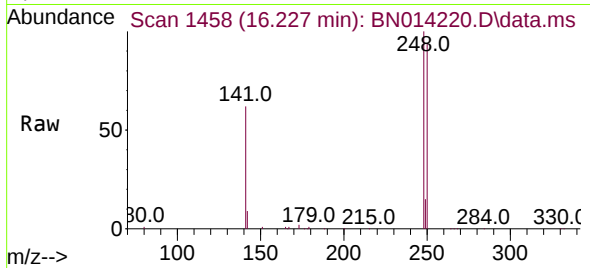

#22
Hexachlorobenzene
Concen: 0.75 ng
RT: 16.337 min Scan# 1467
Delta R.T. -0.001 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:284 Resp: 17854
Ion Ratio Lower Upper
284 100
142 36.3 28.9 43.3
249 31.3 25.0 37.4


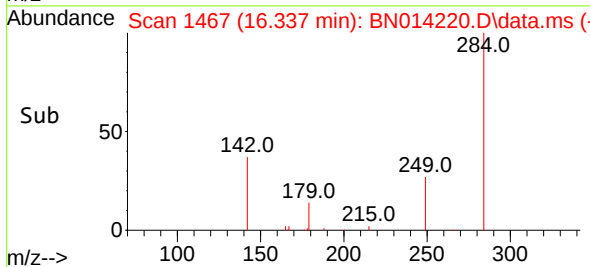

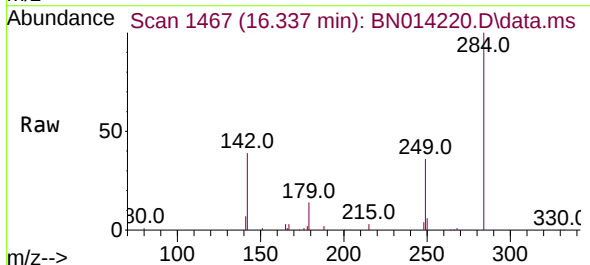




#23
Atrazine
Concen: 0.79 ng
RT: 16.495 min Scan# 1480
Delta R.T. -0.001 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:200 Resp: 11887
Ion Ratio Lower Upper
200 100
173 28.3 21.9 32.9
215 47.1 38.1 57.1

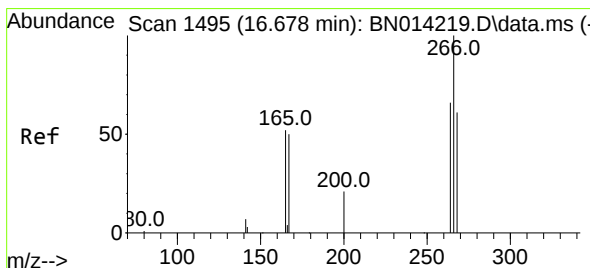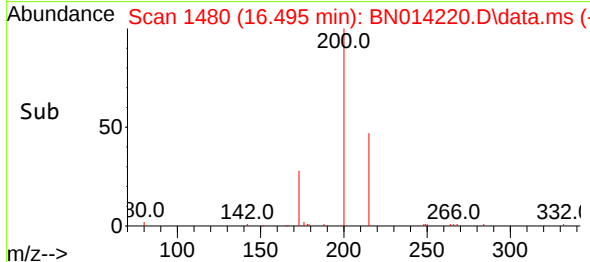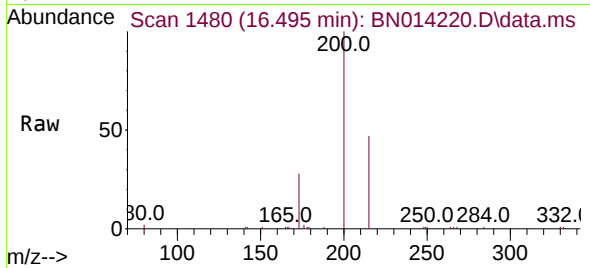

#24
Pentachlorophenol
Concen: 0.71 ng
RT: 16.690 min Scan# 1496
Delta R.T. 0.012 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:266 Resp: 4547
Ion Ratio Lower Upper
266 100
264 62.5 48.8 73.2
268 63.6 48.8 73.2


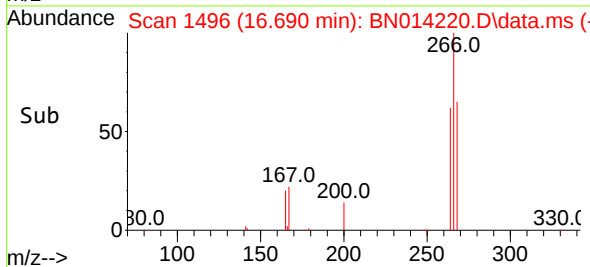

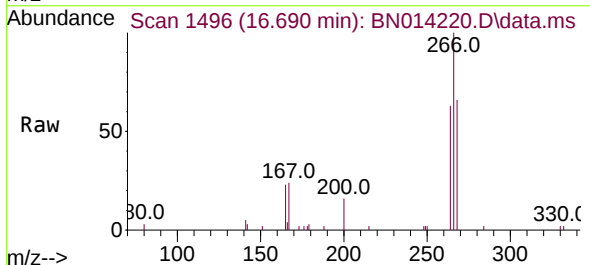




#25
Phenanthrene
Concen: 0.76 ng
RT: 17.067 min Scan# 1527
Delta R.T. -0.001 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:178 Resp: 85605
Ion Ratio Lower Upper
178 100
176 18.8 15.0 22.6
179 15.3 12.2 18.4

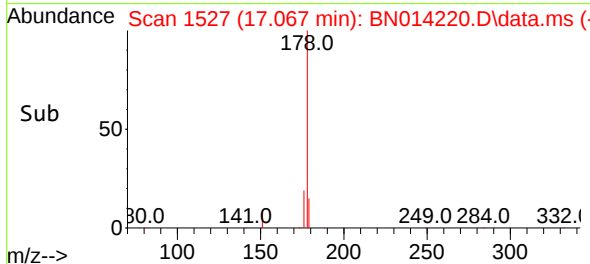

#26
Anthracene
Concen: 0.75 ng
RT: 17.164 min Scan# 1535
Delta R.T. -0.001 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:178 Resp: 72139
Ion Ratio Lower Upper
178 100
176 18.3 14.6 21.8
179 15.3 12.3 18.5


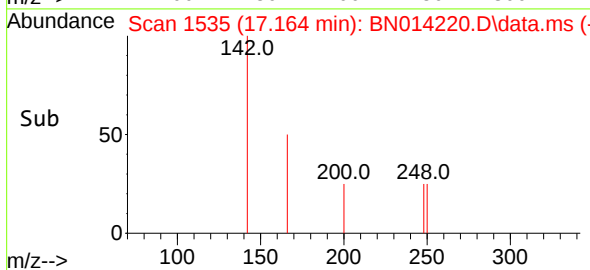

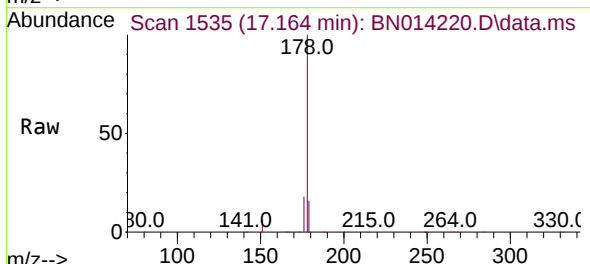




#27
Fluoranthene-d10
Concen: 0.58 ng
RT: 19.066 min Scan# 1818
Delta R.T. 0.002 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:212 Resp: 88338
Ion Ratio Lower Upper
212 100
106 12.6 10.1 15.1
104 7.1 5.6 8.4

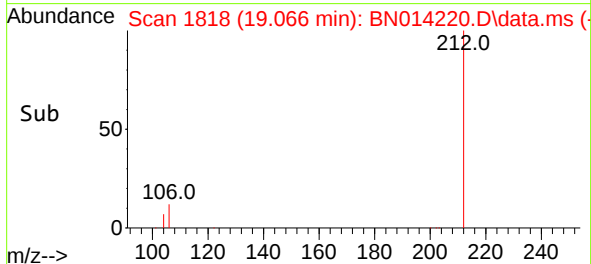

#28
Fluoranthene
Concen: 0.75 ng
RT: 19.096 min Scan# 1824
Delta R.T. 0.002 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:202 Resp: 98772
Ion Ratio Lower Upper
202 100
101 10.8 8.6 13.0
203 17.3 13.8 20.6


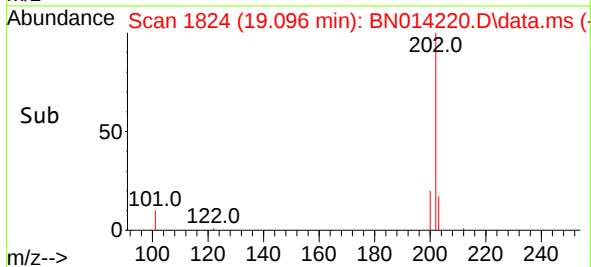

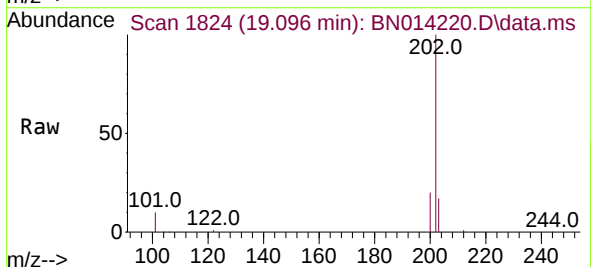




#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.226 min Scan# 2122
Delta R.T. 0.008 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:240 Resp: 39135
Ion Ratio Lower Upper
240 100
120 6.1 10.8 16.2#
236 25.6 21.4 32.2

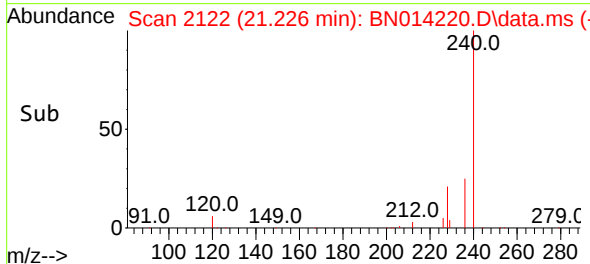

#30
Pyrene
Concen: 0.77 ng
RT: 19.459 min Scan# 1897
Delta R.T. -0.003 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:202 Resp: 97271
Ion Ratio Lower Upper
202 100
200 20.4 16.3 24.5
203 17.4 13.9 20.9


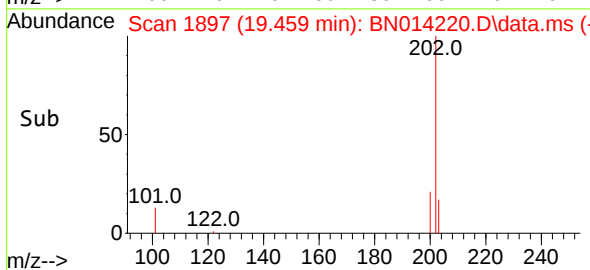

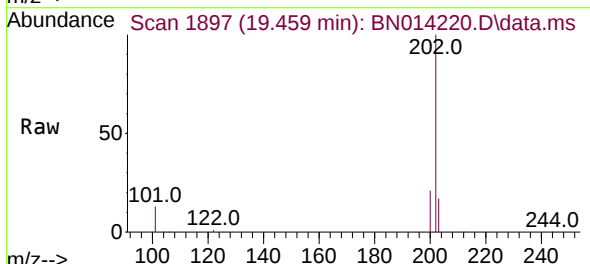




#31
Terphenyl-d14
Concen: 0.82 ng
RT: 19.672 min Scan# 1940
Delta R.T. 0.002 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:244 Resp: 74214
Ion Ratio Lower Upper
244 100
212 7.3 5.9 8.9
122 10.6 9.2 13.8

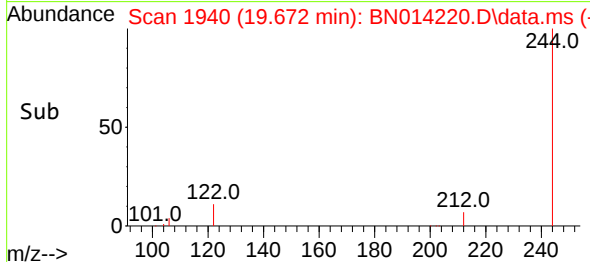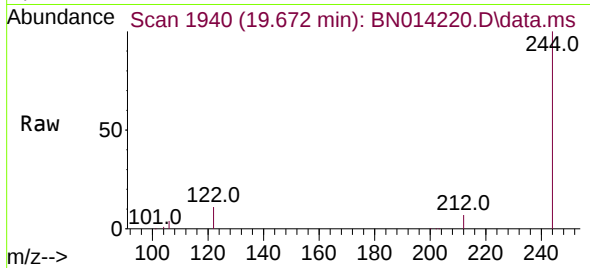

#32
Benzo(a)anthracene
Concen: 0.75 ng
RT: 21.205 min Scan# 2120
Delta R.T. -0.003 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:228 Resp: 90357
Ion Ratio Lower Upper
228 100
226 27.0 21.1 31.7
229 19.3 15.8 23.8


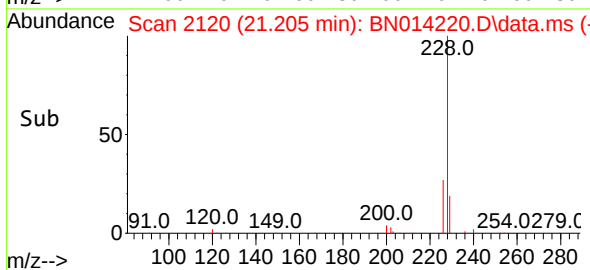

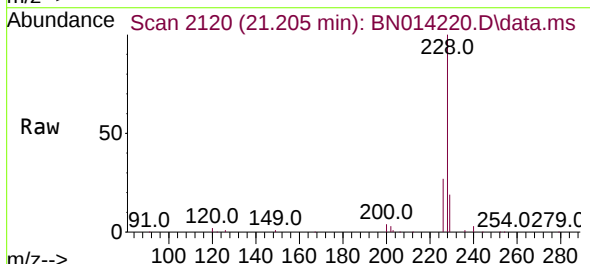


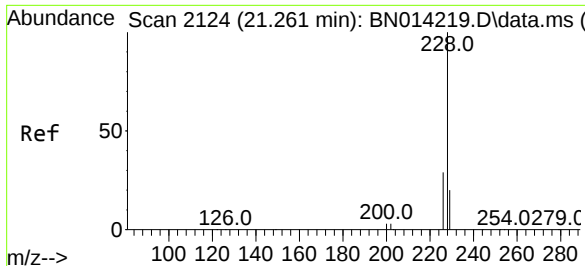

#33
Chrysene
Concen: 0.74 ng
RT: 21.258 min Scan# 2125
Delta R.T. -0.003 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:228	Resp:	98696
Ion Ratio	Lower	Upper
228	100	
226	29.4	23.0 34.6
229	19.3	15.8 23.8

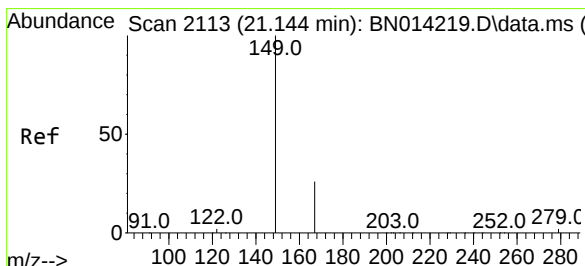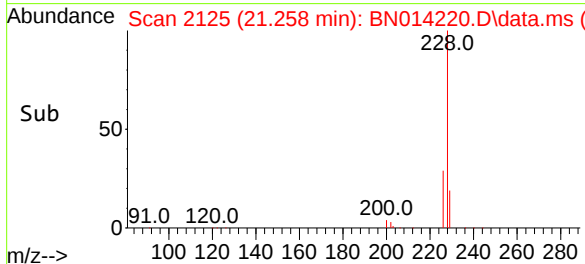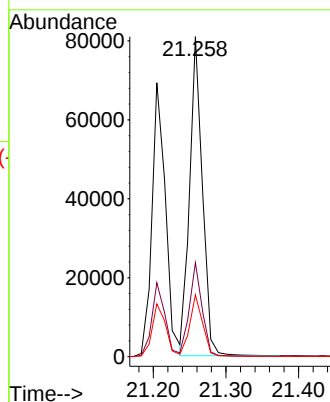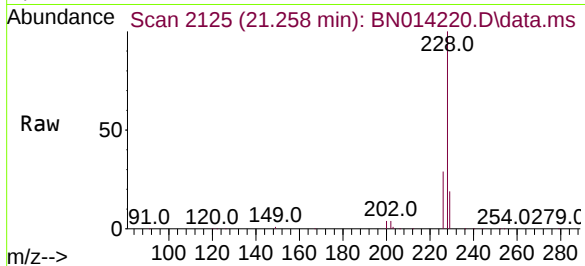

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.65 ng
RT: 21.152 min Scan# 2115
Delta R.T. 0.008 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:149	Resp:	26955
Ion Ratio	Lower	Upper
149	100	
167	27.1	21.4 32.0
279	3.8	3.1 4.7


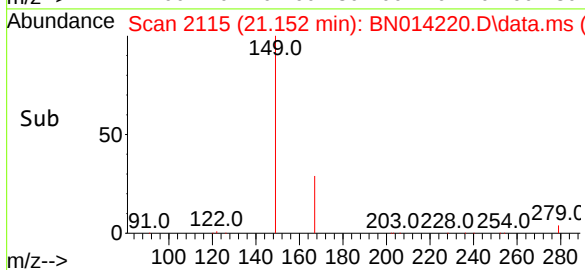
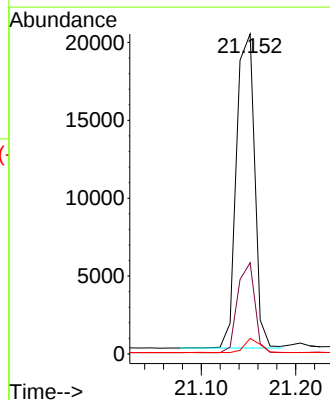
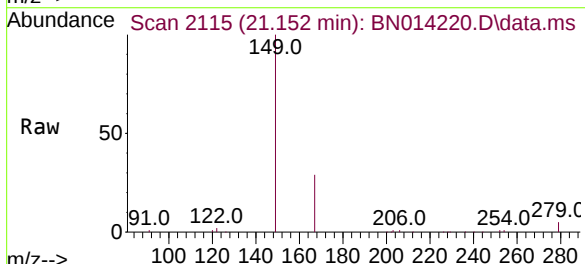




#35
Indeno(1,2,3-cd)pyrene
Concen: 0.59 ng
RT: 25.636 min Scan# 3177
Delta R.T. 0.004 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:	276	Resp:	95271
Ion Ratio	Lower	Upper	
276	100		
138	23.4	18.6	27.8
277	24.8	19.8	29.8

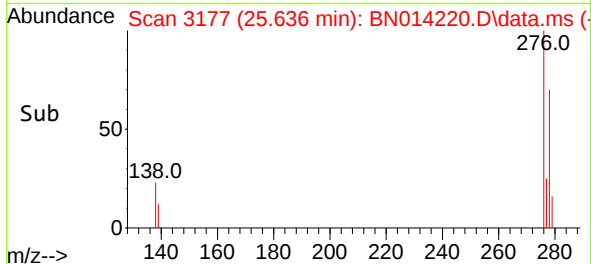

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.428 min Scan# 2532
Delta R.T. 0.001 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:	264	Resp:	33804
Ion Ratio	Lower	Upper	
264	100		
260	24.3	19.7	29.5
265	25.0	19.2	28.8


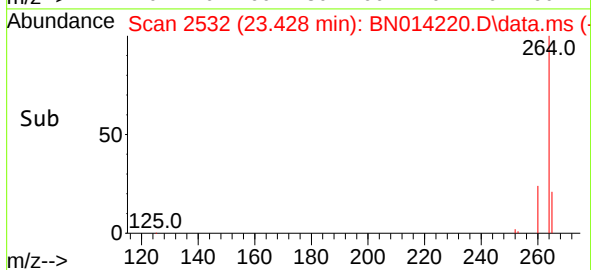

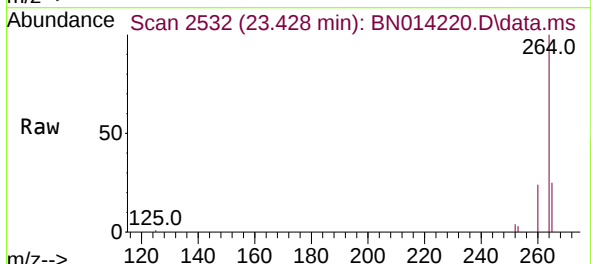




#37
Benzo(b)fluoranthene
Concen: 0.76 ng
RT: 22.768 min Scan# 2339
Delta R.T. 0.001 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8


Tgt Ion:252 Resp: 96433
Ion Ratio Lower Upper
252 100
253 22.5 18.5 27.7
125 10.2 10.3 15.5#

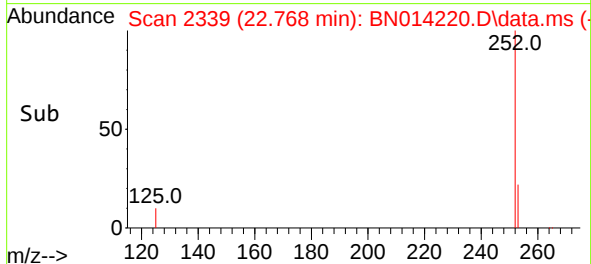

#38
Benzo(k)fluoranthene
Concen: 0.80 ng
RT: 22.812 min Scan# 2352
Delta R.T. 0.001 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:252 Resp: 98962
Ion Ratio Lower Upper
252 100
253 22.2 18.1 27.1
125 9.6 7.8 11.6


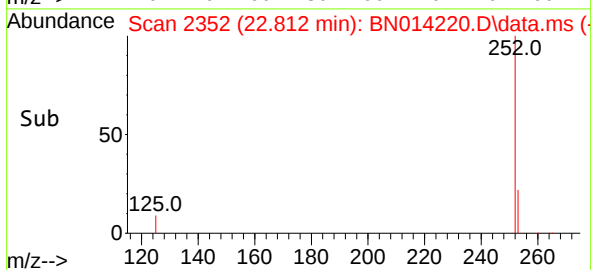

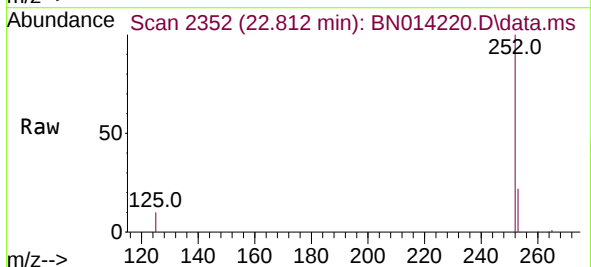




#39
Benzo(a)pyrene
Concen: 0.75 ng
RT: 23.332 min Scan# 2504
Delta R.T. 0.001 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.8


Tgt Ion:252 Resp: 84755
Ion Ratio Lower Upper
252 100
253 22.7 19.4 29.2
125 12.2 16.6 24.8#

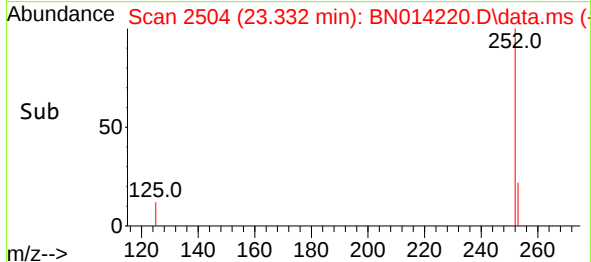

#40
Dibenzo(a,h)anthracene
Concen: 0.67 ng
RT: 25.650 min Scan# 3181
Delta R.T. 0.004 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Tgt Ion:278 Resp: 79362
Ion Ratio Lower Upper
278 100
139 15.6 12.6 19.0
279 24.0 19.4 29.0

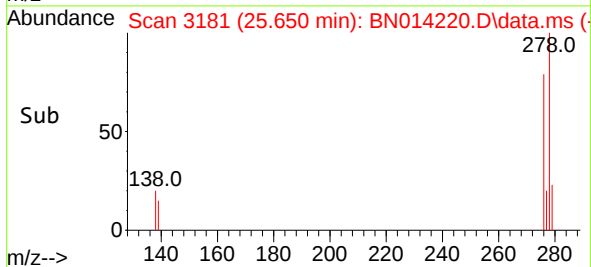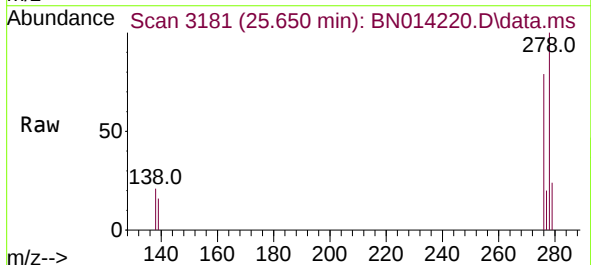

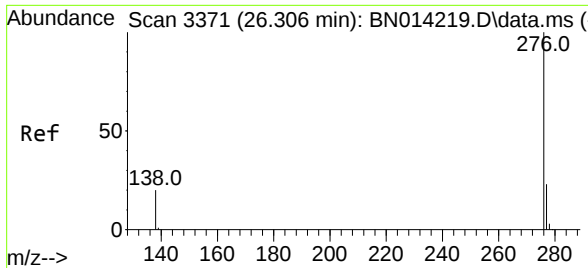

#41
Benzo(g,h,i)perylene
Concen: 0.67 ng
RT: 26.307 min Scan# 3373
Delta R.T. 0.001 min
Lab File: BN014220.D
Acq: 06 Apr 2021 11:54

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.8

Tgt Ion:	276	Resp:	80675
Ion Ratio	Lower	Upper	
276	100		
277	23.7	18.9	28.3
138	20.5	16.4	24.6

