

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040721\
 Data File : BN014221.D
 Acq On : 06 Apr 2021 12:30
 Operator : CG/JU
 Sample : SSTDICC1.6
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Quant Time: Apr 06 13:05:16 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 06 12:12:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.644	152	7419	0.40	ng	0.00
7) Naphthalene-d8	10.416	136	28455	0.40	ng	0.00
13) Acenaphthene-d10	14.283	164	17620	0.40	ng	0.00
19) Phenanthrene-d10	17.031	188	38615	0.40	ng	0.00
29) Chrysene-d12	21.218	240	41513	0.40	ng	0.00
36) Perylene-d12	23.428	264	36431	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.236	112	28445	1.53	ng	0.00
5) Phenol-d6	6.815	99	37775	1.55	ng	0.00
8) Nitrobenzene-d5	8.794	82	32469	1.57	ng	0.00
11) 2-Methylnaphthalene-d10	12.018	152	76296	1.18	ng	0.00
14) 2,4,6-Tribromophenol	15.780	330	11510	1.73	ng	0.00
15) 2-Fluorobiphenyl	12.900	172	101680	1.55	ng	0.00
27) Fluoranthene-d10	19.069	212	184454	1.21	ng	0.00
31) Terphenyl-d14	19.670	244	146741	1.53	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.166	88	14226	1.58	ng	95
3) n-Nitrosodimethylamine	3.488	42	12848	1.74	ng	# 93
6) bis(2-Chloroethyl)ether	7.072	93	32720	1.54	ng	100
9) Naphthalene	10.467	128	115562	1.51	ng	100
10) Hexachlorobutadiene	10.758	225	21122	1.51	ng	# 99
12) 2-Methylnaphthalene	12.093	142	82189	1.53	ng	97
16) Acenaphthylene	14.004	152	118801	1.64	ng	100
17) Acenaphthene	14.346	154	81715	1.58	ng	98
18) Fluorene	15.336	166	105787	1.61	ng	99
20) 4,6-Dinitro-2-methylph...	15.412	198	9700	1.67	ng	# 88
21) 4-Bromophenyl-phenylether	16.228	248	34021	1.55	ng	99
22) Hexachlorobenzene	16.337	284	36456	1.53	ng	99
23) Atrazine	16.496	200	25812	1.72	ng	98
24) Pentachlorophenol	16.690	266	11220	1.74	ng	98
25) Phenanthrene	17.068	178	172215	1.52	ng	100
26) Anthracene	17.165	178	152395	1.58	ng	100
28) Fluoranthene	19.094	202	204148	1.55	ng	100
30) Pyrene	19.461	202	202143	1.51	ng	100
32) Benzo(a)anthracene	21.208	228	196500	1.53	ng	100
33) Chrysene	21.261	228	210560	1.48	ng	100
34) Bis(2-ethylhexyl)phtha...	21.144	149	65910	1.49	ng	100
35) Indeno(1,2,3-cd)pyrene	25.635	276	222493	1.30	ng	100
37) Benzo(b)fluoranthene	22.767	252	213682	1.57	ng	# 96
38) Benzo(k)fluoranthene	22.812	252	208165	1.56	ng	99
39) Benzo(a)pyrene	23.332	252	188507	1.55	ng	# 89
40) Dibenzo(a,h)anthracene	25.646	278	186140	1.46	ng	99
41) Benzo(g,h,i)perylene	26.306	276	186086	1.42	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040721\
Data File : BN014221.D
Acq On : 06 Apr 2021 12:30
Operator : CG/JU
Sample : SSTDICC1.6
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6

Quant Time: Apr 06 13:05:16 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 06 12:12:15 2021
Response via : Initial Calibration




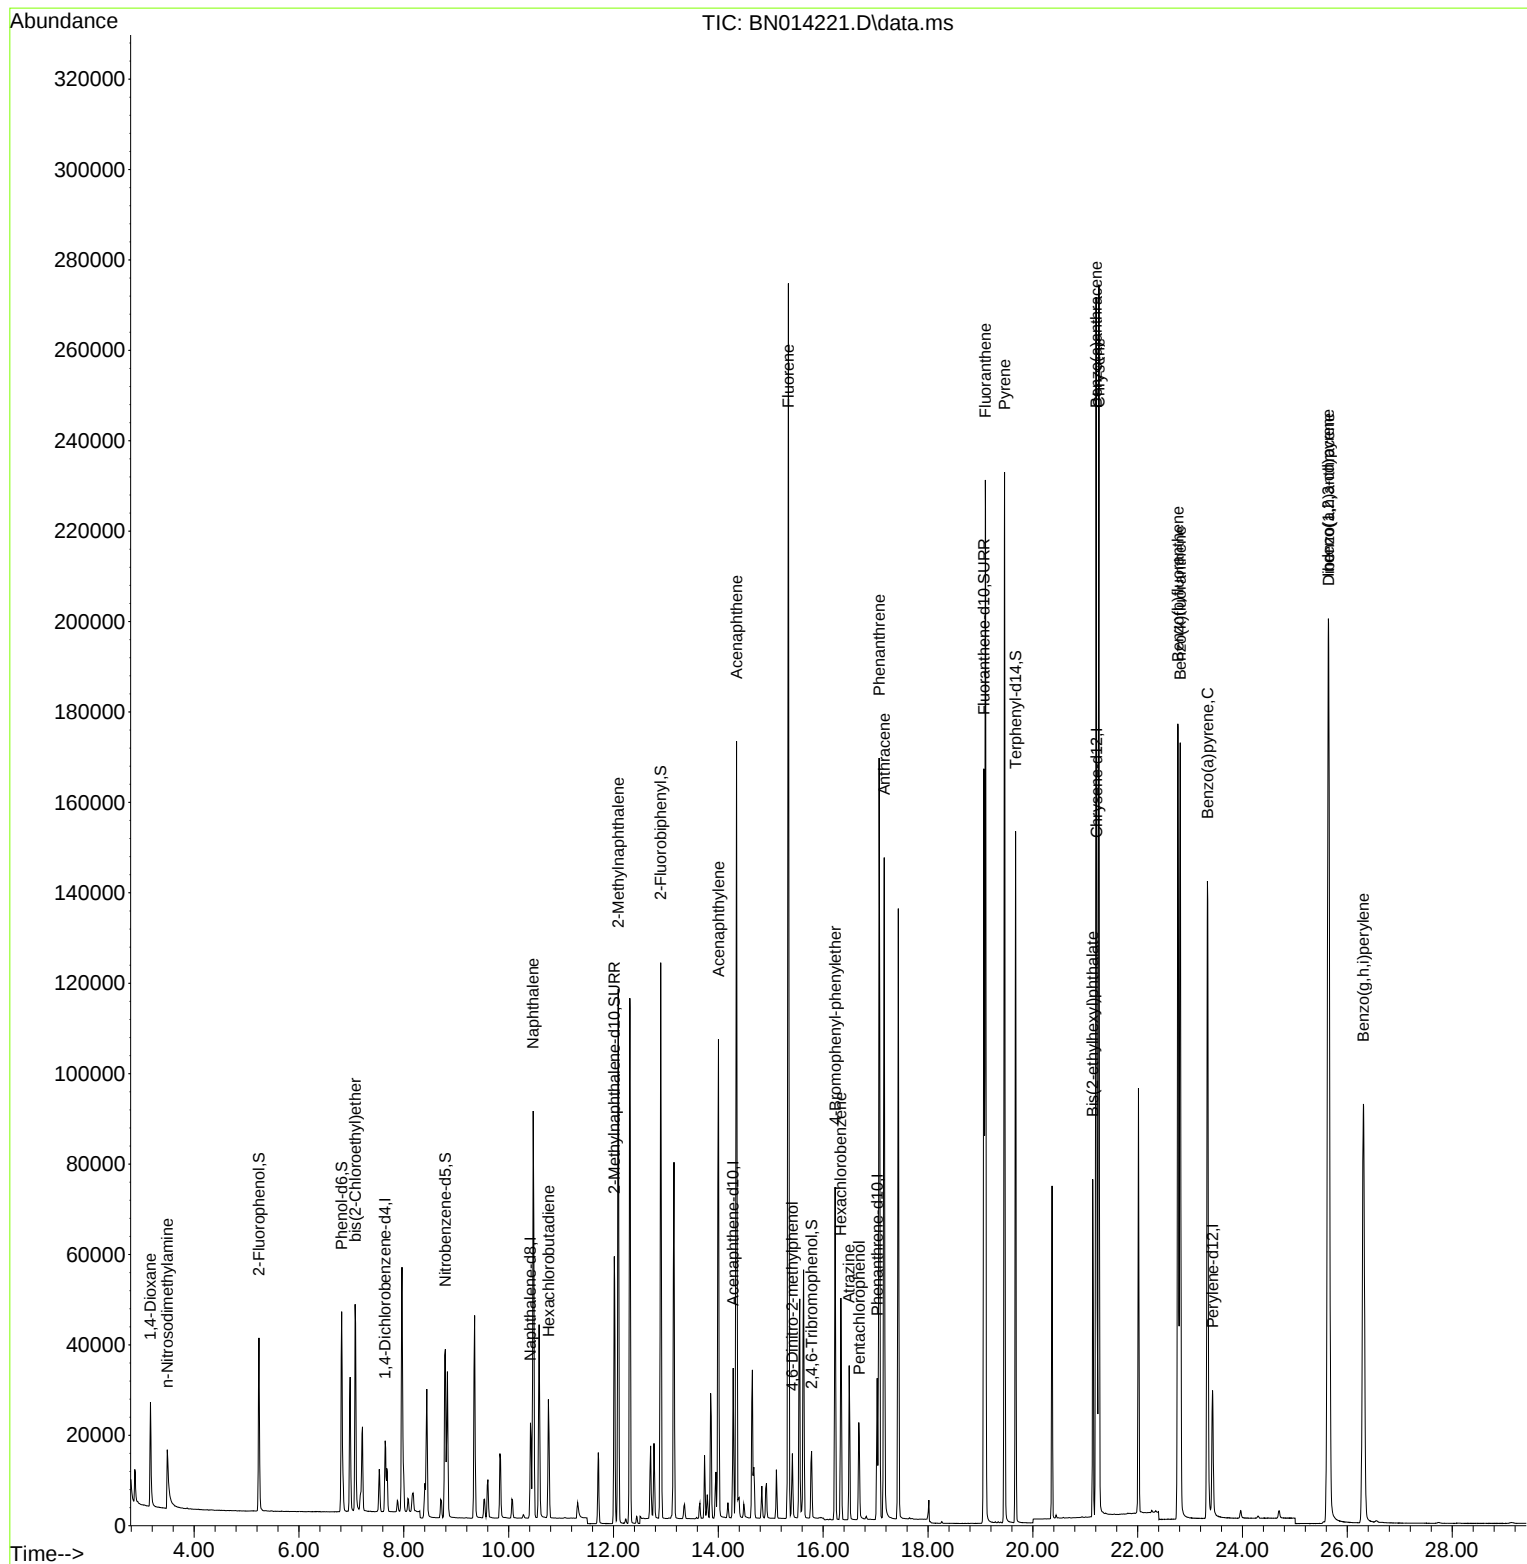


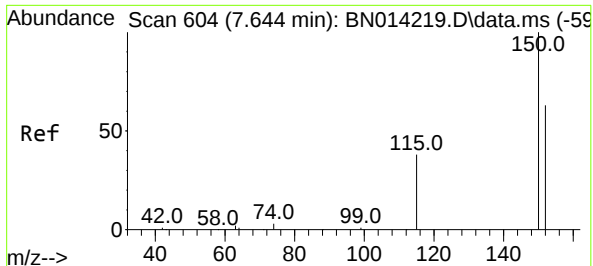

#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.644 min Scan# 604
 Delta R.T. 0.000 min
 Lab File: BN014221.D
 Acq: 06 Apr 2021 12:30




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6


Tgt Ion: 152 Resp: 7419
 Ion Ratio Lower Upper
 152 100
 150 157.9 126.2 189.2
 115 62.1 49.4 74.0

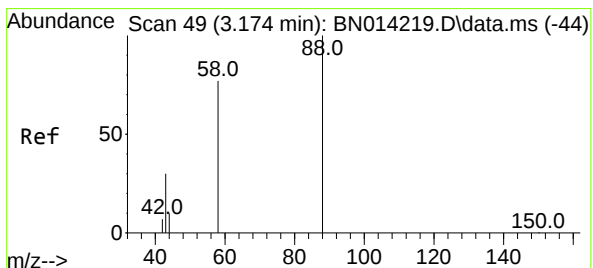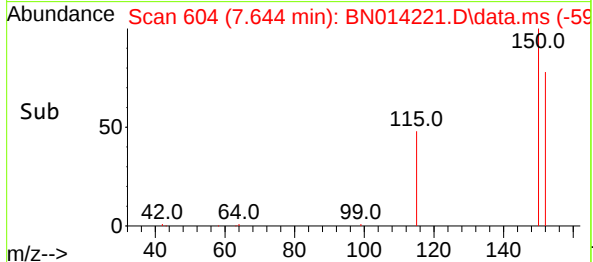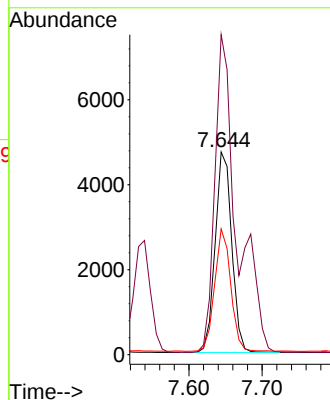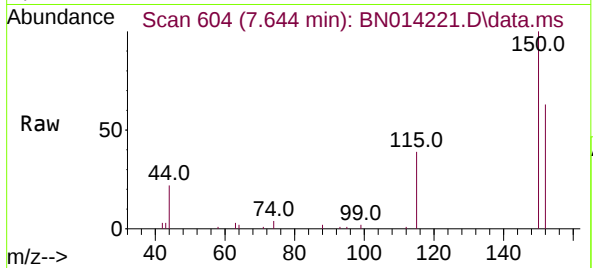

#2
 1,4-Dioxane
 Concen: 1.58 ng
 RT: 3.166 min Scan# 48
 Delta R.T. -0.008 min
 Lab File: BN014221.D
 Acq: 06 Apr 2021 12:30

Tgt Ion: 88 Resp: 14226
 Ion Ratio Lower Upper
 88 100
 58 81.4 70.0 105.0
 43 34.1 28.3 42.5


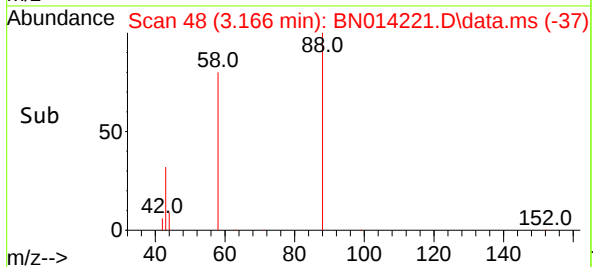
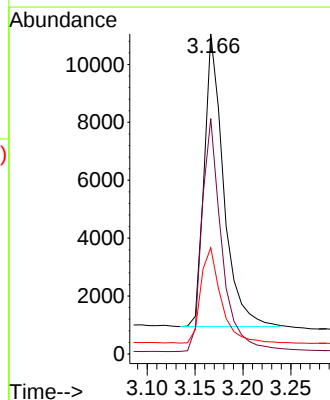
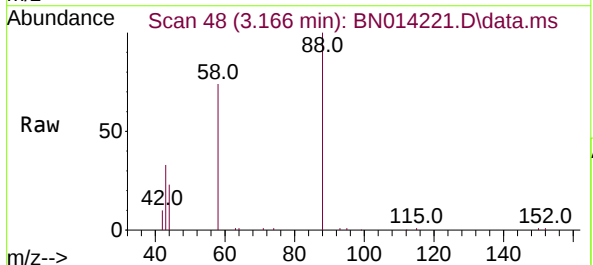


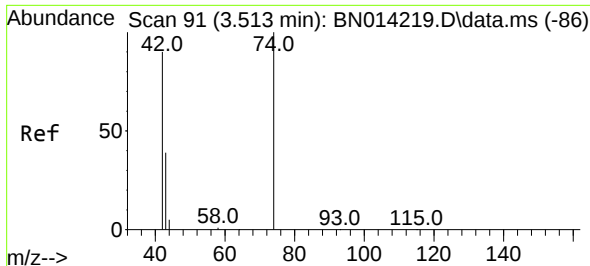

#3
n-Nitrosodimethylamine
Concen: 1.74 ng
RT: 3.488 min Scan# 88
Delta R.T. -0.024 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 42 Resp: 12848
Ion Ratio Lower Upper
42 100
74 112.5 85.0 127.6
44 6.9 9.4 14.0#

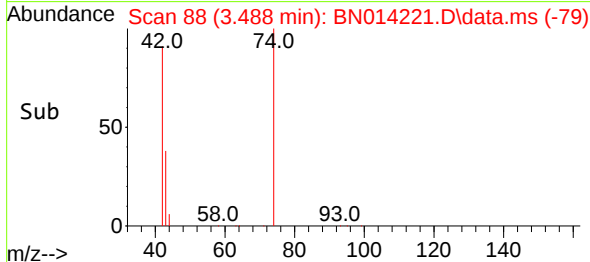

#4
2-Fluorophenol
Concen: 1.53 ng
RT: 5.236 min Scan# 305
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion: 112 Resp: 28445
Ion Ratio Lower Upper
112 100
64 60.9 48.4 72.6
63 32.1 26.1 39.1


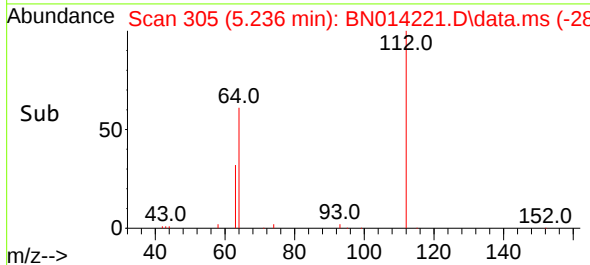

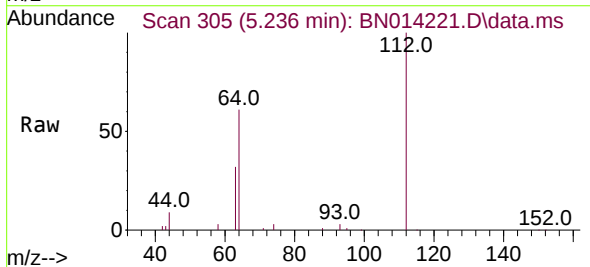


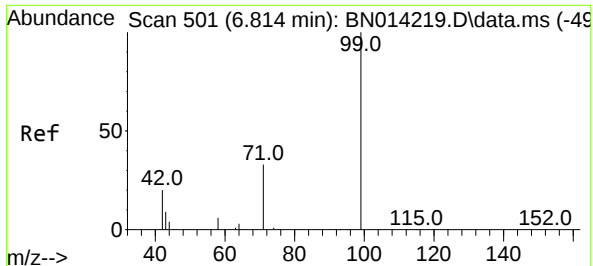

#5
Phenol-d6
Concen: 1.55 ng
RT: 6.815 min Scan# 501
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion: 99 Resp: 37775
Ion Ratio Lower Upper
99 100
42 22.2 17.9 26.9
71 33.7 27.0 40.6

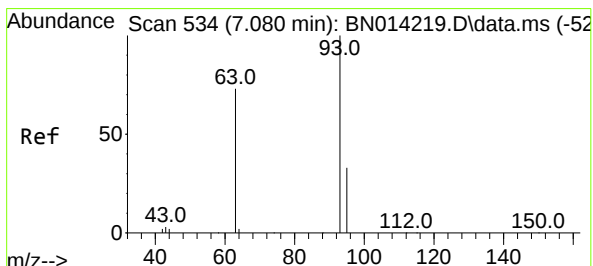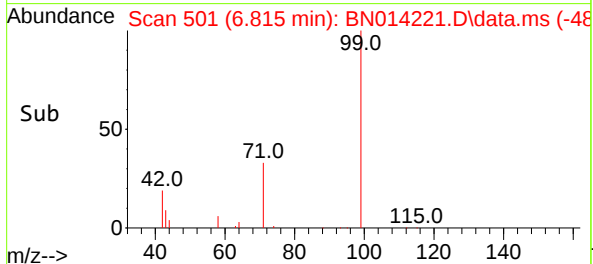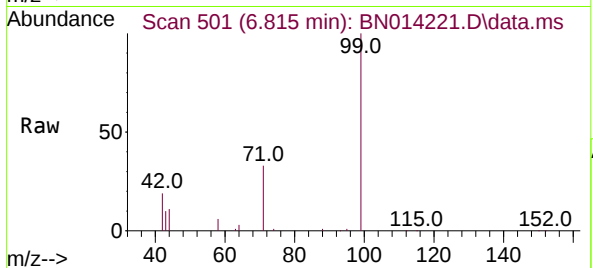

#6
bis(2-Chloroethyl)ether
Concen: 1.54 ng
RT: 7.072 min Scan# 533
Delta R.T. -0.008 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion: 93 Resp: 32720
Ion Ratio Lower Upper
93 100
63 81.6 65.3 97.9
95 32.8 26.3 39.5


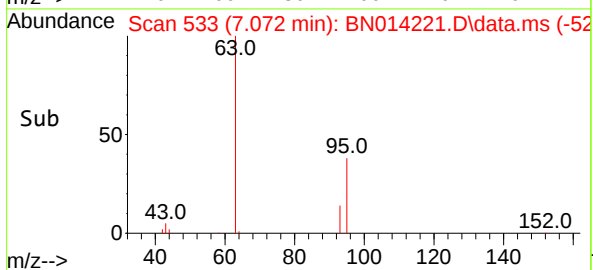

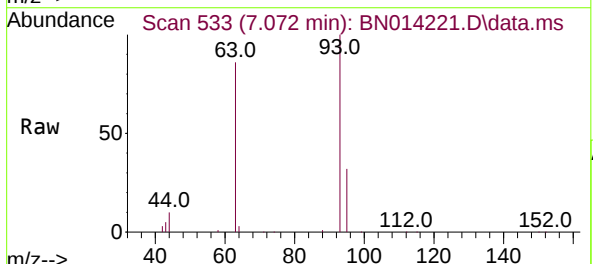




#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.416 min Scan# 853
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	136	Resp:	28455
Ion Ratio	Lower	Upper	
136	100		
137	11.2	8.9	13.3
54	10.7	8.4	12.6
68	7.6	5.8	8.8

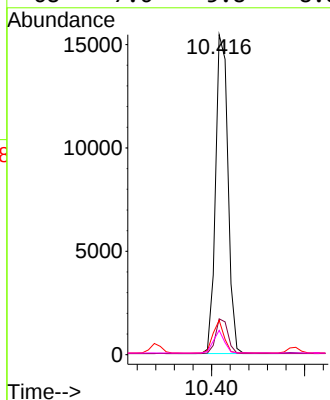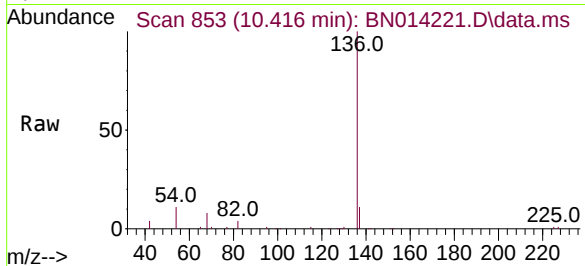

#8
Nitrobenzene-d5
Concen: 1.57 ng
RT: 8.794 min Scan# 725
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:	82	Resp:	32469
Ion Ratio	Lower	Upper	
82	100		
128	45.1	36.1	54.1
54	47.3	39.1	58.7


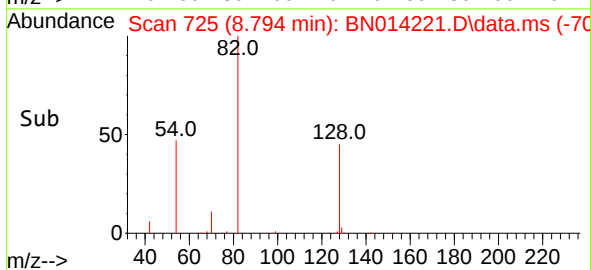
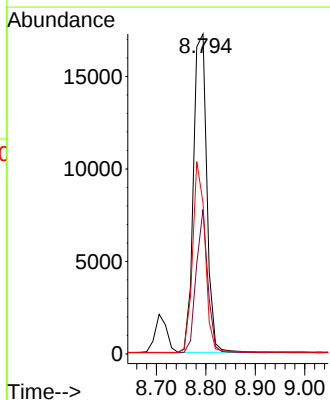
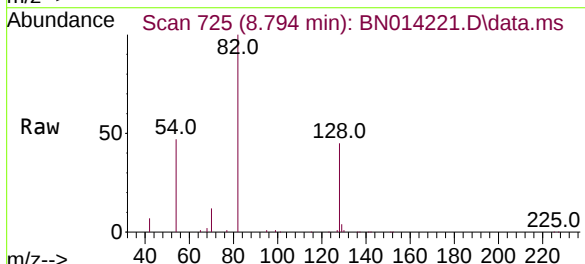




#9
Naphthalene
Concen: 1.51 ng
RT: 10.467 min Scan# 857
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:128 Resp: 115562
Ion Ratio Lower Upper
128 100
129 11.0 8.9 13.3
127 13.1 10.6 16.0



#10
Hexachlorobutadiene
Concen: 1.51 ng
RT: 10.758 min Scan# 880
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:225 Resp: 21122
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 63.7 50.6 75.8


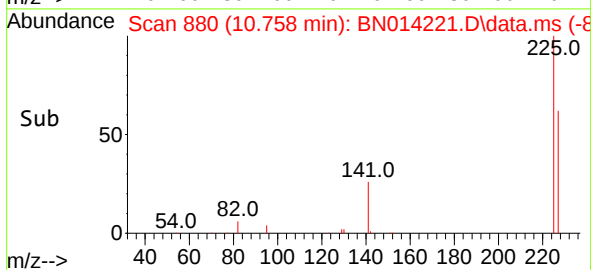






#11
2-Methylnaphthalene-d10
Concen: 1.18 ng
RT: 12.018 min Scan# 1054
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:152 Resp: 76296
Ion Ratio Lower Upper
152 100
151 20.1 16.2 24.2



#12
2-Methylnaphthalene
Concen: 1.53 ng
RT: 12.093 min Scan# 1071
Delta R.T. 0.004 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:142 Resp: 82189
Ion Ratio Lower Upper
142 100
141 86.4 71.4 107.2
115 34.0 29.1 43.7


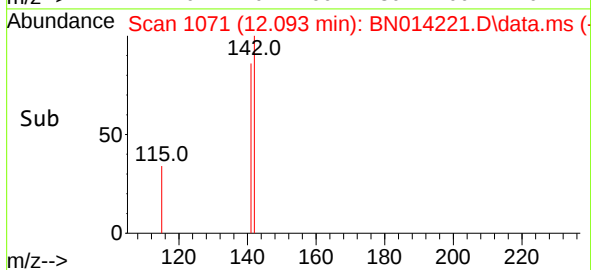

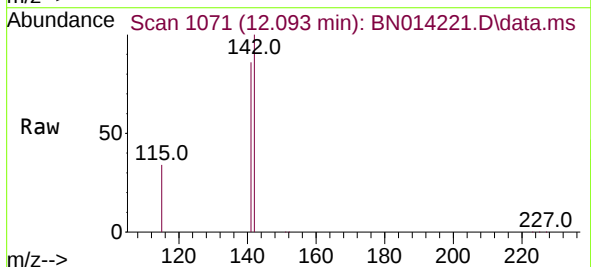


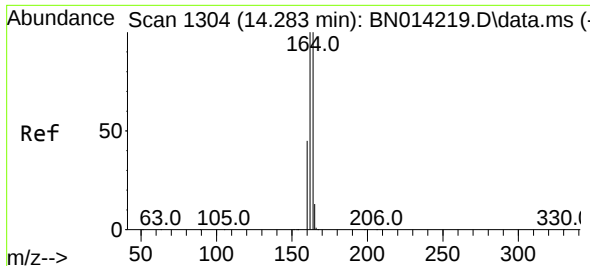

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.283 min Scan# 1304
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:164 Resp: 17620
Ion Ratio Lower Upper
164 100
162 102.6 80.4 120.6
160 46.5 36.0 54.0

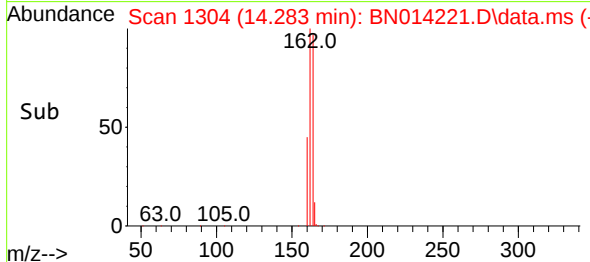

#14
2,4,6-Tribromophenol
Concen: 1.73 ng
RT: 15.780 min Scan# 1422
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:330 Resp: 11510
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 38.6 30.6 45.8


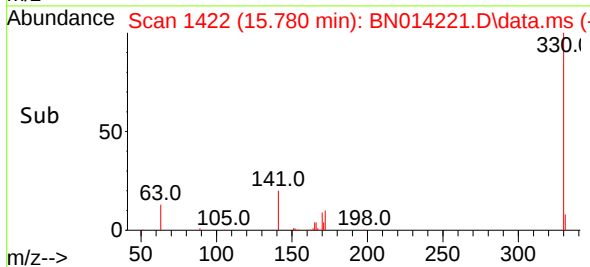

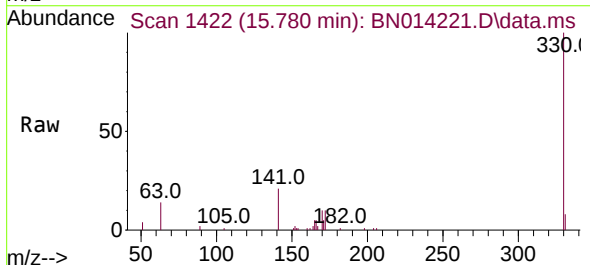




#15
2-Fluorobiphenyl
Concen: 1.55 ng
RT: 12.900 min Scan# 1195
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:172 Resp: 101680
Ion Ratio Lower Upper
172 100
171 34.7 27.8 41.6
170 23.4 18.7 28.1

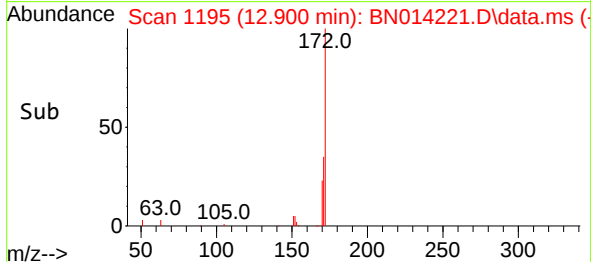

#16
Acenaphthylene
Concen: 1.64 ng
RT: 14.004 min Scan# 1282
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:152 Resp: 118801
Ion Ratio Lower Upper
152 100
151 19.1 15.5 23.3
153 13.0 10.5 15.7


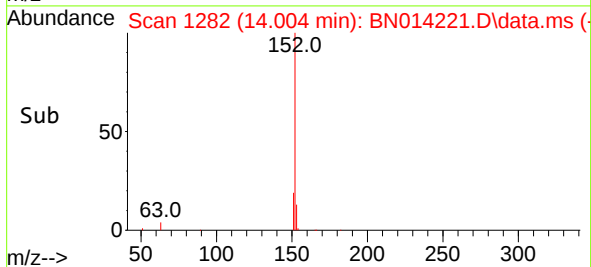

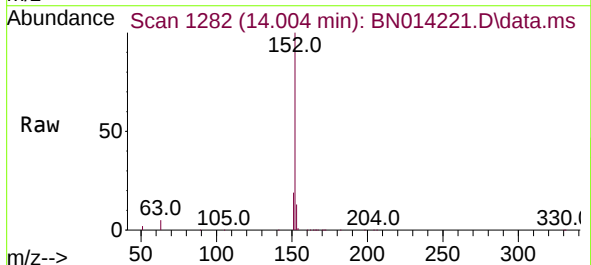




#17
Acenaphthene
Concen: 1.58 ng
RT: 14.346 min Scan# 1309
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:154 Resp: 81715
Ion Ratio Lower Upper
154 100
153 108.9 88.8 133.2
152 52.7 43.8 65.6

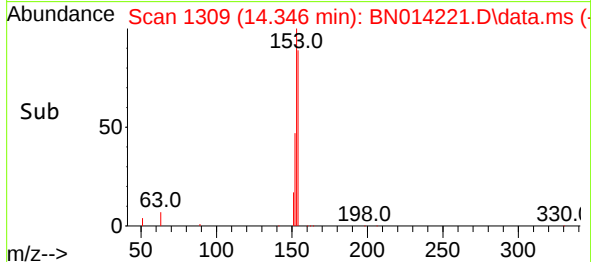

#18
Fluorene
Concen: 1.61 ng
RT: 15.336 min Scan# 1387
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:166 Resp: 105787
Ion Ratio Lower Upper
166 100
165 96.9 78.6 118.0
167 13.4 10.7 16.1


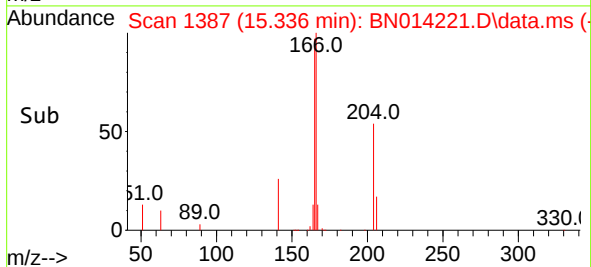

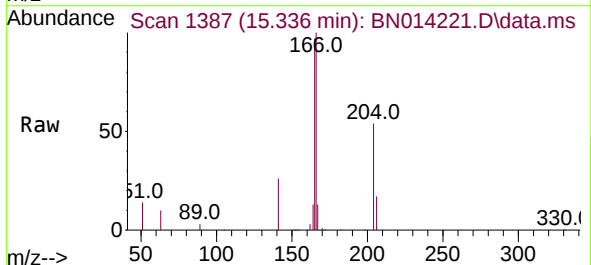




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.031 min Scan# 1524
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:188 Resp: 38615
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.5 6.2 9.2



#20
4,6-Dinitro-2-methylphenol
Concen: 1.67 ng
RT: 15.412 min Scan# 1393
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:198 Resp: 9700
Ion Ratio Lower Upper
198 100
51 45.0 46.3 69.5#
105 41.9 35.5 53.3


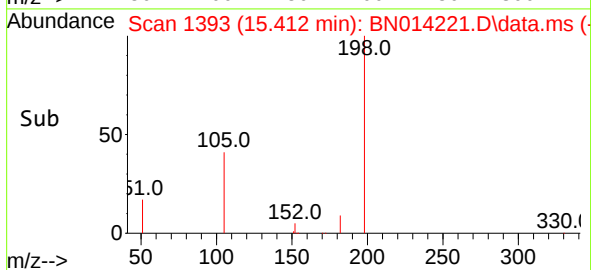






#21
4-Bromophenyl-phenylether
Concen: 1.55 ng
RT: 16.228 min Scan# 1458
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:	248	Resp:	34021
Ion Ratio	Lower	Upper	
248	100		
250	94.7	76.1	114.1
141	58.6	45.5	68.3



#22
Hexachlorobenzene
Concen: 1.53 ng
RT: 16.337 min Scan# 1467
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:	284	Resp:	36456
Ion Ratio	Lower	Upper	
284	100		
142	35.7	28.9	43.3
249	30.8	25.0	37.4


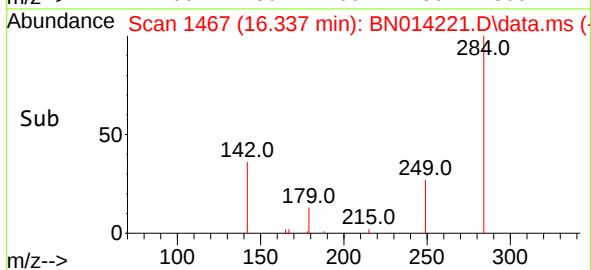




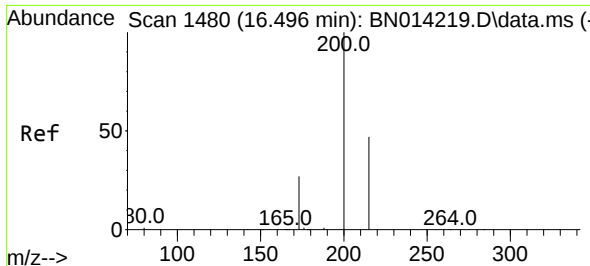

#23
Atrazine
Concen: 1.72 ng
RT: 16.496 min Scan# 1480
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:200 Resp: 25812
Ion Ratio Lower Upper
200 100
173 29.0 21.9 32.9
215 46.5 38.1 57.1

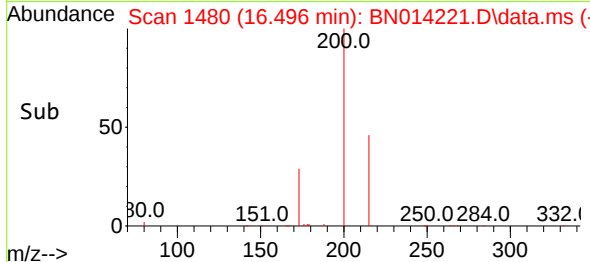

#24
Pentachlorophenol
Concen: 1.74 ng
RT: 16.690 min Scan# 1496
Delta R.T. 0.012 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:266 Resp: 11220
Ion Ratio Lower Upper
266 100
264 62.2 48.8 73.2
268 63.3 48.8 73.2


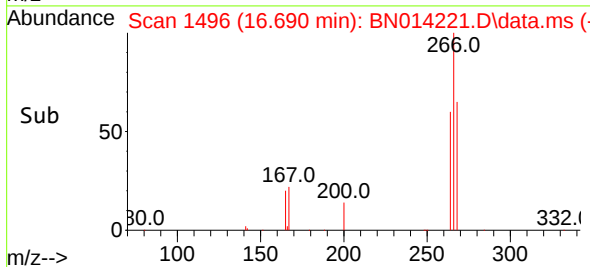

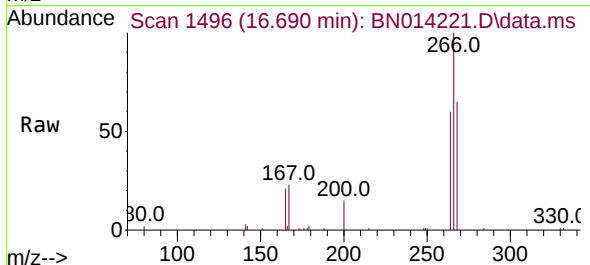


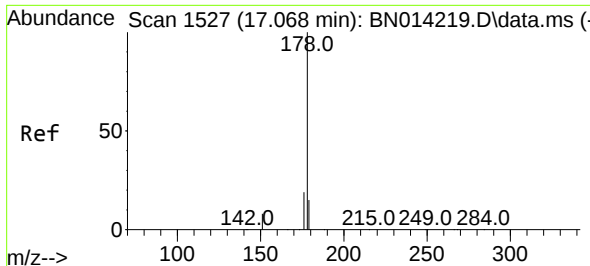

#25
Phenanthrene
Concen: 1.52 ng
RT: 17.068 min Scan# 1527
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:178 Resp: 172215
Ion Ratio Lower Upper
178 100
176 18.8 15.0 22.6
179 15.3 12.2 18.4

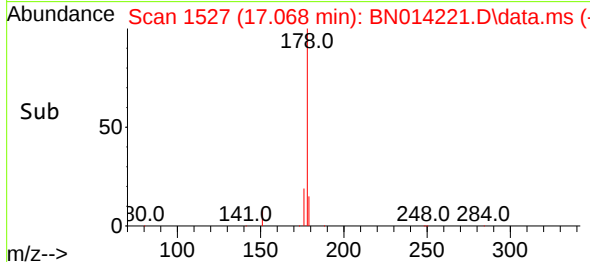

#26
Anthracene
Concen: 1.58 ng
RT: 17.165 min Scan# 1535
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:178 Resp: 152395
Ion Ratio Lower Upper
178 100
176 18.2 14.6 21.8
179 15.4 12.3 18.5


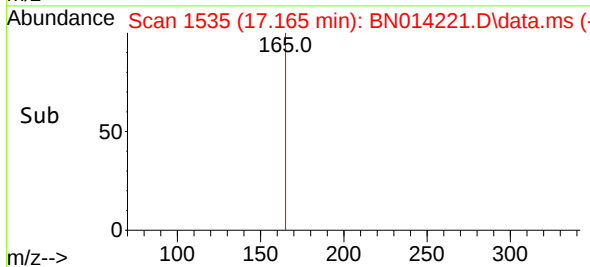

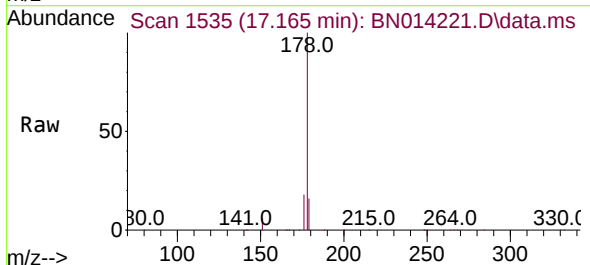


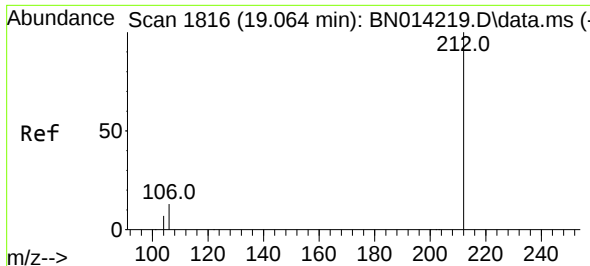

#27
Fluoranthene-d10
Concen: 1.21 ng
RT: 19.069 min Scan# 1817
Delta R.T. 0.005 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:212 Resp: 184454
Ion Ratio Lower Upper
212 100
106 12.6 10.1 15.1
104 7.0 5.6 8.4

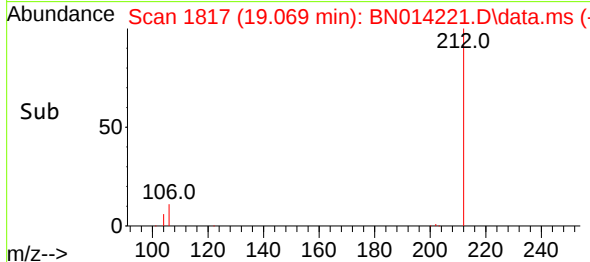

#28
Fluoranthene
Concen: 1.55 ng
RT: 19.094 min Scan# 1822
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:202 Resp: 204148
Ion Ratio Lower Upper
202 100
101 10.9 8.6 13.0
203 17.4 13.8 20.6


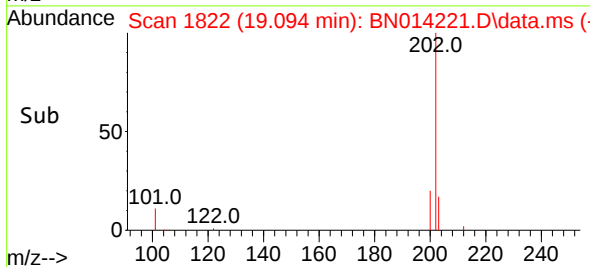

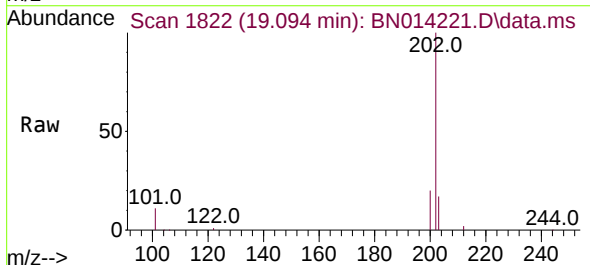




#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.218 min Scan# 2120
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:240 Resp: 41513
Ion Ratio Lower Upper
240 100
120 14.3 10.8 16.2
236 27.2 21.4 32.2

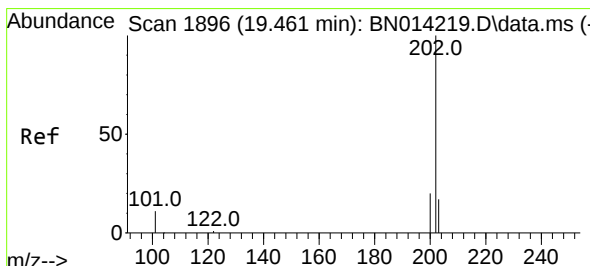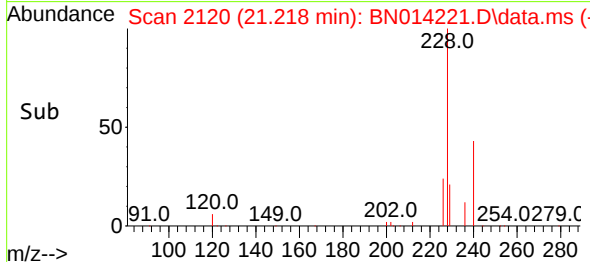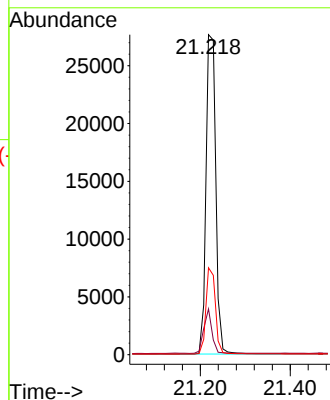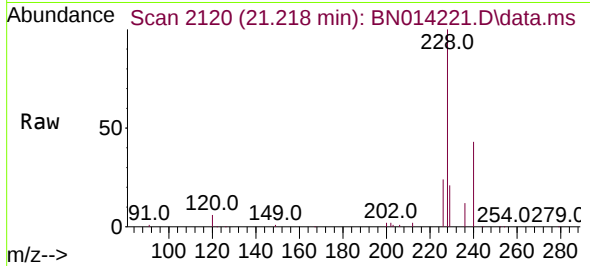

#30
Pyrene
Concen: 1.51 ng
RT: 19.461 min Scan# 1896
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:202 Resp: 202143
Ion Ratio Lower Upper
202 100
200 20.4 16.3 24.5
203 17.4 13.9 20.9


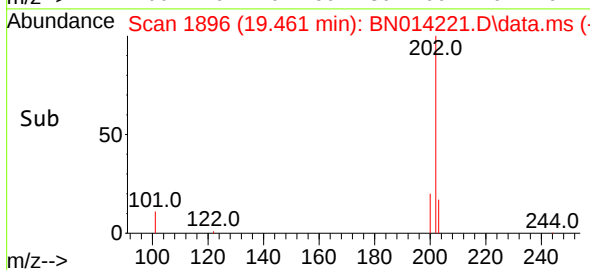
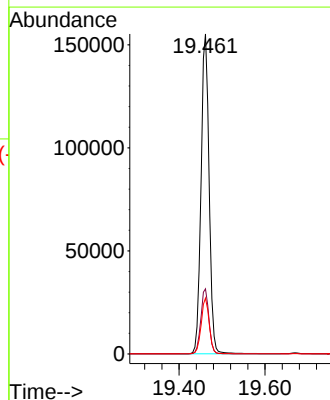
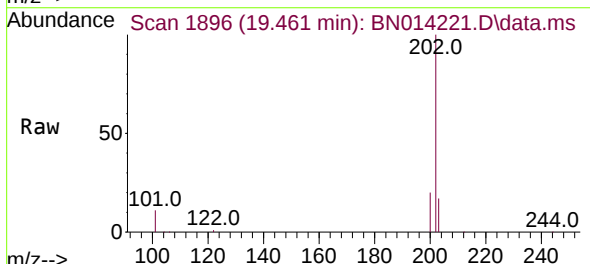




#31
Terphenyl-d14
Concen: 1.53 ng
RT: 19.670 min Scan# 1938
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:244 Resp: 146741
Ion Ratio Lower Upper
244 100
212 7.5 5.9 8.9
122 11.9 9.2 13.8

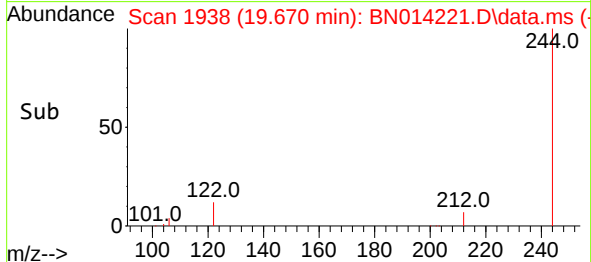

#32
Benzo(a)anthracene
Concen: 1.53 ng
RT: 21.208 min Scan# 2119
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:228 Resp: 196500
Ion Ratio Lower Upper
228 100
226 26.3 21.1 31.7
229 19.5 15.8 23.8



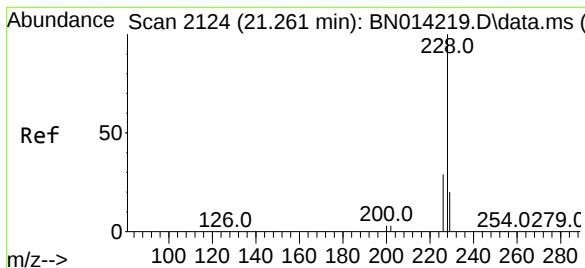

#33

Chrysene

Concen: 1.48 ng

RT: 21.261 min Scan# 2124

Delta R.T. 0.000 min

Lab File: BN014221.D

Acq: 06 Apr 2021 12:30

Instrument :

BNA_N

ClientSampleId :

SSTDICC1.6





Tgt Ion:228 Resp: 210560

Ion Ratio Lower Upper

228 100

226 29.0 23.0 34.6

229 19.6 15.8 23.8

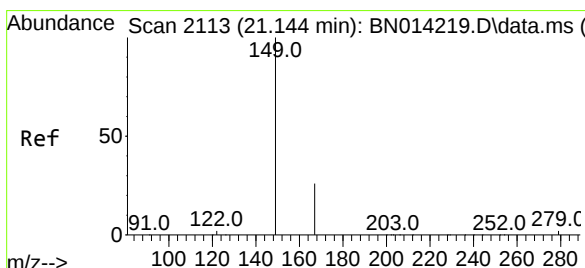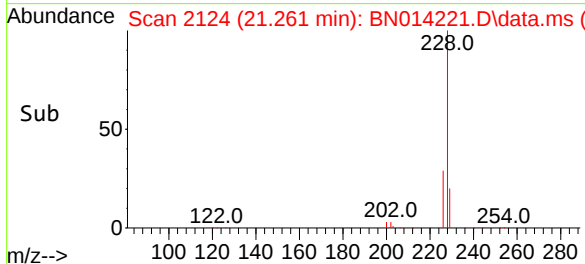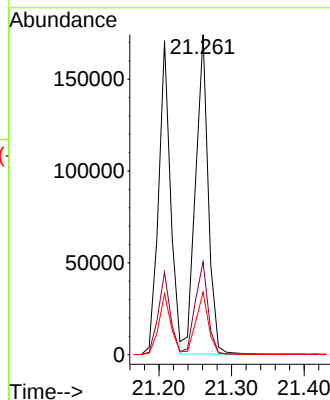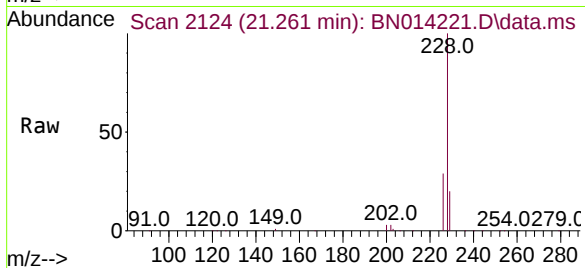

#34

Bis(2-ethylhexyl)phthalate

Concen: 1.49 ng

RT: 21.144 min Scan# 2113

Delta R.T. 0.000 min

Lab File: BN014221.D

Acq: 06 Apr 2021 12:30




Tgt Ion:149 Resp: 65910


Ion Ratio Lower Upper

149 100

167 26.7 21.4 32.0

279 4.0 3.1 4.7


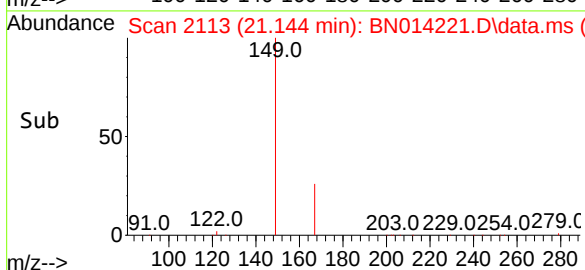
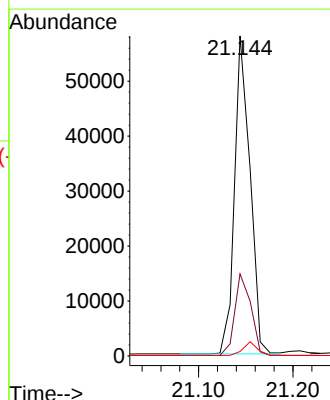
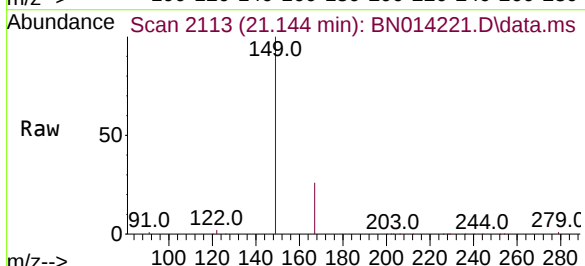




#35
Indeno(1,2,3-cd)pyrene
Concen: 1.30 ng
RT: 25.635 min Scan# 3175
Delta R.T. 0.003 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:276 Resp: 222493
Ion Ratio Lower Upper
276 100
138 23.6 18.6 27.8
277 24.8 19.8 29.8

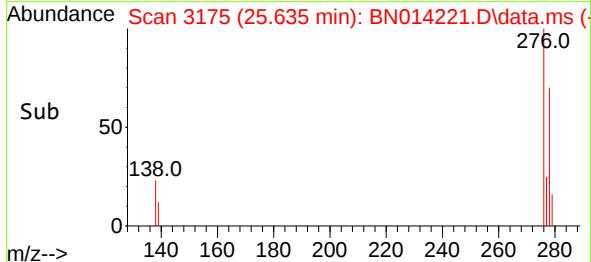

#36
Perylene-d12
Concen: 0.40 ng
RT: 23.428 min Scan# 2530
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:264 Resp: 36431
Ion Ratio Lower Upper
264 100
260 24.5 19.7 29.5
265 24.2 19.2 28.8


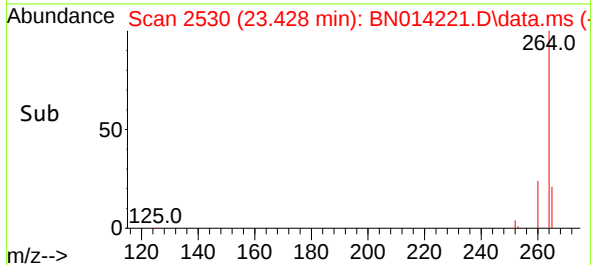

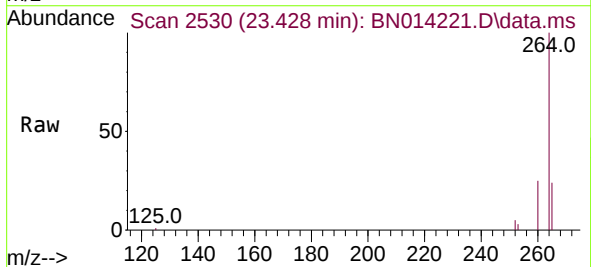




#37
Benzo(b)fluoranthene
Concen: 1.57 ng
RT: 22.767 min Scan# 2337
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 213682
Ion Ratio Lower Upper
252 100
253 22.0 18.5 27.7
125 10.0 10.3 15.5#



#38
Benzo(k)fluoranthene
Concen: 1.56 ng
RT: 22.812 min Scan# 2350
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:252 Resp: 208165
Ion Ratio Lower Upper
252 100
253 22.1 18.1 27.1
125 9.5 7.8 11.6


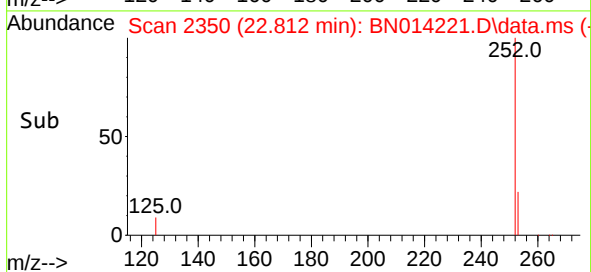






#39
Benzo(a)pyrene
Concen: 1.55 ng
RT: 23.332 min Scan# 2502
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30




Instrument :
BNA_N
ClientSampleId :
SSTDICC1.6


Tgt Ion:252 Resp: 188507
Ion Ratio Lower Upper
252 100
253 22.3 19.4 29.2
125 11.8 16.6 24.8#

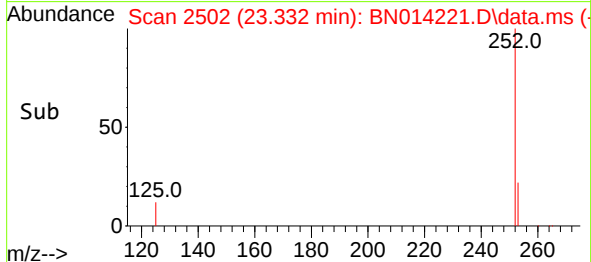

#40
Dibenzo(a,h)anthracene
Concen: 1.46 ng
RT: 25.646 min Scan# 3178
Delta R.T. 0.000 min
Lab File: BN014221.D
Acq: 06 Apr 2021 12:30

Tgt Ion:278 Resp: 186140
Ion Ratio Lower Upper
278 100
139 15.9 12.6 19.0
279 23.4 19.4 29.0

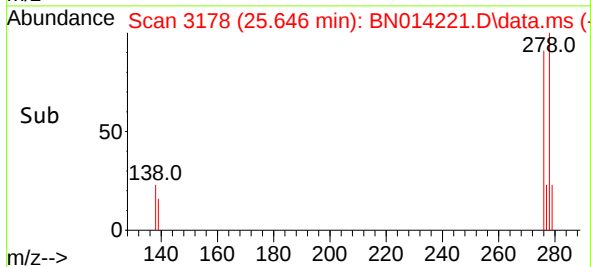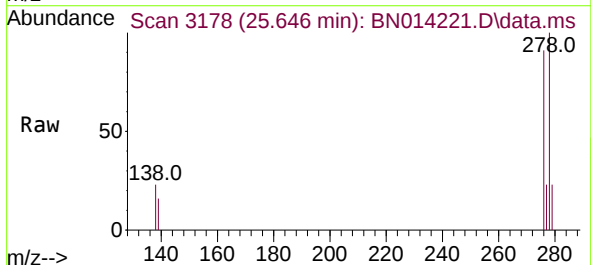

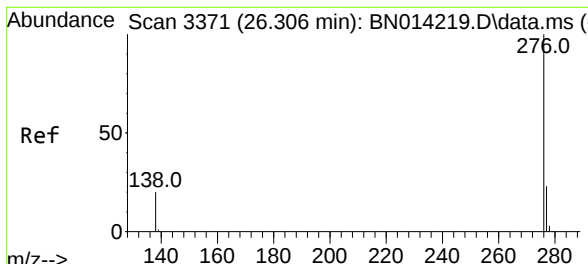

#41
 Benzo(g,h,i)perylene
 Concen: 1.42 ng
 RT: 26.306 min Scan# 3371
 Delta R.T. 0.000 min
 Lab File: BN014221.D
 Acq: 06 Apr 2021 12:30

Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC1.6

Tgt Ion:	276	Resp:	186086
Ion Ratio	Lower	Upper	
276	100		
277	23.7	18.9	28.3
138	20.4	16.4	24.6

