
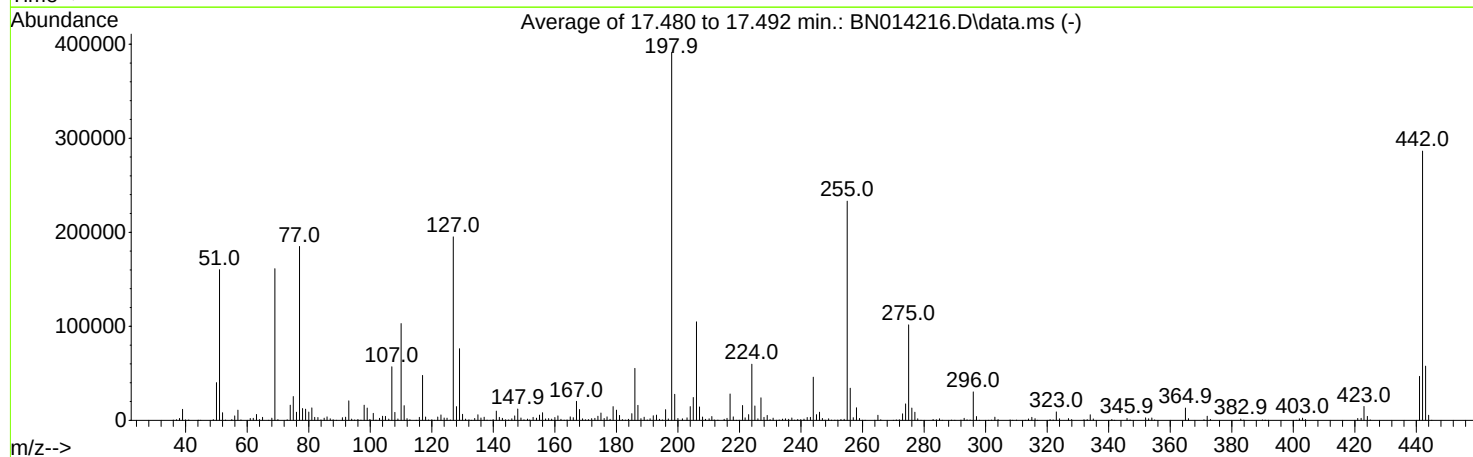


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040721\
 Data File : BN014216.D
 Acq On : 06 Apr 2021 09:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN040721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 06 16:07:07 2021

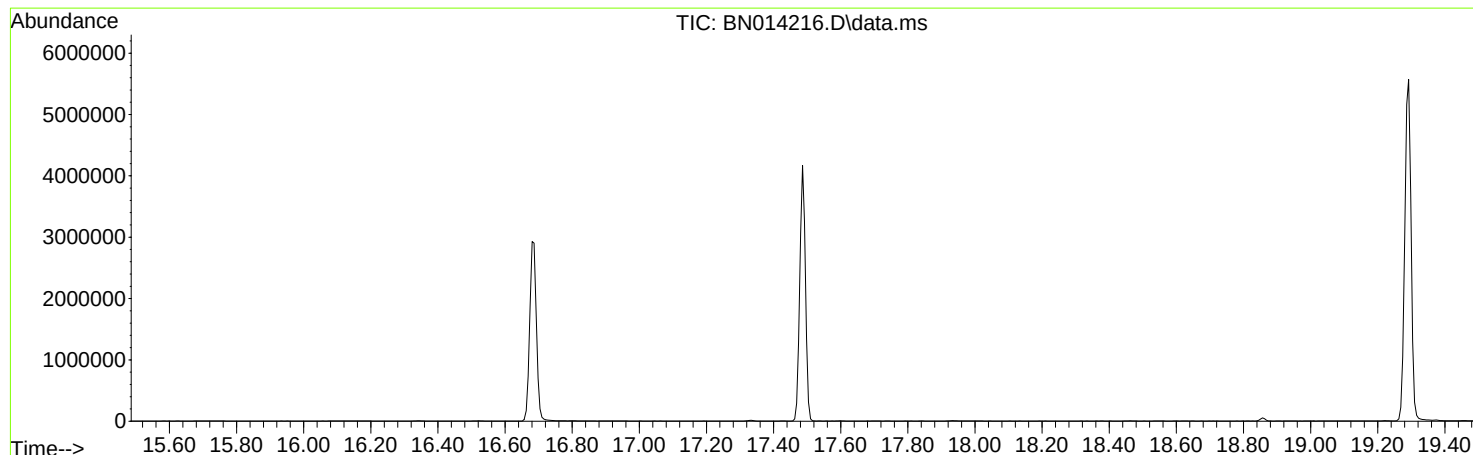

AutoFind: Scans 2447, 2448, 2449; Background Corrected with Scan 2440

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.0	160363	PASS
68	69	0.00	2	1.5	2425	PASS
69	198	0.00	100	41.2	161301	PASS
70	69	0.00	2	0.5	866	PASS
127	198	10	80	49.9	195136	PASS
197	198	0.00	2	0.4	1596	PASS
198	198	100	100	100.0	391168	PASS
199	198	5	9	7.1	27720	PASS
275	198	10	60	26.0	101515	PASS
365	198	1	100	3.3	13059	PASS
441	198	0.01	100	12.0	46768	PASS
442	442	50	100	100.0	286293	PASS
443	442	15	24	20.2	57701	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
4/7/2021	BNA_N	<u>BN014216.D</u>
Compound Name	Response	Retention Time
DDT	1402660	20.527
DDD	2201	20.086
DDE	1413	19.58
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3614	1406274	0.26

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040721\
Data File : BN014216.D
Acq On : 06 Apr 2021 09:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 06 10:53:36 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

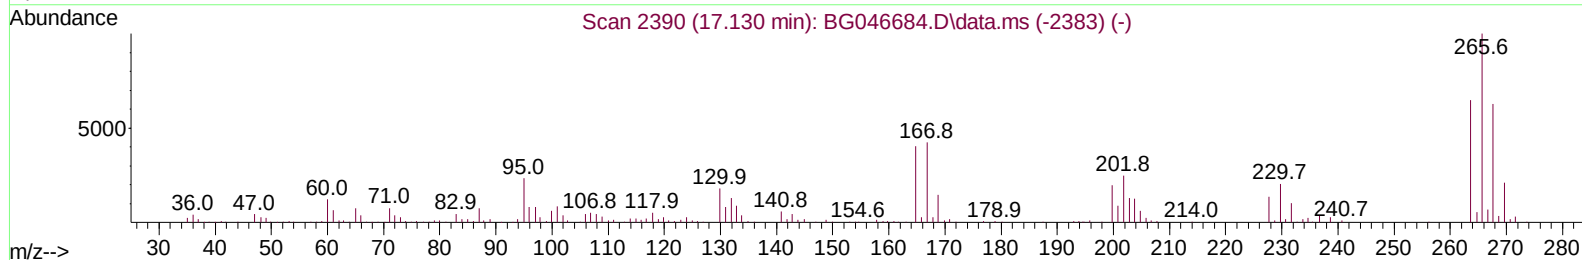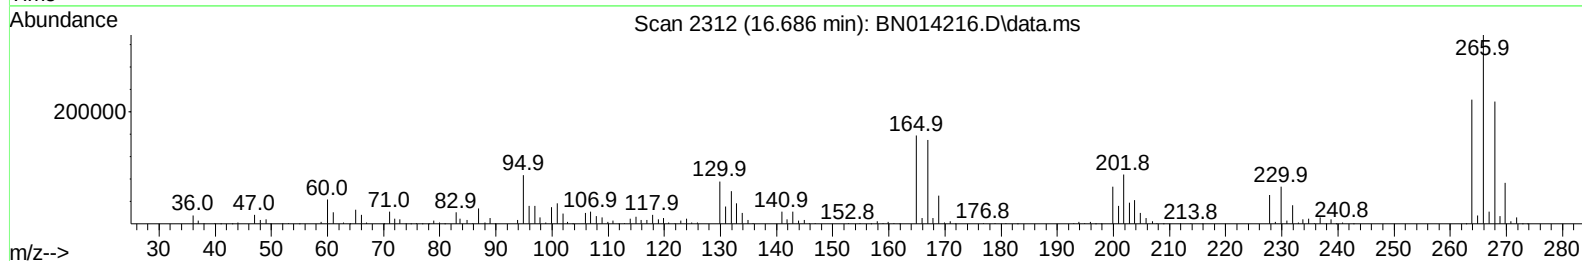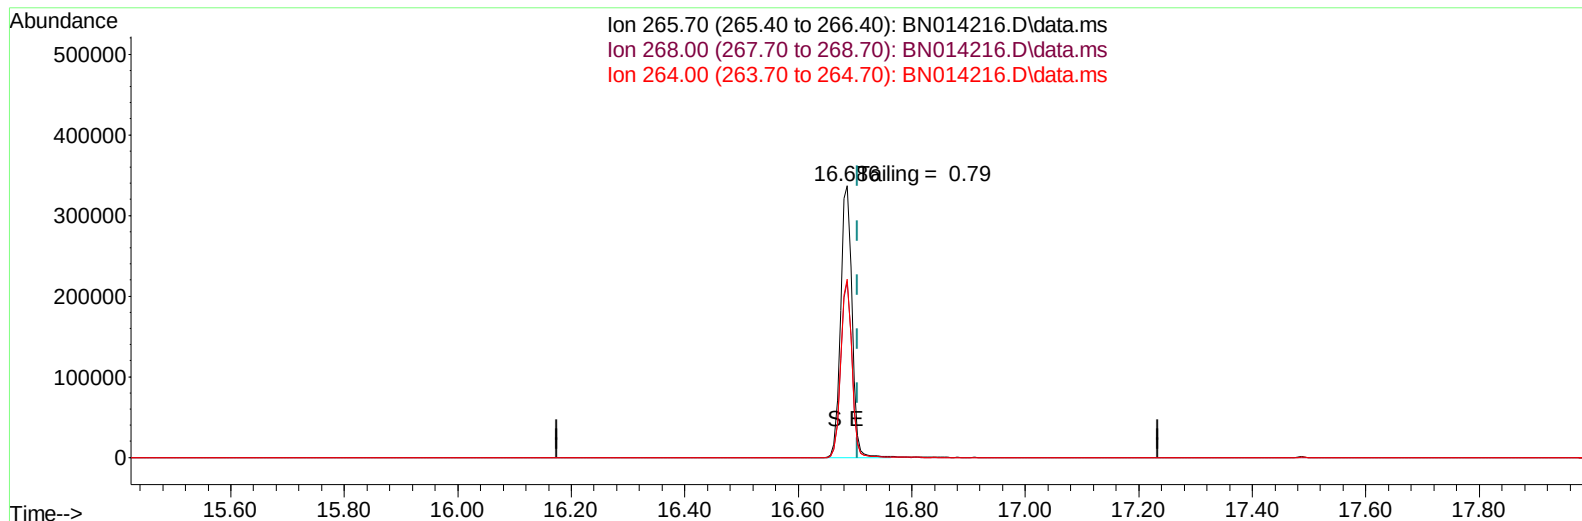

TIC: BN014216.D\data.ms

(70) Pentachlorophenol (C)

16.686min (-0.018) 24167.29 ng




response 466371

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.70
264.00	61.60	65.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040721\
Data File : BN014216.D
Acq On : 06 Apr 2021 09:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Apr 06 10:53:36 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 26 11:50:50 2021
Response via : Initial Calibration

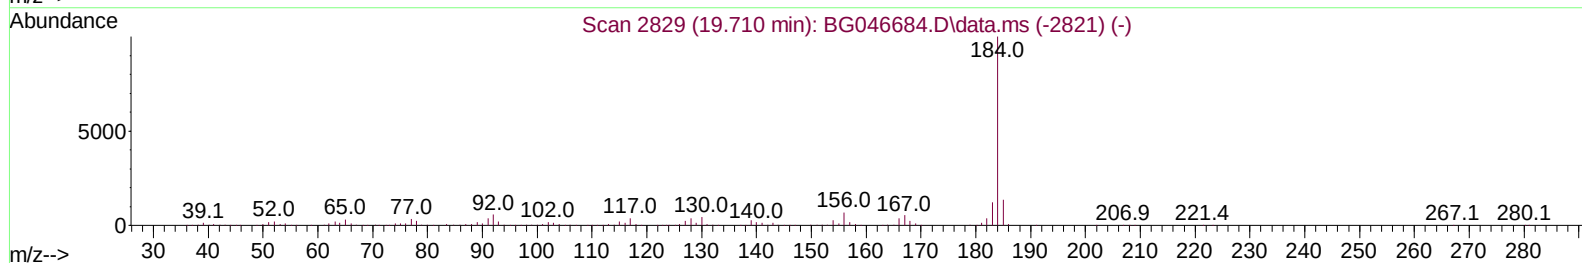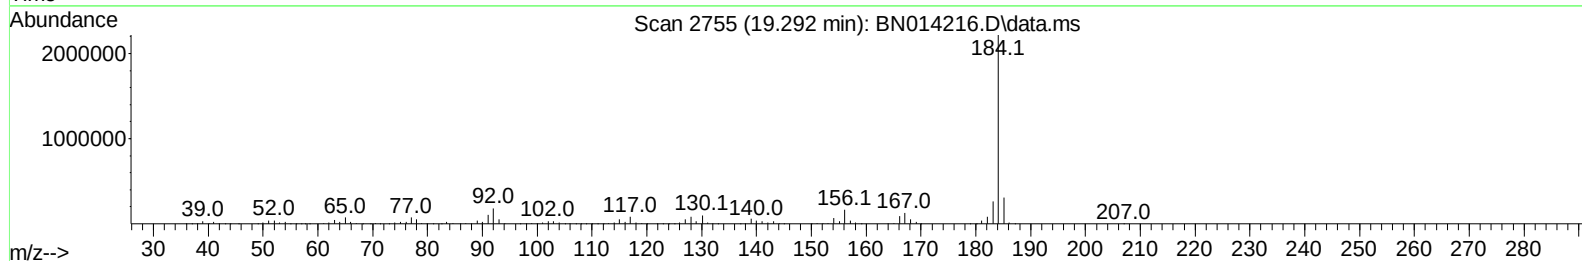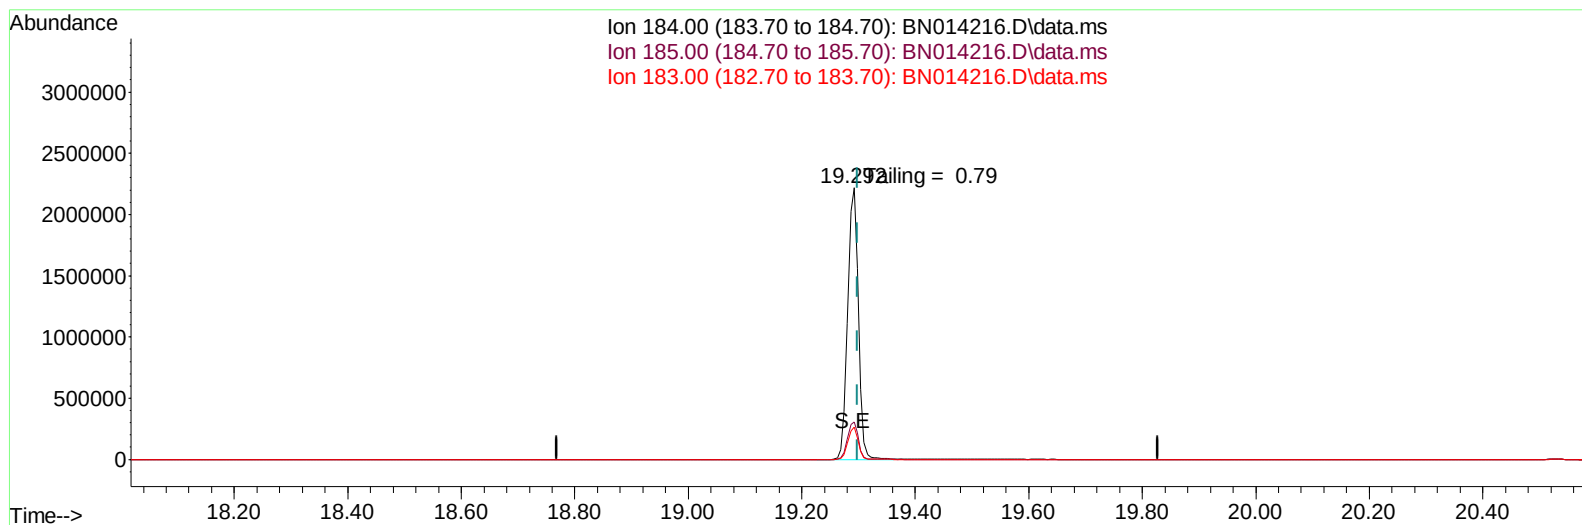

TIC: BN014216.D\data.ms

(77) Benzidine

19.292min (-0.006) 0.00 ng

response 2925137

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.89
183.00	13.20	11.86
0.00	0.00	0.00