




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030740.D
Acq On : 07 Apr 2024 14:07
Operator : MA/JU
Sample : P1987-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R43

Manual IntegrationsAPPROVED

Quant Time: Apr 07 15:04:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/08/2024
Supervised By :mohammad ahmed 04/09/2024

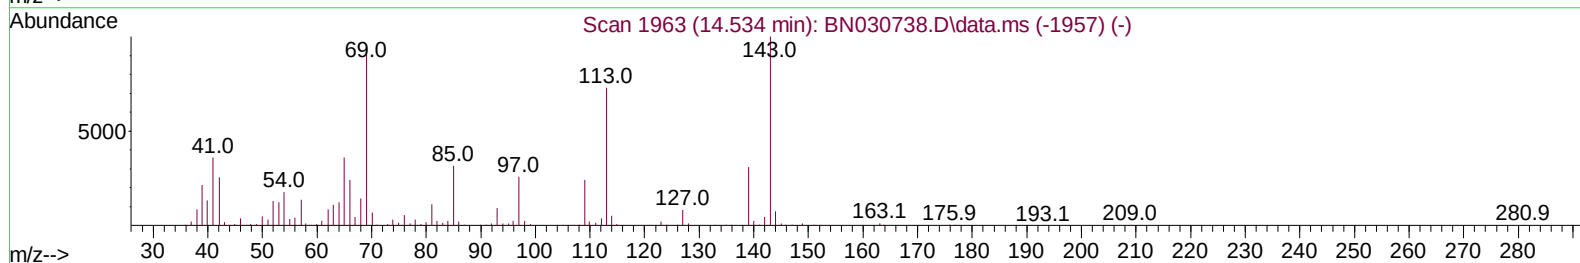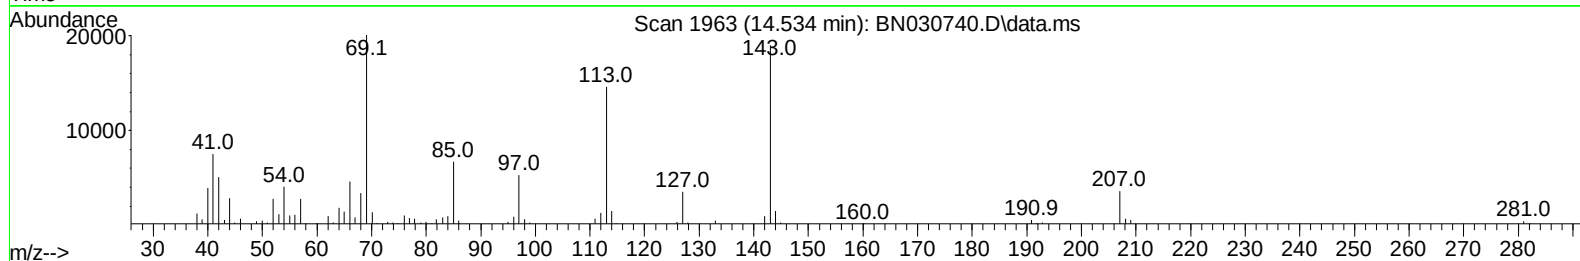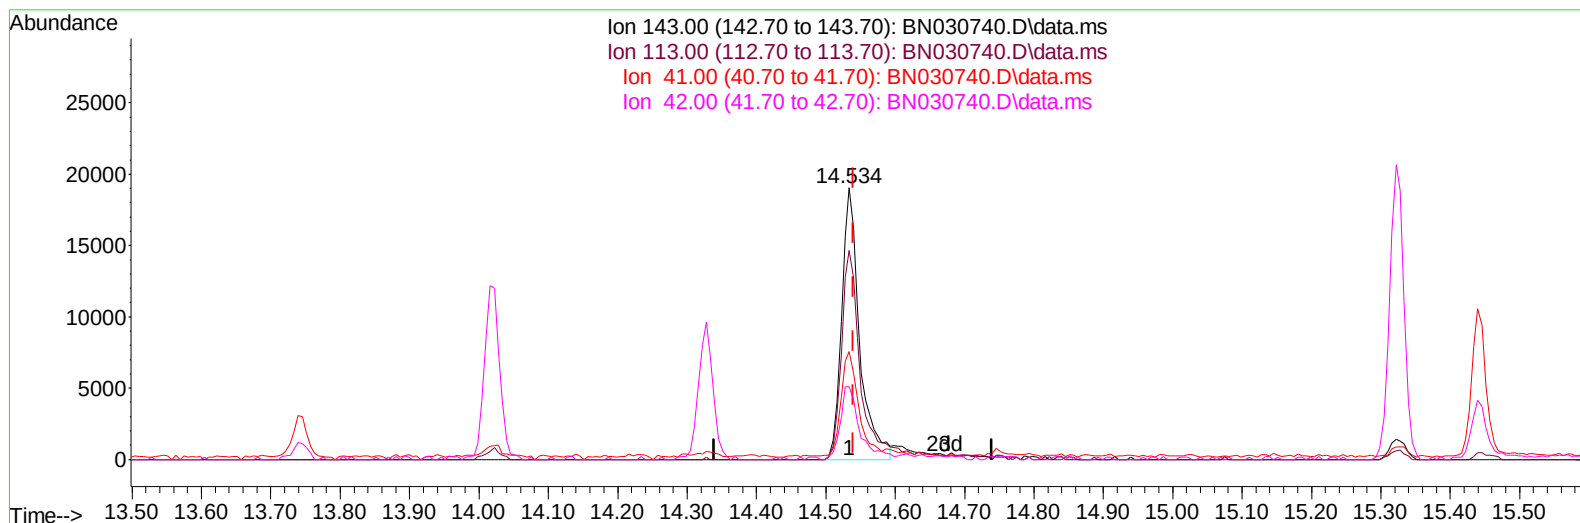

TIC: BN030740.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.534min (-0.006) 5.43 ng/u1

response 34228

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	72.10	76.90
41.00	38.20	39.66
42.00	26.70	26.73




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
 Data File : BN030740.D
 Acq On : 07 Apr 2024 14:07
 Operator : MA/JU
 Sample : P1987-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R43

Manual IntegrationsAPPROVED

Quant Time: Apr 07 15:04:55 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 12:24:07 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/08/2024
 Supervised By :mohammad ahmed 04/09/2024

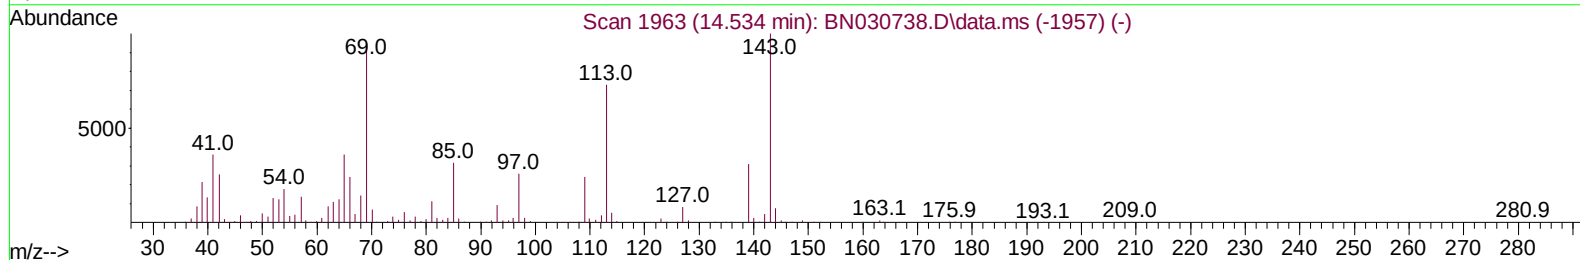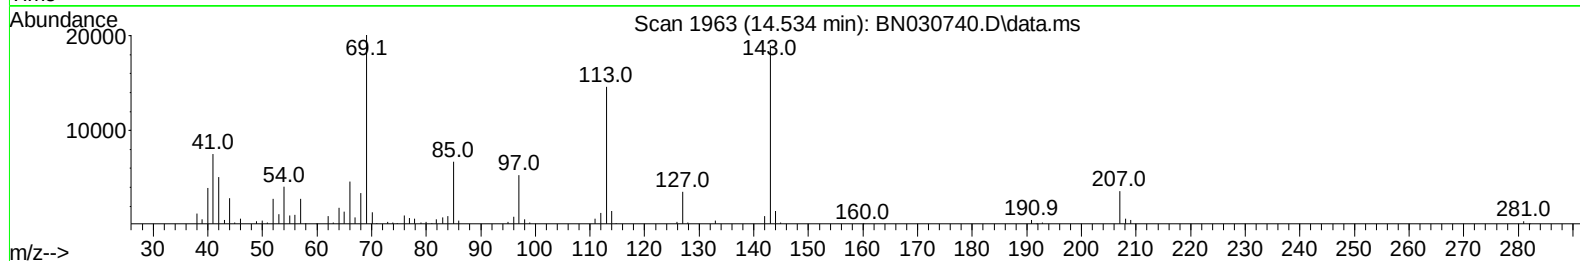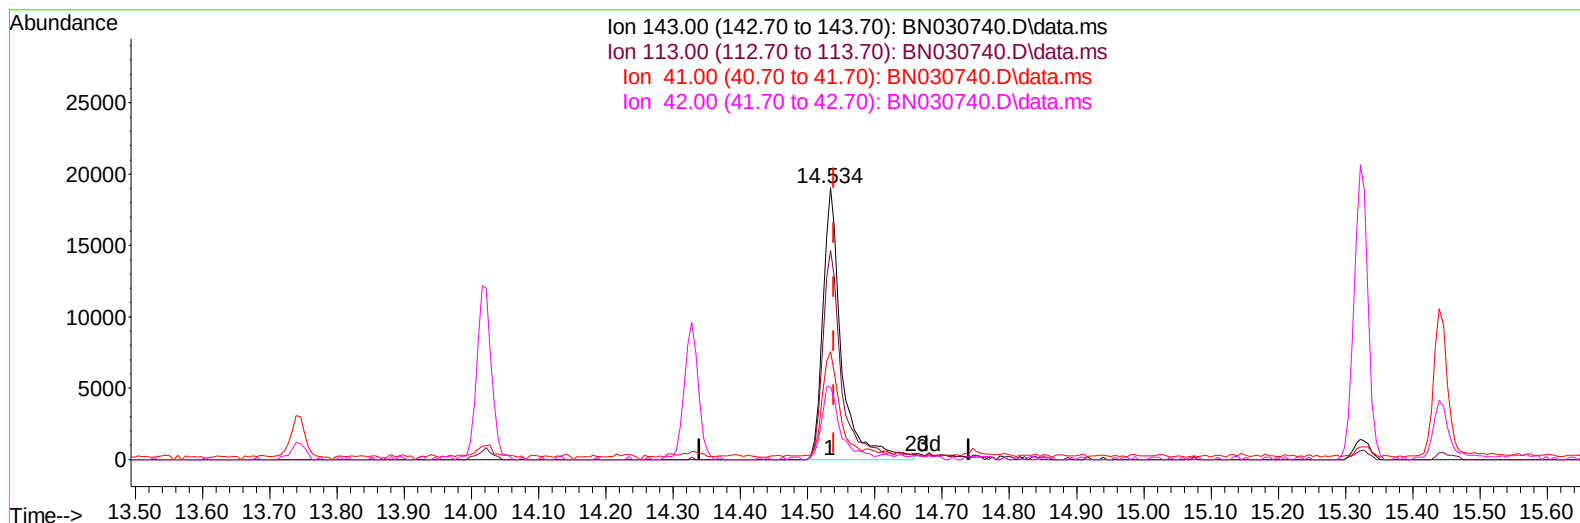

TIC: BN030740.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.534min (-0.006) 5.81 ng/ul m

response 36603

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	72.10	76.90
41.00	38.20	39.66
42.00	26.70	26.73

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
 Data File : BN030740.D
 Acq On : 07 Apr 2024 14:07
 Operator : MA/JU
 Sample : P1987-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R43

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/08/2024
 Supervised By :mohammad ahmed 04/09/2024

Quant Time: Apr 07 16:34:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 12:24:07 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.687	152		136963	20.000	ng/ul	-0.01
20) Naphthalene-d8	10.469	136		677179	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.328	164		493256	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.075	188		1074105	20.000	ng/ul	-0.01
79) Chrysene-d12	21.310	240		1085049	20.000	ng/ul	-0.02
88) Perylene-d12	24.251	264		1220949	20.000	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.187	96		15765	5.397	ng/uL	-0.01
4) Pyridine-d5	3.599	84		57296	6.542	ng/ul	0.00
7) Phenol-d5	6.858	99		80098	7.229	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.022	67		274015	40.041	ng/ul	-0.02
11) 2-Chlorophenol-d4	7.216	132		270201	32.147	ng/ul	-0.01
15) 4-Methylphenol-d8	8.387	113		171611	18.481	ng/ul	-0.01
21) Nitrobenzene-d5	8.840	128		190290	40.508	ng/ul	-0.01
24) 2-Nitrophenol-d4	9.557	143		186689	43.443	ng/ul	-0.01
28) 2,4-Dichlorophenol-d3	10.087	165		341057	36.252	ng/ul	-0.01
31) 4-Chloroaniline-d4	10.610	131		425957	27.502	ng/ul	-0.01
46) Dimethylphthalate-d6	13.746	166		1397537	42.436	ng/ul	-0.01
49) Acenaphthylene-d8	14.022	160		1607893	42.464	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.534	143		36603m	5.811	ng/ul	0.00
60) Fluorene-d10	15.322	176		1262427	43.806	ng/ul	-0.02
65) 4,6-Dinitro-2-methylph...	15.445	200		172162	36.313	ng/ul	0.00
73) Anthracene-d10	17.175	188		2190082	47.323	ng/ul	-0.01
81) Pyrene-d10	19.475	212		2671800	45.800	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.057	264		2798497	49.744	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030740.D
Acq On : 07 Apr 2024 14:07
Operator : MA/JU
Sample : P1987-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R43

Manual IntegrationsAPPROVED

Quant Time: Apr 07 16:34:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/08/2024
Supervised By :mohammad ahmed 04/09/2024

