

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
 Data File : BN030759.D
 Acq On : 08 Apr 2024 03:11
 Operator : MA/JU
 Sample : P2017-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH5F0

Quant Time: Apr 08 05:02:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Mar 31 12:24:07 2024
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.681	152	199186	20.000	ng/u1	-0.02
20) Naphthalene-d8	10.463	136	920632	20.000	ng/u1	-0.02
38) Acenaphthene-d10	14.328	164	640939	20.000	ng/u1	-0.01
64) Phenanthrene-d10	17.075	188	1370173	20.000	ng/u1	-0.01
79) Chrysene-d12	21.310	240	1341939	20.000	ng/u1	-0.02
88) Perylene-d12	24.251	264	1454456	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	20249	4.766	ng/uL	-0.01
4) Pyridine-d5	3.599	84	203386	15.967	ng/u1	0.00
7) Phenol-d5	6.852	99	196735	12.210	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.022	67	351584	35.327	ng/u1	-0.02
11) 2-Chlorophenol-d4	7.216	132	424828	34.755	ng/u1	-0.01
15) 4-Methylphenol-d8	8.387	113	353079	26.145	ng/u1	-0.01
21) Nitrobenzene-d5	8.840	128	250453	39.217	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.552	143	263485	45.099	ng/u1	-0.02
28) 2,4-Dichlorophenol-d3	10.087	165	543296	42.477	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.610	131	383769	18.226	ng/u1	-0.01
46) Dimethylphthalate-d6	13.745	166	1921626	44.905	ng/u1	-0.01
49) Acenaphthylene-d8	14.016	160	2106143	42.806	ng/u1	-0.02
54) 4-Nitrophenol-d4	14.540	143	97615	11.926	ng/u1	0.00
60) Fluorene-d10	15.322	176	1662979	44.409	ng/u1	-0.02
65) 4,6-Dinitro-2-methylph...	15.440	200	257666	42.604	ng/u1	-0.01
73) Anthracene-d10	17.175	188	2657522	45.016	ng/u1	-0.01
81) Pyrene-d10	19.475	212	3177316	44.039	ng/u1	-0.01
92) Benzo(a)pyrene-d12	24.051	264	3175937	47.389	ng/u1	-0.02
Target Compounds						
16) Acetophenone	8.505	105	25878	1.214	ng/u1	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030759.D
Acq On : 08 Apr 2024 03:11
Operator : MA/JU
Sample : P2017-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5F0


Quant Time: Apr 08 05:02:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Mar 31 12:24:07 2024
Response via : Initial Calibration

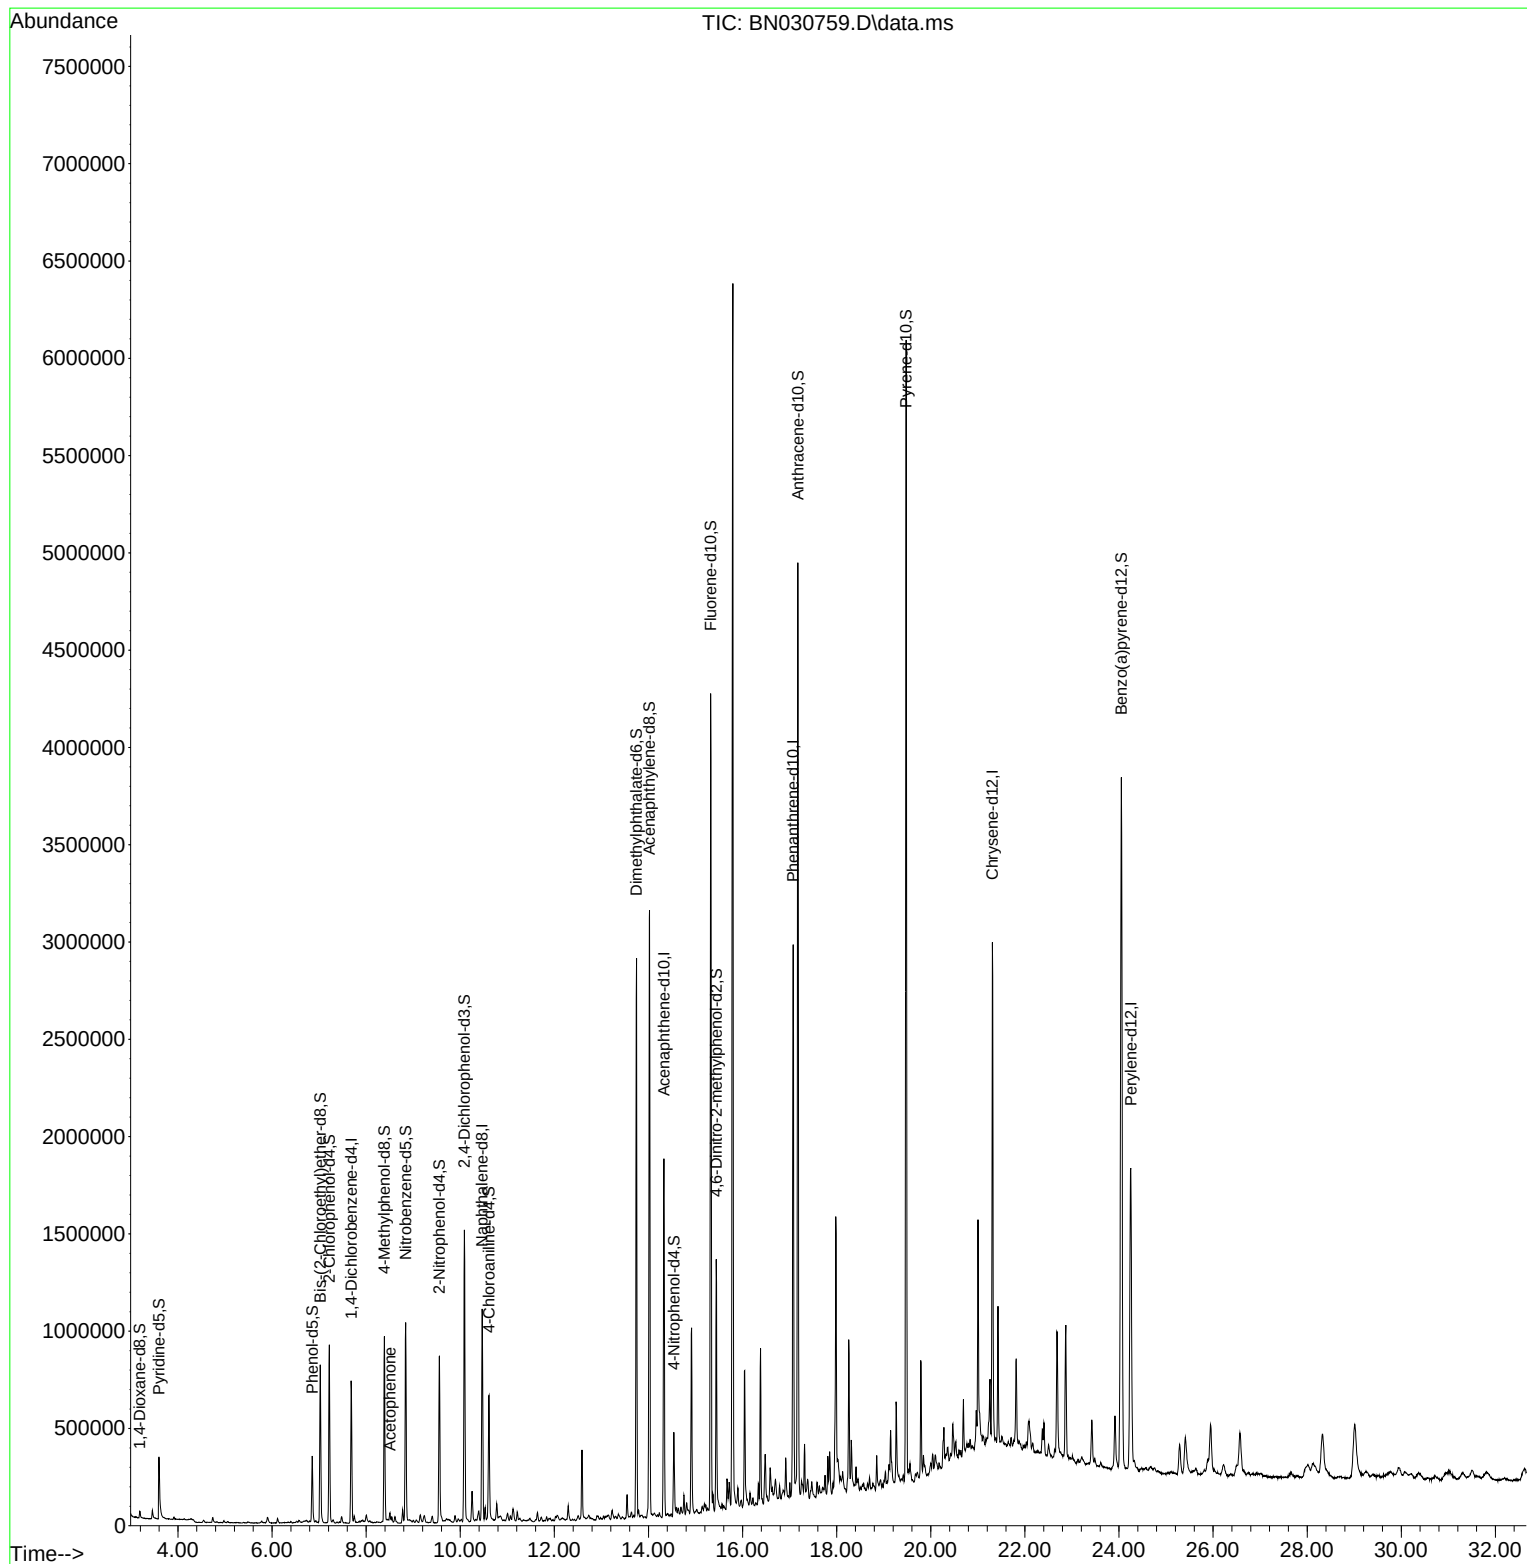

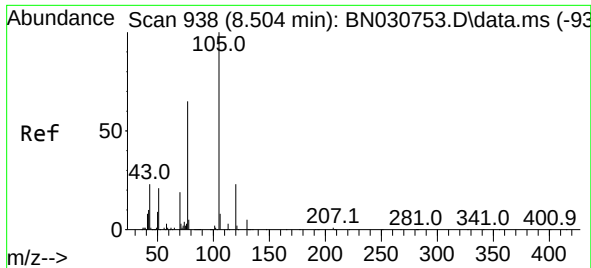

#16
 Acetophenone
 Concen: 1.214 ng/ul
 RT: 8.505 min Scan# 91
 Delta R.T. -0.012 min
 Lab File: BN030759.D
 Acq: 08 Apr 2024 03:11

Instrument :
 BNA_N
 ClientSampleId :
 BH5F0

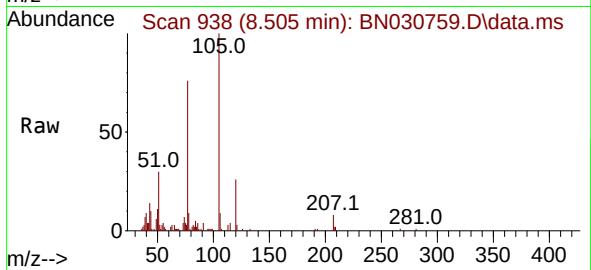

Tgt Ion:	105	Resp:	25878
Ion	Ratio	Lower	Upper
105	100		
77	76.1	61.2	91.8
51	29.9	21.0	31.4

