

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
 Data File : BN030742.D
 Acq On : 07 Apr 2024 15:25
 Operator : MA/JU
 Sample : P1987-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R61

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030742.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	46	rVB	39914	64837	0.65%	0.089%
2	3.599	102	104	122	rBV	191336	334745	3.34%	0.458%
3	6.857	652	658	667	rVB	212031	339829	3.39%	0.465%
4	7.028	680	687	696	rBV	902354	1405014	14.03%	1.924%
5	7.216	712	719	731	rBV	829396	1321249	13.20%	1.809%
6	7.687	790	799	808	rBV	590135	961728	9.60%	1.317%
7	8.387	911	918	931	rBV	686148	1099760	10.98%	1.506%
8	8.840	984	995	1007	rBV	1105575	1804329	18.02%	2.471%
9	9.246	1059	1064	1071	rVB3	13118	24710	0.25%	0.034%
10	9.557	1109	1117	1130	rBV	875964	1410176	14.08%	1.931%
11	10.087	1199	1207	1220	rBV	1269694	2185234	21.82%	2.993%
12	10.469	1264	1272	1280	rBV	962569	1625750	16.24%	2.226%
13	10.610	1284	1296	1313	rBV	1209959	2055988	20.53%	2.816%
14	11.740	1483	1488	1491	rVB3	11125	17282	0.17%	0.024%
15	12.063	1537	1543	1549	rVB	25550	42389	0.42%	0.058%
16	13.228	1736	1741	1745	rBV3	15222	23945	0.24%	0.033%
17	13.745	1822	1829	1841	rBV	2935787	4067403	40.62%	5.570%
18	14.022	1868	1876	1889	rBV2	3283026	4899616	48.93%	6.710%
19	14.328	1922	1928	1938	rBV	1707775	2482602	24.79%	3.400%
20	14.534	1957	1963	1979	rBV	205678	379624	3.79%	0.520%
21	14.751	1994	2000	2005	rVB9	7159	14154	0.14%	0.019%
22	15.328	2091	2098	2110	rBV	4259424	6274878	62.67%	8.593%
23	15.439	2111	2117	2134	rVV	1208115	1754809	17.53%	2.403%
24	15.563	2134	2138	2142	rVB3	21277	29778	0.30%	0.041%
25	16.110	2226	2231	2239	rBV5	15577	24956	0.25%	0.034%
26	16.757	2335	2341	2346	rBV10	7424	14334	0.14%	0.020%
27	17.075	2388	2395	2405	rBV	2160794	3186913	31.83%	4.364%
28	17.175	2405	2412	2425	rVV	5012700	7519401	75.10%	10.298%
29	17.975	2543	2548	2554	rBV3	57970	76739	0.77%	0.105%
30	18.410	2619	2622	2626	rBV6	7029	10582	0.11%	0.014%
31	19.039	2724	2729	2734	rBV	75910	105284	1.05%	0.144%
32	19.110	2736	2741	2746	rBV	71487	103910	1.04%	0.142%
33	19.263	2763	2767	2774	rBV2	57962	80180	0.80%	0.110%
34	19.422	2790	2794	2797	rBV5	19577	24785	0.25%	0.034%
35	19.480	2797	2804	2811	rBV	6515782	9210238	91.98%	12.613%
36	20.527	2980	2982	2986	rBV2	23083	27752	0.28%	0.038%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030742.D
Acq On : 07 Apr 2024 15:25
Operator : MA/JU
Sample : P1987-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R61

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	21.010	3061	3064	3068	rBV3	34245	39092	0.39%	0.054%
38	21.316	3110	3116	3127	rBV	2625147	3795991	37.91%	5.199%
39	24.057	3572	3582	3597	rBV2	4084106	10013077	100.00%	13.713%
40	24.257	3607	3616	3631	rVB	1631964	4167815	41.62%	5.708%




Sum of corrected areas: 73020878

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030742.D
Acq On : 07 Apr 2024 15:25
Operator : MA/JU
Sample : P1987-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R61

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

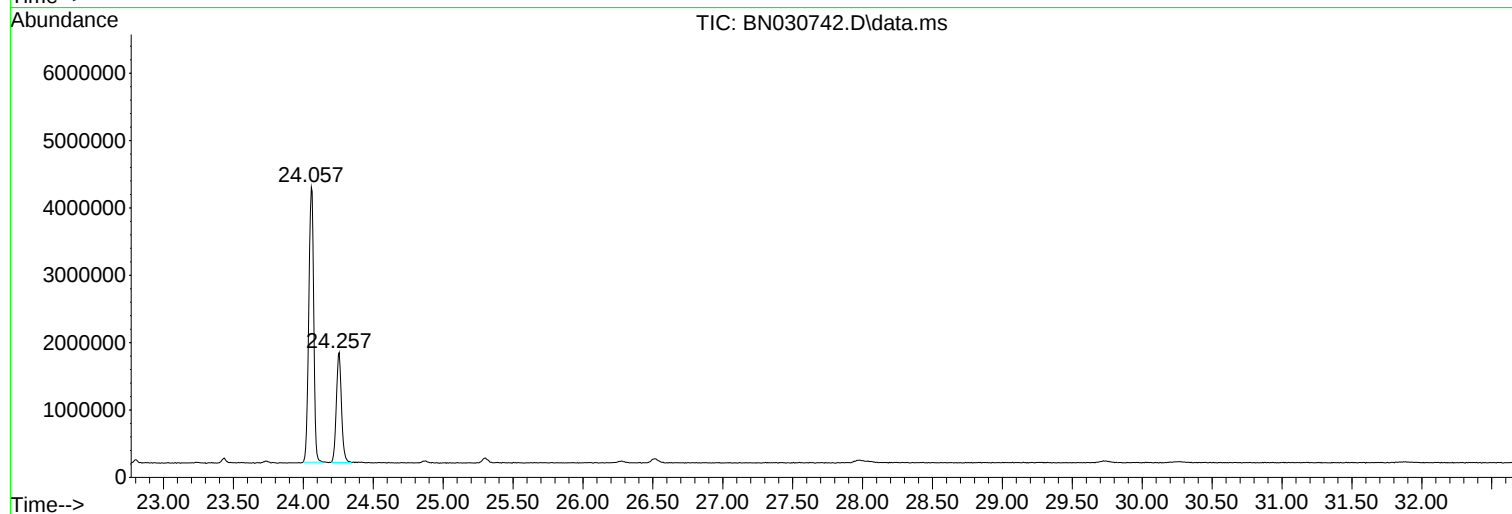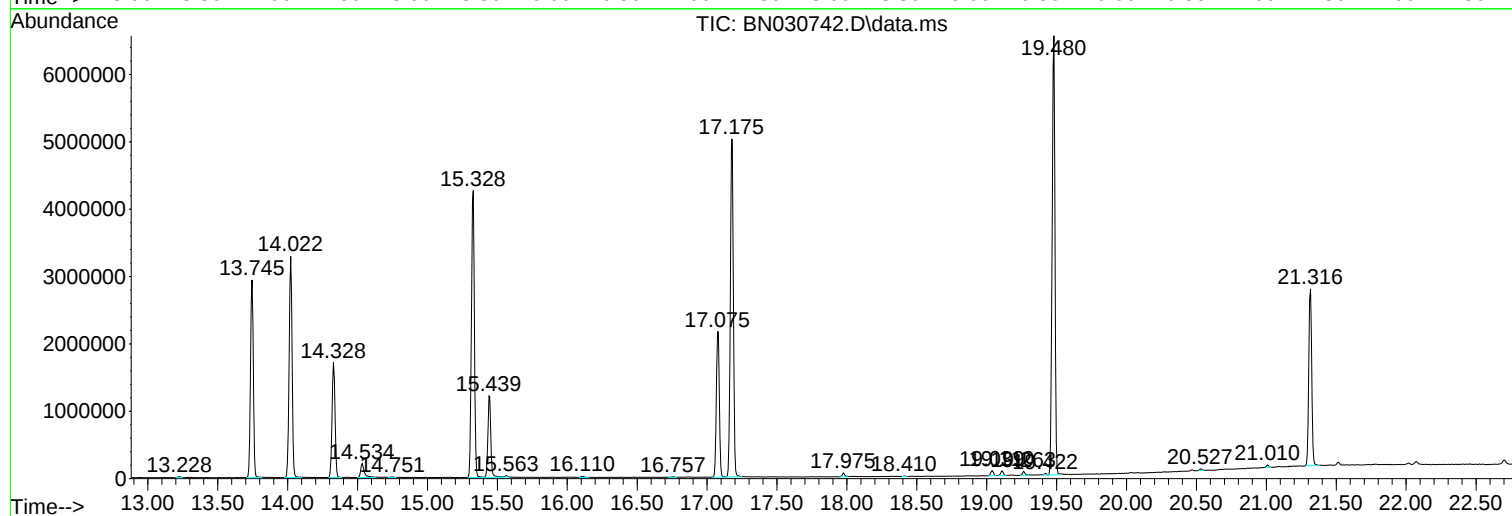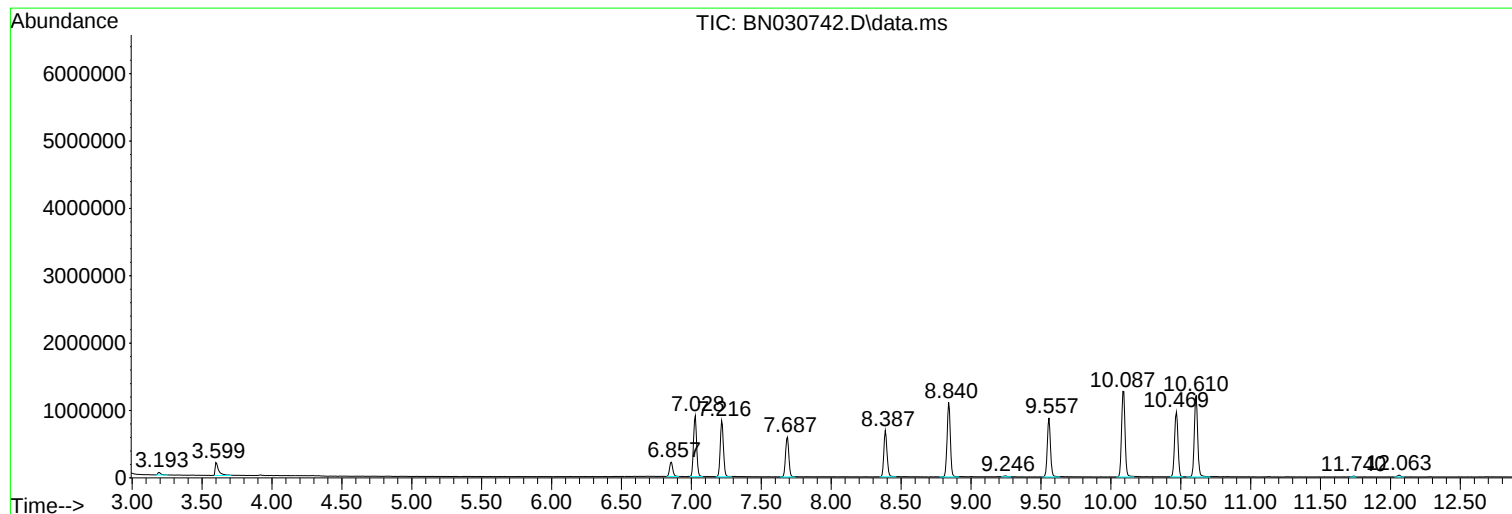

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030742.D
Acq On : 07 Apr 2024 15:25
Operator : MA/JU
Sample : P1987-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R61

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030742.D
Acq On : 07 Apr 2024 15:25
Operator : MA/JU
Sample : P1987-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R61

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc