

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
 Data File : BN030743.D
 Acq On : 07 Apr 2024 16:04
 Operator : MA/JU
 Sample : P1987-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MC0R62

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030743.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	40	rBV	22761	34225	0.42%	0.059%
2	3.599	102	104	118	rBV	103506	171430	2.10%	0.297%
3	6.858	653	658	671	rVB	146640	245065	3.00%	0.425%
4	7.028	680	687	699	rVB	683424	1095955	13.42%	1.901%
5	7.216	712	719	731	rBV	621655	984790	12.06%	1.709%
6	7.299	731	733	740	rVB6	5001	9417	0.12%	0.016%
7	7.687	791	799	806	rBV	485819	763437	9.35%	1.325%
8	8.387	911	918	927	rBV	514608	802783	9.83%	1.393%
9	8.840	987	995	1006	rBV	865890	1365399	16.72%	2.369%
10	9.240	1059	1063	1068	rVB6	5057	9373	0.11%	0.016%
11	9.557	1110	1117	1130	rBV	636762	1037336	12.70%	1.800%
12	10.087	1200	1207	1225	rBV	1005530	1651024	20.22%	2.865%
13	10.469	1264	1272	1283	rBV	783284	1322807	16.20%	2.295%
14	10.610	1288	1296	1306	rBV	879559	1489815	18.24%	2.585%
15	12.063	1537	1543	1549	rBV3	20655	33001	0.40%	0.057%
16	12.716	1651	1654	1660	rVB6	5158	8517	0.10%	0.015%
17	13.745	1822	1829	1842	rBV	2203172	3142583	38.48%	5.452%
18	14.022	1867	1876	1884	rBV	2586814	3824290	46.83%	6.635%
19	14.328	1921	1928	1941	rBV	1400909	2021705	24.76%	3.508%
20	14.534	1957	1963	1973	rBV	138481	252494	3.09%	0.438%
21	14.751	1995	2000	2003	rVB6	7267	10939	0.13%	0.019%
22	15.075	2052	2055	2060	rBV	10527	14453	0.18%	0.025%
23	15.322	2090	2097	2110	rBV	3318329	4934384	60.42%	8.561%
24	15.439	2111	2117	2131	rVV	951792	1351638	16.55%	2.345%
25	15.563	2133	2138	2143	rVB3	18863	32258	0.39%	0.056%
26	16.110	2225	2231	2237	rVB3	11382	18522	0.23%	0.032%
27	17.075	2389	2395	2405	rBV	1859522	2595224	31.78%	4.503%
28	17.175	2405	2412	2423	rBV	4342420	6081587	74.47%	10.552%
29	17.975	2544	2548	2554	rBV3	53892	67979	0.83%	0.118%
30	19.039	2724	2729	2734	rBV2	62105	84794	1.04%	0.147%
31	19.104	2736	2740	2745	rBV	51808	76739	0.94%	0.133%
32	19.263	2763	2767	2772	rBV5	35892	49681	0.61%	0.086%
33	19.416	2791	2793	2797	rBV3	11842	10940	0.13%	0.019%
34	19.475	2797	2803	2812	rBV	5400047	7504507	91.89%	13.020%
35	21.316	3110	3116	3122	rBV	2060190	3013228	36.90%	5.228%
36	24.051	3572	3581	3595	rBV2	3274328	8166600	100.00%	14.169%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030743.D
Acq On : 07 Apr 2024 16:04
Operator : MA/JU
Sample : P1987-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R62

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	24.251	3607	3615	3629	rVB2	1343668	3357589	41.11%	5.825%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 57636508

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030743.D
Acq On : 07 Apr 2024 16:04
Operator : MA/JU
Sample : P1987-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

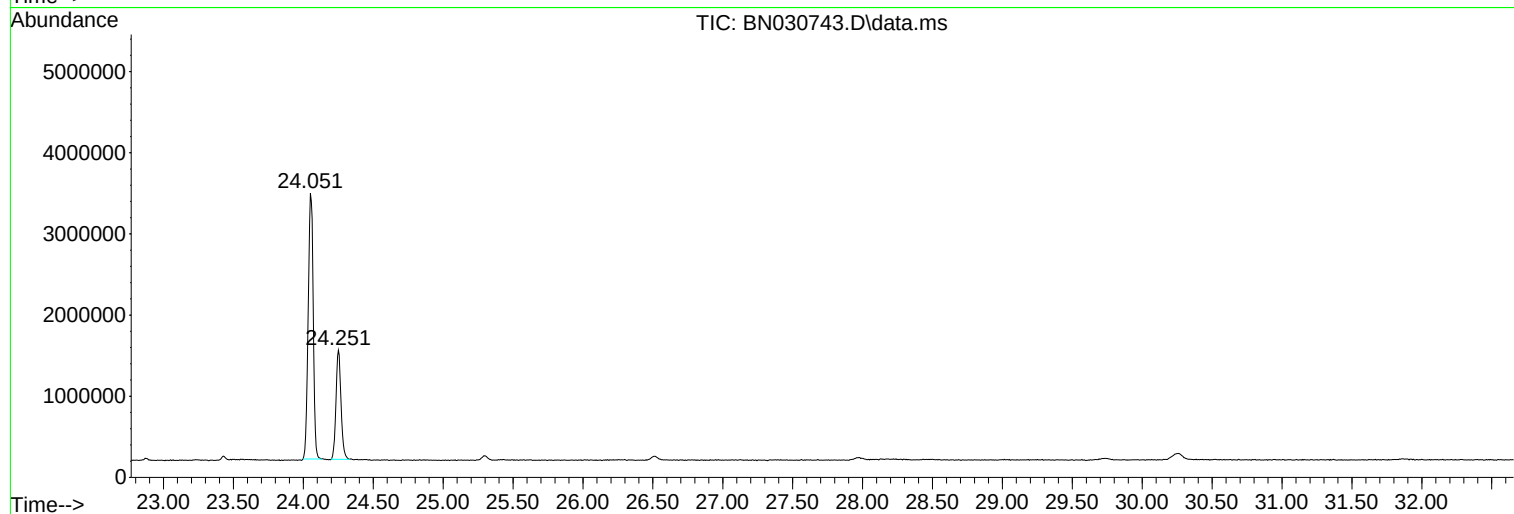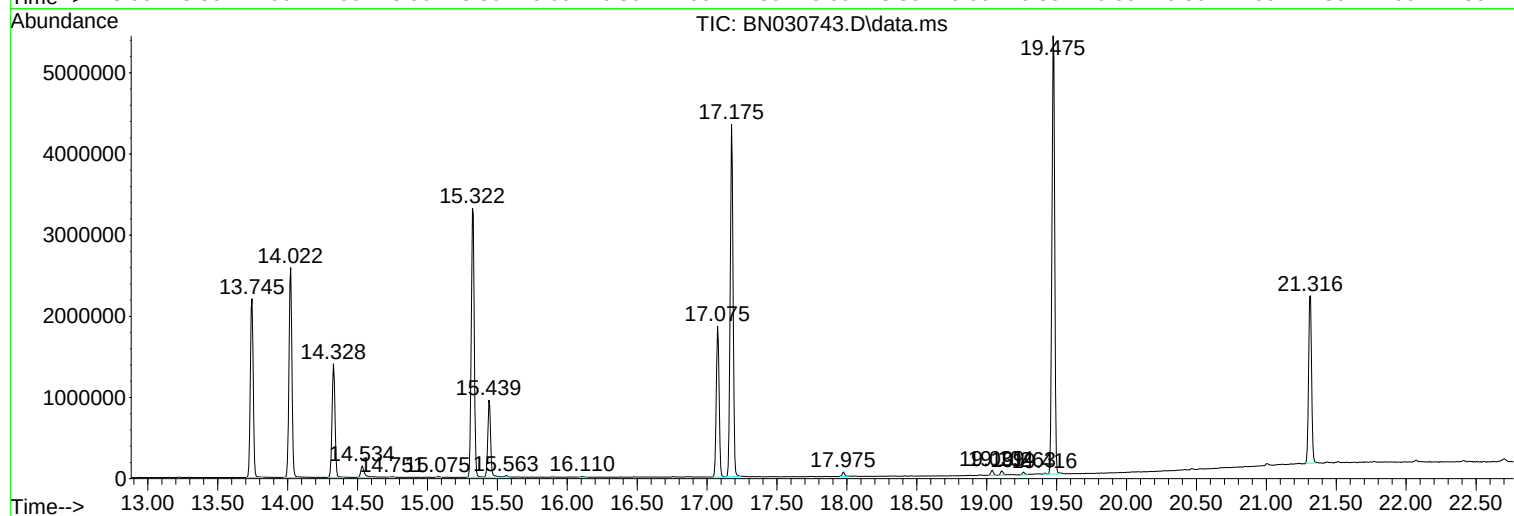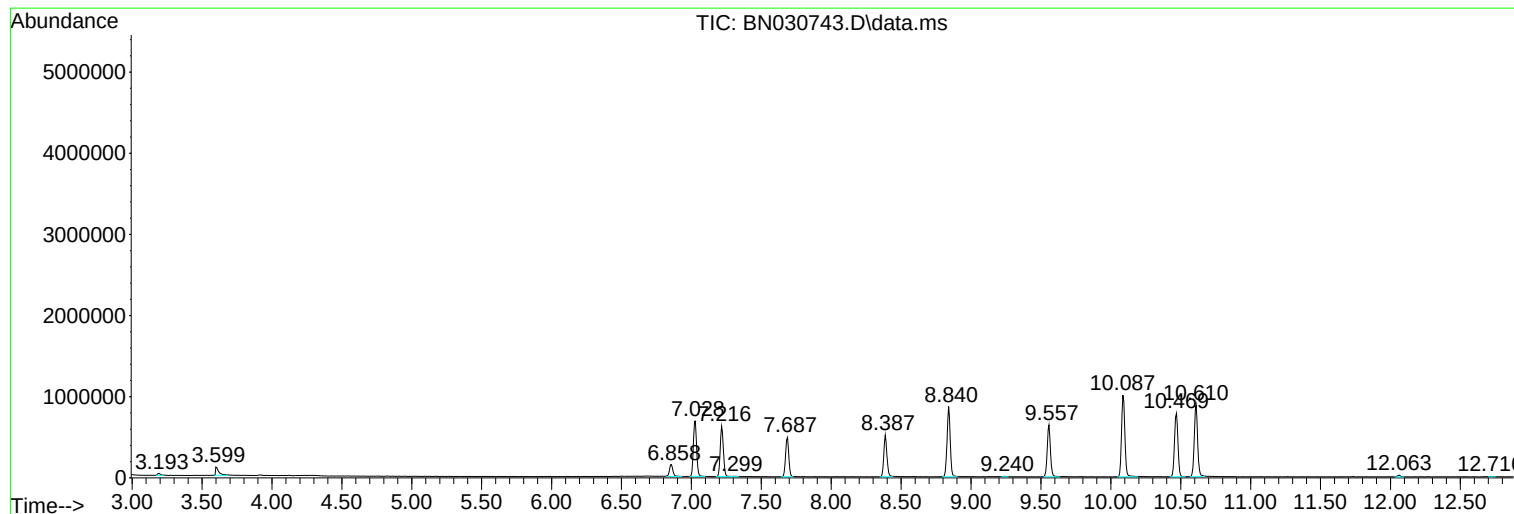

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030743.D
Acq On : 07 Apr 2024 16:04
Operator : MA/JU
Sample : P1987-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030743.D
Acq On : 07 Apr 2024 16:04
Operator : MA/JU
Sample : P1987-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MC0R62

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc