

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
 Data File : BN030746.D
 Acq On : 07 Apr 2024 18:02
 Operator : MA/JU
 Sample : P2017-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH5E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030746.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	31	34	43	rBV	33715	52423	0.65%	0.083%
2	3.458	75	80	84	rBV6	7094	13757	0.17%	0.022%
3	3.599	102	104	116	rBV	197530	331523	4.14%	0.527%
4	3.917	154	158	164	rVB5	7897	13369	0.17%	0.021%
5	4.275	215	219	224	rVB3	15657	22869	0.29%	0.036%
6	4.740	294	298	306	rVB9	5256	10260	0.13%	0.016%
7	5.205	373	377	384	rBV	18993	27065	0.34%	0.043%
8	6.569	605	609	616	rBV6	3288	8060	0.10%	0.013%
9	6.675	623	627	633	rBV4	10122	15236	0.19%	0.024%
10	6.852	651	657	670	rVB	196121	327322	4.09%	0.520%
11	7.028	680	687	698	rVB	704502	1123337	14.03%	1.785%
12	7.216	712	719	731	rBV	676486	1061960	13.27%	1.687%
13	7.310	731	735	740	rVB7	6913	12489	0.16%	0.020%
14	7.687	791	799	806	rBV	594005	966116	12.07%	1.535%
15	7.752	806	810	817	rVB4	11546	21235	0.27%	0.034%
16	8.387	911	918	933	rBV	617184	992640	12.40%	1.577%
17	8.504	933	938	944	rVB3	10220	19454	0.24%	0.031%
18	8.840	987	995	1004	rBV	875343	1416152	17.69%	2.250%
19	9.004	1019	1023	1029	rBV7	9920	15289	0.19%	0.024%
20	9.240	1056	1063	1071	rVB9	7459	17977	0.22%	0.029%
21	9.404	1087	1091	1099	rVB6	11923	21081	0.26%	0.033%
22	9.557	1108	1117	1131	rBV	676266	1103856	13.79%	1.754%
23	9.781	1150	1155	1160	rVB9	5390	11665	0.15%	0.019%
24	9.969	1180	1187	1190	rBV3	7718	13455	0.17%	0.021%
25	10.087	1197	1207	1219	rBV	1066730	1769714	22.11%	2.812%
26	10.251	1230	1235	1243	rVB7	8330	15186	0.19%	0.024%
27	10.469	1264	1272	1282	rBV	944298	1571651	19.63%	2.497%
28	10.610	1285	1296	1316	rBV	952658	1661405	20.75%	2.640%
29	10.869	1338	1340	1345	rVB5	5478	8669	0.11%	0.014%
30	10.934	1345	1351	1358	rVB6	7656	14681	0.18%	0.023%
31	11.010	1358	1364	1368	rBV	23818	40659	0.51%	0.065%
32	11.069	1369	1374	1379	rVV	20807	34147	0.43%	0.054%
33	11.122	1379	1383	1393	rVB4	15027	31399	0.39%	0.050%
34	11.210	1393	1398	1402	rBV2	14828	26362	0.33%	0.042%
35	11.251	1402	1405	1410	rVB7	5394	9345	0.12%	0.015%
36	12.063	1535	1543	1549	rVB2	22400	40579	0.51%	0.064%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
 Data File : BN030746.D
 Acq On : 07 Apr 2024 18:02
 Operator : MA/JU
 Sample : P2017-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH5E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	12.504	1610	1618	1623	rBV8	6339	14671	0.18%	0.023%
38	12.587	1627	1632	1637	rVV7	7440	14255	0.18%	0.023%
39	13.116	1717	1722	1726	rBV6	5758	9580	0.12%	0.015%
40	13.245	1736	1744	1749	rVB4	21876	52882	0.66%	0.084%

41	13.745	1822	1829	1835	rBV	2409231	3423320	42.76%	5.439%
42	13.787	1835	1836	1843	rVB	21657	24342	0.30%	0.039%
43	14.022	1865	1876	1886	rBV	2665554	4007282	50.06%	6.367%
44	14.328	1921	1928	1939	rBV	1652115	2361258	29.50%	3.752%
45	14.534	1957	1963	1978	rBV	193684	358865	4.48%	0.570%

46	14.745	1993	1999	2005	rVB5	13460	31416	0.39%	0.050%
47	14.816	2007	2011	2013	rBV4	8194	10618	0.13%	0.017%
48	14.904	2021	2026	2032	rBV2	38254	58754	0.73%	0.093%
49	15.139	2060	2066	2067	rBV3	6490	9898	0.12%	0.016%
50	15.322	2090	2097	2104	rBV	3557796	5337177	66.67%	8.480%

51	15.375	2104	2106	2111	rVV3	24988	34660	0.43%	0.055%
52	15.439	2111	2117	2134	rVV	984505	1396082	17.44%	2.218%
53	15.563	2134	2138	2142	rBV2	17441	26988	0.34%	0.043%
54	15.657	2150	2154	2158	rBV7	10287	16493	0.21%	0.026%
55	15.781	2171	2175	2182	rVB4	17955	28522	0.36%	0.045%

56	15.969	2204	2207	2211	rVV6	7504	8978	0.11%	0.014%
57	16.016	2211	2215	2218	rVV5	4875	9134	0.11%	0.015%
58	16.051	2219	2221	2227	rVV7	5983	11170	0.14%	0.018%
59	16.110	2227	2231	2237	rVB4	14239	20532	0.26%	0.033%
60	16.228	2246	2251	2255	rBV7	6247	10720	0.13%	0.017%

61	16.275	2255	2259	2263	rVB5	6096	8540	0.11%	0.014%
62	16.375	2273	2276	2280	rBV6	10499	12843	0.16%	0.020%
63	16.481	2287	2294	2299	rBV9	9426	17926	0.22%	0.028%
64	16.845	2351	2356	2359	rBV6	10855	18631	0.23%	0.030%
65	17.004	2379	2383	2387	rVB4	25405	31942	0.40%	0.051%

66	17.075	2387	2395	2405	rBV	2110831	3089632	38.60%	4.909%
67	17.175	2406	2412	2423	rVB	4383371	6277430	78.42%	9.974%
68	17.369	2441	2445	2450	rBV4	6758	11161	0.14%	0.018%
69	17.463	2457	2461	2467	rBV6	10629	22263	0.28%	0.035%
70	17.851	2523	2527	2532	rVB8	6429	10038	0.13%	0.016%

71	17.975	2544	2548	2555	rBV	118651	165609	2.07%	0.263%
72	18.051	2558	2561	2567	rVB	10742	17190	0.21%	0.027%
73	18.410	2619	2622	2626	rVB4	15484	18533	0.23%	0.029%
74	18.669	2661	2666	2669	rBV6	11693	19566	0.24%	0.031%
75	18.851	2693	2697	2702	rBV6	15413	24849	0.31%	0.039%

76	19.039	2724	2729	2734	rBV2	64615	88565	1.11%	0.141%
----	--------	------	------	------	------	-------	-------	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030746.D
Acq On : 07 Apr 2024 18:02
Operator : MA/JU
Sample : P2017-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5E7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M

Title : SVOA CALIBRATION

77	19.110	2736	2741	2744	rBV	57976	80916	1.01%	0.129%
78	19.145	2744	2747	2754	rVB2	71494	96696	1.21%	0.154%
79	19.263	2763	2767	2775	rBV	58424	89201	1.11%	0.142%
80	19.480	2797	2804	2816	rBV	5407459	7544418	94.25%	11.987%
81	21.010	3061	3064	3070	rVB5	46692	57551	0.72%	0.091%
82	21.316	3110	3116	3126	rBV	2308420	3420648	42.73%	5.435%
83	24.051	3572	3581	3597	rVB2	3195856	8004985	100.00%	12.719%
84	24.251	3606	3615	3630	rVB	1456406	3687445	46.06%	5.859%




Sum of corrected areas: 62936562

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030746.D
Acq On : 07 Apr 2024 18:02
Operator : MA/JU
Sample : P2017-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5E7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

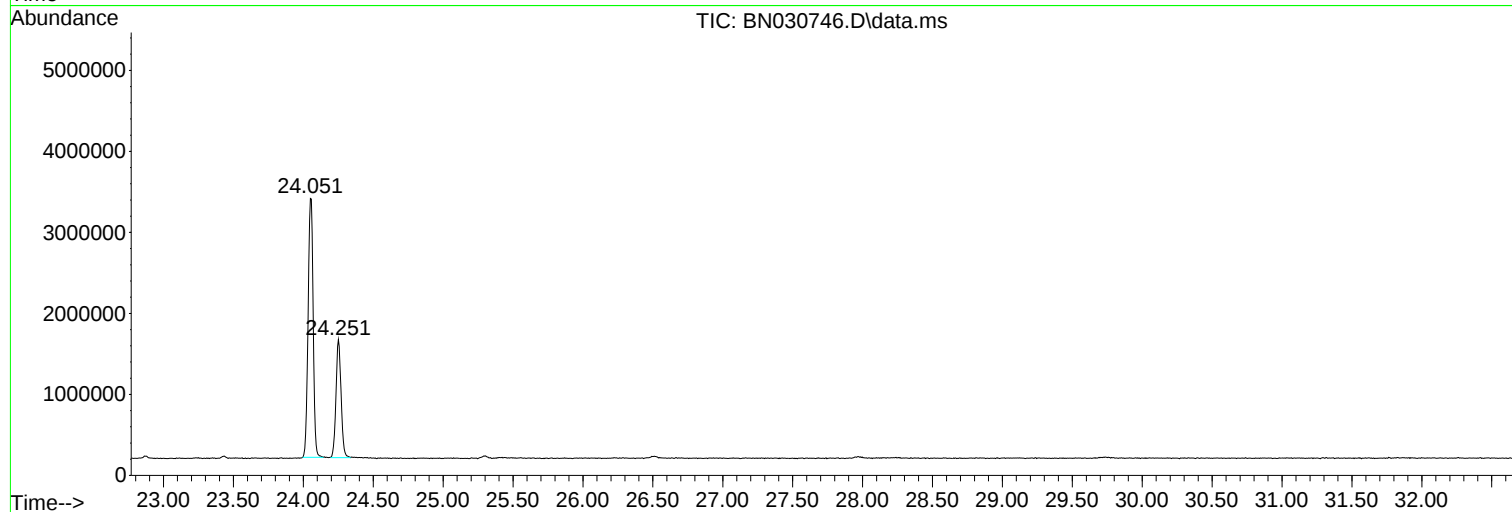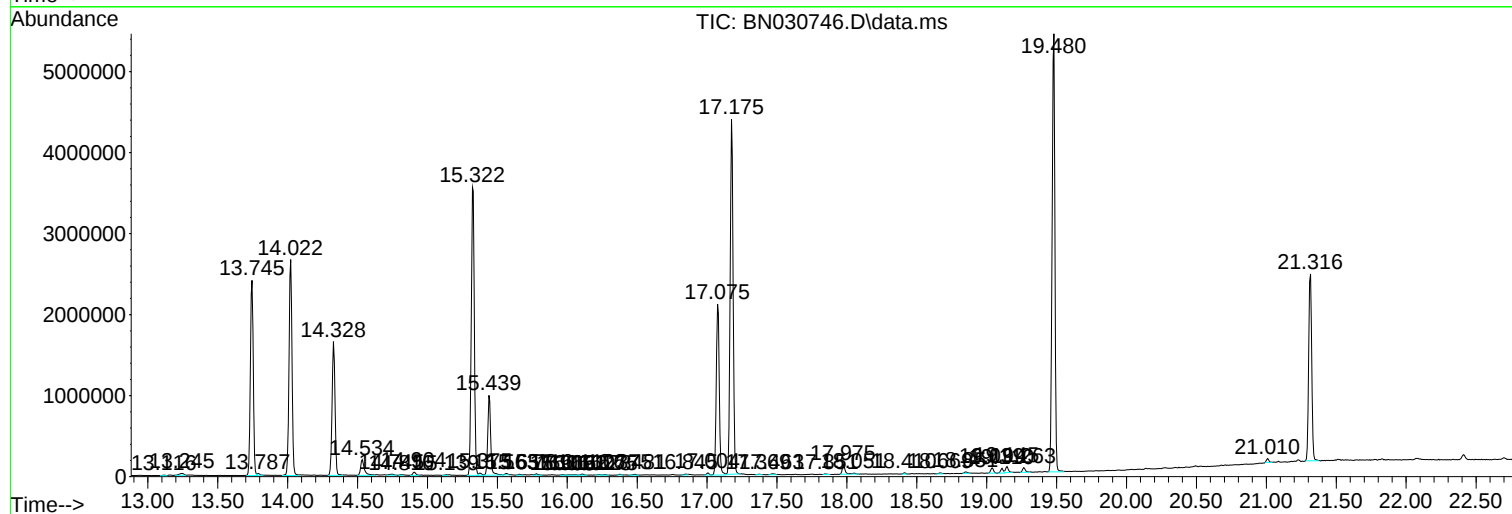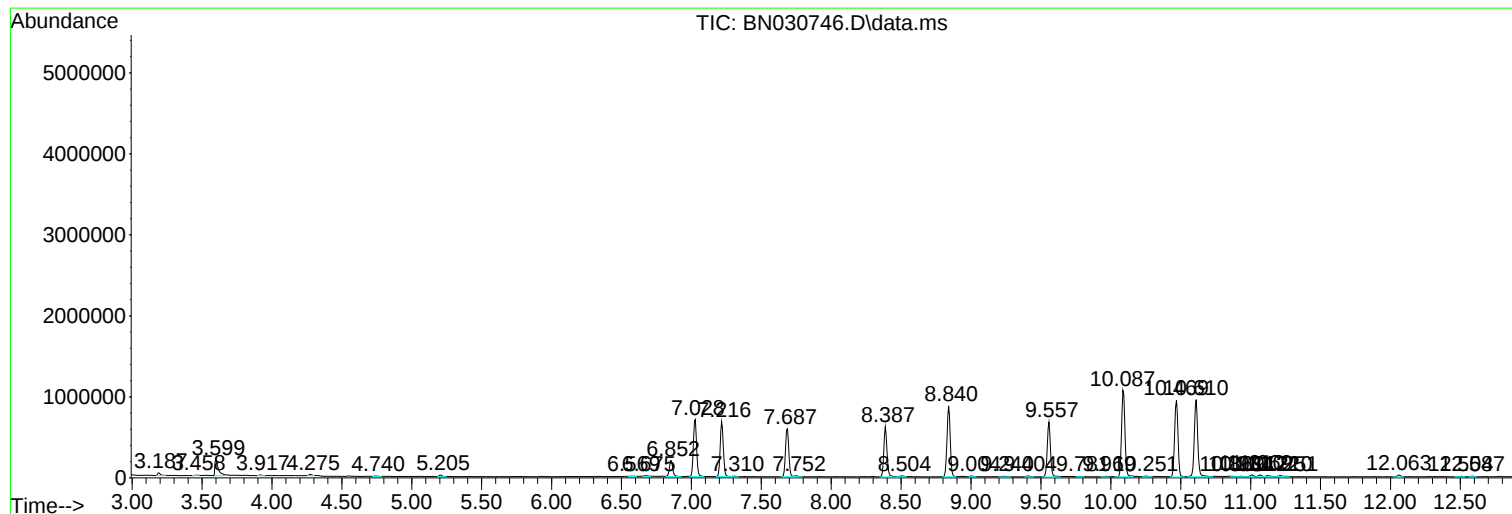

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030746.D
Acq On : 07 Apr 2024 18:02
Operator : MA/JU
Sample : P2017-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5E7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030746.D
Acq On : 07 Apr 2024 18:02
Operator : MA/JU
Sample : P2017-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5E7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc