

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
 Data File : BN030748.D
 Acq On : 07 Apr 2024 19:21
 Operator : MA/JU
 Sample : P2017-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH5E4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030748.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	31	34	41	rBV	28791	40845	0.61%	0.077%
2	3.599	101	104	119	rBV	148480	266657	3.97%	0.502%
3	3.917	155	158	164	rVB3	6001	9893	0.15%	0.019%
4	4.275	216	219	223	rBV5	5618	7512	0.11%	0.014%
5	6.858	652	658	665	rBV	165432	271783	4.04%	0.512%
6	7.022	680	686	701	rVB	587110	957860	14.24%	1.804%
7	7.216	711	719	730	rBV	578348	901823	13.41%	1.698%
8	7.687	792	799	806	rBV	555746	912514	13.57%	1.718%
9	7.746	807	809	814	rVB3	5315	6862	0.10%	0.013%
10	8.387	911	918	932	rBV	527883	833860	12.40%	1.570%
11	8.499	932	937	943	rVB6	5363	11661	0.17%	0.022%
12	8.840	987	995	1003	rBV	731282	1176384	17.49%	2.215%
13	8.999	1019	1022	1031	rVB10	7643	15310	0.23%	0.029%
14	9.558	1109	1117	1132	rBV	540686	891189	13.25%	1.678%
15	9.716	1139	1144	1149	rVB8	4400	8340	0.12%	0.016%
16	9.887	1169	1173	1179	rVB6	4691	7989	0.12%	0.015%
17	9.969	1182	1187	1193	rVB7	4756	7203	0.11%	0.014%
18	10.087	1200	1207	1224	rBV	896248	1475522	21.94%	2.778%
19	10.469	1264	1272	1280	rBV	897366	1496467	22.25%	2.818%
20	10.610	1284	1296	1314	rBV	680173	1186615	17.65%	2.234%
21	10.934	1345	1351	1356	rVB9	4408	8245	0.12%	0.016%
22	11.005	1358	1363	1368	rVV	12071	19068	0.28%	0.036%
23	11.063	1368	1373	1379	rVV	14167	25396	0.38%	0.048%
24	11.116	1379	1382	1390	rVB4	6132	12392	0.18%	0.023%
25	11.263	1401	1407	1408	rBV5	3716	6884	0.10%	0.013%
26	11.281	1408	1410	1415	rVB6	5202	7434	0.11%	0.014%
27	12.057	1538	1542	1548	rBV	17439	28555	0.42%	0.054%
28	12.781	1660	1665	1671	rVB4	4512	7740	0.12%	0.015%
29	12.940	1687	1692	1696	rVB6	4855	8568	0.13%	0.016%
30	13.222	1735	1740	1748	rBV2	14918	31531	0.47%	0.059%
31	13.746	1820	1829	1835	rBV	1921276	2713765	40.36%	5.110%
32	14.022	1867	1876	1886	rBV	2173208	3280225	48.78%	6.177%
33	14.328	1920	1928	1936	rBV	1557710	2263451	33.66%	4.262%
34	14.534	1957	1963	1981	rBV	152595	303752	4.52%	0.572%
35	14.746	1996	1999	2005	rVB7	5569	9261	0.14%	0.017%
36	14.904	2020	2026	2031	rBV4	13325	22483	0.33%	0.042%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
 Data File : BN030748.D
 Acq On : 07 Apr 2024 19:21
 Operator : MA/JU
 Sample : P2017-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH5E4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	15.322	2090	2097	2103	rBV	3020704	4289676	63.79%	8.078%
38	15.440	2111	2117	2129	rBV	753584	1073810	15.97%	2.022%
39	15.563	2133	2138	2143	rVB4	16323	27501	0.41%	0.052%
40	16.104	2226	2230	2236	rVB7	10291	16520	0.25%	0.031%
41	16.863	2353	2359	2364	rBV5	8769	13949	0.21%	0.026%
42	17.075	2389	2395	2405	rBV	2078993	2895765	43.06%	5.453%
43	17.175	2405	2412	2429	rVV	3528004	5096906	75.80%	9.598%
44	17.475	2458	2463	2469	rVB8	7050	13524	0.20%	0.025%
45	17.751	2506	2510	2515	rVB7	10434	14244	0.21%	0.027%
46	17.810	2515	2520	2522	rBV5	5536	7977	0.12%	0.015%
47	17.975	2543	2548	2555	rBV	72384	103370	1.54%	0.195%
48	18.051	2558	2561	2565	rVB4	7914	11945	0.18%	0.022%
49	18.410	2619	2622	2626	rVB4	12939	16146	0.24%	0.030%
50	19.039	2724	2729	2733	rBV2	52679	67376	1.00%	0.127%
51	19.110	2737	2741	2744	rBV	42767	54604	0.81%	0.103%
52	19.139	2744	2746	2750	rVB4	12956	15854	0.24%	0.030%
53	19.263	2764	2767	2773	rBV3	33230	40348	0.60%	0.076%
54	19.475	2797	2803	2813	rBV	4389163	6144073	91.37%	11.569%
55	21.316	3110	3116	3123	rBV	2382622	3446967	51.26%	6.491%
56	24.057	3572	3582	3592	rBV2	2775837	6724447	100.00%	12.662%
57	24.251	3606	3615	3627	rBV2	1515318	3796300	56.46%	7.148%




Sum of corrected areas: 53106341

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030748.D
Acq On : 07 Apr 2024 19:21
Operator : MA/JU
Sample : P2017-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5E4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

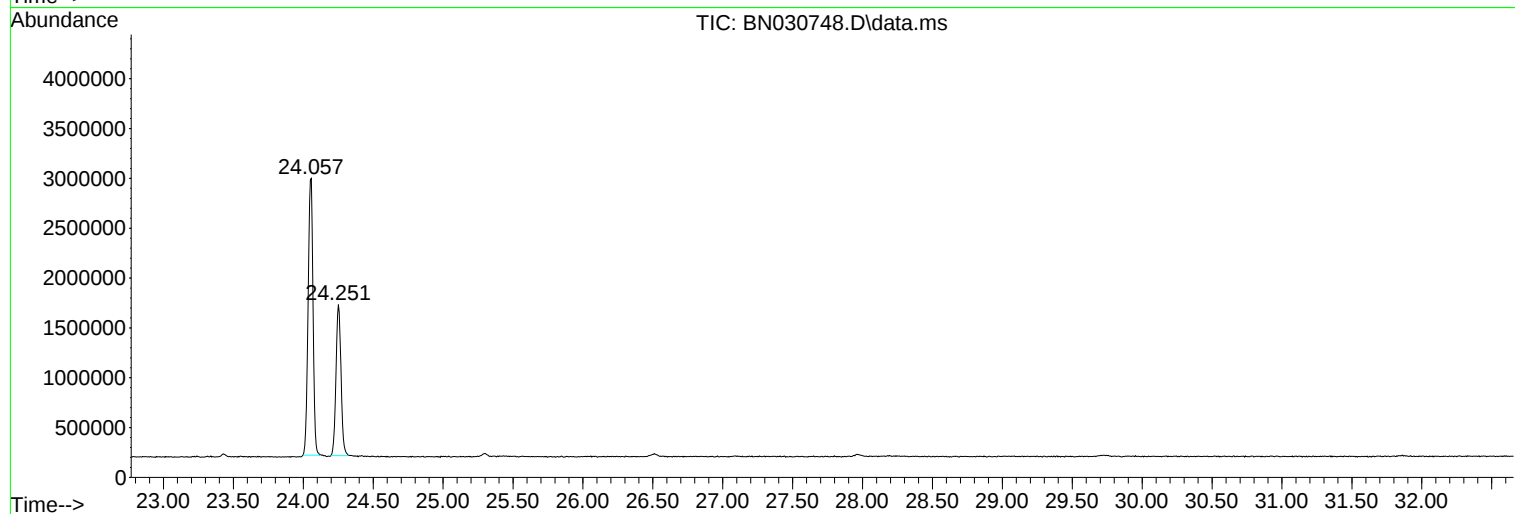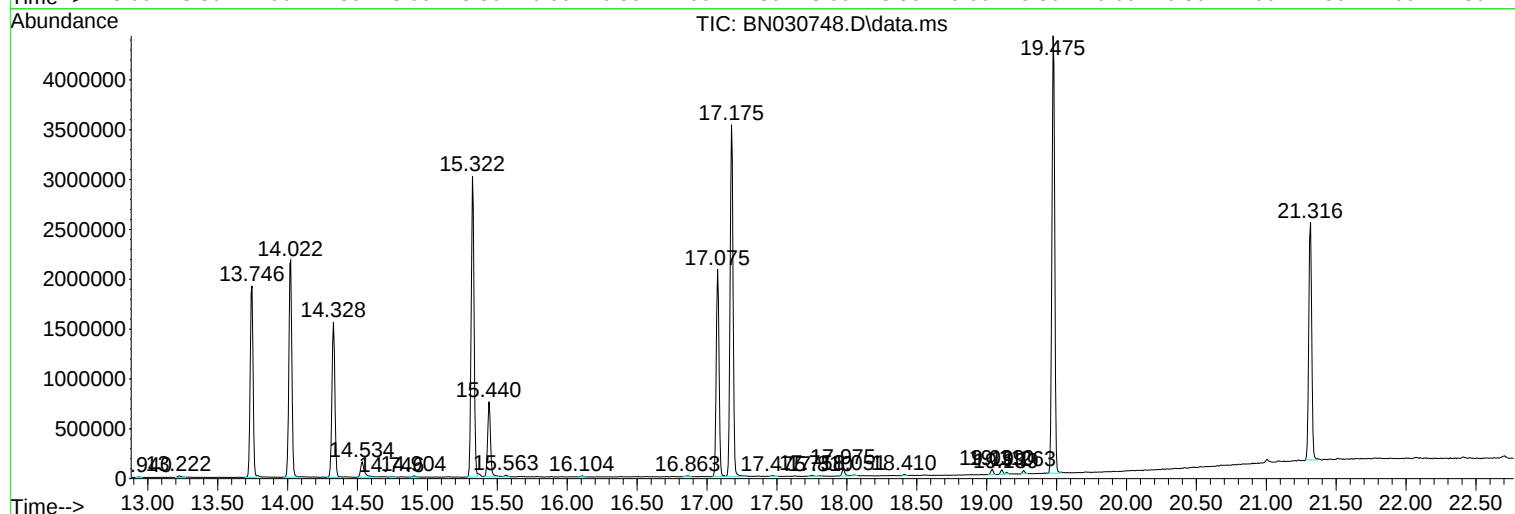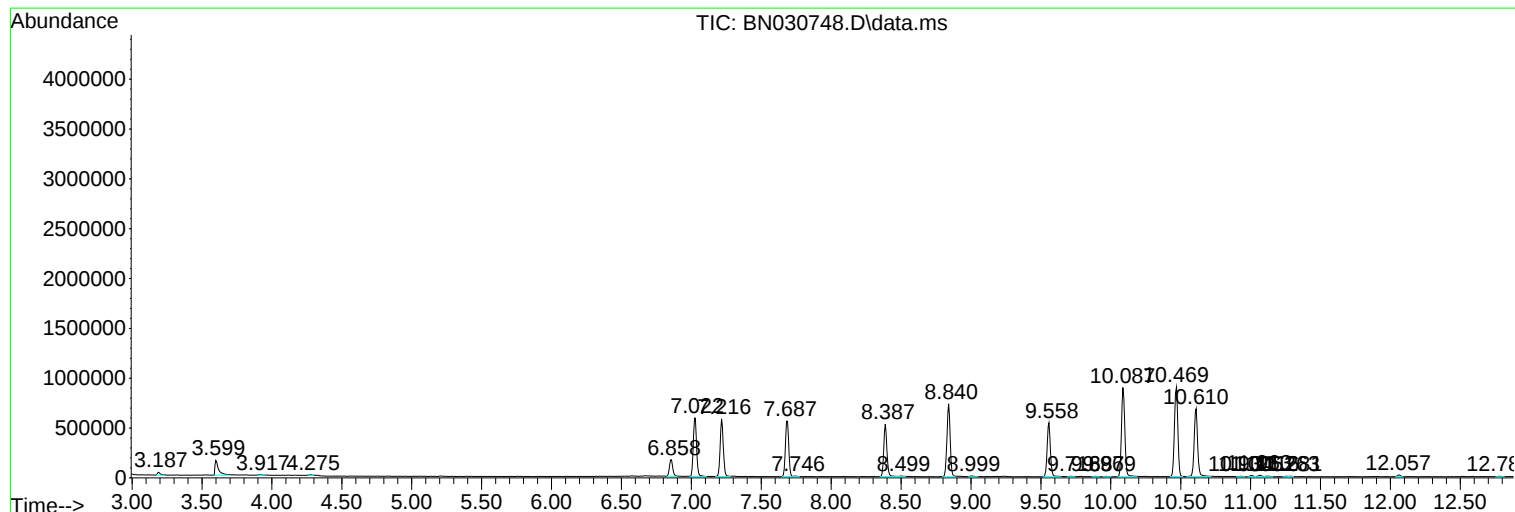

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030748.D
Acq On : 07 Apr 2024 19:21
Operator : MA/JU
Sample : P2017-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5E4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030748.D
Acq On : 07 Apr 2024 19:21
Operator : MA/JU
Sample : P2017-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5E4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc