

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
 Data File : BN030750.D
 Acq On : 07 Apr 2024 20:39
 Operator : MA/JU
 Sample : PB160077BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK077

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030750.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	31	34	47	rVB	33788	52145	0.98%	0.106%
2	3.593	101	103	126	rBV	454950	782620	14.76%	1.590%
3	3.917	153	158	161	rBV5	8269	10946	0.21%	0.022%
4	6.852	650	657	667	rBV	593145	944942	17.82%	1.920%
5	7.028	680	687	700	rVB	502547	813636	15.34%	1.653%
6	7.216	710	719	731	rBV	614436	970856	18.31%	1.973%
7	7.687	792	799	807	rBV	586448	947796	17.87%	1.926%
8	8.387	911	918	929	rBV	777924	1251233	23.59%	2.542%
9	8.840	988	995	1011	rBV	610779	991863	18.70%	2.015%
10	9.557	1110	1117	1132	rBV	472862	772320	14.56%	1.569%
11	10.087	1199	1207	1218	rBV	800573	1330768	25.09%	2.704%
12	10.469	1263	1272	1280	rBV	918261	1536517	28.97%	3.122%
13	10.610	1288	1296	1311	rBV	852275	1467141	27.66%	2.981%
14	12.057	1538	1542	1550	rVB2	14524	24681	0.47%	0.050%
15	13.228	1734	1741	1746	rBV3	8387	15088	0.28%	0.031%
16	13.745	1822	1829	1838	rBV	1612462	2301948	43.41%	4.677%
17	14.022	1869	1876	1886	rBV	1798594	2758888	52.02%	5.606%
18	14.328	1921	1928	1938	rBV	1614408	2337891	44.08%	4.750%
19	14.528	1956	1962	1979	rBV	620890	1053117	19.86%	2.140%
20	15.322	2090	2097	2110	rBV	2495800	3562735	67.18%	7.239%
21	15.439	2111	2117	2126	rBV	590272	800393	15.09%	1.626%
22	15.563	2133	2138	2143	rVB3	12434	19052	0.36%	0.039%
23	16.110	2225	2231	2238	rBV8	7561	13563	0.26%	0.028%
24	17.075	2389	2395	2405	rBV	2166677	2966802	55.94%	6.028%
25	17.175	2405	2412	2427	rVV	2943656	4018328	75.77%	8.165%
26	19.039	2724	2729	2735	rBV2	34004	50497	0.95%	0.103%
27	19.110	2737	2741	2747	rVB	29961	41041	0.77%	0.083%
28	19.475	2797	2803	2812	rBV	3497621	4843709	91.33%	9.842%
29	21.310	3110	3115	3123	rBV2	2330261	3435585	64.78%	6.981%
30	24.051	3572	3581	3598	rVB2	2199597	5303308	100.00%	10.776%
31	24.251	3606	3615	3628	rVB	1548303	3794572	71.55%	7.710%




Sum of corrected areas: 49213981

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030750.D
Acq On : 07 Apr 2024 20:39
Operator : MA/JU
Sample : PB160077BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK077

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

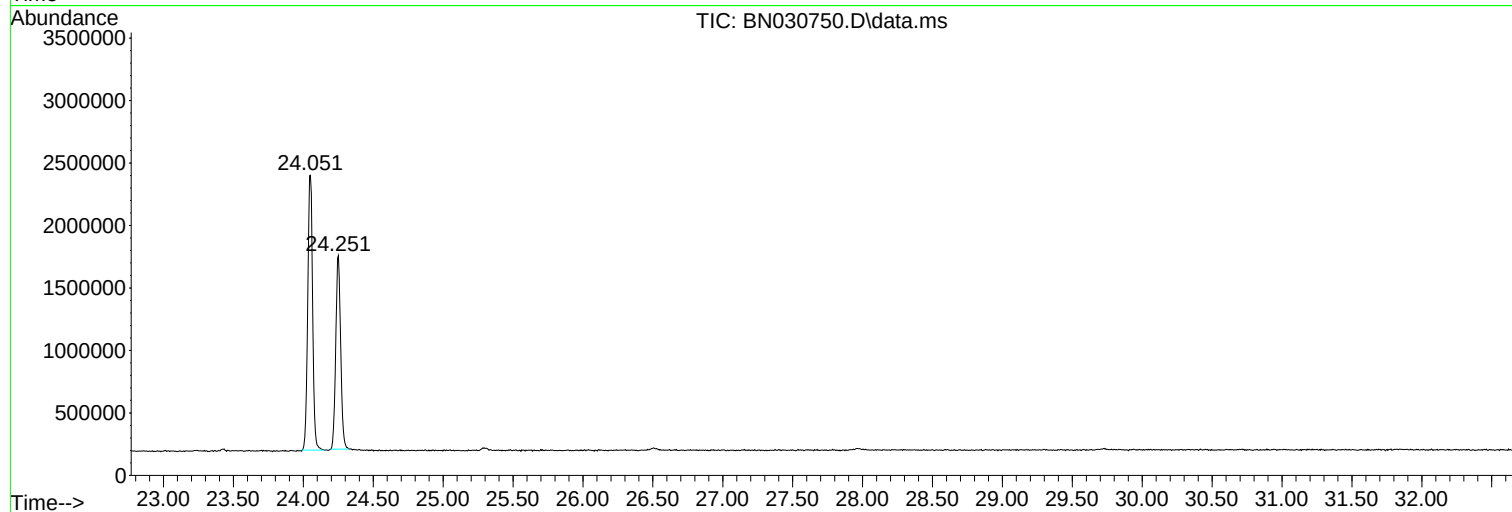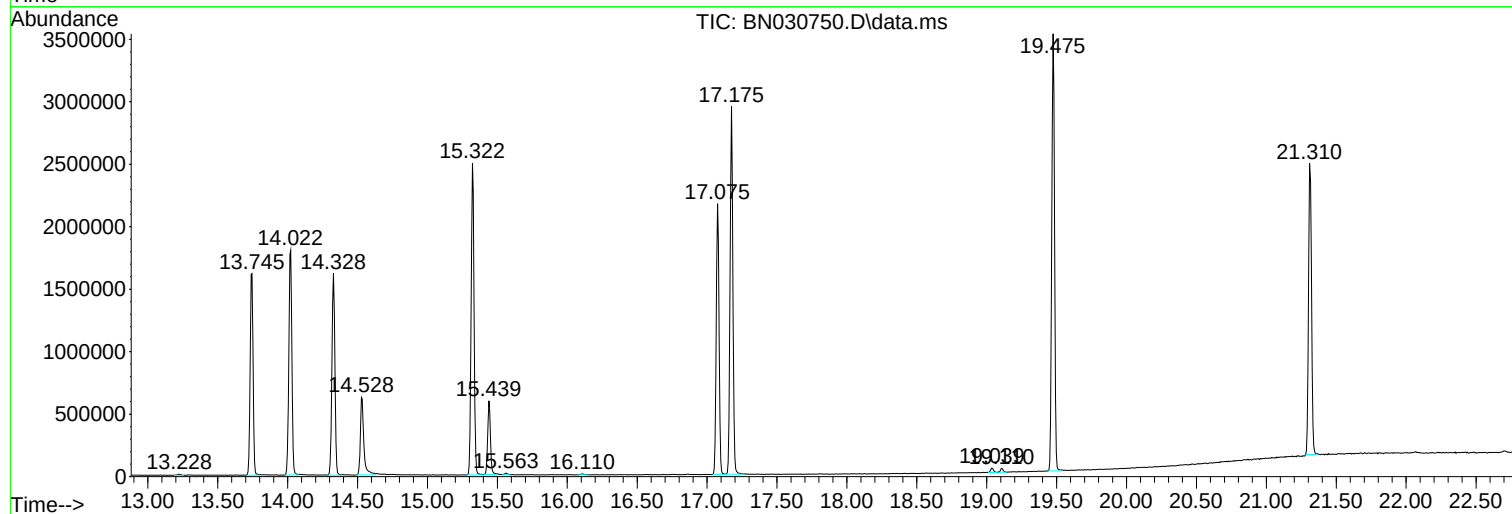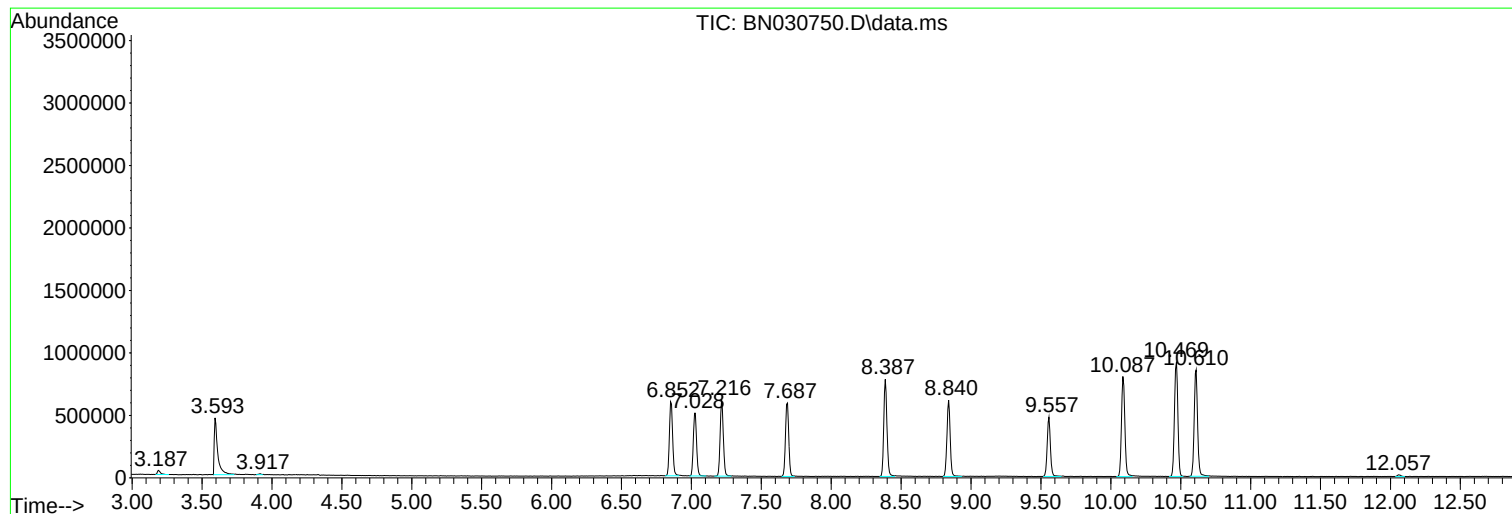

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030750.D
Acq On : 07 Apr 2024 20:39
Operator : MA/JU
Sample : PB160077BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK077

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030750.D
Acq On : 07 Apr 2024 20:39
Operator : MA/JU
Sample : PB160077BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK077

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------