

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
 Data File : BN030756.D
 Acq On : 08 Apr 2024 01:14
 Operator : MA/JU
 Sample : P2017-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH5E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030756.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	47	rVB	33156	54121	0.71%	0.094%
2	3.599	101	104	124	rBV	152691	275106	3.60%	0.476%
3	3.911	154	157	161	rBV4	6645	10392	0.14%	0.018%
4	4.993	336	341	348	rVB5	8442	14601	0.19%	0.025%
5	5.199	374	376	385	rVB8	5840	10658	0.14%	0.018%
6	6.852	651	657	667	rVB	204569	322596	4.22%	0.558%
7	7.022	680	686	700	rVB	666019	1072800	14.04%	1.855%
8	7.216	712	719	731	rBV	672659	1038753	13.59%	1.796%
9	7.681	791	798	806	rBV	571512	920978	12.05%	1.592%
10	7.746	806	809	818	rVB6	6679	13919	0.18%	0.024%
11	8.387	910	918	929	rBV	623004	972395	12.72%	1.681%
12	8.505	934	938	944	rVB3	7179	13156	0.17%	0.023%
13	8.840	987	995	1005	rBV	839206	1339370	17.52%	2.316%
14	9.557	1106	1117	1124	rBV	626083	1025922	13.42%	1.774%
15	9.710	1141	1143	1151	rVB8	5915	9871	0.13%	0.017%
16	9.775	1151	1154	1159	rBV6	4097	8071	0.11%	0.014%
17	9.969	1181	1187	1190	rBV3	5184	9289	0.12%	0.016%
18	10.087	1198	1207	1229	rBV	1027053	1702919	22.28%	2.945%
19	10.257	1231	1236	1240	rVB6	6440	11530	0.15%	0.020%
20	10.469	1264	1272	1285	rBV	872291	1495606	19.57%	2.586%
21	10.604	1285	1295	1318	rBV	699658	1240353	16.23%	2.145%
22	10.928	1346	1350	1358	rBV8	4838	9181	0.12%	0.016%
23	11.004	1358	1363	1369	rVV2	12123	20491	0.27%	0.035%
24	11.063	1369	1373	1378	rVV	15865	24753	0.32%	0.043%
25	11.122	1378	1383	1388	rVB	10702	19110	0.25%	0.033%
26	12.057	1536	1542	1548	rVB	19848	33426	0.44%	0.058%
27	13.222	1734	1740	1747	rBV6	11541	19233	0.25%	0.033%
28	13.740	1821	1828	1834	rBV	2230310	3064489	40.09%	5.299%
29	13.787	1834	1836	1844	rVB4	17127	26266	0.34%	0.045%
30	14.022	1869	1876	1885	rBV	2423283	3691564	48.30%	6.383%
31	14.328	1921	1928	1938	rBV	1516259	2238742	29.29%	3.871%
32	14.410	1938	1942	1944	rVB4	6874	8206	0.11%	0.014%
33	14.534	1956	1963	1978	rBV	186284	354438	4.64%	0.613%
34	14.692	1986	1990	1993	rVB6	7171	10730	0.14%	0.019%
35	14.745	1995	1999	2004	rVB8	7259	12614	0.17%	0.022%
36	14.810	2007	2010	2015	rVB6	5953	8326	0.11%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
 Data File : BN030756.D
 Acq On : 08 Apr 2024 01:14
 Operator : MA/JU
 Sample : P2017-04
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH5E5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	14.904	2022	2026	2030	rBV4	11981	15877	0.21%	0.027%
38	15.322	2090	2097	2104	rBV	3374070	4805110	62.86%	8.309%
39	15.439	2111	2117	2134	rBV	910494	1268816	16.60%	2.194%
40	15.563	2134	2138	2144	rVB3	18495	28356	0.37%	0.049%
41	16.010	2210	2214	2218	rBV7	5119	8616	0.11%	0.015%
42	16.104	2226	2230	2235	rBV5	12418	17733	0.23%	0.031%
43	16.751	2337	2340	2345	rVB7	7473	8338	0.11%	0.014%
44	16.851	2352	2357	2362	rBV5	5550	12304	0.16%	0.021%
45	17.075	2389	2395	2405	rBV	1990602	2856879	37.38%	4.940%
46	17.175	2405	2412	2423	rBV2	3882037	5686970	74.40%	9.833%
47	17.751	2506	2510	2515	rVB7	10664	14825	0.19%	0.026%
48	17.975	2540	2548	2556	rBV2	73856	113933	1.49%	0.197%
49	18.045	2559	2560	2565	rVB3	5981	8545	0.11%	0.015%
50	19.039	2724	2729	2734	rBV2	59323	79510	1.04%	0.137%
51	19.110	2736	2741	2744	rBV	50162	70841	0.93%	0.122%
52	19.139	2744	2746	2755	rVB6	22113	33933	0.44%	0.059%
53	19.263	2763	2767	2772	rBV4	35039	52216	0.68%	0.090%
54	19.475	2797	2803	2810	rBV	5152200	6983921	91.37%	12.076%
55	21.310	3109	3115	3124	rBV	2295735	3368848	44.07%	5.825%
56	24.045	3571	3580	3595	rBV2	3108910	7643686	100.00%	13.217%
57	24.245	3606	3614	3630	rVB	1408341	3650122	47.75%	6.311%




Sum of corrected areas: 57833354

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030756.D
Acq On : 08 Apr 2024 01:14
Operator : MA/JU
Sample : P2017-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5E5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

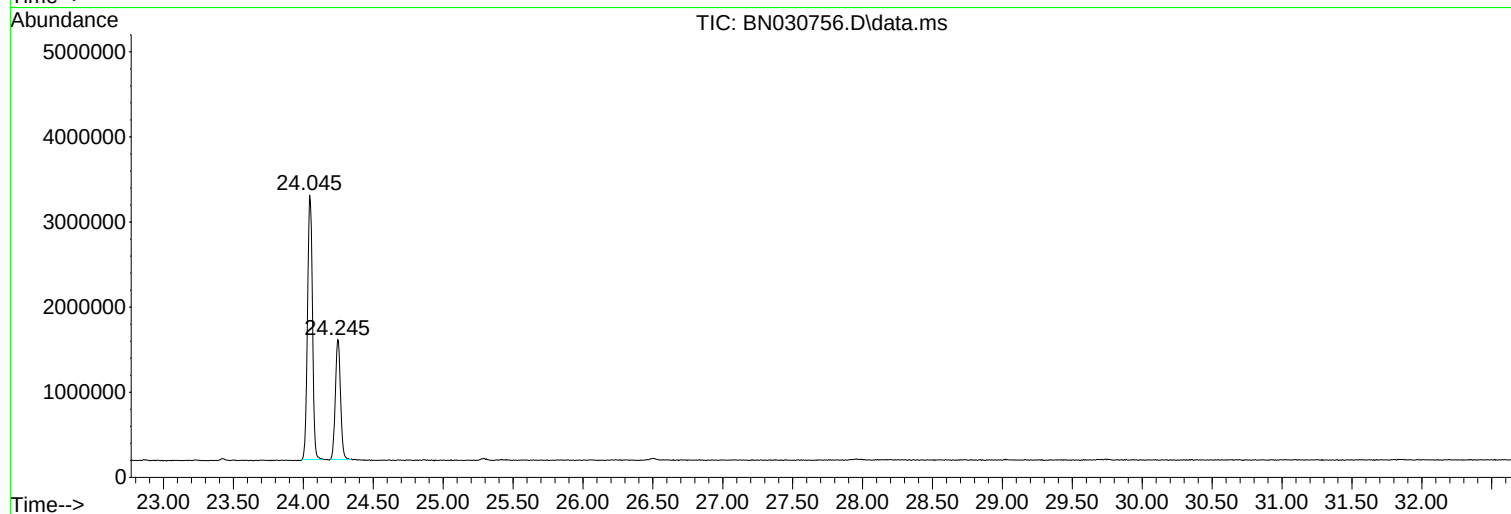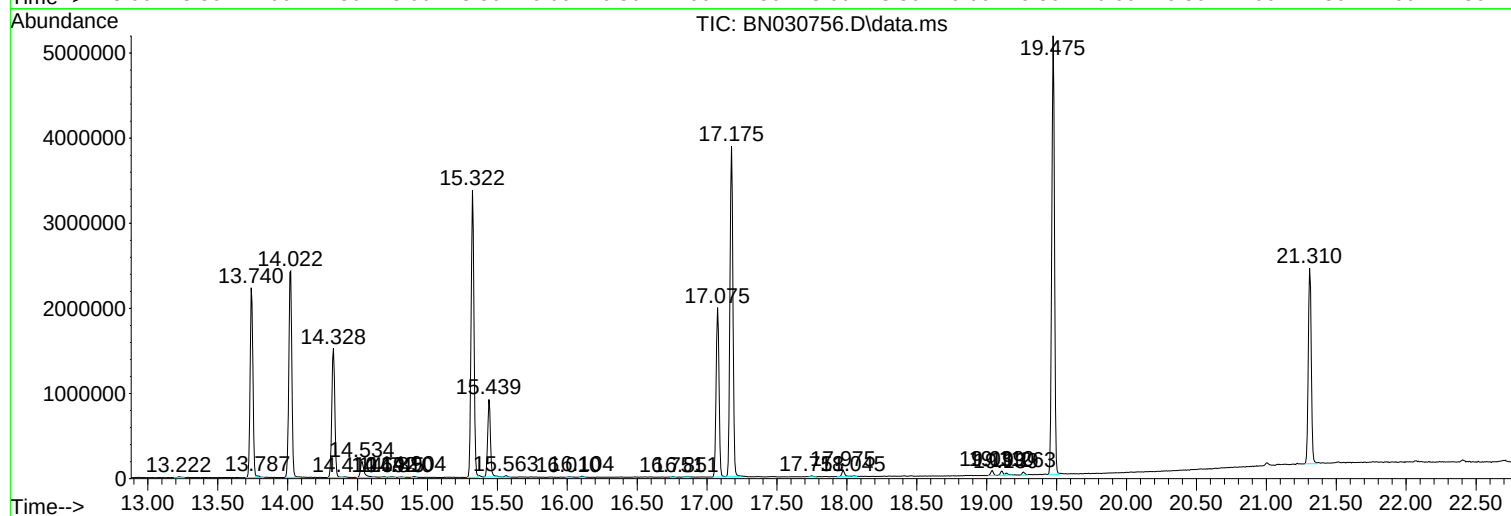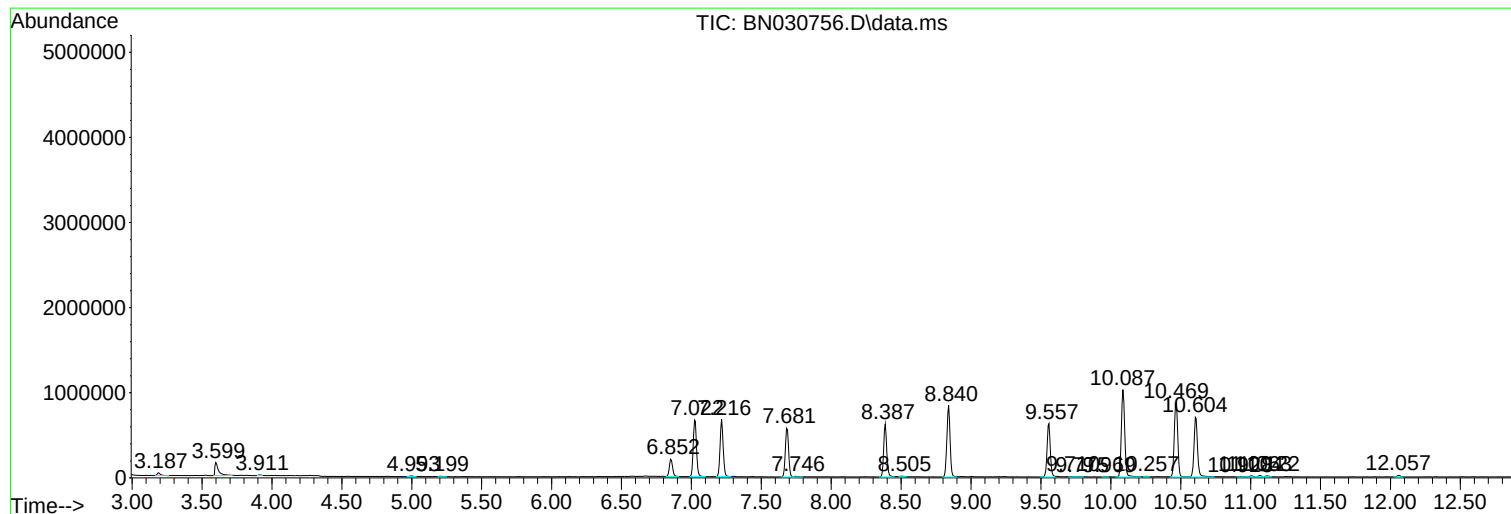

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030756.D
Acq On : 08 Apr 2024 01:14
Operator : MA/JU
Sample : P2017-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5E5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030756.D
Acq On : 08 Apr 2024 01:14
Operator : MA/JU
Sample : P2017-04
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5E5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------