

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
 Data File : BN030758.D
 Acq On : 08 Apr 2024 02:32
 Operator : MA/JU
 Sample : P2017-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH5E9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030758.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.193	31	35	41	rBV	24506	33429	0.42%	0.063%
2	3.599	102	104	124	rBV	211912	369901	4.61%	0.693%
3	3.911	154	157	161	rBV3	7278	10503	0.13%	0.020%
4	6.852	652	657	668	rVB	142127	236827	2.95%	0.444%
5	7.022	680	686	699	rVB	586538	931673	11.60%	1.745%
6	7.216	712	719	730	rBV	484833	758879	9.45%	1.421%
7	7.311	730	735	741	rVB10	6516	12297	0.15%	0.023%
8	7.681	791	798	806	rBV	542465	879797	10.95%	1.648%
9	7.740	806	808	815	rVB5	8143	14906	0.19%	0.028%
10	8.387	911	918	930	rBV	461486	731377	9.11%	1.370%
11	8.505	935	938	944	rVB4	7399	10840	0.13%	0.020%
12	8.840	985	995	1012	rBV	717311	1160185	14.44%	2.173%
13	8.999	1018	1022	1027	rVB7	9064	13484	0.17%	0.025%
14	9.240	1058	1063	1071	rVB6	7891	17575	0.22%	0.033%
15	9.410	1087	1092	1096	rVB6	8713	13668	0.17%	0.026%
16	9.557	1109	1117	1131	rBV	267910	454114	5.65%	0.851%
17	10.087	1200	1207	1220	rBV	694897	1152163	14.34%	2.158%
18	10.463	1264	1271	1282	rBV	817991	1389056	17.29%	2.602%
19	10.604	1289	1295	1306	rBV	709782	1198702	14.92%	2.245%
20	11.010	1358	1364	1368	rBV	12957	22209	0.28%	0.042%
21	11.069	1369	1374	1379	rVV2	13534	21790	0.27%	0.041%
22	11.210	1391	1398	1405	rBV2	15278	30287	0.38%	0.057%
23	12.057	1535	1542	1547	rBV	17578	29729	0.37%	0.056%
24	13.228	1733	1741	1748	rBV3	17184	35279	0.44%	0.066%
25	13.740	1822	1828	1835	rBV	1899944	2709784	33.74%	5.075%
26	14.022	1865	1876	1886	rBV	2119727	3214980	40.03%	6.021%
27	14.328	1921	1928	1935	rBV	1432055	2078368	25.88%	3.893%
28	14.551	1958	1966	1977	rBV5	19829	57028	0.71%	0.107%
29	14.904	2021	2026	2033	rBV2	18691	28763	0.36%	0.054%
30	15.140	2061	2066	2073	rVB4	6642	11416	0.14%	0.021%
31	15.322	2090	2097	2108	rBV	3062963	4354348	54.21%	8.155%
32	15.440	2113	2117	2126	rVB3	22010	40111	0.50%	0.075%
33	15.563	2132	2138	2143	rBV3	11356	18062	0.22%	0.034%
34	16.104	2227	2230	2235	rVB4	10064	14990	0.19%	0.028%
35	16.845	2351	2356	2358	rBV4	6366	10855	0.14%	0.020%
36	17.004	2379	2383	2387	rVB2	22152	25260	0.31%	0.047%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
 Data File : BN030758.D
 Acq On : 08 Apr 2024 02:32
 Operator : MA/JU
 Sample : P2017-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH5E9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

37	17.075	2389	2395	2405	rBV	1957868	2747591	34.21%	5.146%
38	17.175	2405	2412	2425	rVV	4052686	5630800	70.11%	10.546%
39	17.275	2425	2429	2433	rVB5	10950	16238	0.20%	0.030%
40	17.463	2456	2461	2468	rBV9	11247	23874	0.30%	0.045%
41	17.751	2507	2510	2515	rVB5	9158	15520	0.19%	0.029%
42	17.804	2515	2519	2524	rBV8	6191	12437	0.15%	0.023%
43	17.975	2545	2548	2553	rVB5	12154	13720	0.17%	0.026%
44	18.410	2618	2622	2626	rBV4	18365	19919	0.25%	0.037%
45	18.845	2692	2696	2705	rBV7	20536	47852	0.60%	0.090%
46	19.039	2724	2729	2735	rVB2	53070	76911	0.96%	0.144%
47	19.110	2736	2741	2744	rBV	47335	70452	0.88%	0.132%
48	19.263	2764	2767	2772	rBV5	10325	17439	0.22%	0.033%
49	19.475	2797	2803	2815	rBV2	5177524	7028128	87.50%	13.163%
50	21.010	3059	3064	3073	rBV5	68656	139917	1.74%	0.262%
51	21.310	3109	3115	3122	rBV2	2318511	3376514	42.04%	6.324%
52	22.869	3375	3380	3388	rVB	195016	318753	3.97%	0.597%
53	24.051	3571	3581	3598	rVB2	3249650	8031910	100.00%	15.043%
54	24.245	3606	3614	3629	rVB	1471073	3712419	46.22%	6.953%




Sum of corrected areas: 53393029

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030758.D
Acq On : 08 Apr 2024 02:32
Operator : MA/JU
Sample : P2017-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5E9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

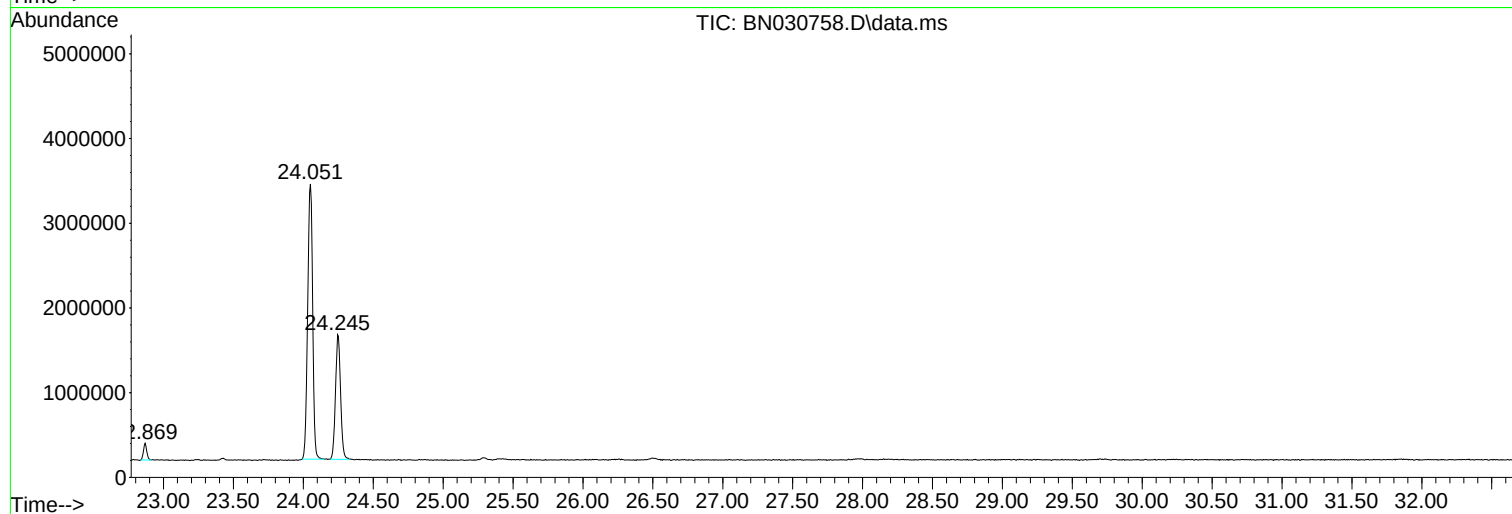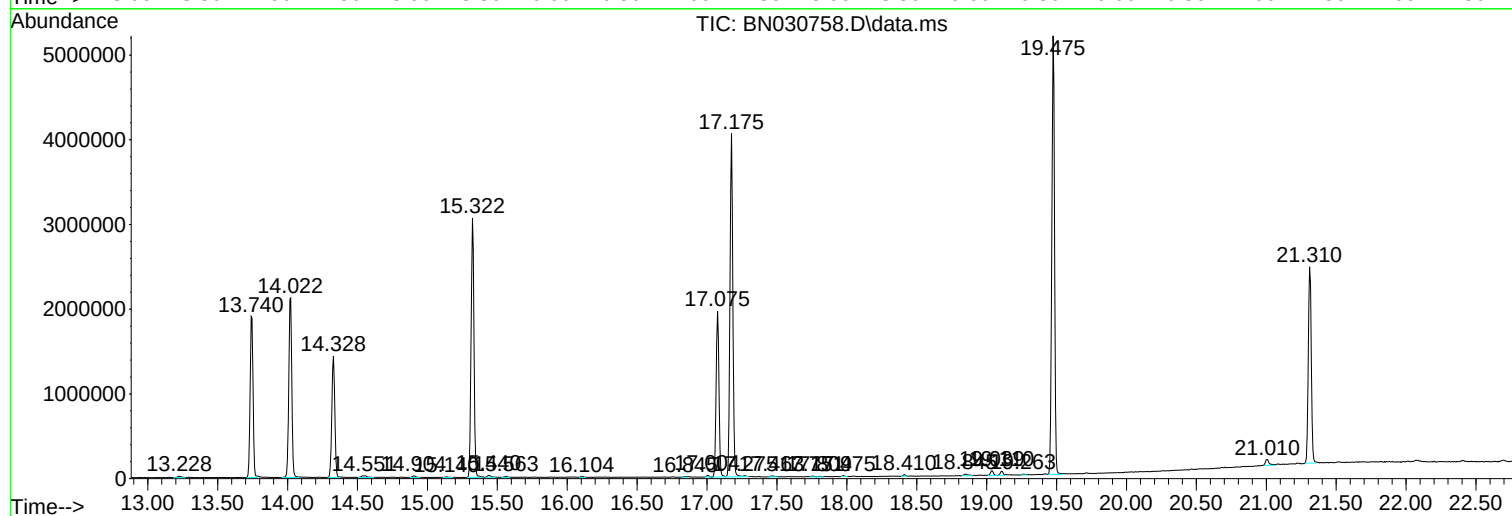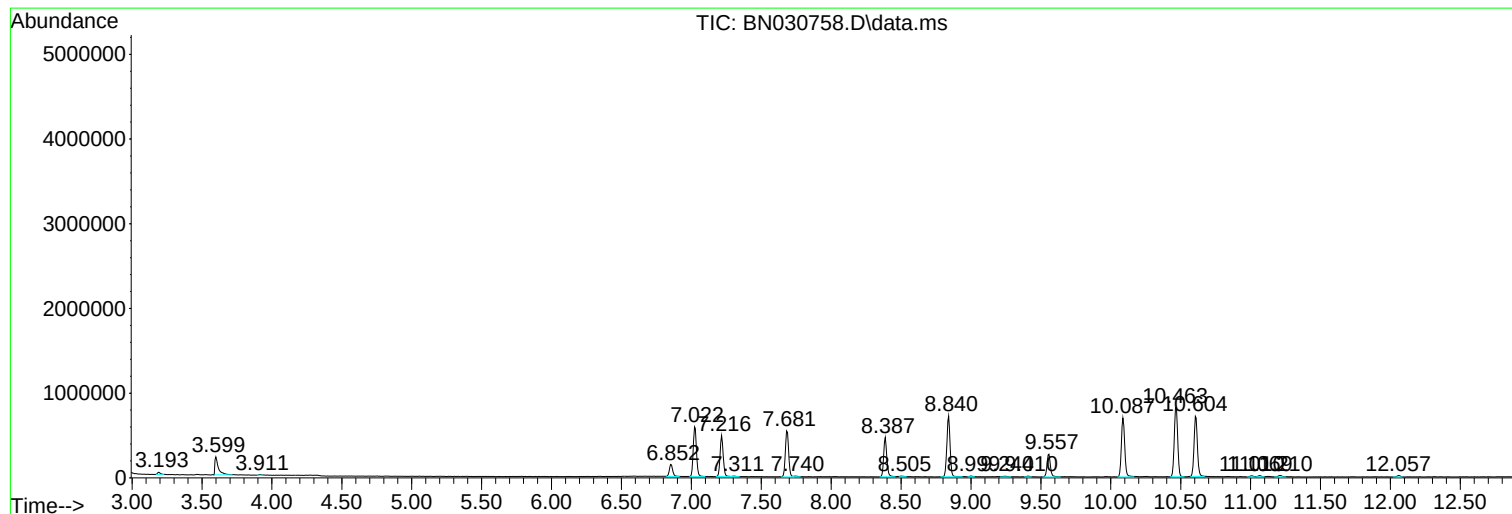

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030758.D
Acq On : 08 Apr 2024 02:32
Operator : MA/JU
Sample : P2017-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5E9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040724\
Data File : BN030758.D
Acq On : 08 Apr 2024 02:32
Operator : MA/JU
Sample : P2017-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BH5E9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc