




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030798.D
Acq On : 09 Apr 2024 20:32
Operator : MA/JU
Sample : P2013-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC0

Manual IntegrationsAPPROVED

Quant Time: Apr 09 21:58:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 09 12:10:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

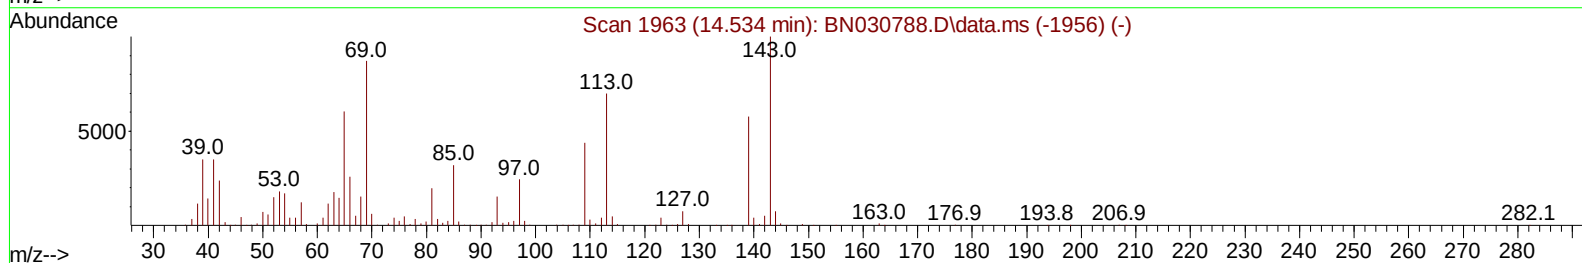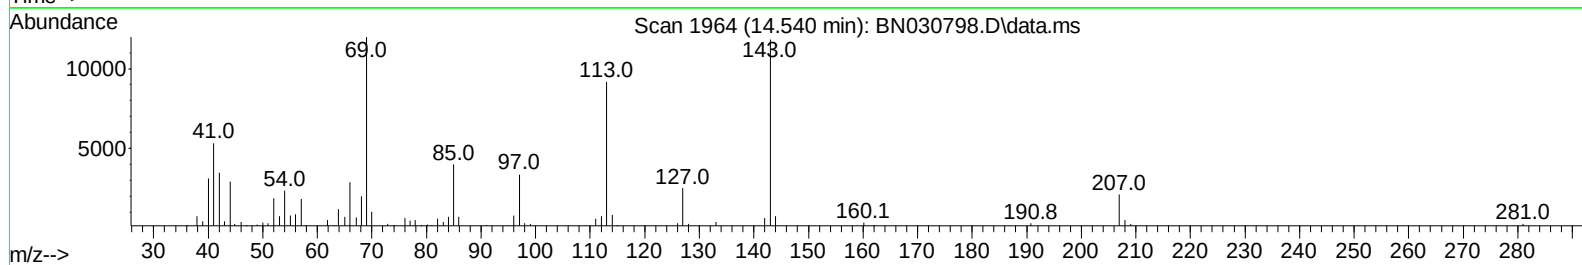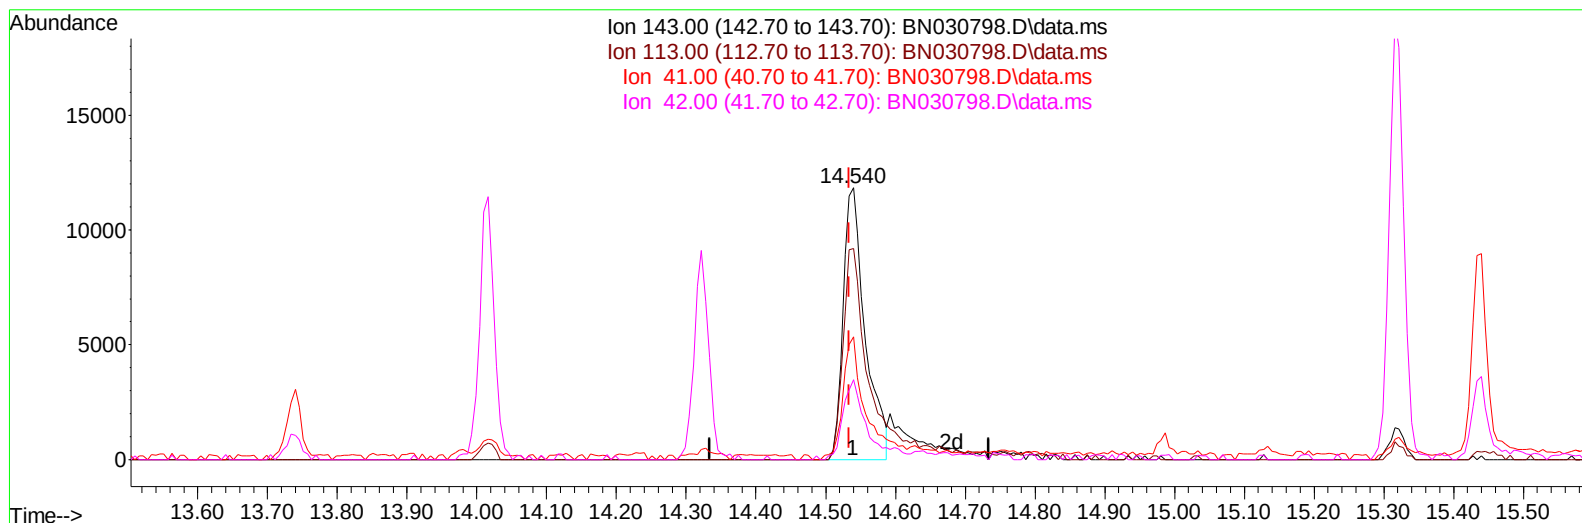

TIC: BN030798.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.540min (+ 0.006) 4.47 ng/ul

response 25887

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	72.10	77.74
41.00	38.20	45.20
42.00	26.70	29.47




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030798.D
Acq On : 09 Apr 2024 20:32
Operator : MA/JU
Sample : P2013-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC0

Manual IntegrationsAPPROVED

Quant Time: Apr 09 21:58:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 09 12:10:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

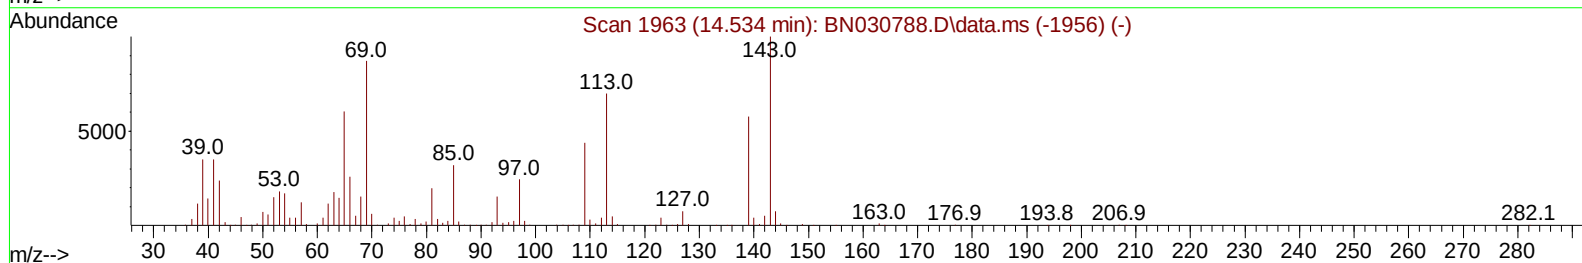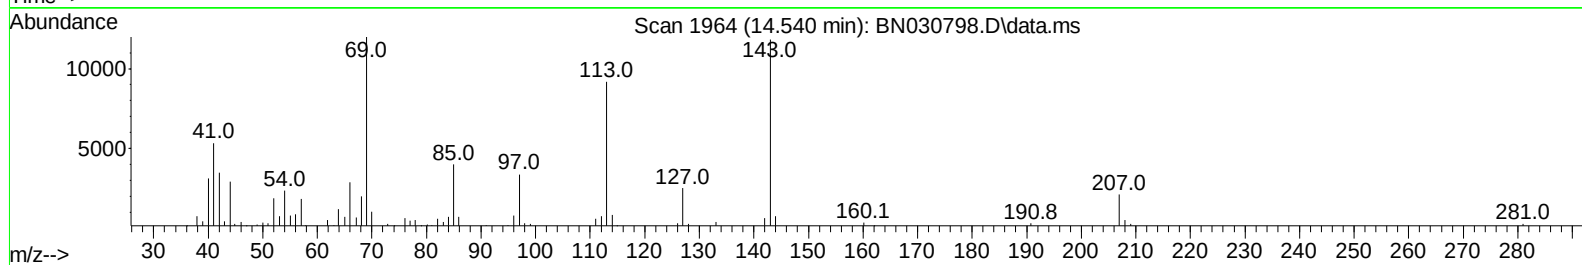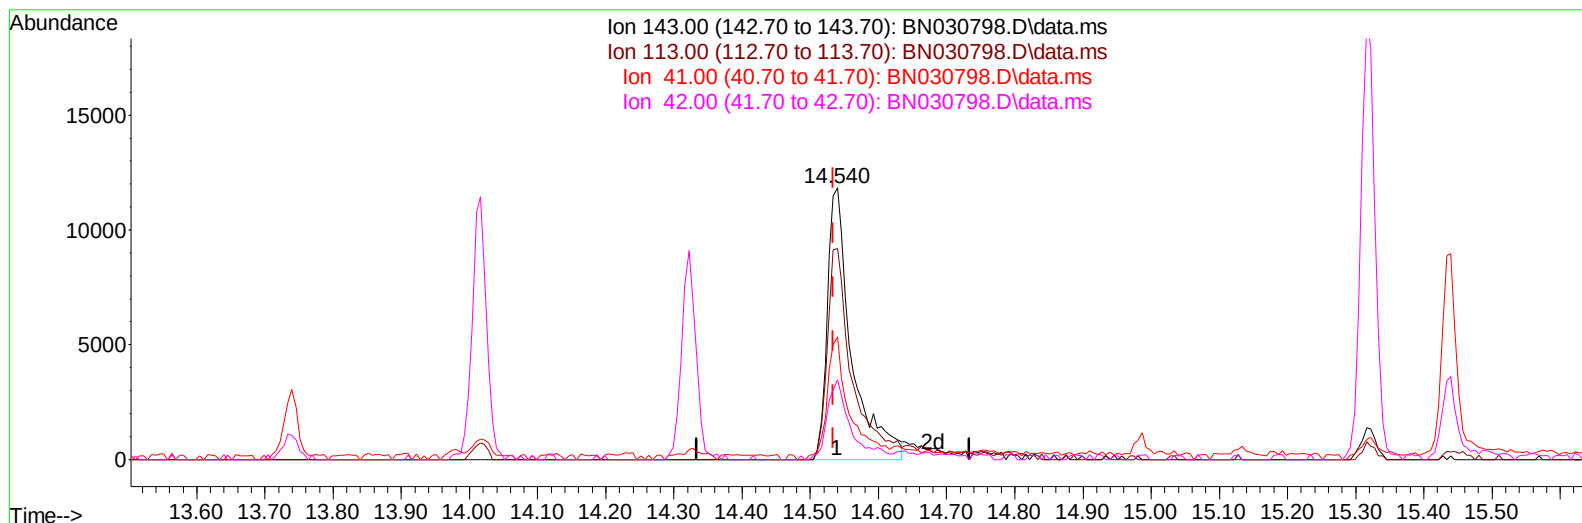

TIC: BN030798.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.540min (+ 0.006) 5.06 ng/ul m

response 29294

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	72.10	77.74
41.00	38.20	45.20
42.00	26.70	29.47

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
 Data File : BN030798.D
 Acq On : 09 Apr 2024 20:32
 Operator : MA/JU
 Sample : P2013-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0MC0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 04/10/2024
 Supervised By :mohammad ahmed 04/10/2024

Quant Time: Apr 09 21:59:31 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 09 12:10:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.681	152	141254	20.000	ng/ul	0.00
20) Naphthalene-d8	10.463	136	644413	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.322	164	453582	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.069	188	1017124	20.000	ng/ul	0.00
79) Chrysene-d12	21.310	240	1063019	20.000	ng/ul	0.00
88) Perylene-d12	24.239	264	1210082	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	12146	4.031	ng/uL	0.00
4) Pyridine-d5	3.599	84	106089	11.744	ng/ul	0.00
7) Phenol-d5	6.852	99	80874	7.078	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.022	67	239933	33.996	ng/ul	0.00
11) 2-Chlorophenol-d4	7.216	132	235809	27.203	ng/ul	0.00
15) 4-Methylphenol-d8	8.381	113	163065	17.027	ng/ul	0.00
21) Nitrobenzene-d5	8.834	128	163062	36.477	ng/ul	0.00
24) 2-Nitrophenol-d4	9.552	143	151918	37.149	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.087	165	290830	32.485	ng/ul	0.00
31) 4-Chloroaniline-d4	10.604	131	435658	29.558	ng/ul	0.00
46) Dimethylphthalate-d6	13.740	166	1259714	41.597	ng/ul	0.00
49) Acenaphthylene-d8	14.016	160	1380440	39.646	ng/ul	0.00
54) 4-Nitrophenol-d4	14.540	143	29294m	5.057	ng/ul	0.00
60) Fluorene-d10	15.322	176	1142962	43.130	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.439	200	146237	32.573	ng/ul	0.00
73) Anthracene-d10	17.169	188	1910008	43.584	ng/ul	0.00
81) Pyrene-d10	19.475	212	2443053	42.746	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.045	264	2533149	45.431	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030798.D
Acq On : 09 Apr 2024 20:32
Operator : MA/JU
Sample : P2013-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC0

Manual IntegrationsAPPROVED

Quant Time: Apr 09 21:59:31 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 09 12:10:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

