

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
 Data File : BN030792.D
 Acq On : 09 Apr 2024 12:43
 Operator : MA/JU
 Sample : P1970-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 COAK0

Quant Time: Apr 09 14:55:23 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 09 12:10:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.681	152	199053	20.000	ng/u1	0.00
20) Naphthalene-d8	10.463	136	935936	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.322	164	676880	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.075	188	1475150	20.000	ng/u1	0.00
79) Chrysene-d12	21.310	240	1399024	20.000	ng/u1	0.00
88) Perylene-d12	24.239	264	1376862	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	32597	7.678	ng/uL	0.00
4) Pyridine-d5	3.593	84	269583	21.178	ng/u1	0.00
7) Phenol-d5	6.852	99	190872	11.854	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.022	67	559452	56.251	ng/u1	0.00
11) 2-Chlorophenol-d4	7.210	132	581792	47.628	ng/u1	0.00
15) 4-Methylphenol-d8	8.387	113	403969	29.934	ng/u1	0.00
21) Nitrobenzene-d5	8.840	128	423346	65.205	ng/u1	0.00
24) 2-Nitrophenol-d4	9.552	143	451878	76.081	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.087	165	763488	58.717	ng/u1	0.00
31) 4-Chloroaniline-d4	10.604	131	826067	38.589	ng/u1	0.00
46) Dimethylphthalate-d6	13.740	166	2905420	64.290	ng/u1	0.00
49) Acenaphthylene-d8	14.016	160	3269948	62.931	ng/u1	0.00
54) 4-Nitrophenol-d4	14.534	143	88645	10.255	ng/u1	0.00
60) Fluorene-d10	15.322	176	2503275	63.299	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.439	200	459901	70.632	ng/u1	0.00
73) Anthracene-d10	17.175	188	4061833	63.907	ng/u1	0.00
81) Pyrene-d10	19.475	212	4714436	62.678	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.051	264	4517476	71.206	ng/u1	0.01


Target Compounds					Qvalue
2) 1,4-Dioxane	3.222	88	17067	3.753	ng/uL 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030792.D
Acq On : 09 Apr 2024 12:43
Operator : MA/JU
Sample : P1970-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AK0


Quant Time: Apr 09 14:55:23 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Apr 09 12:10:11 2024
Response via : Initial Calibration

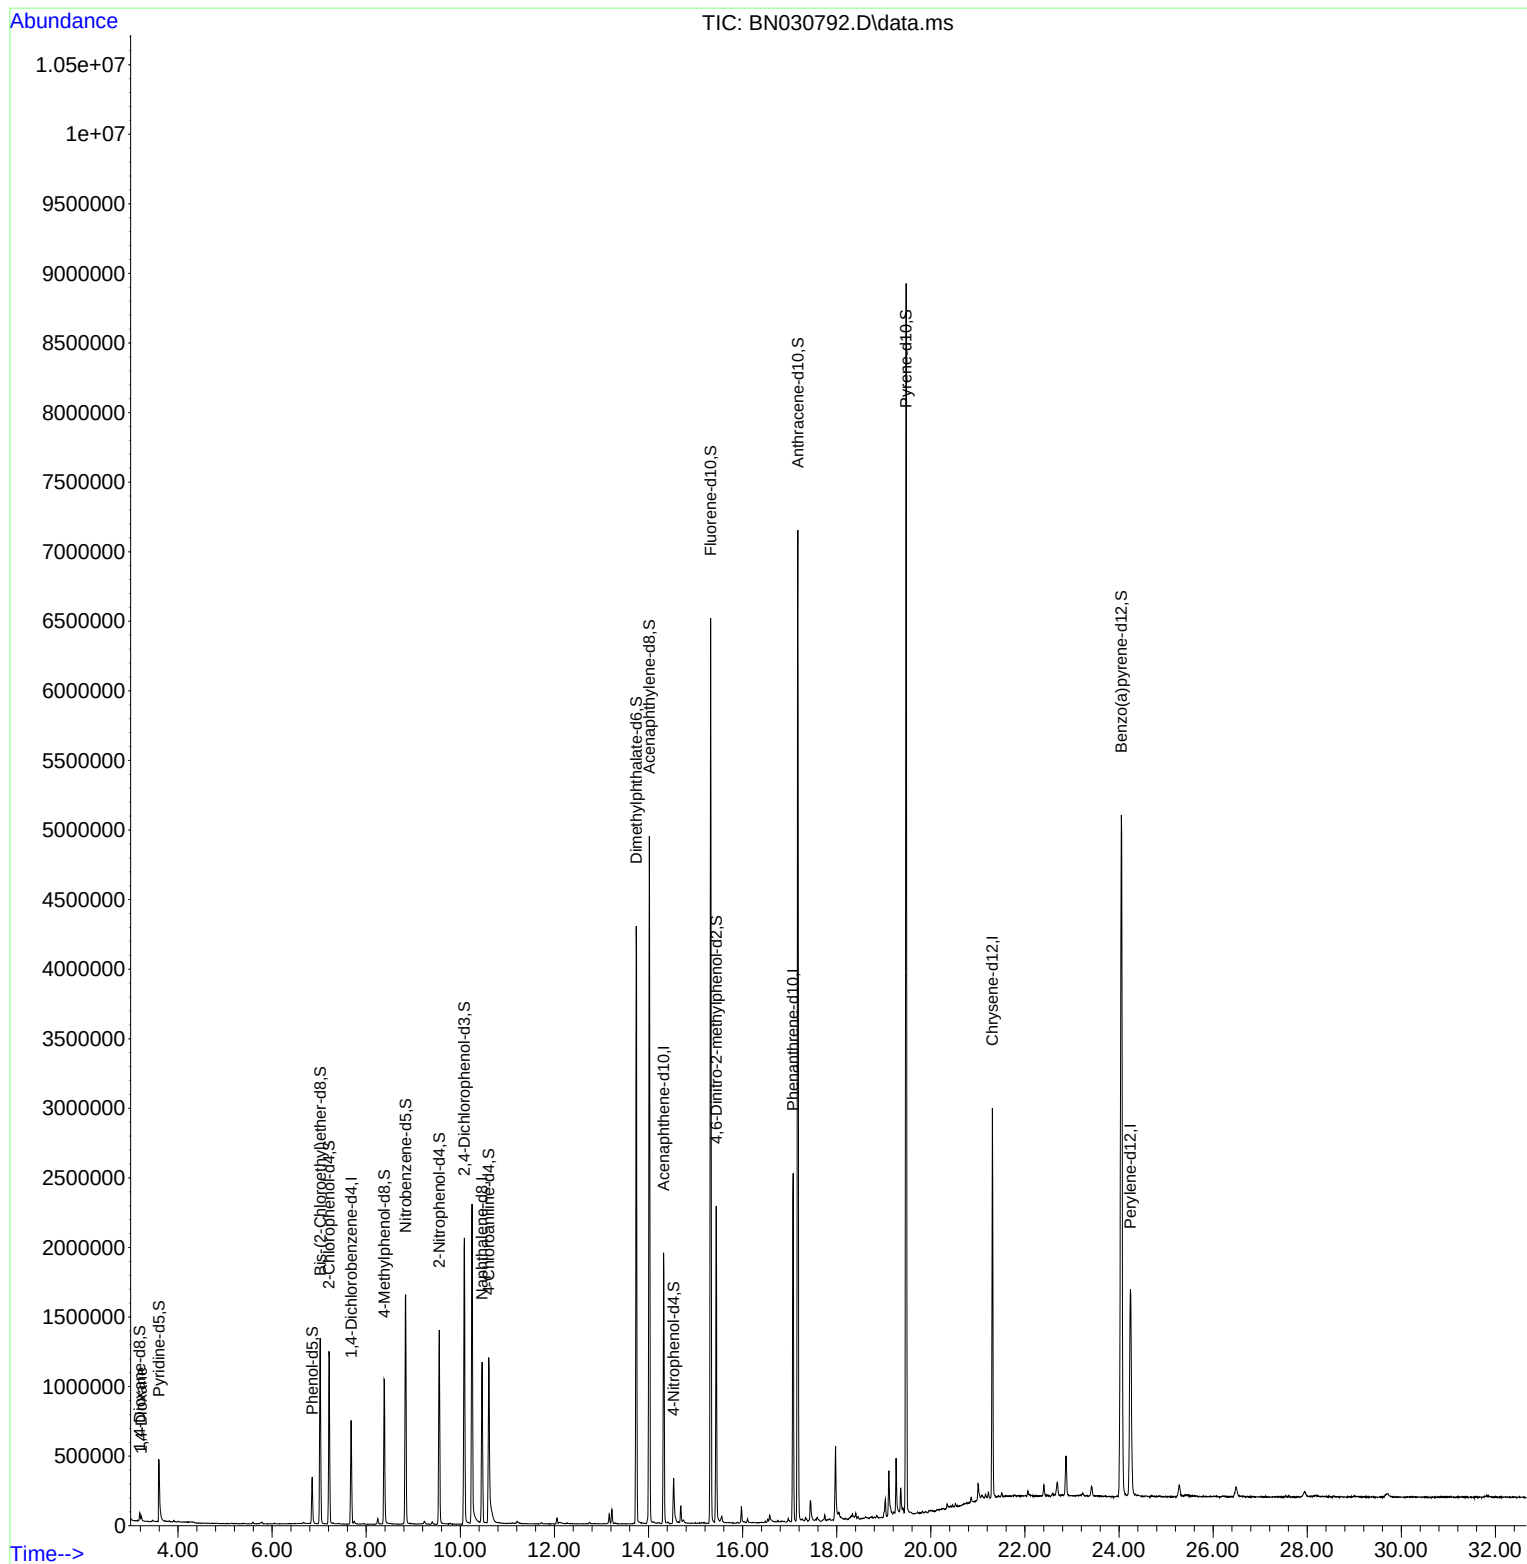

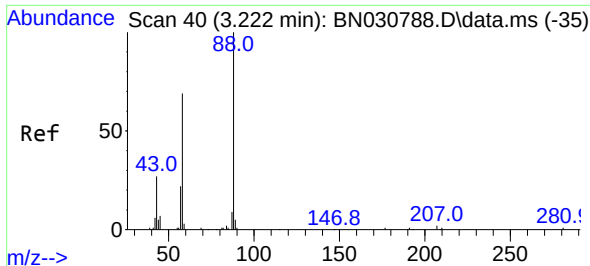

#2
1,4-Dioxane
Concen: 3.753 ng/uL
RT: 3.222 min Scan# 40
Delta R.T. 0.000 min
Lab File: BN030792.D
Acq: 09 Apr 2024 12:43

Instrument :
BNA_N
ClientSampleId :
C0AK0

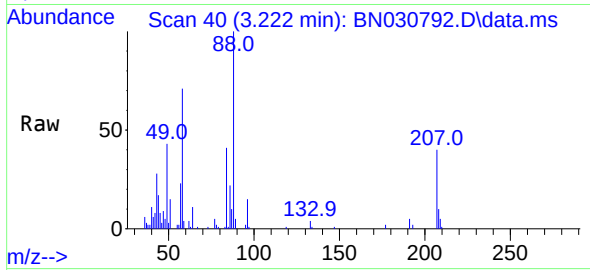

Tgt Ion:	88	Resp:	17067
Ion	Ratio	Lower	Upper
88	100		
43	28.4	23.8	35.8
58	70.8	56.6	84.8

