

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
 Data File : BN030799.D
 Acq On : 09 Apr 2024 21:11
 Operator : MA/JU
 Sample : P2013-15MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0MC0MS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/10/2024
 Supervised By :mohammad ahmed 04/10/2024

Quant Time: Apr 09 22:23:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Apr 09 12:10:11 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.681	152	196500	20.000	ng/u1	0.00
20) Naphthalene-d8	10.463	136	916560	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.322	164	624263	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.075	188	1365722	20.000	ng/u1	0.00
79) Chrysene-d12	21.316	240	1290623	20.000	ng/u1	0.00
88) Perylene-d12	24.245	264	1494538	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.187	96	20794	4.961	ng/uL	0.00
4) Pyridine-d5	3.599	84	155764	12.396	ng/u1	0.00
7) Phenol-d5	6.852	99	139816	8.796	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.022	67	355203	36.179	ng/u1	0.00
11) 2-Chlorophenol-d4	7.216	132	367023	30.436	ng/u1	0.00
15) 4-Methylphenol-d8	8.387	113	266307	19.989	ng/u1	0.00
21) Nitrobenzene-d5	8.840	128	253665	39.896	ng/u1	0.00
24) 2-Nitrophenol-d4	9.551	143	253421	43.569	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.087	165	468366	36.782	ng/u1	0.00
31) 4-Chloroaniline-d4	10.604	131	695631	33.183	ng/u1	0.00
46) Dimethylphthalate-d6	13.745	166	1812517	43.487	ng/u1	0.00
49) Acenaphthylene-d8	14.016	160	2000646	41.748	ng/u1	0.00
54) 4-Nitrophenol-d4	14.534	143	82580	10.358	ng/u1	0.00
60) Fluorene-d10	15.322	176	1548252	42.450	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.445	200	292928	48.593	ng/u1	0.00
73) Anthracene-d10	17.175	188	2509594	42.648	ng/u1	0.00
81) Pyrene-d10	19.474	212	2969449	42.794	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.051	264	3082788	44.766	ng/u1	0.01
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.222	88	20229	4.506	ng/uL	99
5) Pyridine	3.616	79	160486	12.657	ng/u1	98
6) Benzaldehyde	6.834	77	340465m	45.993	ng/u1	
8) Phenol	6.881	94	153960	9.297	ng/u1	98
10) Bis(2-Chloroethyl)ether	7.116	93	474847	35.164	ng/u1	99
12) 2-Chlorophenol	7.246	128	384477	29.722	ng/u1	97
13) 2-Methylphenol	8.122	108	294962	23.115	ng/u1	98
14) 2,2'-oxybis(1-Chloropr...	8.204	45	611174	32.142	ng/u1	98
16) Acetophenone	8.504	105	776909	36.935	ng/u1	98
17) N-Nitroso-di-n-propyla...	8.487	70	388018	36.626	ng/u1	96
18) 4-Methylphenol	8.452	108	293202	20.525	ng/u1	99
19) Hexachloroethane	8.752	117	132877	24.501	ng/u1	97
22) Nitrobenzene	8.881	77	566048	36.470	ng/u1	100
23) Isophorone	9.404	82	1162265	37.549	ng/u1	99
25) 2-Nitrophenol	9.587	139	275940	40.366	ng/u1	98
26) 2,4-Dimethylphenol	9.646	107	434713	28.612	ng/u1	100
27) Bis(2-Chloroethoxy)met...	9.887	93	702266	35.684	ng/u1	100
29) 2,4-Dichlorophenol	10.116	162	458695	35.291	ng/u1	99
30) Naphthalene	10.516	128	1540884	32.779	ng/u1	99
32) 4-Chloroaniline	10.628	127	656434	32.491	ng/u1	97
33) Hexachlorobutadiene	10.793	225	224796	27.477	ng/u1	97
34) Caprolactam	11.416	113	28597	5.890	ng/u1	98
35) 4-Chloro-3-methylphenol	11.751	107	521831	35.646	ng/u1	99
36) 2-Methylnaphthalene	12.134	142	1187057	36.159	ng/u1	97

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
 Data File : BN030799.D
 Acq On : 09 Apr 2024 21:11
 Operator : MA/JU
 Sample : P2013-15MS
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :

BNA_N

ClientSampleId :

E0MC0MS

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 04/10/2024

Supervised By :mohammad ahmed 04/10/2024

Quant Time: Apr 09 22:23:26 2024

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M


Quant Title : SVOA CALIBRATION

QLast Update : Tue Apr 09 12:10:11 2024

Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.351	142	1219700	36.599	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.498	216	609929	37.859	ng/ul	96
40) Hexachlorocyclopentadiene	12.475	237	208891	22.832	ng/ul	96
41) 2,4,6-Trichlorophenol	12.745	196	438880	43.595	ng/ul	100
42) 2,4,5-Trichlorophenol	12.816	196	473399	41.638	ng/ul	94
43) 1,1'-Biphenyl	13.157	154	1651996	38.825	ng/ul	97
44) 2-Chloronaphthalene	13.192	162	1280686	38.235	ng/ul	99
45) 2-Nitroaniline	13.410	65	417822	46.873	ng/ul	97
47) Dimethylphthalate	13.792	163	1777108	41.276	ng/ul	99
48) 2,6-Dinitrotoluene	13.910	165	369694	46.313	ng/ul	94
50) Acenaphthylene	14.045	152	2200646	39.745	ng/ul	99
51) 3-Nitroaniline	14.239	138	406938	48.029	ng/ul	96
52) Acenaphthene	14.387	153	1452057	39.353	ng/ul	99
53) 2,4-Dinitrophenol	14.445	184	176922	48.254	ng/ul	95
55) 4-Nitrophenol	14.545	109	66112	10.467	ng/ul	96
56) Dibenzofuran	14.728	168	2057382	40.112	ng/ul	96
57) 2,4-Dinitrotoluene	14.698	165	564154	48.407	ng/ul	97
58) 2,3,4,6-Tetrachlorophenol	14.951	232	434945	46.063	ng/ul	98
59) Diethylphthalate	15.157	149	1848709	42.267	ng/ul	100
61) Fluorene	15.375	166	1664535	40.829	ng/ul	100
62) 4-Chlorophenyl-phenyle...	15.375	204	789132	39.453	ng/ul	96
63) 4-Nitroaniline	15.410	138	440455	53.472	ng/ul	100
66) 4,6-Dinitro-2-methylph...	15.463	198	302939	46.769	ng/ul	95
67) N-Nitrosodiphenylamine	15.592	169	1517490	40.800	ng/ul	97
68) 4-Bromophenyl-phenylether	16.269	248	537158	41.420	ng/ul	98
69) Hexachlorobenzene	16.369	284	583765	38.227	ng/ul	94
70) Atrazine	16.551	200	555769	43.111	ng/ul	99
71) Pentachlorophenol	16.722	266	387891	43.081	ng/ul	95
72) Phenanthrene	17.116	178	2859255	40.749	ng/ul	99
74) Anthracene	17.210	178	2892832	40.783	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.116	216	632752	37.712	ng/ul	96
76) Pentachlorobenzene	14.639	250	659046	38.671	ng/ul	91
77) Carbazole	17.480	167	2787635	44.813	ng/ul	98
78) Di-n-butylphthalate	18.045	149	3406468	44.889	ng/ul	99
80) Fluoranthene	19.139	202	3420580	41.469	ng/ul	97
82) Pyrene	19.504	202	3603127	41.361	ng/ul	100
83) Butylbenzylphthalate	20.416	149	1636493	49.191	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.227	252	941762	39.712	ng/ul	96
85) Benzo(a)anthracene	21.298	228	3610161	41.913	ng/ul	98
86) Bis(2-ethylhexyl)phtha...	21.227	149	2305232	46.987	ng/ul	98
87) Chrysene	21.357	228	3504120	43.101	ng/ul	95
89) Di-n-octyl phthalate	22.339	149	4323968	45.686	ng/ul	100
90) Benzo(b)fluoranthene	23.321	252	3702890	42.099	ng/ul	98
91) Benzo(k)fluoranthene	23.386	252	3729248	41.749	ng/ul	98
93) Benzo(a)pyrene	24.115	252	3137656	37.763	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	27.545	276	3978050	44.291	ng/ul	98
95) Dibenzo(a,h)anthracene	27.603	278	3194907	42.255	ng/ul	95
96) Benzo(g,h,i)perylene	28.574	276	2964560m	42.044	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 4.506 ng/uL
RT: 3.222 min Scan# 40
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion: 88 Resp: 20229
Ion Ratio Lower Upper
88 100
43 30.5 23.8 35.8
58 69.8 56.6 84.8


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024






04/10/2024
Supervised By :mohammad
ahmed


04/10/2024



#5
Pyridine
Concen: 12.657 ng/uL
RT: 3.616 min Scan# 107
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11

Tgt Ion: 79 Resp: 160486
Ion Ratio Lower Upper
79 100
52 71.5 56.2 84.4
51 35.6 27.0 40.4

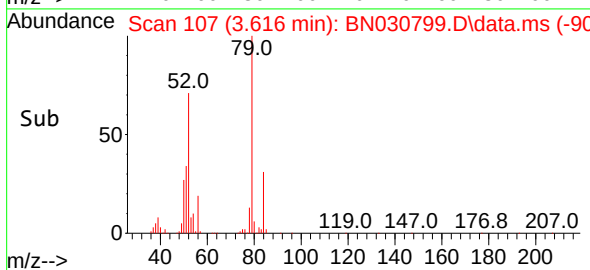





#6
Benzaldehyde
Concen: 45.993 ng/ul m
RT: 6.834 min Scan# 61
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11

Instrument :
BNA_N
ClientSampleId :
EOMCOMS

Tgt Ion: 77 Resp: 34046
Ion Ratio Lower Upper
77 100
105 102.2 78.1 117.1
106 96.6 75.6 113.4



Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

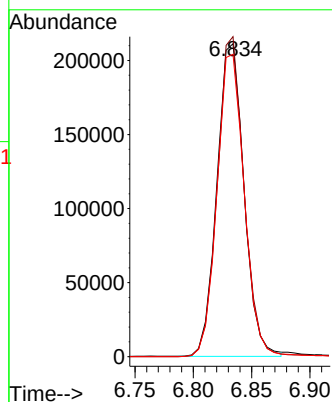




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024



#8
Phenol
Concen: 9.297 ng/ul
RT: 6.881 min Scan# 662
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11


Tgt Ion: 94 Resp: 153960
Ion Ratio Lower Upper
94 100
65 25.2 21.4 32.0
66 35.1 28.5 42.7

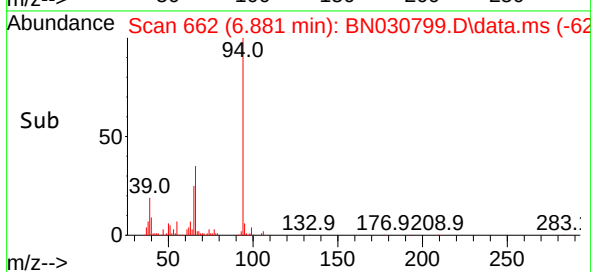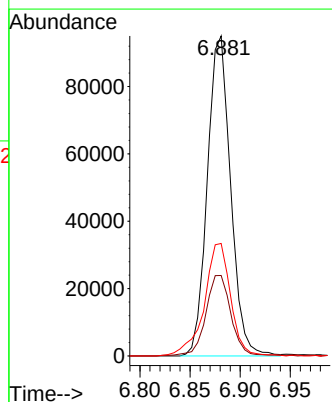



#10
Bis(2-Chloroethyl)ether
Concen: 35.164 ng/ul
RT: 7.116 min Scan# 701
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion: 93 Resp: 47484
Ion Ratio Lower Upper
93 100
63 71.8 58.2 87.4
95 32.3 26.0 39.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

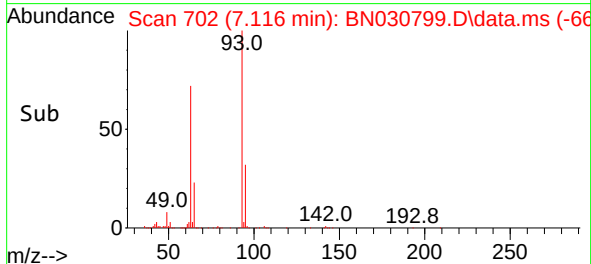




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024



#12
2-Chlorophenol
Concen: 29.722 ng/ul
RT: 7.246 min Scan# 724
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11


Tgt Ion:128 Resp: 384477
Ion Ratio Lower Upper
128 100
64 43.0 37.0 55.4
130 32.0 26.3 39.5

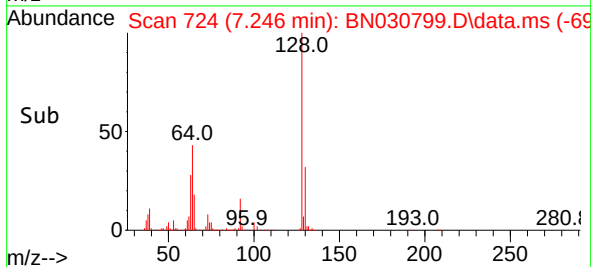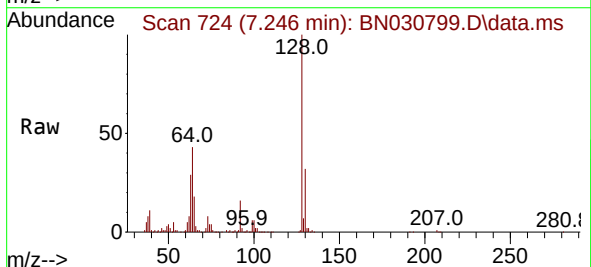



#13
2-Methylphenol
Concen: 23.115 ng/ul
RT: 8.122 min Scan# 81
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion:108 Resp: 294962
Ion Ratio Lower Upper
108 100
107 87.5 71.8 107.8


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

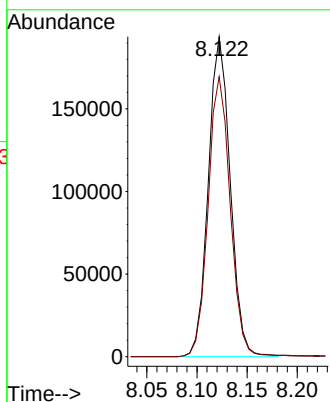


04/10/2024
Supervised By :mohammad
ahmed



04/10/2024




#14
2,2'-oxybis(1-Chloropropane)
Concen: 32.142 ng/ul
RT: 8.204 min Scan# 887
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Tgt Ion: 45 Resp: 611174
Ion Ratio Lower Upper
45 100
77 16.1 12.1 18.1
79 11.3 8.6 13.0

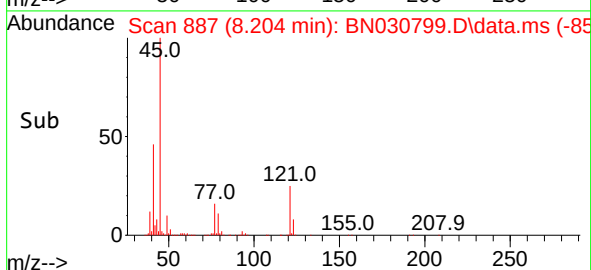





#16
Acetophenone
Concen: 36.935 ng/ul
RT: 8.504 min Scan# 91
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11

Instrument :
BNA_N
ClientSampleId :
E0MC0MS

Tgt Ion: 105 Resp: 776909
Ion Ratio Lower Upper
105 100
77 75.2 61.2 91.8
51 24.4 21.0 31.4



Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

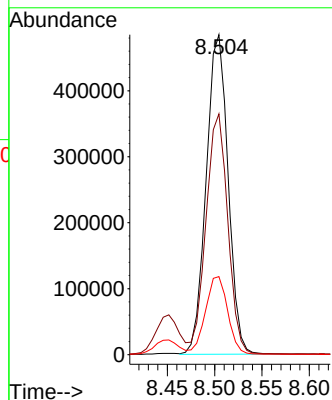




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024

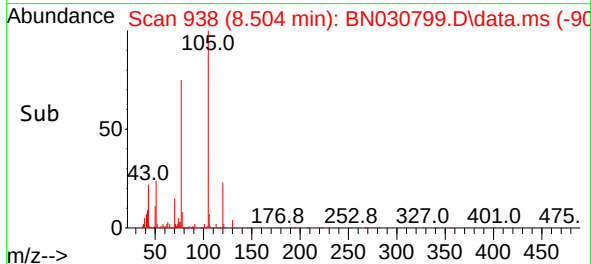

#17
N-Nitroso-di-n-propylamine
Concen: 36.626 ng/ul
RT: 8.487 min Scan# 935
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11


Tgt Ion: 70 Resp: 388018
Ion Ratio Lower Upper
70 100
42 55.4 47.4 71.0
101 10.1 7.9 11.9
130 22.5 19.0 28.4

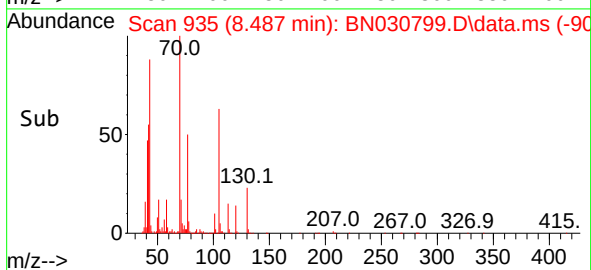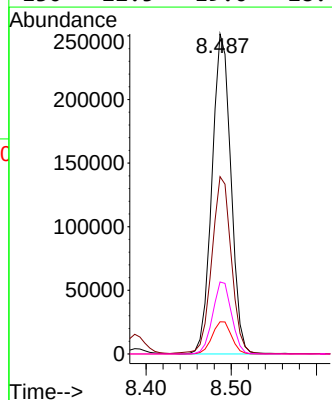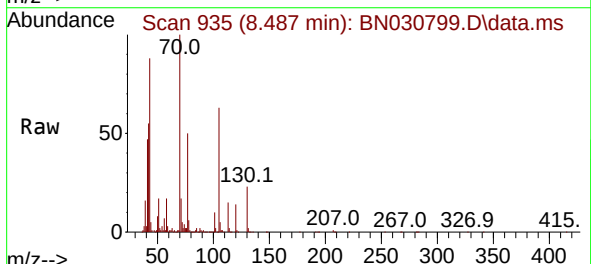



#18
4-Methylphenol
Concen: 20.525 ng/ul
RT: 8.452 min Scan# 91
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion:108 Resp: 29320
Ion Ratio Lower Upper
108 100
107 111.1 88.1 132.1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

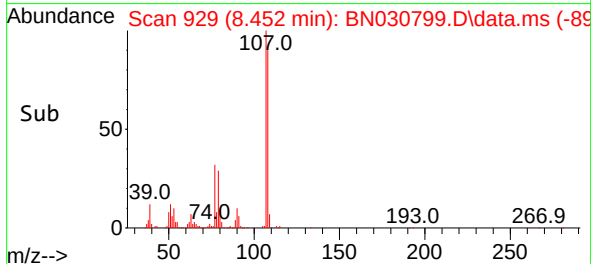




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024



#19
Hexachloroethane
Concen: 24.501 ng/ul
RT: 8.752 min Scan# 980
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11


Tgt Ion:117 Resp: 132877
Ion Ratio Lower Upper
117 100
201 99.4 76.5 114.7
199 62.2 48.5 72.7

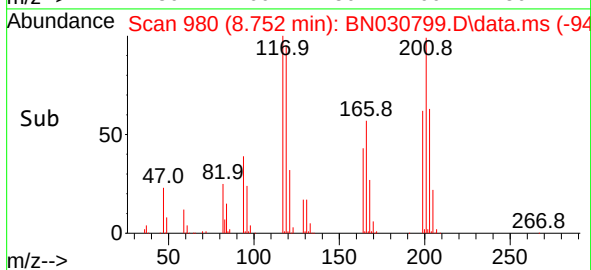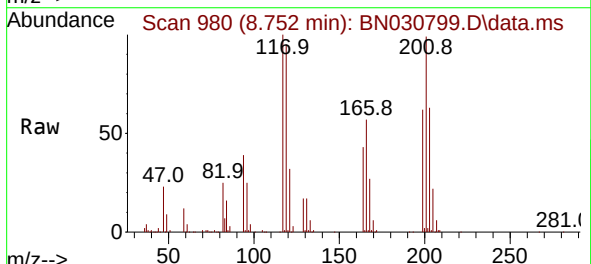



#22
Nitrobenzene
Concen: 36.470 ng/ul
RT: 8.881 min Scan# 1002
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion: 77 Resp: 566048
Ion Ratio Lower Upper
77 100
123 46.9 37.5 56.3
65 13.1 10.6 15.8


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

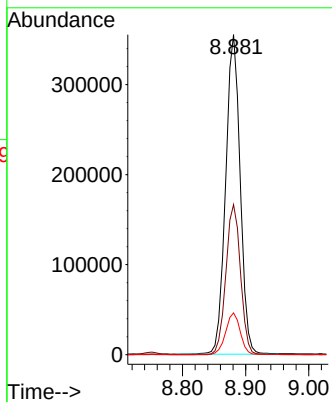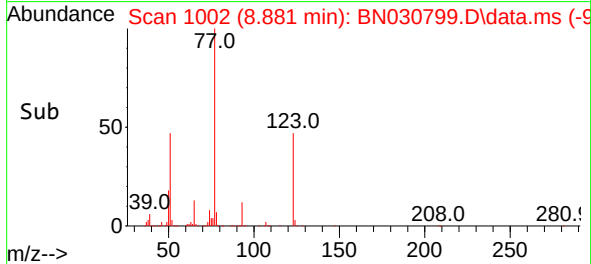




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024



#23
Isophorone
Concen: 37.549 ng/ul
RT: 9.404 min Scan# 1091
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11

Tgt Ion: 82 Resp: 1162265
Ion Ratio Lower Upper
82 100
95 7.2 5.7 8.5
138 18.9 14.6 21.8

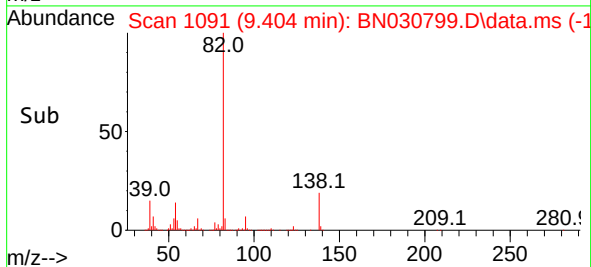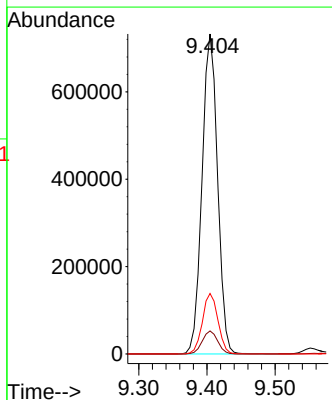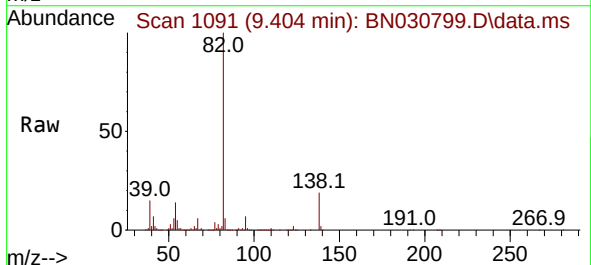

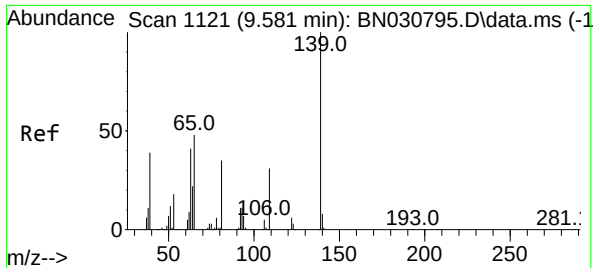



#25
2-Nitrophenol
Concen: 40.366 ng/ul
RT: 9.587 min Scan# 1121
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11

Instrument :
BNA_N
ClientSampleId :
EOMCOMS

Tgt Ion:139 Resp: 275940
Ion Ratio Lower Upper
139 100
65 47.7 39.5 59.3
109 30.6 23.8 35.8



Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

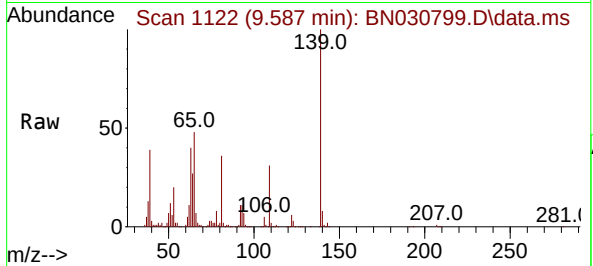




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024

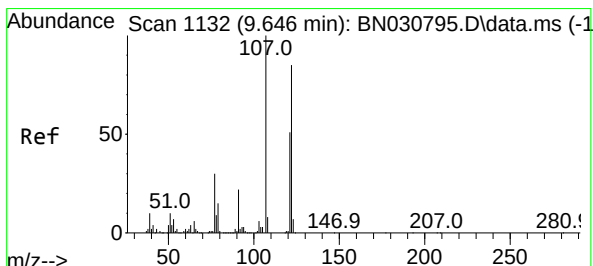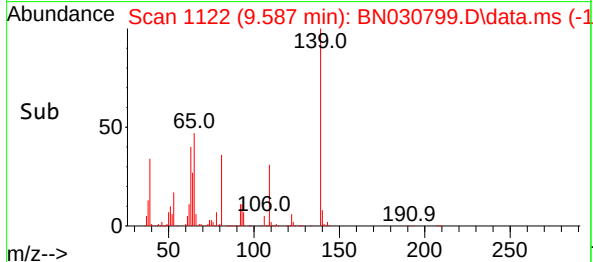

#26
2,4-Dimethylphenol
Concen: 28.612 ng/ul
RT: 9.646 min Scan# 1132
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11

Tgt Ion:107 Resp: 434713
Ion Ratio Lower Upper
107 100
121 51.6 41.6 62.4
122 89.4 71.3 106.9

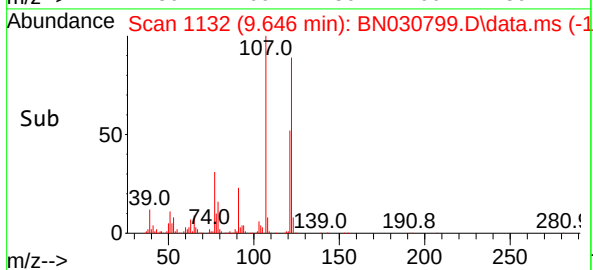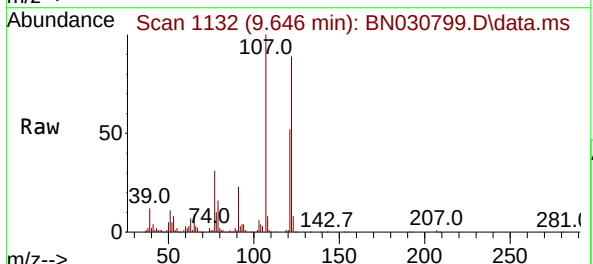



#27

Bis(2-Chloroethoxy)methane

Concen: 35.684 ng/ul

RT: 9.887 min Scan# 1173

Delta R.T. -0.000 min

Lab File: BN030799.D

Acq: 09 Apr 2024 21:11

Instrument :

BNA_N

ClientSampleId :

EOMCOMS

Tgt Ion: 93 Resp: 702260

Ion Ratio Lower Upper

93 100

95 31.4 25.4 38.0



123 11.5 9.4 14.0

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 04/10/2024



Supervised By :mohammad ahmed 04/10/2024



04/10/2024

Supervised By :mohammad
ahmed

04/10/2024

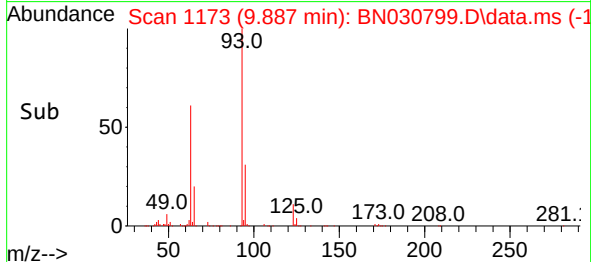

#29

2,4-Dichlorophenol

Concen: 35.291 ng/ul

RT: 10.116 min Scan# 1212

Delta R.T. 0.006 min

Lab File: BN030799.D

Acq: 09 Apr 2024 21:11




Tgt Ion:162 Resp: 458695


Ion Ratio Lower Upper

162 100

164 65.0 51.8 77.8

98 35.9 28.0 42.0

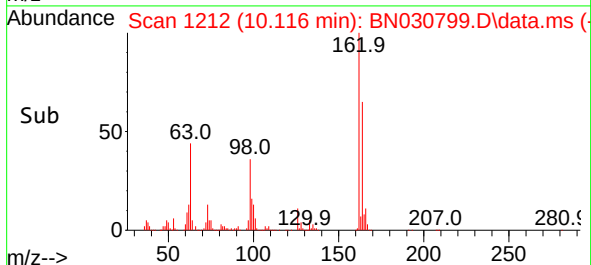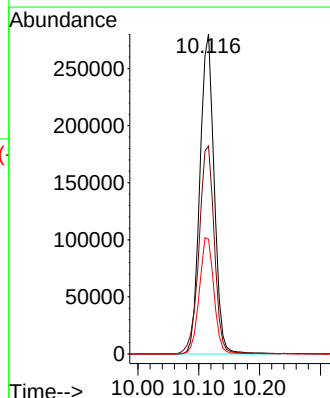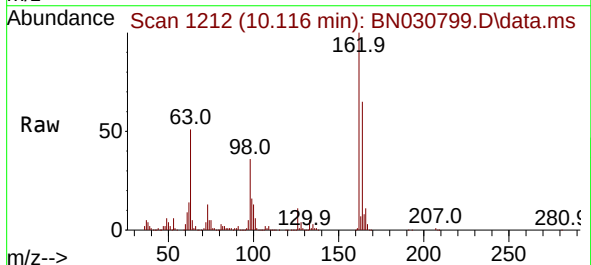





#30
Naphthalene
Concen: 32.779 ng/ul
RT: 10.516 min Scan# 1279
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11

Instrument :
BNA_N
ClientSampleId :
EOMCOMS

Tgt Ion:128 Resp: 1540884
Ion Ratio Lower Upper
128 100
129 11.0 8.7 13.1
127 13.5 10.5 15.7



Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

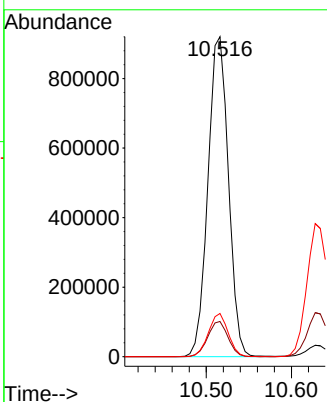




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024



#32
4-Chloroaniline
Concen: 32.491 ng/ul
RT: 10.628 min Scan# 1299
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11


Tgt Ion:127 Resp: 656434
Ion Ratio Lower Upper
127 100
129 33.0 25.3 37.9

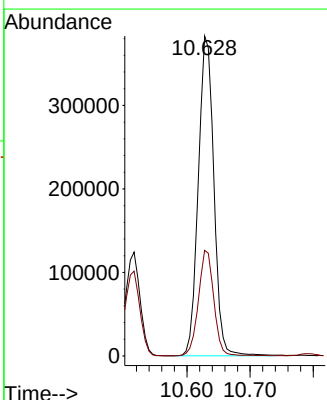



#33
Hexachlorobutadiene
Concen: 27.477 ng/ul
RT: 10.793 min Scan# 11
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument : BNA_N
ClientSampleId : E0MC0MS



Tgt Ion: 225 Resp: 224790


Ion	Ratio	Lower	Upper
225	100		
223	59.4	50.9	76.3
227	63.7	51.6	77.4

Manual Integrations
APPROVED
Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

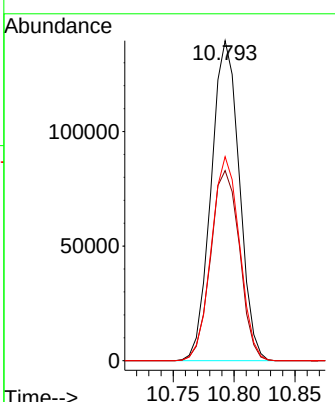


04/10/2024
Supervised By :mohammad ahmed

04/10/2024






#34
Caprolactam
Concen: 5.890 ng/ul
RT: 11.416 min Scan# 1433
Delta R.T. 0.012 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Tgt Ion: 113 Resp: 28597


Ion	Ratio	Lower	Upper
113	100		
55	152.8	124.7	187.1
56	114.2	90.6	135.8

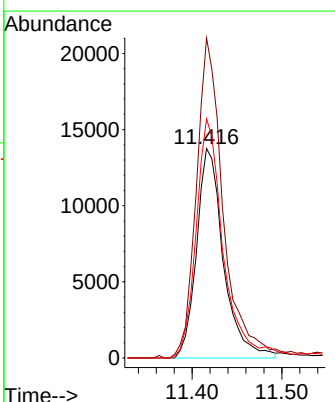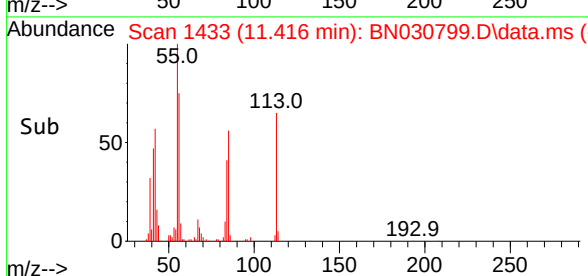



#35
4-Chloro-3-methylphenol
Concen: 35.646 ng/ul
RT: 11.751 min Scan# 1490
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion:107 Resp: 52183
Ion Ratio Lower Upper
107 100
144 25.8 21.4 32.0
142 81.3 65.9 98.9


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

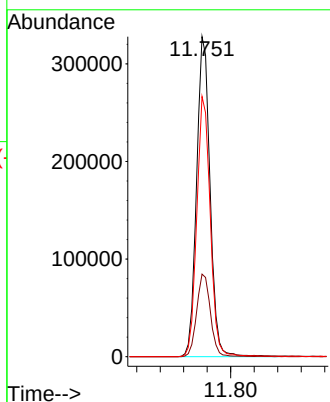




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024



#36
2-Methylnaphthalene
Concen: 36.159 ng/ul
RT: 12.134 min Scan# 1555
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11


Tgt Ion:142 Resp: 1187057
Ion Ratio Lower Upper
142 100
141 91.0 70.8 106.2

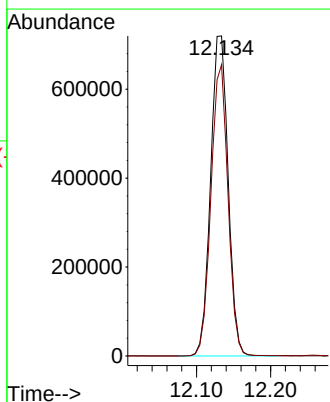



#37
1-Methylnaphthalene
Concen: 36.599 ng/ul
RT: 12.351 min Scan# 1592
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
E0MC0MS



Tgt Ion:142 Resp: 1219700
Ion Ratio Lower Upper
142 100
141 89.5 73.0 109.4
116 3.7 2.9 4.3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

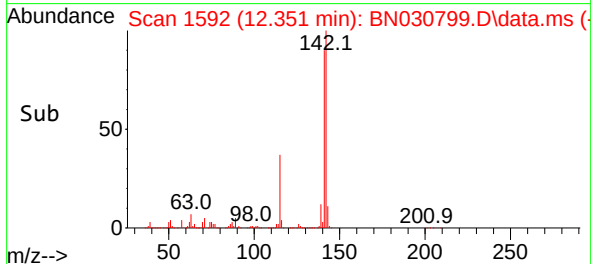




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024



#39
1,2,4,5-Tetrachlorobenzene
Concen: 37.859 ng/ul
RT: 12.498 min Scan# 1617
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11


Tgt Ion:216 Resp: 609929
Ion Ratio Lower Upper
216 100
214 80.5 60.9 91.3
179 22.6 17.4 26.0
108 19.2 14.2 21.4

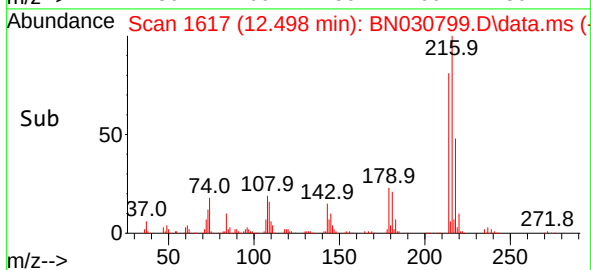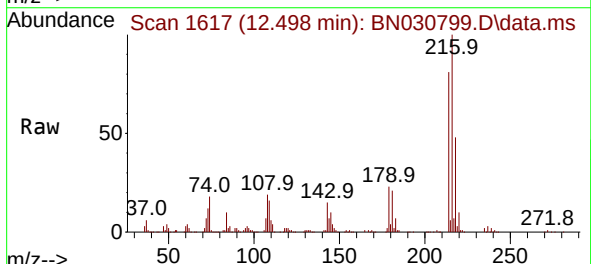



#40
Hexachlorocyclopentadiene
Concen: 22.832 ng/ul
RT: 12.475 min Scan# 1613
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion:237 Resp: 20889
Ion Ratio Lower Upper
237 100
235 66.8 50.6 76.0
272 13.5 10.2 15.4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

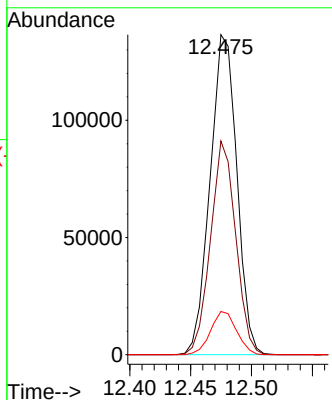


04/10/2024
Supervised By :mohammad
ahmed



04/10/2024




#41
2,4,6-Trichlorophenol
Concen: 43.595 ng/ul
RT: 12.745 min Scan# 1659
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11

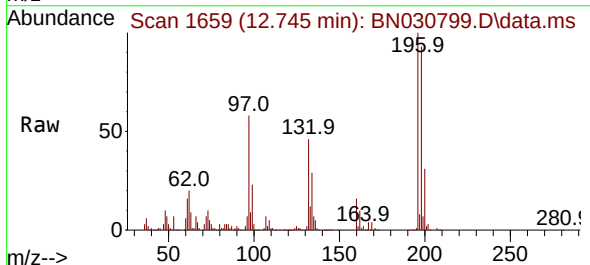


Tgt Ion:196 Resp: 438880
Ion Ratio Lower Upper
196 100
198 93.5 74.6 111.8
200 30.9 24.8 37.2

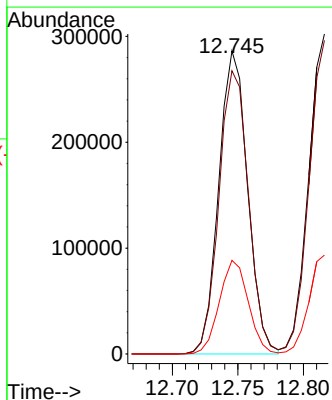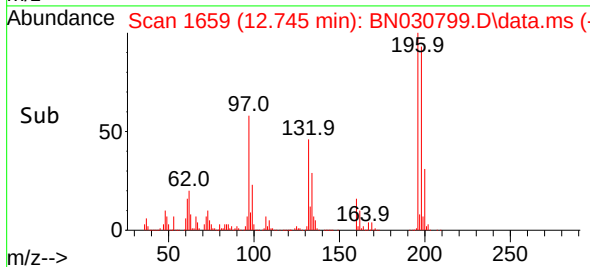



#42
 2,4,5-Trichlorophenol
 Concen: 41.638 ng/ul
 RT: 12.816 min Scan# 1671
 Delta R.T. -0.000 min
 Lab File: BN030799.D
 Acq: 09 Apr 2024 21:11



Instrument : BNA_N
 ClientSampleId : EOMCOMS



Tgt Ion:196 Resp: 473399


Ion	Ratio	Lower	Upper
196	100		
198	98.0	73.0	109.6
200	30.9	25.2	37.8

Manual Integrations
APPROVED
 Reviewed By :Yogesh Patel 04/10/2024
 Supervised By :mohammad ahmed 04/10/2024

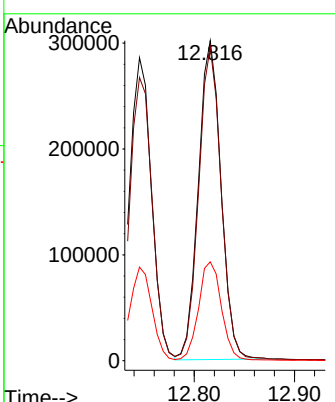


04/10/2024
 Supervised By :mohammad ahmed

04/10/2024






#43
 1,1'-Biphenyl
 Concen: 38.825 ng/ul
 RT: 13.157 min Scan# 1729
 Delta R.T. 0.006 min
 Lab File: BN030799.D
 Acq: 09 Apr 2024 21:11



Tgt Ion:154 Resp: 1651996


Ion	Ratio	Lower	Upper
154	100		
153	41.9	31.5	47.3
76	12.7	9.8	14.6

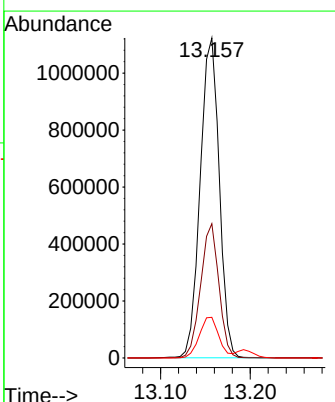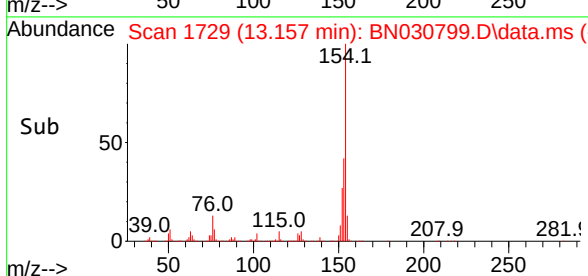



#44
2-Chloronaphthalene
Concen: 38.235 ng/ul
RT: 13.192 min Scan# 1735
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion:162 Resp: 1280680
Ion Ratio Lower Upper
162 100
164 33.2 25.7 38.5
127 40.6 32.2 48.2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

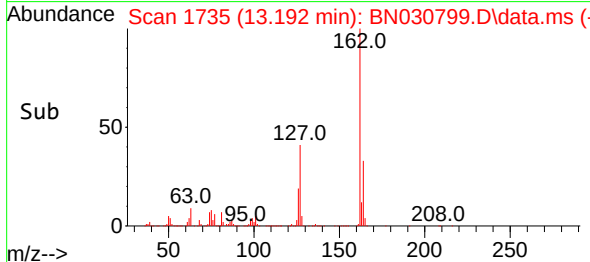


04/10/2024
Supervised By :mohammad
ahmed



04/10/2024




#45
2-Nitroaniline
Concen: 46.873 ng/ul
RT: 13.410 min Scan# 1772
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11




Tgt Ion: 65 Resp: 417822
Ion Ratio Lower Upper
65 100
92 72.7 57.7 86.5
138 117.3 90.6 135.8

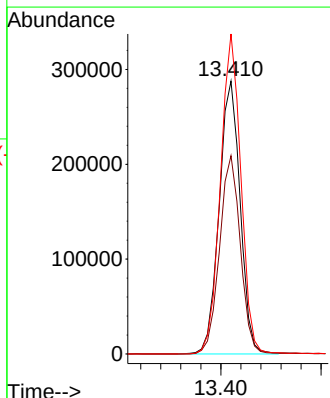



#47
Dimethylphthalate
Concen: 41.276 ng/ul
RT: 13.792 min Scan# 1837
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion:163 Resp: 1777108
Ion Ratio Lower Upper
163 100
194 4.3 3.3 4.9
164 9.8 8.2 12.4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024




04/10/2024
Supervised By :mohammad
ahmed



04/10/2024




#48
2,6-Dinitrotoluene
Concen: 46.313 ng/ul
RT: 13.910 min Scan# 1857
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11




Tgt Ion:165 Resp: 369694
Ion Ratio Lower Upper
165 100
89 59.0 43.5 65.3
121 22.2 15.7 23.5

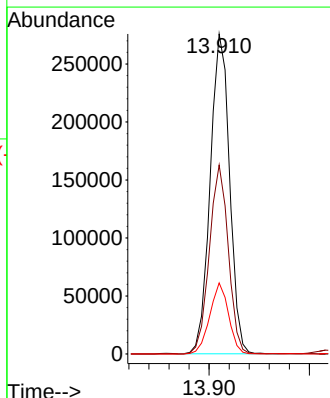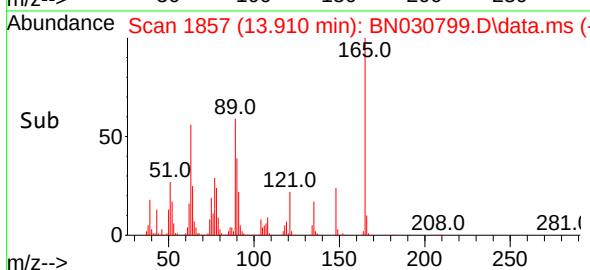

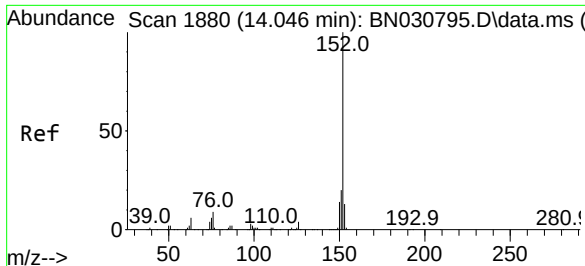

#50
Acenaphthylene
Concen: 39.745 ng/ul
RT: 14.045 min Scan# 1880
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS

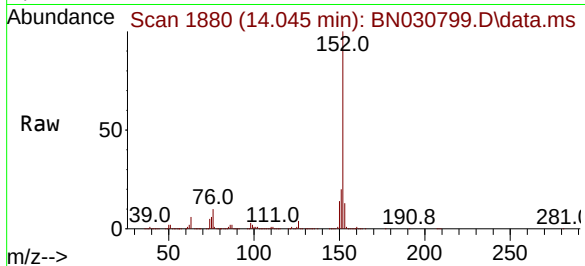

Tgt Ion:152 Resp: 2200640
Ion Ratio Lower Upper
152 100
151 19.9 15.8 23.8
153 12.8 10.7 16.1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

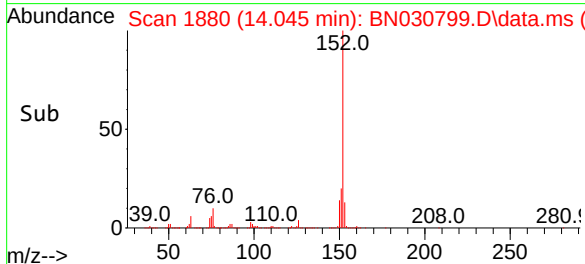




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024

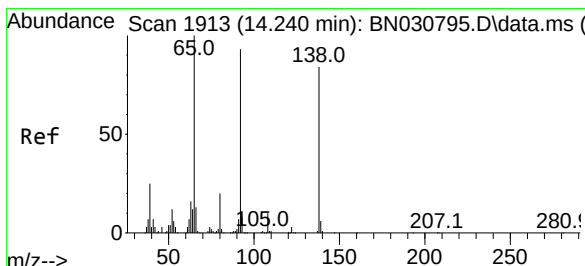

#51
3-Nitroaniline
Concen: 48.029 ng/ul
RT: 14.239 min Scan# 1913
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11

Tgt Ion:138 Resp: 406938
Ion Ratio Lower Upper
138 100
108 10.9 9.6 14.4
92 108.1 89.6 134.4

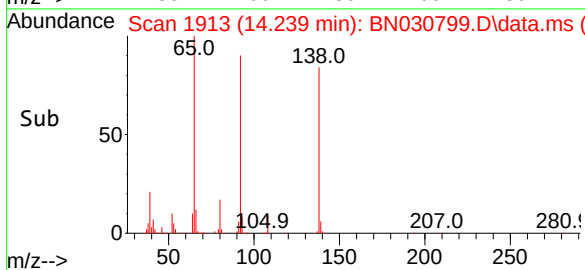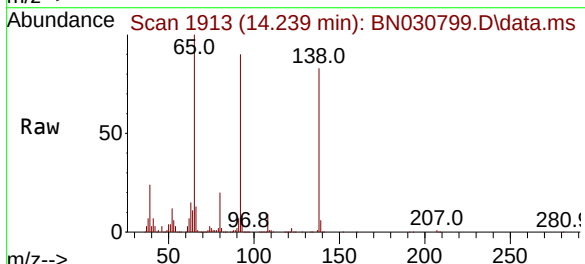





#52
 Acenaphthene
 Concen: 39.353 ng/ul
 RT: 14.387 min Scan# 1938
 Delta R.T. -0.000 min
 Lab File: BN030799.D
 Acq: 09 Apr 2024 21:11

Instrument : BNA_N
 ClientSampleId : E0MC0MS

Tgt Ion:153 Resp: 145205



Ion	Ratio	Lower	Upper
153	100		
152	47.1	37.6	56.4
154	88.7	70.3	105.5

Manual Integrations
APPROVED
 Reviewed By :Yogesh Patel 04/10/2024
 Supervised By :mohammad ahmed 04/10/2024

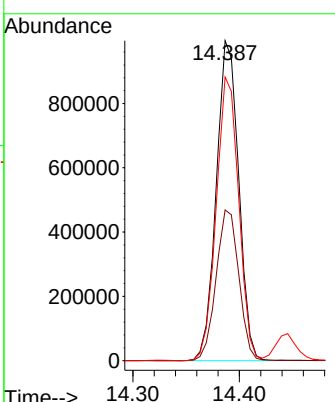

04/10/2024
 Supervised By :mohammad ahmed




04/10/2024




#53
 2,4-Dinitrophenol
 Concen: 48.254 ng/ul
 RT: 14.445 min Scan# 1948
 Delta R.T. 0.006 min
 Lab File: BN030799.D
 Acq: 09 Apr 2024 21:11

Tgt Ion:184 Resp: 176922


Ion	Ratio	Lower	Upper
184	100		
63	59.8	49.9	74.9
154	67.2	49.5	74.3

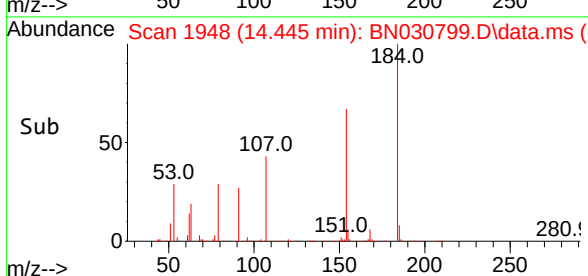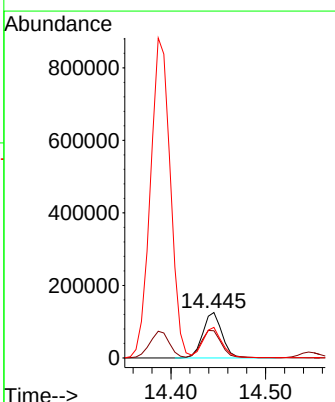



#55
4-Nitrophenol
Concen: 10.467 ng/ul
RT: 14.545 min Scan# 1965
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11

Instrument :
BNA_N
ClientSampleId :
EOMC0MS





Tgt Ion:109 Resp: 66112

Ion	Ratio	Lower	Upper
109	100		
139	137.4	111.8	167.6
65	131.2	98.7	148.1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

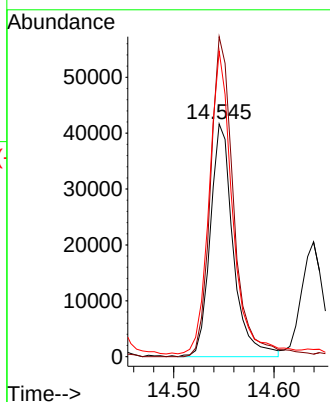

04/10/2024
Supervised By :mohammad
ahmed




04/10/2024




#56
Dibenzofuran
Concen: 40.112 ng/ul
RT: 14.728 min Scan# 1996
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11

Tgt Ion:168 Resp: 2057382


Ion	Ratio	Lower	Upper
168	100		
139	39.9	30.2	45.4

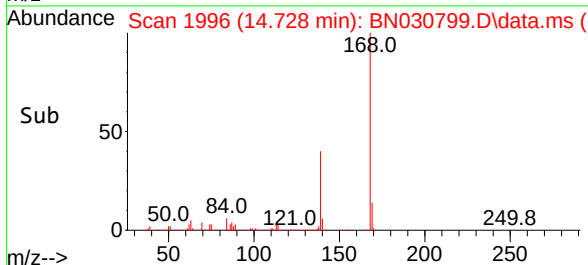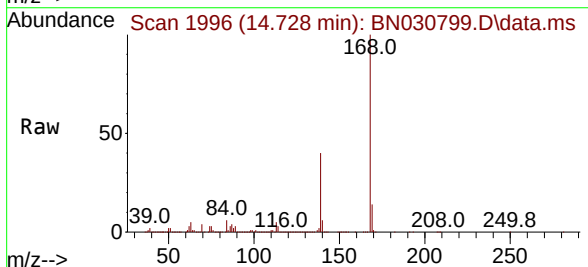



#57
2,4-Dinitrotoluene
Concen: 48.407 ng/ul
RT: 14.698 min Scan# 1991
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion:165 Resp: 564154
Ion Ratio Lower Upper
165 100
63 41.4 34.7 52.1
182 3.0 2.4 3.6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024






04/10/2024
Supervised By :mohammad
ahmed


04/10/2024



#58
2,3,4,6-Tetrachlorophenol
Concen: 46.063 ng/ul
RT: 14.951 min Scan# 2034
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11


Tgt Ion:232 Resp: 434945
Ion Ratio Lower Upper
232 100
131 48.2 36.6 55.0
130 2.5 2.2 3.2
166 32.2 26.0 39.0

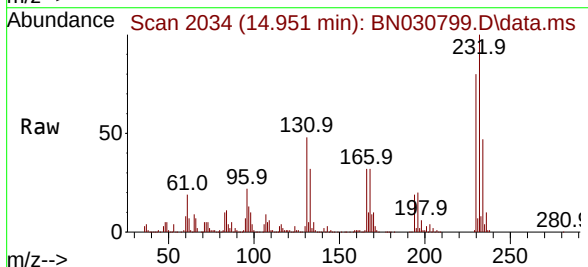

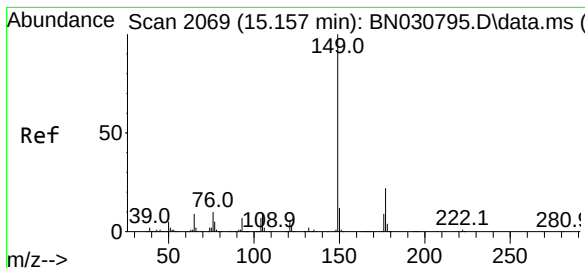

#59
Diethylphthalate
Concen: 42.267 ng/ul
RT: 15.157 min Scan# 2069
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS

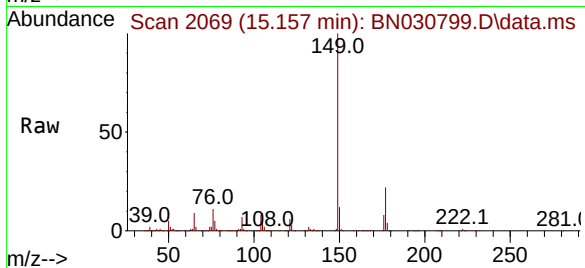

Tgt Ion:149 Resp: 1848709
Ion Ratio Lower Upper
149 100
177 21.7 17.4 26.2
150 12.4 9.8 14.8


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

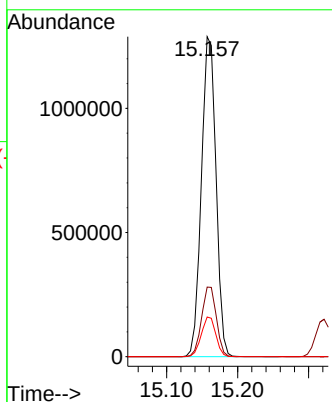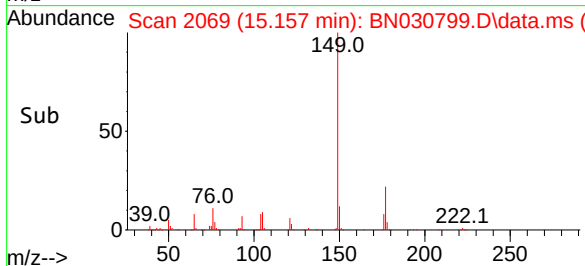




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024

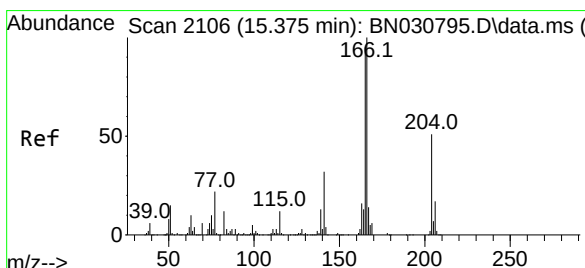

#61
Fluorene
Concen: 40.829 ng/ul
RT: 15.375 min Scan# 2106
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11


Tgt Ion:166 Resp: 1664535
Ion Ratio Lower Upper
166 100
165 97.5 78.2 117.4
167 13.6 11.0 16.4

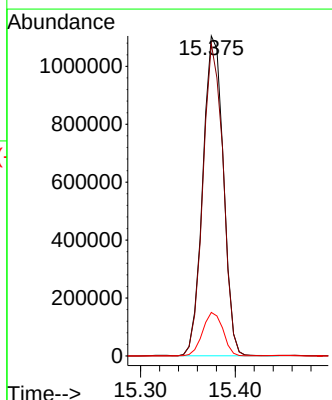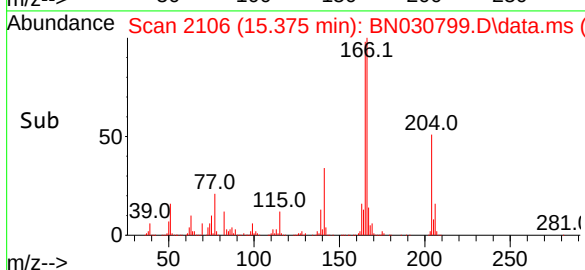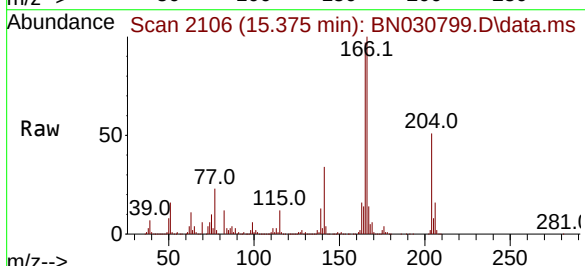



#62
4-Chlorophenyl-phenylether
Concen: 39.453 ng/ul
RT: 15.375 min Scan# 2106
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion:204 Resp: 789132
Ion Ratio Lower Upper
204 100
206 31.6 25.8 38.6
141 65.7 49.1 73.7


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

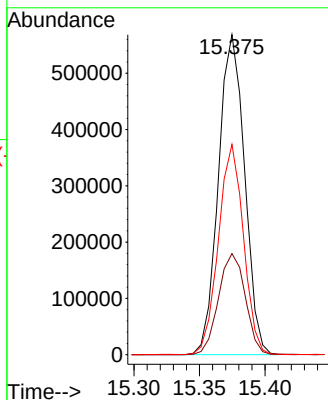




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024



#63
4-Nitroaniline
Concen: 53.472 ng/ul
RT: 15.410 min Scan# 2112
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11


Tgt Ion:138 Resp: 440455
Ion Ratio Lower Upper
138 100
92 49.5 39.7 59.5
108 78.0 62.6 94.0

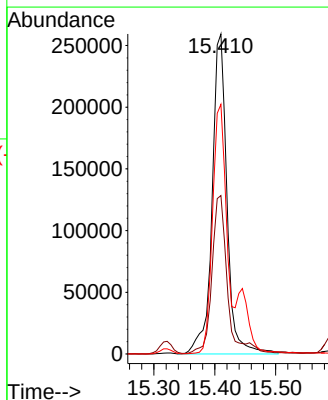



#66
4,6-Dinitro-2-methylphenol
Concen: 46.769 ng/ul
RT: 15.463 min Scan# 2121
Delta R.T. 0.012 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion:198 Resp: 302939
Ion Ratio Lower Upper
198 100
182 4.2 3.6 5.4
77 24.7 22.2 33.4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

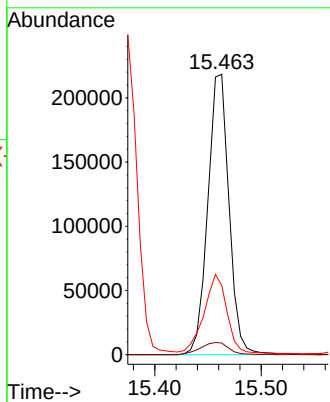




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024



#67
N-Nitrosodiphenylamine
Concen: 40.800 ng/ul
RT: 15.592 min Scan# 2143
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11


Tgt Ion:169 Resp: 1517490
Ion Ratio Lower Upper
169 100
168 68.2 51.9 77.9
167 36.7 29.0 43.4

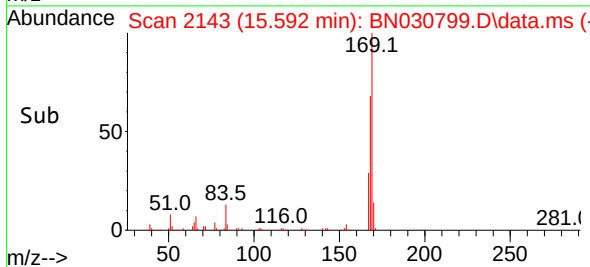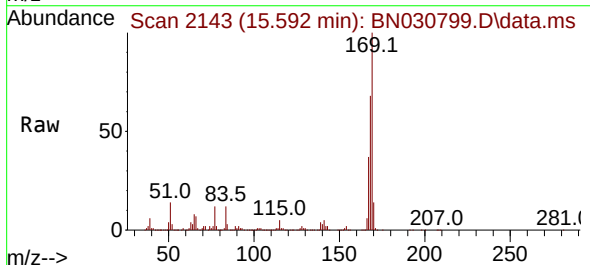



#68
4-Bromophenyl-phenylether
Concen: 41.420 ng/ul
RT: 16.269 min Scan# 21
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion:248 Resp: 537158
Ion Ratio Lower Upper
248 100
250 100.4 80.0 120.0
141 78.6 60.5 90.7


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024




04/10/2024
Supervised By :mohammad
ahmed



04/10/2024




#69
Hexachlorobenzene
Concen: 38.227 ng/ul
RT: 16.369 min Scan# 2275
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11

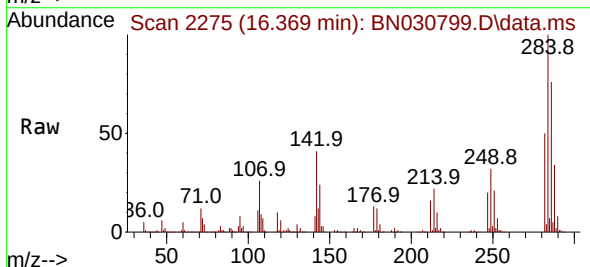


Tgt Ion:284 Resp: 583765
Ion Ratio Lower Upper
284 100
142 41.4 28.6 43.0
249 31.7 25.0 37.4

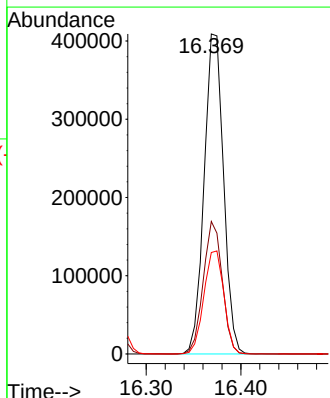



#70
Atrazine
Concen: 43.111 ng/ul
RT: 16.551 min Scan# 21
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion:200 Resp: 555769
Ion Ratio Lower Upper
200 100
173 25.9 21.5 32.3
215 47.8 37.8 56.8


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024






04/10/2024
Supervised By :mohammad
ahmed


04/10/2024



#71
Pentachlorophenol
Concen: 43.081 ng/ul
RT: 16.722 min Scan# 2335
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11


Tgt Ion:266 Resp: 387891
Ion Ratio Lower Upper
266 100
264 69.0 51.0 76.6
268 68.5 52.5 78.7

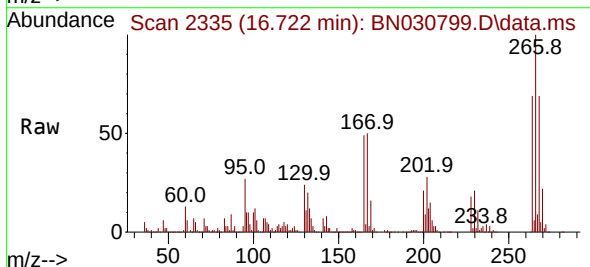



#72
Phenanthrene
Concen: 40.749 ng/u1
RT: 17.116 min Scan# 2402
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion:178 Resp: 285925
Ion Ratio Lower Upper
178 100
179 15.1 12.4 18.6
176 19.4 15.0 22.6


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

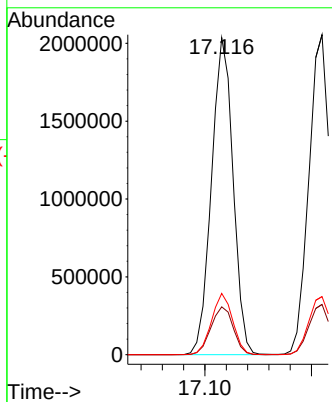




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024



#74
Anthracene
Concen: 40.783 ng/u1
RT: 17.210 min Scan# 2418
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11


Tgt Ion:178 Resp: 2892832
Ion Ratio Lower Upper
178 100
179 15.7 12.0 18.0
176 18.2 15.0 22.4

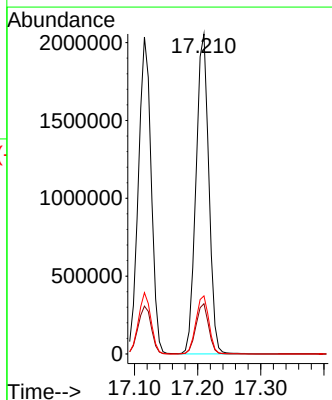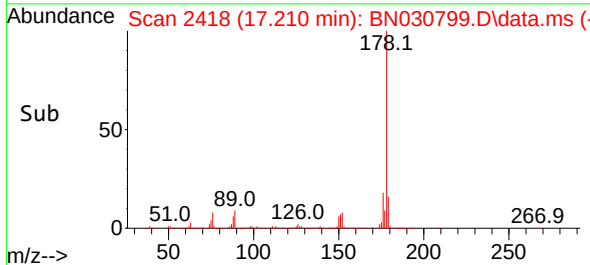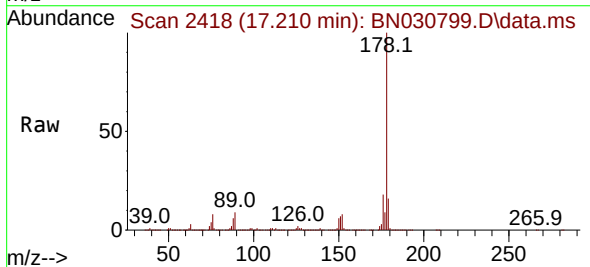



#75
1,2,3,4-Tetrachlorobenzene
Concen: 37.712 ng/uL
RT: 13.116 min Scan# 1722
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMC0MS



Tgt Ion:216 Resp: 632752
Ion Ratio Lower Upper
216 100
214 75.9 63.1 94.7
218 46.7 39.5 59.3


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024




04/10/2024
Supervised By :mohammad
ahmed



04/10/2024




#76
Pentachlorobenzene
Concen: 38.671 ng/uL
RT: 14.639 min Scan# 1981
Delta R.T. -0.000 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11

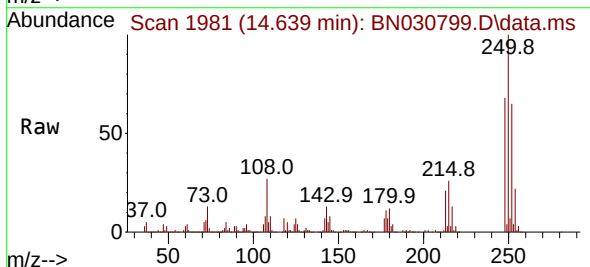


Tgt Ion:250 Resp: 659046
Ion Ratio Lower Upper
250 100
248 67.5 45.8 68.6
252 64.5 48.7 73.1

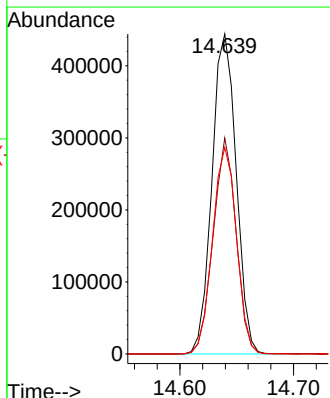



#77
 Carbazole
 Concen: 44.813 ng/ul
 RT: 17.480 min Scan# 2464
 Delta R.T. -0.000 min
 Lab File: BN030799.D
 Acq: 09 Apr 2024 21:11

Instrument :
 BNA_N
 ClientSampleId :
 E0MC0MS





Tgt Ion:167 Resp: 2787639

Ion	Ratio	Lower	Upper
167	100		
166	22.0	16.6	24.8
139	13.2	10.5	15.7


Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 04/10/2024
 Supervised By :mohammad ahmed 04/10/2024

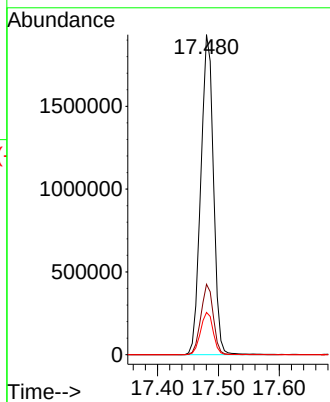


04/10/2024
 Supervised By :mohammad
 ahmed

04/10/2024






#78
 Di-n-butylphthalate
 Concen: 44.889 ng/ul
 RT: 18.045 min Scan# 2560
 Delta R.T. -0.000 min
 Lab File: BN030799.D
 Acq: 09 Apr 2024 21:11

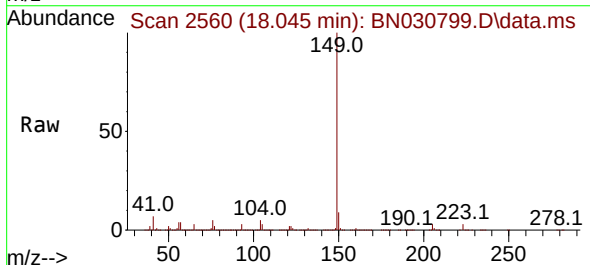

Tgt Ion:149 Resp: 3406468


Ion	Ratio	Lower	Upper
149	100		
150	9.3	7.2	10.8
104	5.2	4.1	6.1

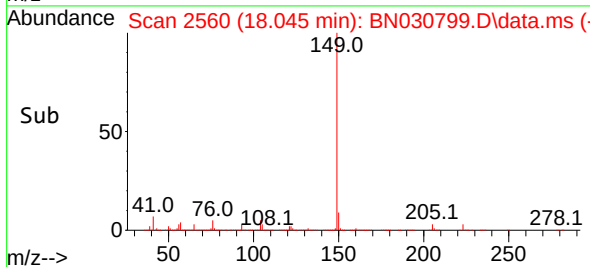



#80
Fluoranthene
Concen: 41.469 ng/ul
RT: 19.139 min Scan# 2746
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion:202 Resp: 3420580
Ion Ratio Lower Upper
202 100
101 12.3 9.0 13.6
100 9.4 6.8 10.2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024






04/10/2024
Supervised By :mohammad
ahmed


04/10/2024



#82
Pyrene
Concen: 41.361 ng/ul
RT: 19.504 min Scan# 2808
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11


Tgt Ion:202 Resp: 3603127
Ion Ratio Lower Upper
202 100
101 14.3 11.3 16.9
100 11.5 9.2 13.8

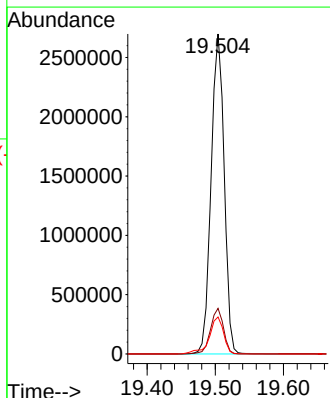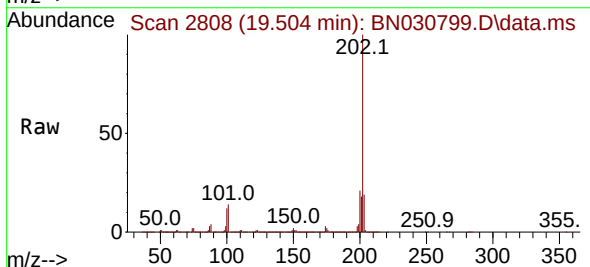



#83
Butylbenzylphthalate
Concen: 49.191 ng/ul
RT: 20.416 min Scan# 2963
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion:149 Resp: 163649
Ion Ratio Lower Upper
149 100
91 71.5 58.2 87.2
206 22.0 15.4 23.0


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

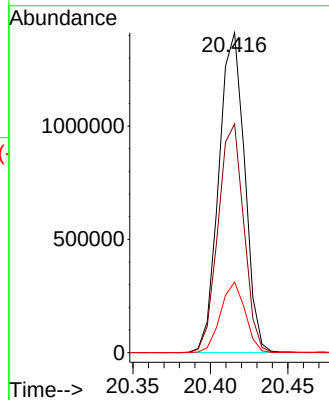




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024

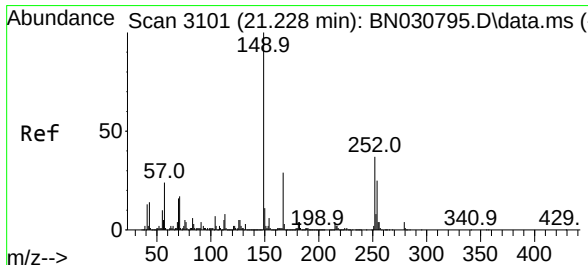

#84
3,3'-Dichlorobenzidine
Concen: 39.712 ng/ul
RT: 21.227 min Scan# 3101
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11


Tgt Ion:252 Resp: 941762
Ion Ratio Lower Upper
252 100
254 67.2 51.1 76.7
126 12.6 9.3 13.9

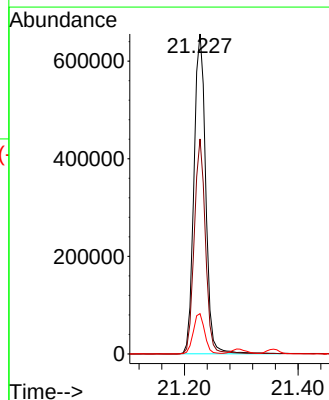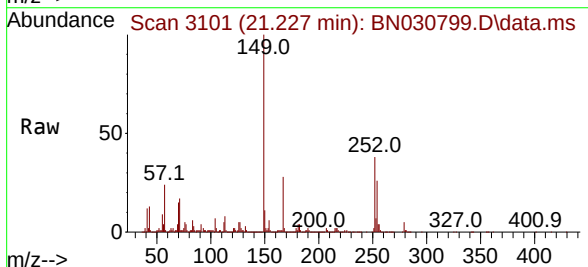



#85
Benzo(a)anthracene
Concen: 41.913 ng/ul
RT: 21.298 min Scan# 3113
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11



Instrument :
BNA_N
ClientSampleId :
EOMCOMS



Tgt Ion:228 Resp: 361016
Ion Ratio Lower Upper
228 100
229 20.4 15.8 23.6
226 27.0 20.5 30.7


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 04/10/2024
Supervised By :mohammad ahmed 04/10/2024

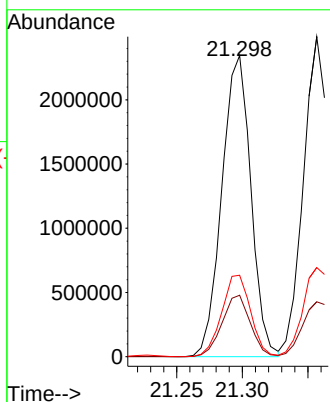




04/10/2024
Supervised By :mohammad
ahmed


04/10/2024



#86
Bis(2-ethylhexyl)phthalate
Concen: 46.987 ng/ul
RT: 21.227 min Scan# 3101
Delta R.T. 0.006 min
Lab File: BN030799.D
Acq: 09 Apr 2024 21:11

Tgt Ion:149 Resp: 2305232
Ion Ratio Lower Upper
149 100
167 27.6 21.4 32.0
279 4.6 3.5 5.3

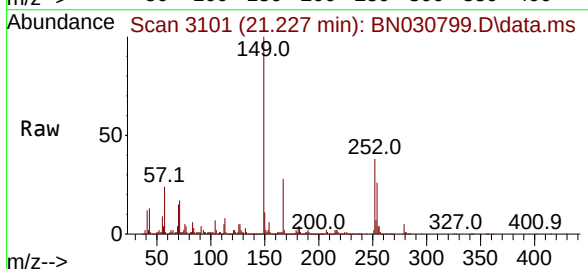



#87

Chrysene

Concen: 43.101 ng/ul

RT: 21.357 min Scan# 3123

Delta R.T. 0.006 min

Lab File: BN030799.D

Acq: 09 Apr 2024 21:11

Instrument :

BNA_N

ClientSampleId :

EOMCOMS

Tgt Ion:228 Resp: 3504120

Ion Ratio Lower Upper

228 100

226 27.9 24.3 36.5



229 17.2 15.9 23.9

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 04/10/2024



Supervised By :mohammad ahmed 04/10/2024



04/10/2024

Supervised By :mohammad
ahmed

04/10/2024



#89

Di-n-octyl phthalate

Concen: 45.686 ng/ul




RT: 22.339 min Scan# 3290


Delta R.T. 0.006 min

Lab File: BN030799.D

Acq: 09 Apr 2024 21:11

Tgt Ion:149 Resp: 4323968





#90

Benzo(b)fluoranthene

Concen: 42.099 ng/ul

RT: 23.321 min Scan# 3457

Delta R.T. 0.006 min

Lab File: BN030799.D

Acq: 09 Apr 2024 21:11

Instrument :

BNA_N

ClientSampleId :

EOMCOMS

Tgt Ion:252 Resp: 3702890

Ion Ratio Lower Upper

252 100

253 22.0 16.7 25.1



125 11.1 8.5 12.7

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 04/10/2024



Supervised By :mohammad ahmed 04/10/2024

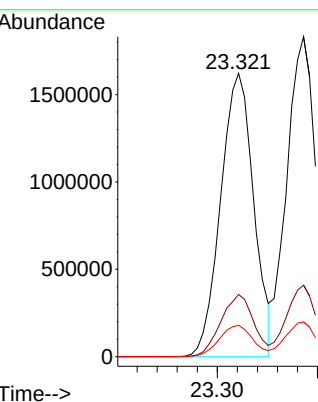

04/10/2024

Supervised By :mohammad
ahmed

04/10/2024



#91

Benzo(k)fluoranthene

Concen: 41.749 ng/ul

RT: 23.386 min Scan# 3468

Delta R.T. 0.012 min

Lab File: BN030799.D

Acq: 09 Apr 2024 21:11




Tgt Ion:252 Resp: 3729248


Ion Ratio Lower Upper

252 100

253 22.4 16.9 25.3

125 10.9 8.5 12.7

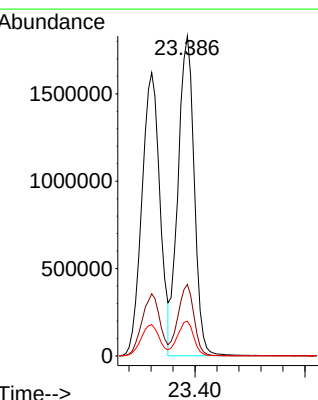



#93

Benzo(a)pyrene

Concen: 37.763 ng/u1

RT: 24.115 min Scan# 3

Delta R.T. 0.012 min

Lab File: BN030799.D


Acq: 09 Apr 2024 21:11

Instrument :

BNA_N

ClientSampleId :

EOMCOMS

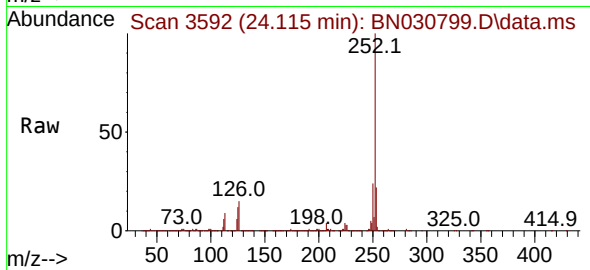

Tgt Ion:252 Resp: 3137650

Ion Ratio Lower Upper

252 100

253 22.4 16.7 25.1



125 11.8 9.6 14.4

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 04/10/2024


Supervised By :mohammad ahmed 04/10/2024

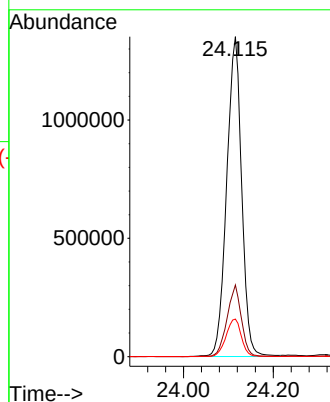

04/10/2024

Supervised By :mohammad
ahmed

04/10/2024



#94

Indeno(1,2,3-cd)pyrene

Concen: 44.291 ng/u1

RT: 27.545 min Scan# 4175

Delta R.T. 0.012 min

Lab File: BN030799.D

Acq: 09 Apr 2024 21:11




Tgt Ion:276 Resp: 3978050


Ion Ratio Lower Upper

276 100

138 21.8 17.8 26.8

277 24.1 18.4 27.6

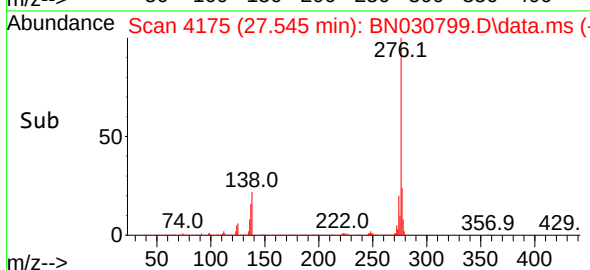



#95

Dibenzo(a,h)anthracene

Concen: 42.255 ng/ul

RT: 27.603 min Scan# 4185

Delta R.T. 0.018 min

Lab File: BN030799.D


Acq: 09 Apr 2024 21:11

Instrument :

BNA_N

ClientSampleId :

EOMCOMS

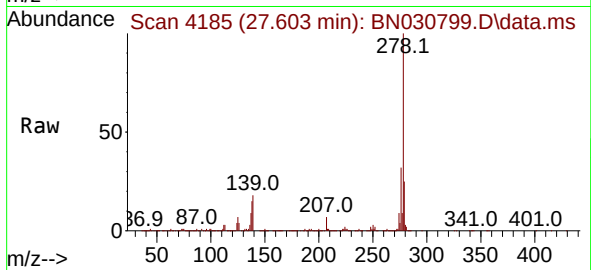

Tgt Ion:278 Resp: 319490

Ion Ratio Lower Upper

278 100

139 17.9 13.2 19.8



279 24.6 17.4 26.2

Manual Integrations

APPROVED

Reviewed By :Yogesh Patel 04/10/2024


Supervised By :mohammad ahmed 04/10/2024

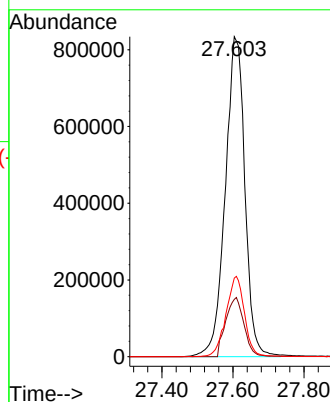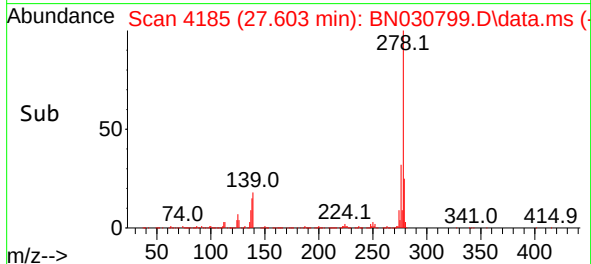

04/10/2024

Supervised By :mohammad
ahmed

04/10/2024



#96

Benzo(g,h,i)perylene

Concen: 42.044 ng/ul m

RT: 28.574 min Scan# 4350

Delta R.T. 0.012 min

Lab File: BN030799.D

Acq: 09 Apr 2024 21:11

Tgt Ion:276 Resp: 2964560

Ion Ratio Lower Upper

276 100

138 24.0 19.3 28.9

277 24.3 20.1 30.1

