

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
 Data File : BN030796.D
 Acq On : 09 Apr 2024 19:13
 Operator : MA/JU
 Sample : PB160094BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK094

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030796.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	41	rVB	41560	56323	0.97%	0.100%
2	3.593	100	103	124	rBV	605090	1006463	17.35%	1.791%
3	3.911	153	157	162	rBV4	8699	13935	0.24%	0.025%
4	6.852	650	657	672	rBV	747991	1177059	20.30%	2.094%
5	7.022	679	686	697	rVB	636526	984061	16.97%	1.751%
6	7.211	711	718	732	rBV	748020	1197061	20.64%	2.130%
7	7.681	790	798	810	rBV	631134	984295	16.97%	1.751%
8	8.381	908	917	931	rBV	966651	1590309	27.42%	2.829%
9	8.834	987	994	1005	rBV	767780	1241036	21.40%	2.208%
10	9.552	1109	1116	1128	rBV	611646	992202	17.11%	1.765%
11	10.087	1198	1207	1218	rBV	985301	1679634	28.96%	2.988%
12	10.463	1263	1271	1282	rBV	969380	1592592	27.46%	2.833%
13	10.604	1286	1295	1316	rBV	1234580	2113139	36.44%	3.759%
14	12.057	1537	1542	1548	rVB	17836	28852	0.50%	0.051%
15	13.222	1735	1740	1747	rVB3	8244	13327	0.23%	0.024%
16	13.740	1821	1828	1842	rBV	2101380	2849396	49.13%	5.069%
17	14.016	1868	1875	1887	rBV2	2286107	3409398	58.79%	6.066%
18	14.322	1921	1927	1936	rBV	1688284	2396583	41.32%	4.264%
19	14.528	1954	1962	1984	rBV	669893	1336732	23.05%	2.378%
20	15.322	2090	2097	2110	rBV	2924891	4372011	75.38%	7.778%
21	15.440	2110	2117	2127	rVV	780775	1106856	19.08%	1.969%
22	15.557	2133	2137	2143	rVB3	14550	23609	0.41%	0.042%
23	16.104	2225	2230	2236	rVB4	11162	14999	0.26%	0.027%
24	16.857	2353	2358	2364	rVB5	4392	8938	0.15%	0.016%
25	17.075	2388	2395	2405	rBV	2074268	3042048	52.45%	5.412%
26	17.169	2405	2411	2431	rVB2	3438315	4975430	85.79%	8.852%
27	19.033	2724	2728	2733	rBV2	41433	55734	0.96%	0.099%
28	19.104	2736	2740	2747	rVV	35246	49300	0.85%	0.088%
29	19.475	2796	2803	2812	rBV	4205126	5799715	100.00%	10.318%
30	21.310	3109	3115	3123	rBV	2352959	3341915	57.62%	5.946%
31	24.045	3571	3580	3592	rBV2	2326073	5468800	94.29%	9.729%
32	24.245	3606	3614	3628	rVB	1346835	3286965	56.67%	5.848%




Sum of corrected areas: 56208717

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030796.D
Acq On : 09 Apr 2024 19:13
Operator : MA/JU
Sample : PB160094BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK094

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

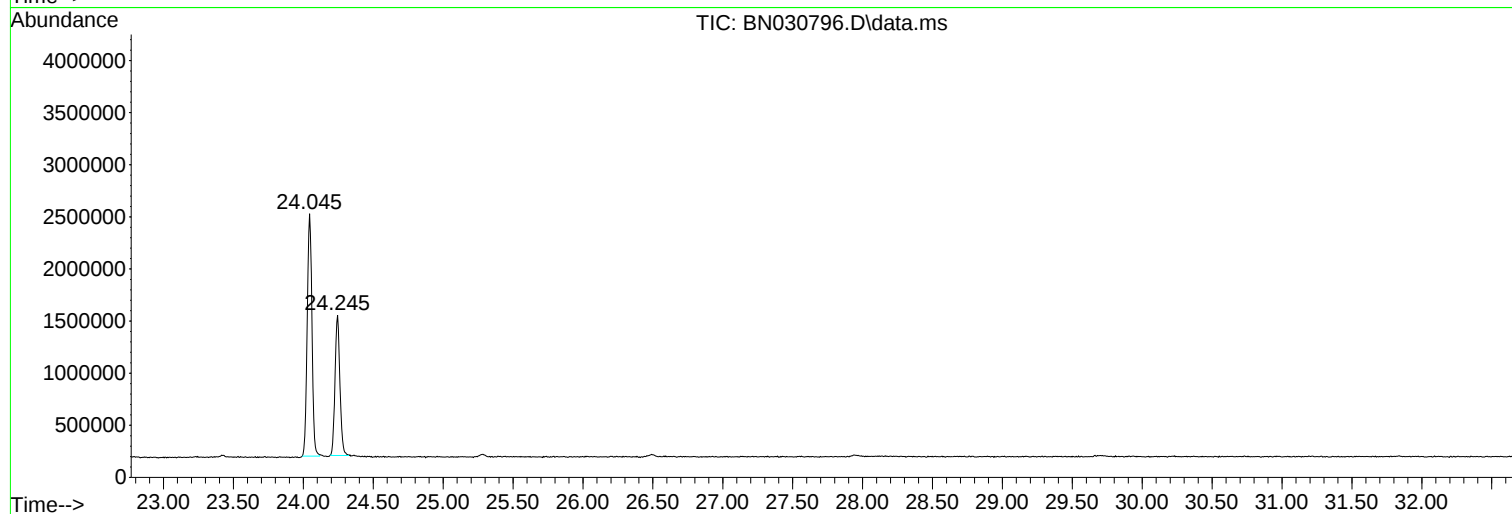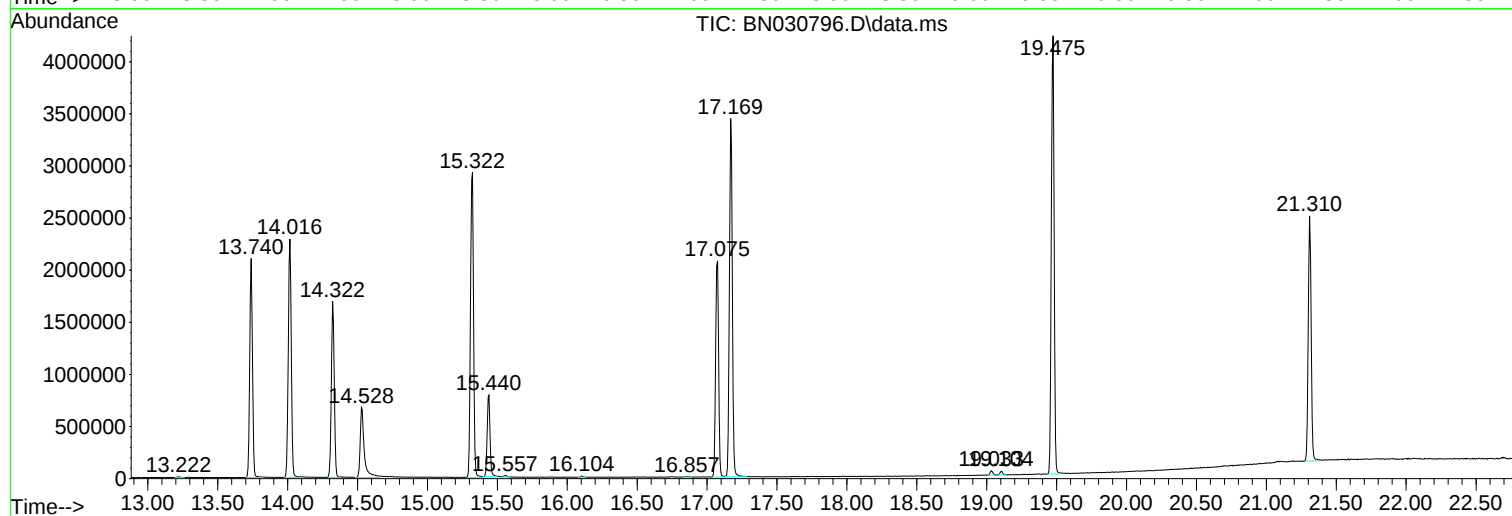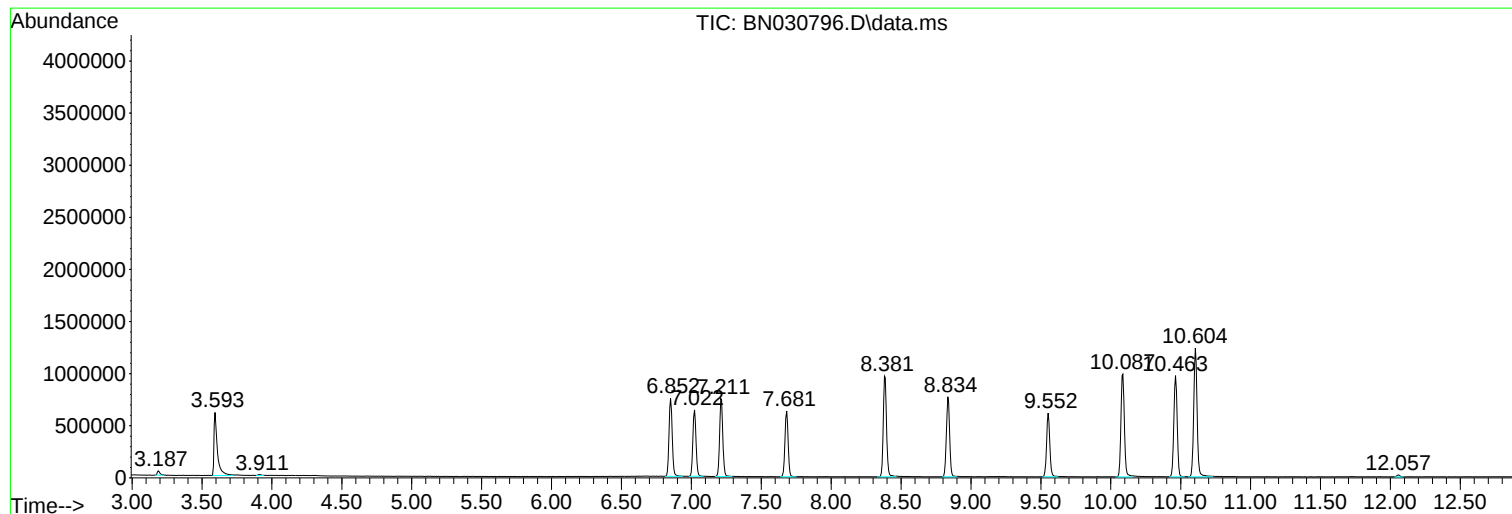

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030796.D
Acq On : 09 Apr 2024 19:13
Operator : MA/JU
Sample : PB160094BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK094

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030796.D
Acq On : 09 Apr 2024 19:13
Operator : MA/JU
Sample : PB160094BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK094

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc