

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
 Data File : BN030797.D
 Acq On : 09 Apr 2024 19:52
 Operator : MA/JU
 Sample : PB160103BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK103

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	43	rVB	39796	57024	0.99%	0.103%
2	3.593	99	103	123	rBV	606028	1011243	17.52%	1.824%
3	6.852	650	657	672	rVB	767479	1170060	20.27%	2.110%
4	7.022	680	686	702	rVB	642139	986871	17.10%	1.780%
5	7.216	712	719	732	rBV	722510	1180223	20.45%	2.129%
6	7.681	791	798	810	rBV	602548	942475	16.33%	1.700%
7	8.381	911	917	930	rBV	949627	1558264	27.00%	2.811%
8	8.834	986	994	1004	rBV	760337	1220630	21.15%	2.202%
9	9.551	1109	1116	1125	rBV	596935	964549	16.71%	1.740%
10	10.087	1199	1207	1223	rBV	968469	1658220	28.73%	2.991%
11	10.463	1263	1271	1281	rBV	918378	1535484	26.60%	2.770%
12	10.604	1287	1295	1316	rBV	1216972	2099856	36.38%	3.788%
13	12.057	1536	1542	1547	rBV2	16109	26474	0.46%	0.048%
14	13.222	1733	1740	1745	rBV4	12260	20432	0.35%	0.037%
15	13.739	1821	1828	1840	rBV	2037801	2795762	48.44%	5.043%
16	14.016	1868	1875	1889	rBV	2357808	3378044	58.52%	6.093%
17	14.322	1920	1927	1935	rBV	1580452	2291258	39.70%	4.133%
18	14.528	1956	1962	1981	rBV	684199	1291448	22.37%	2.329%
19	15.322	2089	2097	2110	rBV	2901385	4321187	74.86%	7.794%
20	15.439	2110	2117	2131	rVV	805055	1119593	19.40%	2.019%
21	15.557	2133	2137	2142	rVB3	14913	22028	0.38%	0.040%
22	16.104	2227	2230	2239	rVB4	11129	14386	0.25%	0.026%
23	16.857	2355	2358	2363	rBV3	4912	6333	0.11%	0.011%
24	17.075	2388	2395	2404	rBV	1994810	2918709	50.57%	5.265%
25	17.169	2405	2411	2427	rVV2	3417436	4890984	84.74%	8.822%
26	17.975	2544	2548	2554	rBV8	2821	6799	0.12%	0.012%
27	19.033	2724	2728	2733	rBV	42352	56676	0.98%	0.102%
28	19.104	2736	2740	2746	rVV	33481	47317	0.82%	0.085%
29	19.469	2796	2802	2817	rBV	4044112	5772014	100.00%	10.411%
30	21.310	3109	3115	3126	rBV	2229127	3245186	56.22%	5.853%
31	24.045	3571	3580	3597	rVB2	2254609	5520825	95.65%	9.958%
32	24.245	3605	3614	3629	rVB	1290668	3310837	57.36%	5.972%




Sum of corrected areas: 55441191

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030797.D
Acq On : 09 Apr 2024 19:52
Operator : MA/JU
Sample : PB160103BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK103

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

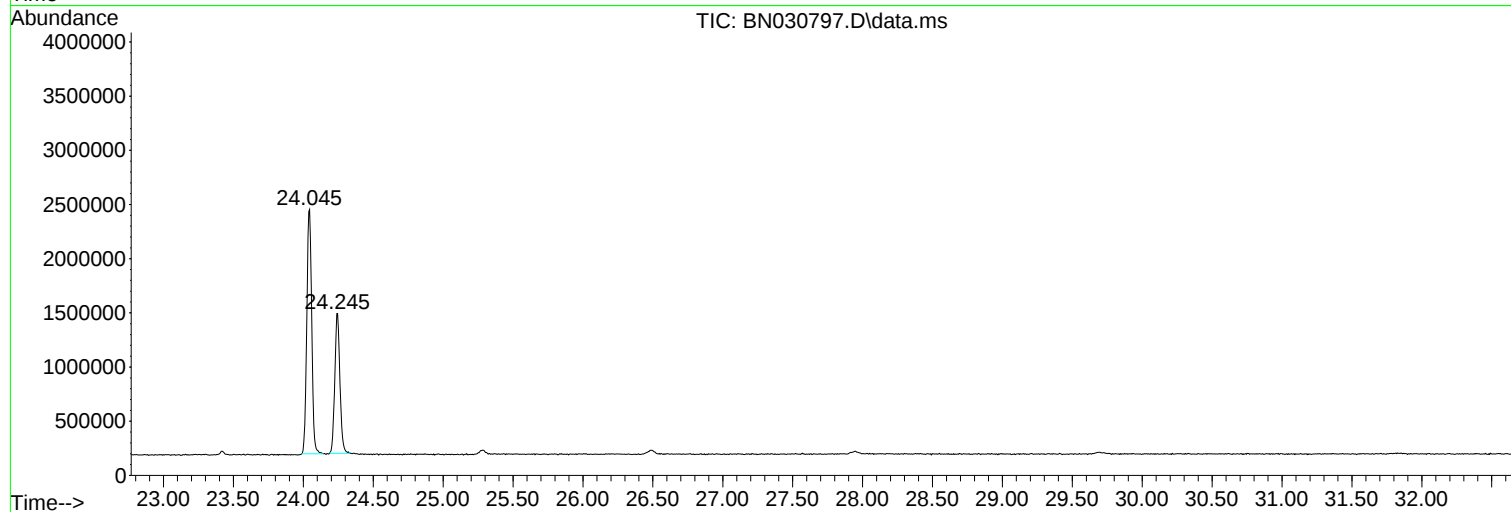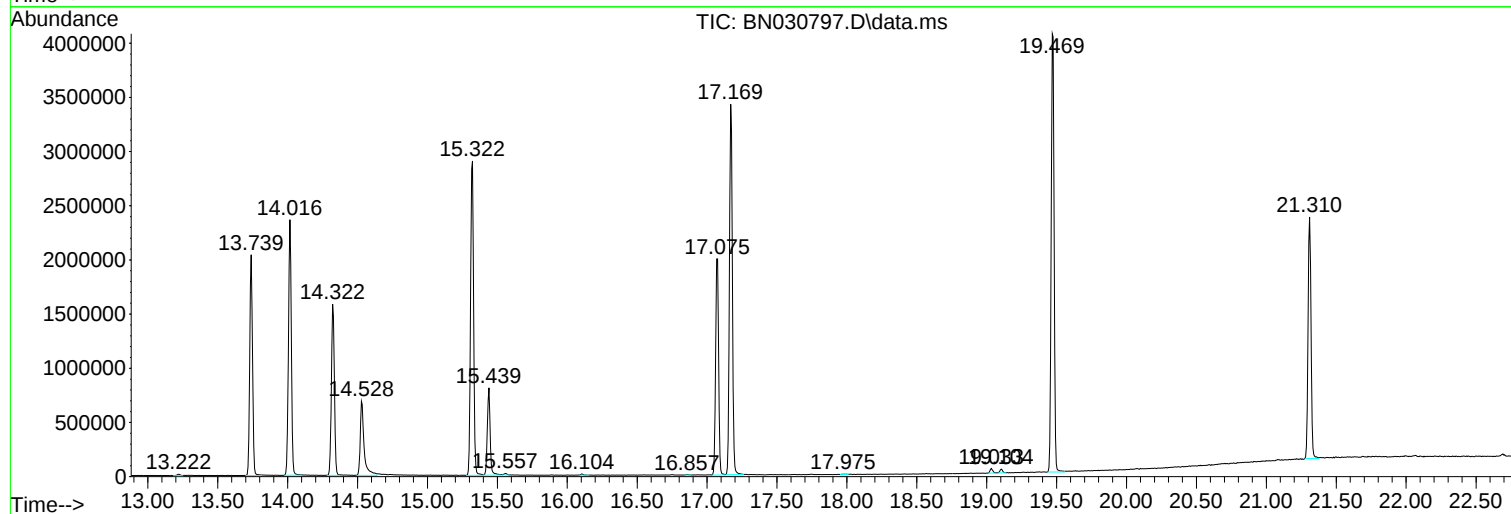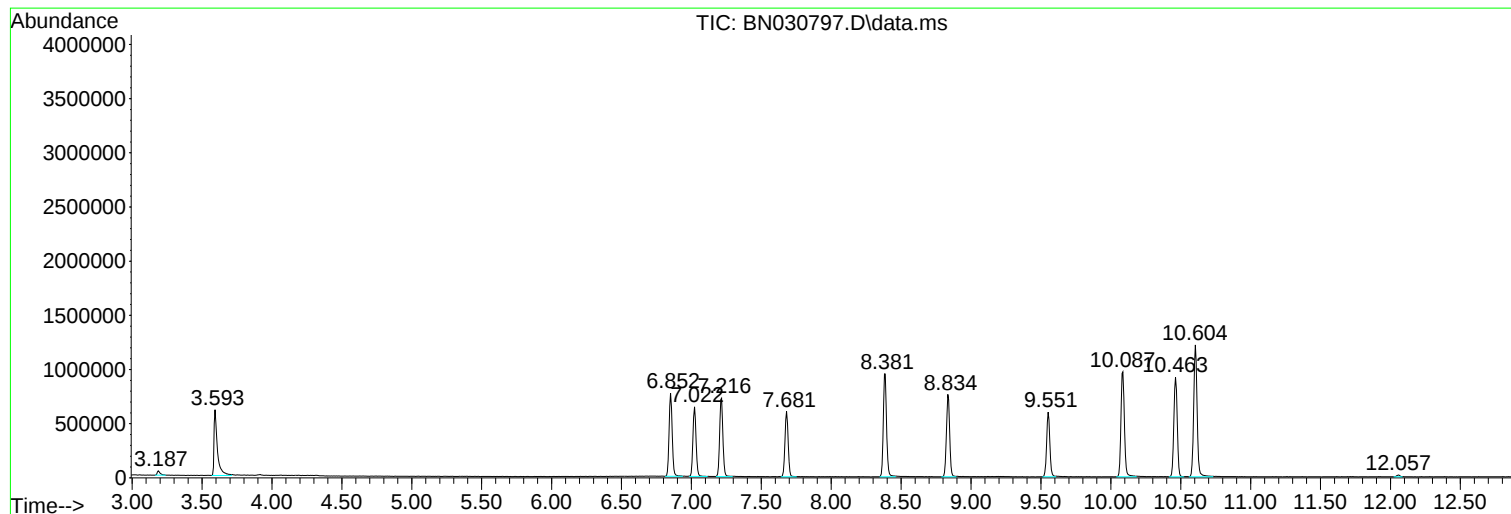

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030797.D
Acq On : 09 Apr 2024 19:52
Operator : MA/JU
Sample : PB160103BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK103

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030797.D
Acq On : 09 Apr 2024 19:52
Operator : MA/JU
Sample : PB160103BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK103

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc