

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
 Data File : BN030798.D
 Acq On : 09 Apr 2024 20:32
 Operator : MA/JU
 Sample : P2013-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0MC0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030798.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	31	34	43	rVB	23130	37470	0.54%	0.073%
2	3.599	102	104	120	rBV	161451	310433	4.44%	0.608%
3	3.911	155	157	162	rVB3	6793	8952	0.13%	0.018%
4	5.340	394	400	408	rBV	10343	22461	0.32%	0.044%
5	6.852	652	657	666	rVB	137668	220959	3.16%	0.433%
6	7.022	676	686	697	rBV	552793	879586	12.58%	1.724%
7	7.210	712	718	730	rBV	489472	810509	11.59%	1.589%
8	7.681	791	798	806	rBV	514738	820196	11.73%	1.608%
9	8.381	908	917	928	rBV	432472	708256	10.13%	1.388%
10	8.834	987	994	1006	rBV	656611	1088022	15.56%	2.133%
11	9.234	1059	1062	1068	rVB5	4701	8518	0.12%	0.017%
12	9.552	1109	1116	1127	rBV	492399	796407	11.39%	1.561%
13	9.957	1178	1185	1193	rBV2	8207	15162	0.22%	0.030%
14	10.087	1199	1207	1224	rBV	780190	1327972	19.00%	2.603%
15	10.463	1264	1271	1280	rBV	805247	1298945	18.58%	2.546%
16	10.604	1288	1295	1314	rBV	798583	1386989	19.84%	2.719%
17	12.057	1535	1542	1548	rBV2	14182	25862	0.37%	0.051%
18	12.669	1643	1646	1650	rBV4	6815	8918	0.13%	0.017%
19	12.928	1684	1690	1696	rBV4	11308	16815	0.24%	0.033%
20	13.222	1735	1740	1745	rBV4	12594	20505	0.29%	0.040%
21	13.740	1821	1828	1845	rBV	1973800	2677285	38.30%	5.248%
22	14.016	1863	1875	1891	rBV	2146877	3152300	45.09%	6.179%
23	14.322	1920	1927	1937	rBV	1343704	1948934	27.88%	3.820%
24	14.540	1958	1964	1980	rBV	82534	210830	3.02%	0.413%
25	14.981	2036	2039	2043	rBV6	7195	9418	0.13%	0.018%
26	15.128	2060	2064	2070	rBV5	7905	11488	0.16%	0.023%
27	15.322	2090	2097	2107	rBV	2809729	4235861	60.59%	8.303%
28	15.439	2111	2117	2134	rVV	742123	1091823	15.62%	2.140%
29	15.557	2134	2137	2143	rVB4	15192	23675	0.34%	0.046%
30	16.098	2226	2229	2235	rVB4	8627	13605	0.19%	0.027%
31	16.745	2336	2339	2344	rBV5	5211	7352	0.11%	0.014%
32	16.851	2352	2357	2361	rBV5	4300	7746	0.11%	0.015%
33	16.998	2377	2382	2386	rVB6	7504	9142	0.13%	0.018%
34	17.069	2388	2394	2405	rBV	1687494	2514447	35.97%	4.929%
35	17.169	2405	2411	2424	rVV	3512778	4991839	71.41%	9.785%
36	17.745	2504	2509	2515	rBV6	15697	20819	0.30%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030798.D
Acq On : 09 Apr 2024 20:32
Operator : MA/JU
Sample : P2013-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC0

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	17.969	2543	2547	2554	rBV	64170	93867	1.34%	0.184%
38	19.033	2724	2728	2734	rBV2	50925	70820	1.01%	0.139%
39	19.104	2736	2740	2744	rBV	40193	55484	0.79%	0.109%
40	19.257	2762	2766	2771	rBV5	35379	54948	0.79%	0.108%
41	19.475	2796	2803	2815	rBV	4470499	6362502	91.01%	12.471%
42	21.310	3109	3115	3127	rBV	2061846	3133922	44.83%	6.143%
43	24.045	3570	3580	3599	rVB	2859590	6990698	100.00%	13.703%
44	24.239	3605	3613	3635	rVB2	1370371	3514648	50.28%	6.889%




Sum of corrected areas: 51016390

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030798.D
Acq On : 09 Apr 2024 20:32
Operator : MA/JU
Sample : P2013-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

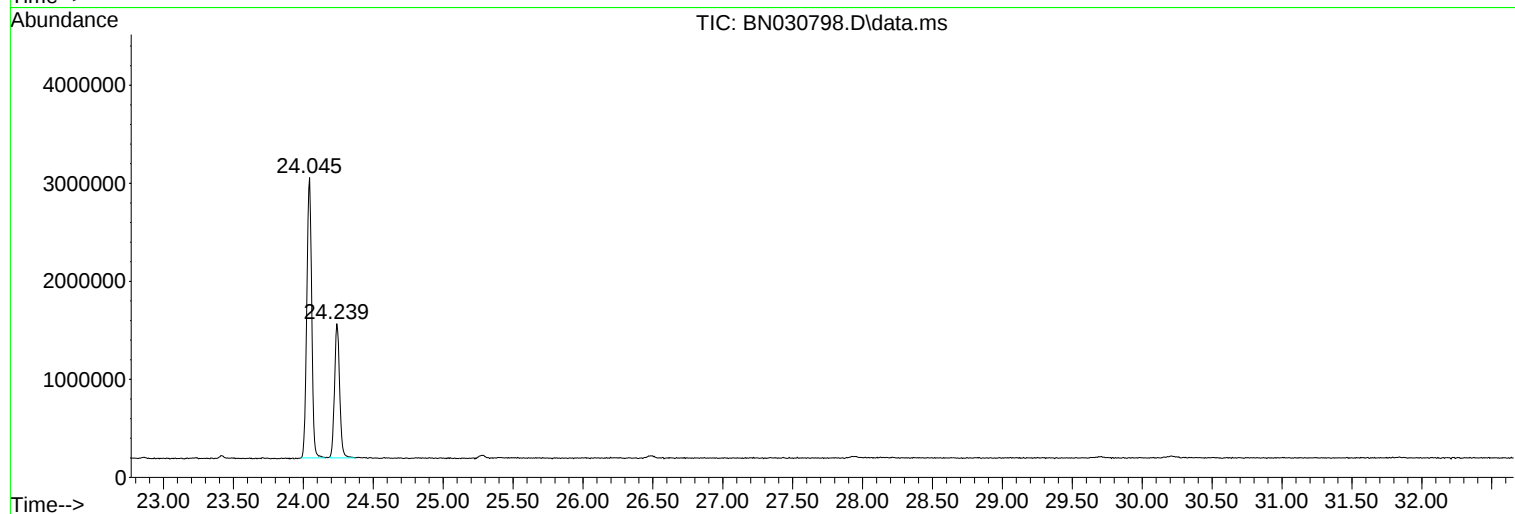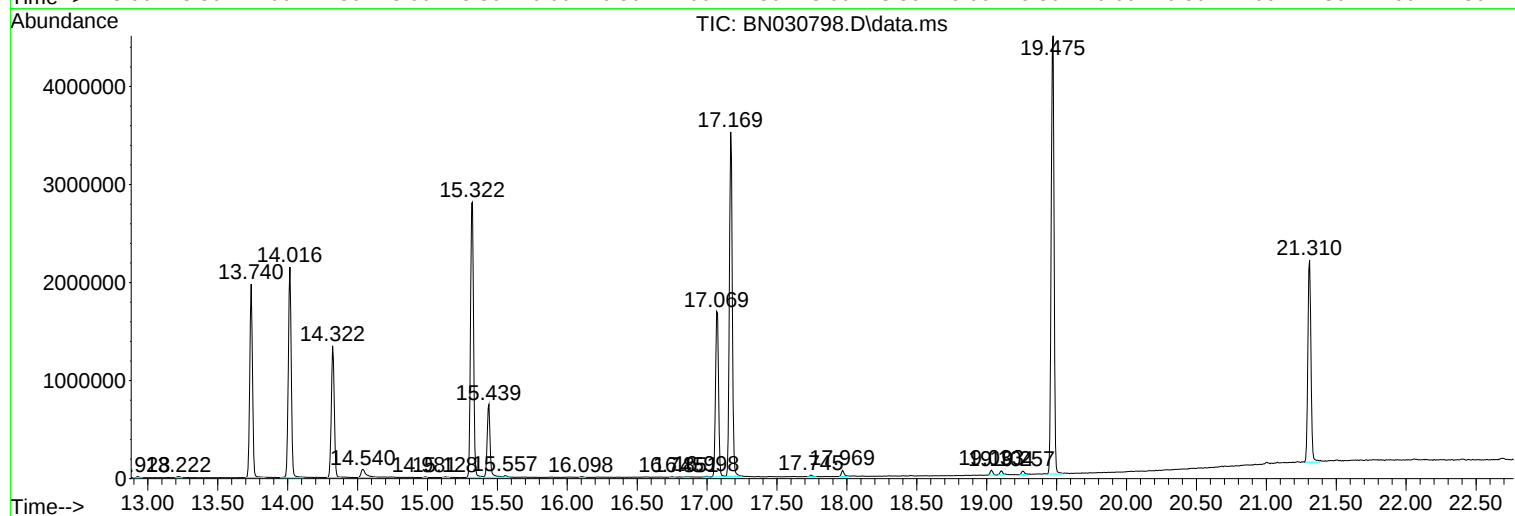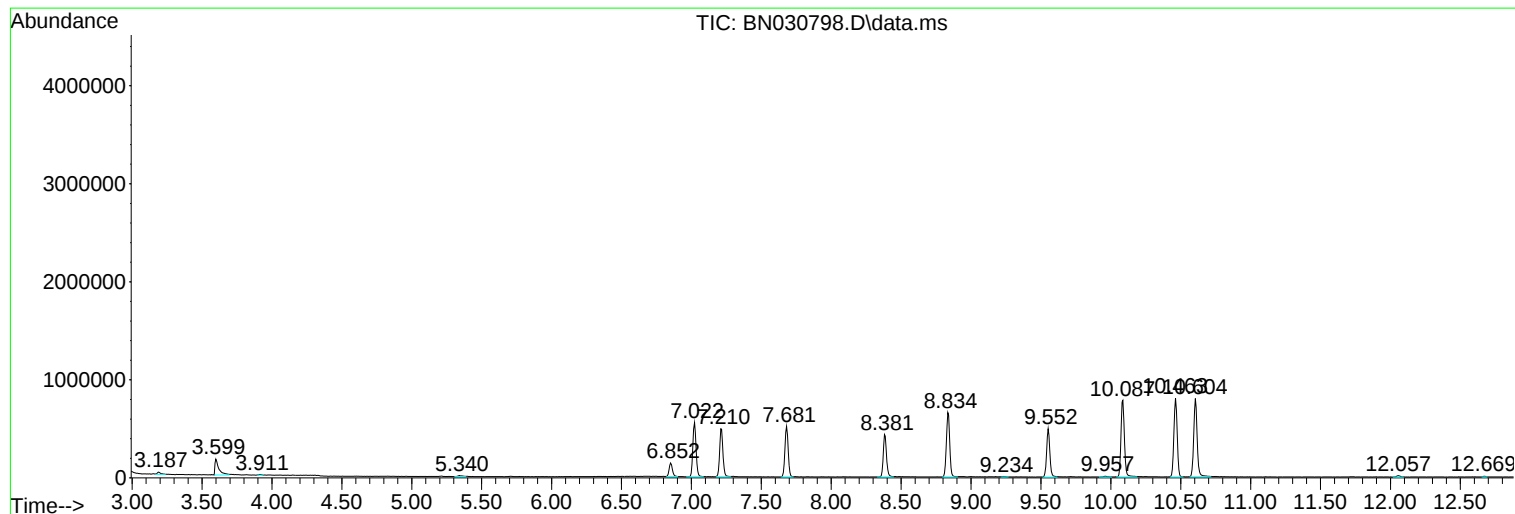

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030798.D
Acq On : 09 Apr 2024 20:32
Operator : MA/JU
Sample : P2013-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030798.D
Acq On : 09 Apr 2024 20:32
Operator : MA/JU
Sample : P2013-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc