

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
 Data File : BN030802.D
 Acq On : 09 Apr 2024 23:10
 Operator : MA/JU
 Sample : P2013-19
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0MC3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN030802.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	30	34	39	rBV	23593	33228	0.49%	0.063%
2	3.599	102	104	119	rBV	165404	292295	4.32%	0.550%
3	3.911	153	157	161	rBV2	7173	9786	0.14%	0.018%
4	5.211	375	378	384	rVB3	5889	7879	0.12%	0.015%
5	5.340	395	400	411	rVB	15047	34920	0.52%	0.066%
6	5.705	458	462	467	rBV3	6864	9643	0.14%	0.018%
7	6.852	651	657	666	rVB	137615	215259	3.18%	0.405%
8	7.022	679	686	699	rBV	612961	965132	14.25%	1.816%
9	7.211	711	718	729	rBV	547215	863736	12.75%	1.625%
10	7.681	791	798	806	rBV	538807	856609	12.65%	1.612%
11	8.381	911	917	930	rBV	453351	728423	10.76%	1.370%
12	8.834	987	994	1003	rBV	753152	1212427	17.90%	2.281%
13	9.552	1108	1116	1129	rBV	556005	901626	13.31%	1.696%
14	10.081	1197	1206	1218	rBV	844658	1432132	21.15%	2.694%
15	10.463	1264	1271	1281	rBV	843443	1394913	20.60%	2.624%
16	10.605	1288	1295	1308	rBV	813492	1415532	20.90%	2.663%
17	12.057	1537	1542	1547	rBV	15899	25894	0.38%	0.049%
18	13.216	1734	1739	1748	rVB3	13685	22506	0.33%	0.042%
19	13.740	1819	1828	1843	rBV	2183304	2948631	43.54%	5.547%
20	14.016	1867	1875	1893	rBV	2318195	3448716	50.93%	6.488%
21	14.322	1920	1927	1938	rBV	1458646	2109594	31.15%	3.969%
22	14.534	1957	1963	1981	rBV	75999	201006	2.97%	0.378%
23	14.745	1995	1999	2005	rVB9	6717	11833	0.17%	0.022%
24	15.316	2087	2096	2111	rBV	3184511	4639138	68.50%	8.728%
25	15.440	2111	2117	2133	rVV	811456	1194810	17.64%	2.248%
26	15.557	2133	2137	2143	rVB4	14708	25638	0.38%	0.048%
27	16.104	2226	2230	2234	rBV5	9615	14354	0.21%	0.027%
28	16.751	2336	2340	2345	rVB8	4609	7821	0.12%	0.015%
29	16.863	2354	2359	2365	rBV4	4488	8140	0.12%	0.015%
30	17.069	2388	2394	2405	rBV	1851275	2696906	39.82%	5.074%
31	17.169	2405	2411	2426	rVV2	3762410	5457205	80.58%	10.267%
32	17.469	2456	2462	2468	rBV8	7851	16917	0.25%	0.032%
33	17.745	2504	2509	2513	rVB7	6955	12358	0.18%	0.023%
34	17.969	2542	2547	2556	rBV2	52706	81322	1.20%	0.153%
35	18.404	2617	2621	2626	rVB7	16221	20151	0.30%	0.038%
36	18.457	2626	2630	2635	rBV8	4142	6834	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030802.D
Acq On : 09 Apr 2024 23:10
Operator : MA/JU
Sample : P2013-19
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC3

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Title : SVOA CALIBRATION

37	19.033	2723	2728	2733	rBV2	49961	72684	1.07%	0.137%
38	19.104	2736	2740	2745	rBV	48100	64633	0.95%	0.122%
39	19.257	2762	2766	2775	rBV4	49862	80373	1.19%	0.151%
40	19.469	2796	2802	2811	rBV	4702770	6604399	97.52%	12.425%
41	21.304	3109	3114	3127	rBV2	2156060	3035691	44.83%	5.711%
42	24.039	3570	3579	3594	rBV2	2836662	6772121	100.00%	12.740%
43	24.239	3605	3613	3627	rVB2	1297597	3202098	47.28%	6.024%




Sum of corrected areas: 53155313

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030802.D
Acq On : 09 Apr 2024 23:10
Operator : MA/JU
Sample : P2013-19
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

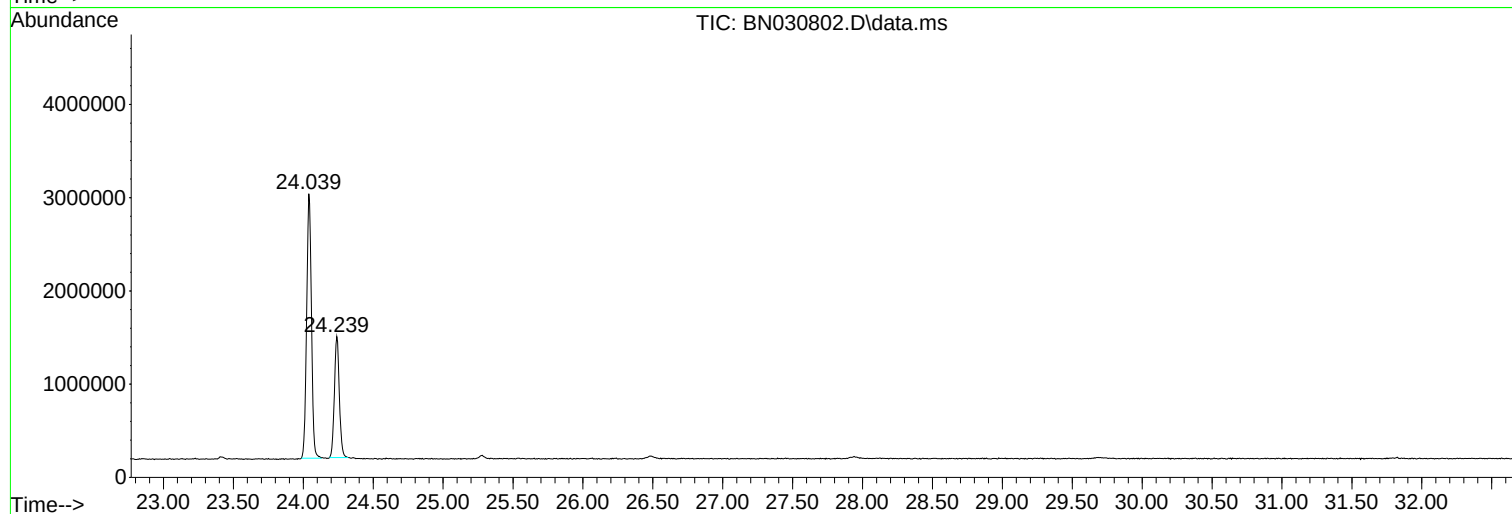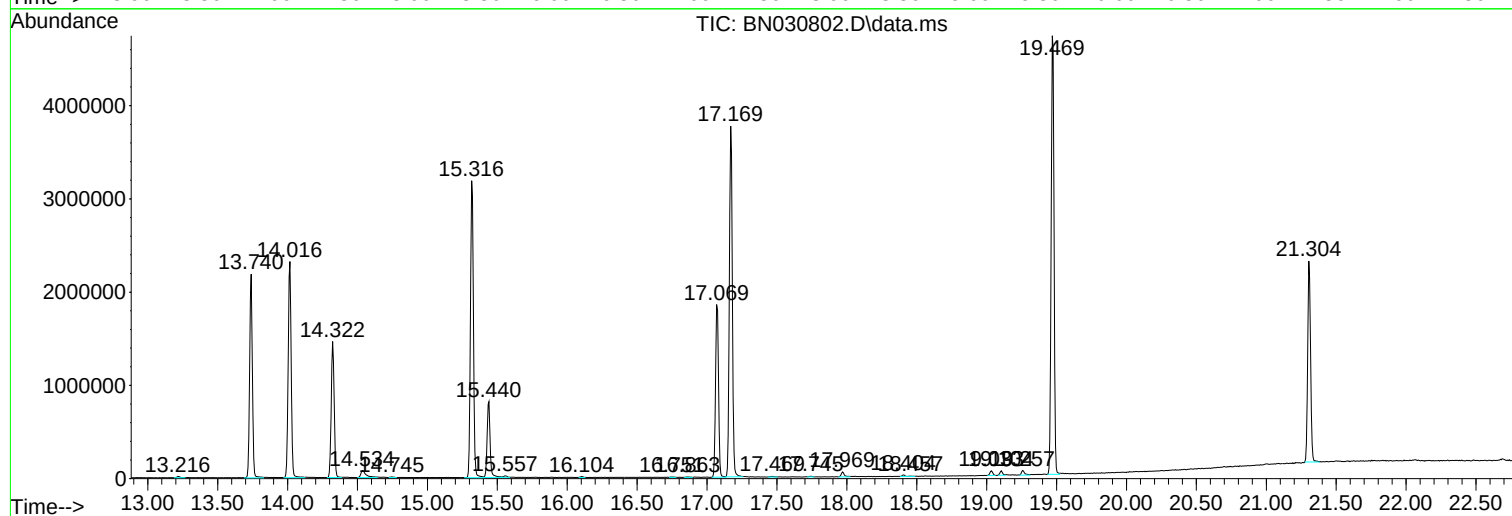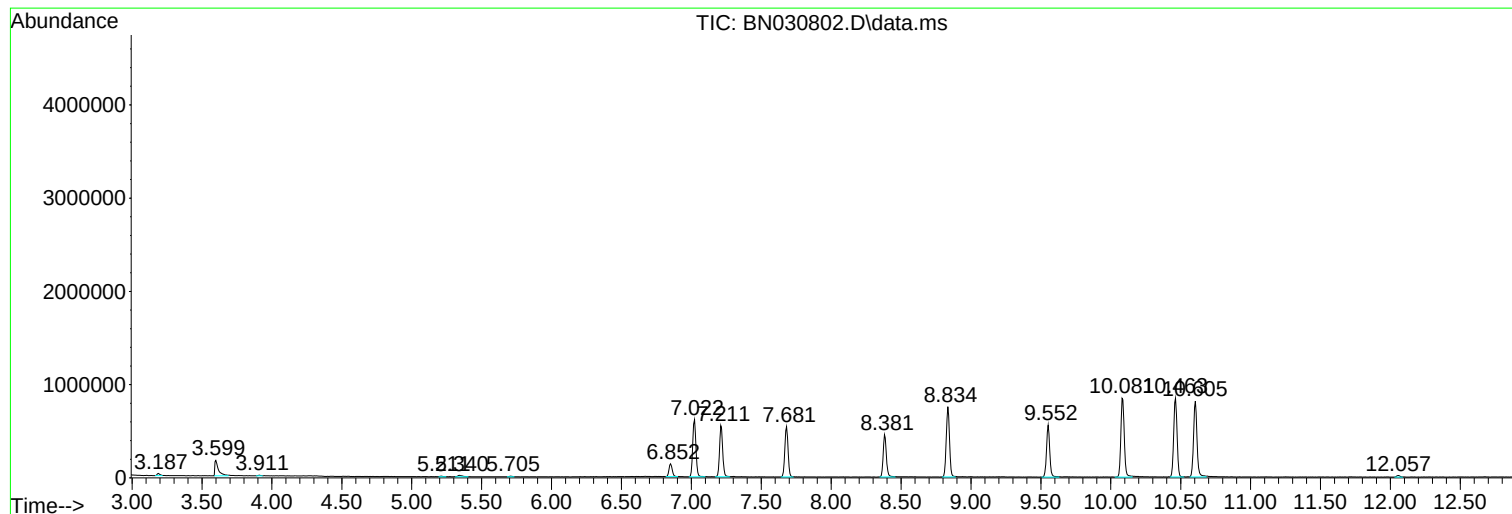

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030802.D
Acq On : 09 Apr 2024 23:10
Operator : MA/JU
Sample : P2013-19
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN040924\
Data File : BN030802.D
Acq On : 09 Apr 2024 23:10
Operator : MA/JU
Sample : P2013-19
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0MC3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN032824.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------